


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101118\
Data File : VN051801.D
Acq On : 11 Oct 2018 7:44
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101118W.M
Title : SW846 8260
Last Update : Fri Oct 12 09:51:20 2018

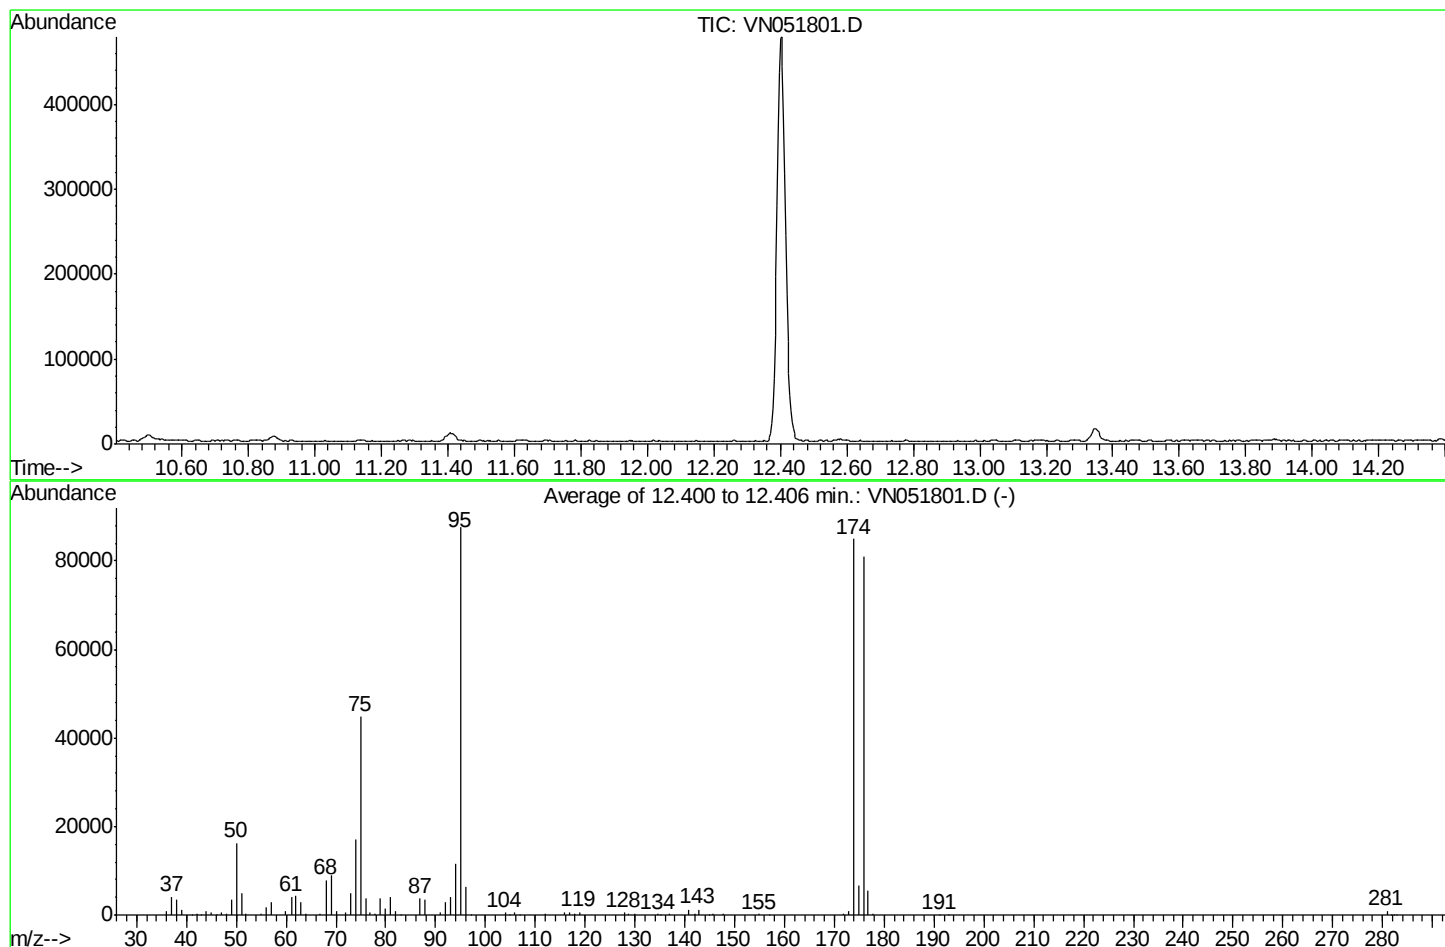

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	16216	PASS
75	95	30	60	51.1	44757	PASS
95	95	100	100	100.0	87600	PASS
96	95	5	9	7.2	6315	PASS
173	174	0.00	2	0.9	798	PASS
174	95	50	100	97.0	84970	PASS
175	174	5	9	7.9	6690	PASS
176	174	95	101	95.3	80981	PASS
177	176	5	9	6.6	5380	PASS