

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101122\
 Data File : VN074852.D
 Acq On : 11 Oct 2022 17:25
 Operator : JC\MD
 Sample : PB148255ZHE#01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB148255ZHE#01

Quant Time: Oct 12 03:55:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 05:37:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	374159	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.112	114	727072	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	761749	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	324590	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	271219	30.593	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	61.180%#		
35) Dibromofluoromethane	8.177	113	243400	33.134	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	66.260%#		
50) Toluene-d8	10.571	98	897741	28.481	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	56.960%#		
62) 4-Bromofluorobenzene	12.853	95	319437	33.338	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	66.680%#		
Target Compounds						Qvalue
3) Chloromethane	2.377	50	3085	0.270	ug/l #	41
11) Tert butyl alcohol	5.542	59	5159	1.737	ug/l #	89
13) Acrolein	4.201	56	283	Below Cal		95
16) Acetone	4.459	43	117496	23.387	ug/l #	84
18) Methyl Acetate	5.065	43	16871	0.907	ug/l	96
20) Methylene Chloride	5.306	84	29840	1.583	ug/l #	75
25) 2-Butanone	7.512	43	13201	1.448	ug/l #	83
29) Tetrahydrofuran	7.853	42	3631	0.571	ug/l #	89
31) Cyclohexane	8.236	56	9848	0.643	ug/l #	41
36) 1,1-Dichloropropene	8.236	75	35224	2.962	ug/l #	45
37) Ethyl Acetate	7.512	43	13201	0.277	ug/l #	92
38) Carbon Tetrachloride	8.241	117	41232	3.677	ug/l #	19
43) Isopropyl Acetate	8.700	43	499791	16.958	ug/l #	91
48) Methyl methacrylate	9.671	41	13818	1.142	ug/l #	90
49) 1,4-Dioxane	9.706	88	269	1.026	ug/l #	24
51) 4-Methyl-2-Pentanone	10.453	43	42937	2.262	ug/l #	74
54) cis-1,3-Dichloropropene	10.365	75	156852	9.758	ug/l #	67
57) 1,3-Dichloropropane	11.212	76	18686	1.115	ug/l #	46
59) 2-Hexanone	11.177	43	439836	30.638	ug/l #	24
74) N-amyl acetate	12.494	43	7220	0.382	ug/l #	71
75) 1,1,2,2-Tetrachloroethane	12.941	83	1000	Below Cal	#	24
76) 1,2,3-Trichloropropane	12.853	75	191487	19.765	ug/l #	1
77) Bromobenzene	12.976	156	1366	Below Cal		51
81) trans-1,4-Dichloro-2-b...	12.853	75	191487	38.510	ug/l #	14
88) 1,4-Dichlorobenzene	13.800	146	3366	0.288	ug/l #	1
92) 1,2-Dibromo-3-Chloropr...	14.717	75	1180	0.456	ug/l #	51
93) 1,2,4-Trichlorobenzene	15.406	180	2372	0.455	ug/l	76
95) Naphthalene	15.653	128	24118	1.069	ug/l #	83
96) 1,2,3-Trichlorobenzene	15.847	180	2488	Below Cal	#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101122\
Data File : VN074852.D
Acq On : 11 Oct 2022 17:25
Operator : JC\MD
Sample : PB148255ZHE#01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB148255ZHE#01

Quant Time: Oct 12 03:55:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 05:37:50 2022
Response via : Initial Calibration




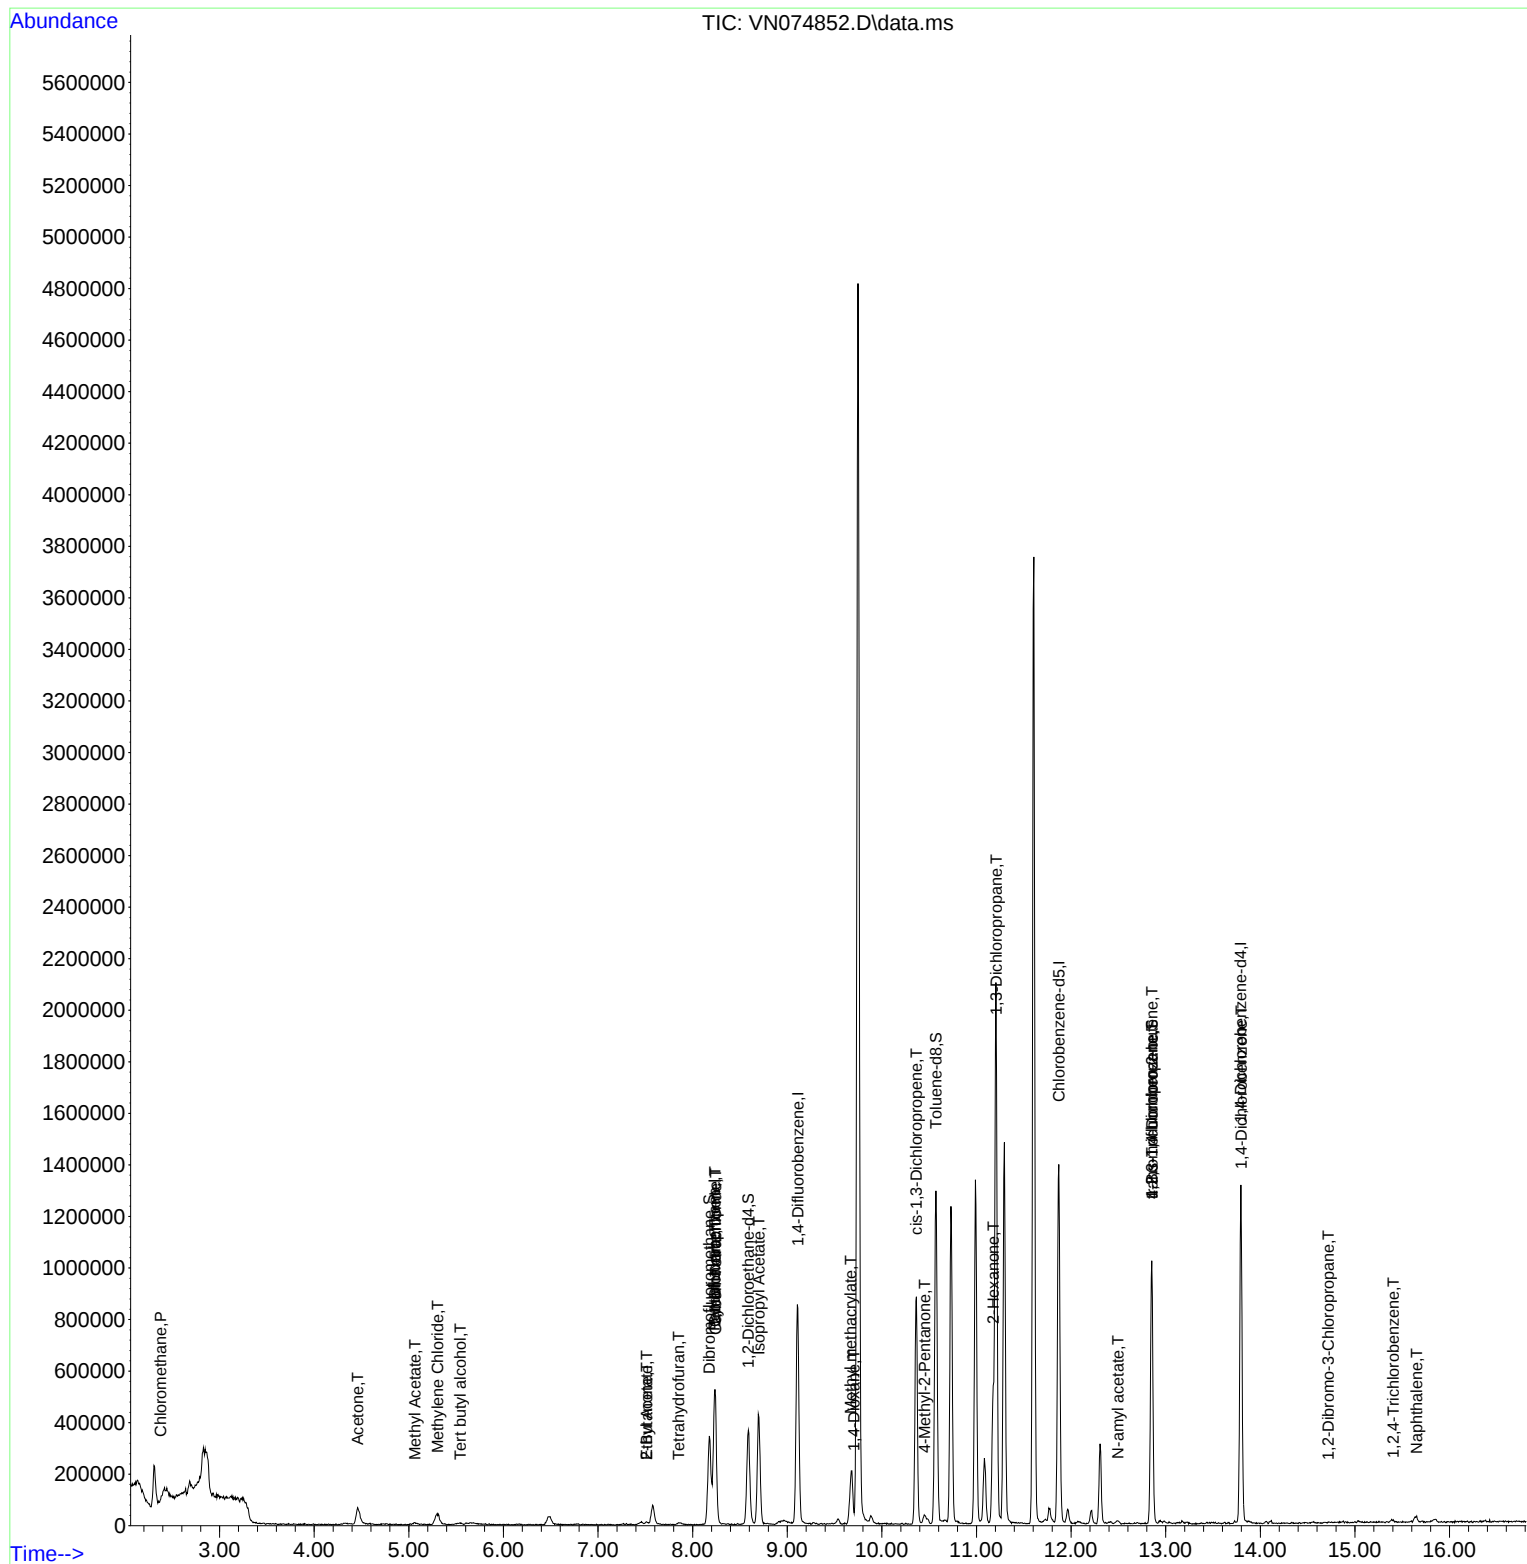




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 10
Delta R.T. -0.006 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25




Instrument :
MSVOA_N
ClientSampleId :
PB148255ZHE#01


Tgt Ion:168 Resp: 374159
Ion Ratio Lower Upper
168 100
99 58.3 42.8 64.2

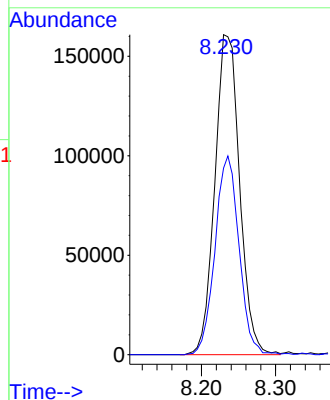

#3
Chloromethane
Concen: 0.270 ug/l
RT: 2.377 min Scan# 55
Delta R.T. -0.000 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25

Tgt Ion: 50 Resp: 3085
Ion Ratio Lower Upper
50 100
52 0.0 26.7 40.1#


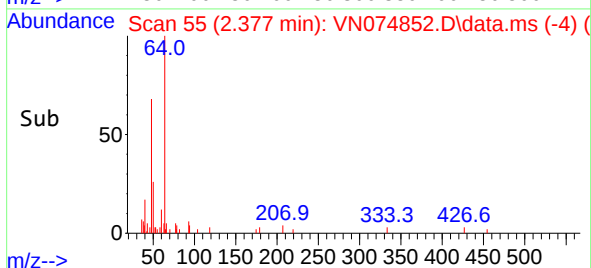
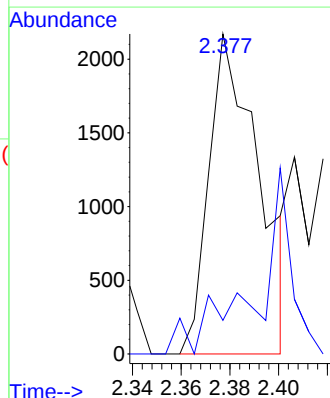





#11
Tert butyl alcohol
Concen: 1.737 ug/l
RT: 5.542 min Scan# 51
Delta R.T. -0.018 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25




Instrument :
MSVOA_N
ClientSampleId :
PB148255ZHE#01


Tgt Ion: 59 Resp: 5159
Ion Ratio Lower Upper
59 100
57 5.4 7.7 11.5#



#13
Acrolein
Concen: Below Cal
RT: 4.201 min Scan# 365
Delta R.T. -0.000 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25

Tgt Ion: 56 Resp: 283
Ion Ratio Lower Upper
56 100
55 72.8 54.9 82.3


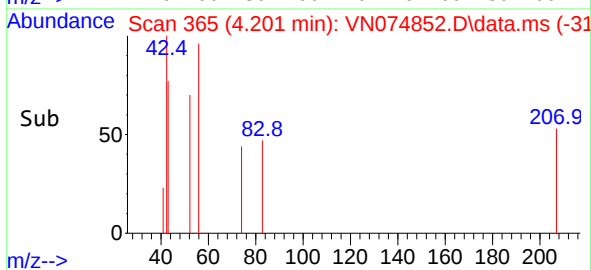






#16
Acetone
Concen: 23.387 ug/l
RT: 4.459 min Scan# 409
Delta R.T. -0.000 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25




Instrument :
MSVOA_N
ClientSampleId :
PB148255ZHE#01


Tgt Ion: 43 Resp: 117496
Ion Ratio Lower Upper
43 100
58 39.7 24.9 37.3#

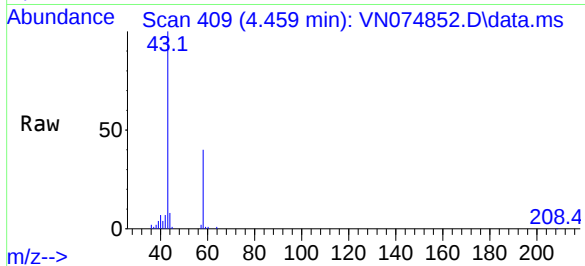

#18
Methyl Acetate
Concen: 0.907 ug/l
RT: 5.065 min Scan# 512
Delta R.T. 0.018 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25

Tgt Ion: 43 Resp: 16871
Ion Ratio Lower Upper
43 100
74 24.8 18.5 27.7


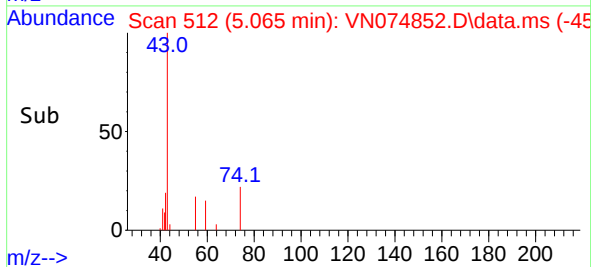

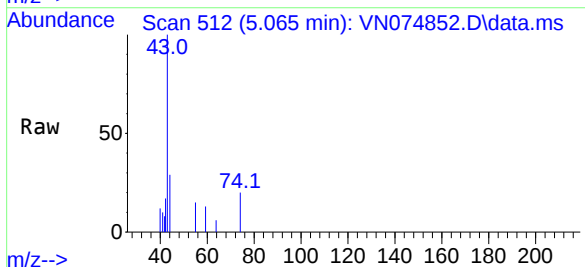




#20
Methylene Chloride
Concen: 1.583 ug/l
RT: 5.306 min Scan# 51
Delta R.T. 0.011 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25




Instrument :
MSVOA_N
ClientSampleId :
PB148255ZHE#01


Tgt Ion: 84 Resp: 29840
Ion Ratio Lower Upper
84 100
49 91.8 107.4 161.0#
51 36.9 35.1 52.7
86 54.6 50.4 75.6

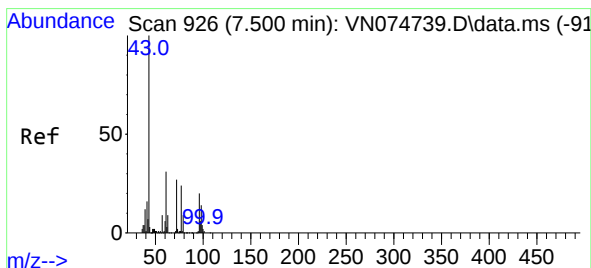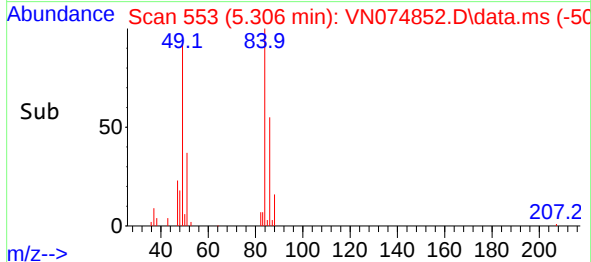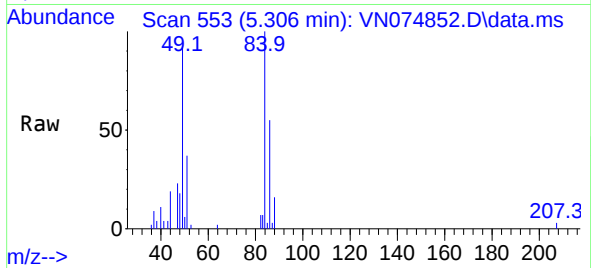

#25
2-Butanone
Concen: 1.448 ug/l
RT: 7.512 min Scan# 928
Delta R.T. 0.012 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25


Tgt Ion: 43 Resp: 13201
Ion Ratio Lower Upper
43 100
72 17.9 21.4 32.0#

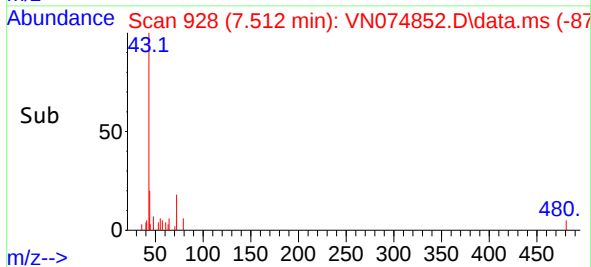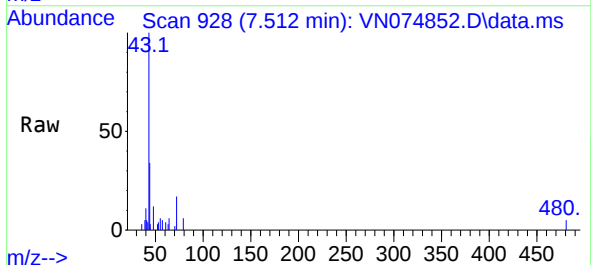






#29
Tetrahydrofuran
Concen: 0.571 ug/l
RT: 7.853 min Scan# 91
Delta R.T. -0.000 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25

Instrument :
MSVOA_N
ClientSampleId :
PB148255ZHE#01



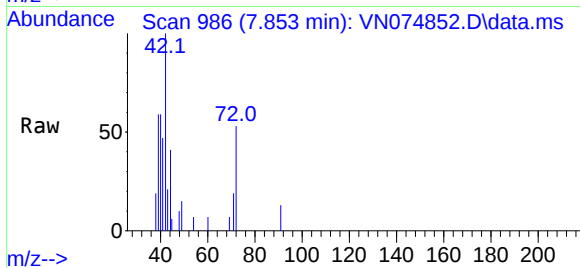



Tgt Ion: 42 Resp: 3631
Ion Ratio Lower Upper
42 100
72 38.4 33.0 49.6
71 27.2 30.4 45.6#

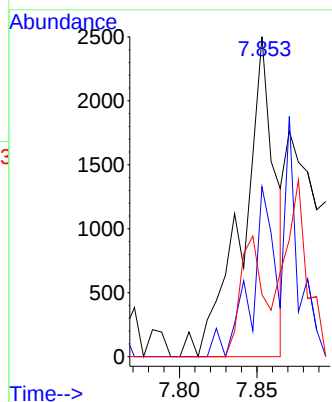

#31
Cyclohexane
Concen: 0.643 ug/l
RT: 8.236 min Scan# 1051
Delta R.T. -0.029 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25

Tgt Ion: 56 Resp: 9848
Ion Ratio Lower Upper
56 100
69 110.7 23.1 34.7#
84 108.0 67.1 100.7#


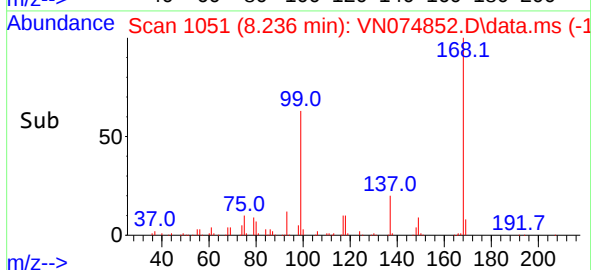

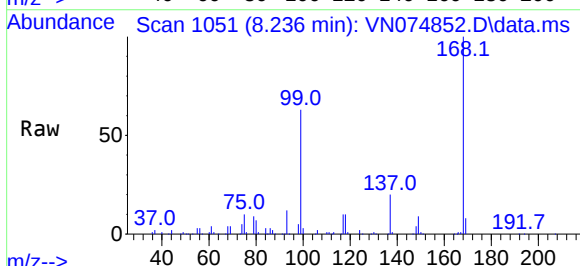


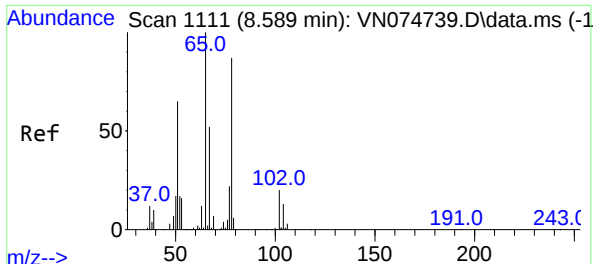

#33
1,2-Dichloroethane-d4
Concen: 30.593 ug/l
RT: 8.588 min Scan# 1111
Delta R.T. -0.000 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25




Instrument :
MSVOA_N
ClientSampleId :
PB148255ZHE#01


Tgt Ion: 65 Resp: 271219
Ion Ratio Lower Upper
65 100
67 53.9 0.0 109.0

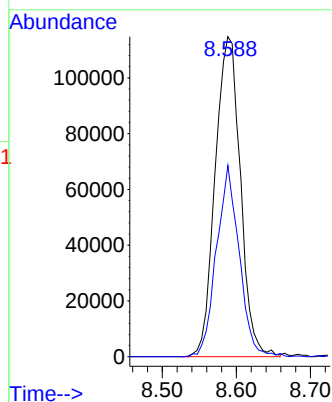

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.112 min Scan# 1200
Delta R.T. 0.006 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25

Tgt Ion: 114 Resp: 727072
Ion Ratio Lower Upper
114 100
63 23.2 0.0 41.2
88 13.9 0.0 30.2


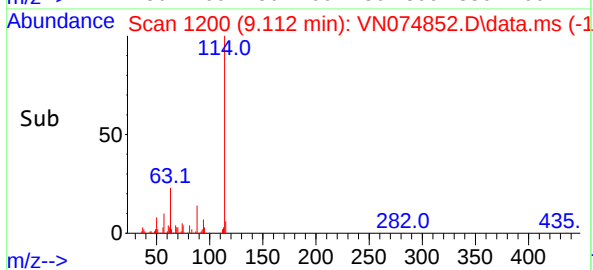
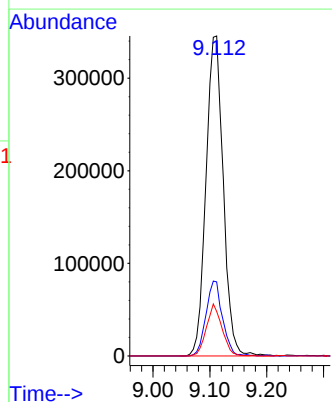
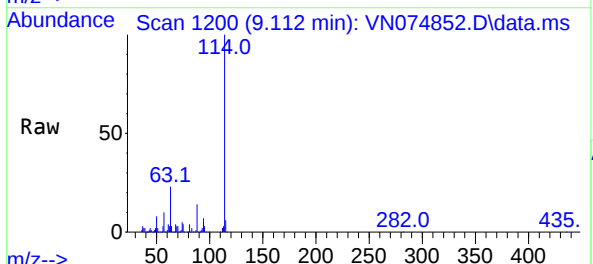




#35
Dibromofluoromethane
Concen: 33.134 ug/l
RT: 8.177 min Scan# 1040
Delta R.T. 0.006 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25




Instrument :
MSVOA_N
ClientSampleId :
PB148255ZHE#01


Tgt Ion:113 Resp: 243400
Ion Ratio Lower Upper
113 100
111 101.0 83.0 124.6
192 16.9 12.6 18.8

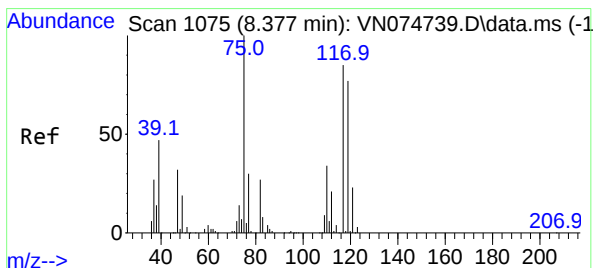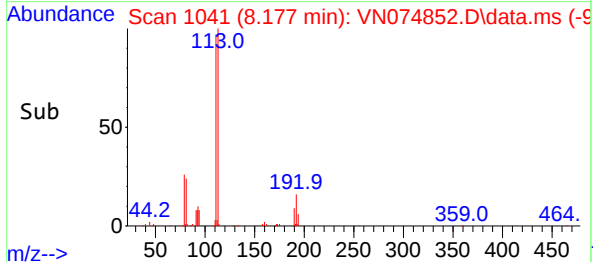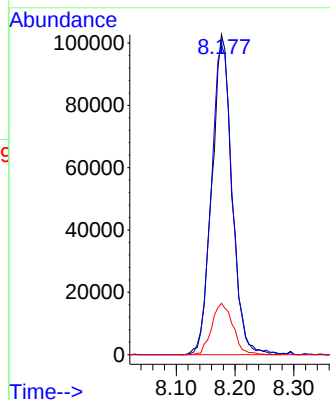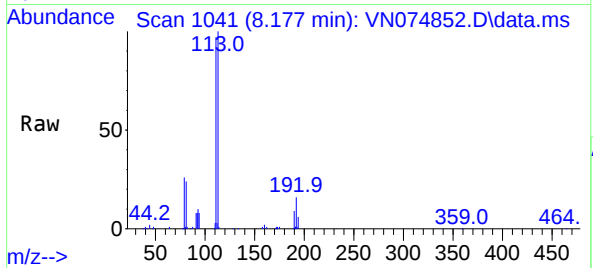

#36
1,1-Dichloropropene
Concen: 2.962 ug/l
RT: 8.236 min Scan# 1051
Delta R.T. -0.141 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25

Tgt Ion: 75 Resp: 35224
Ion Ratio Lower Upper
75 100
110 2.3 17.2 51.5#
77 0.7 24.3 36.5#


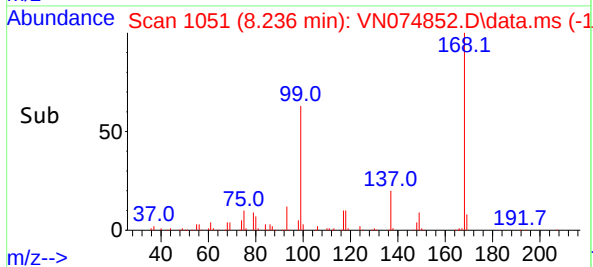
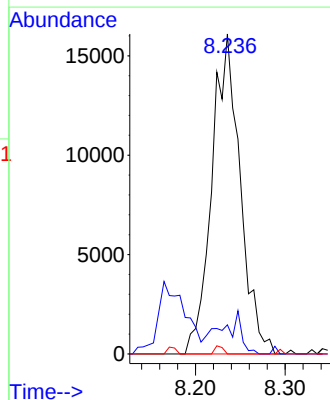
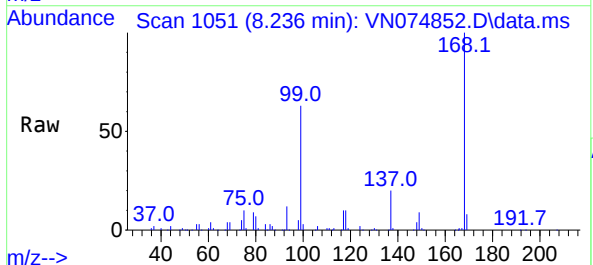


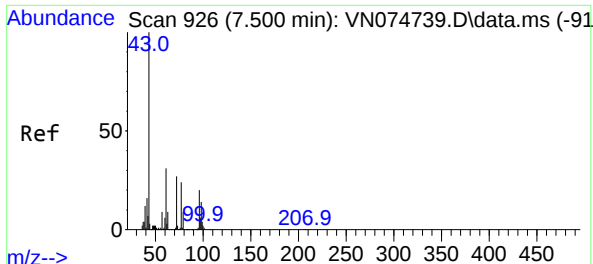

#37
Ethyl Acetate
Concen: 0.277 ug/l
RT: 7.512 min Scan# 91
Delta R.T. 0.012 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25




Instrument :
MSVOA_N
ClientSampleId :
PB148255ZHE#01


Tgt Ion: 43 Resp: 13201
Ion Ratio Lower Upper
43 100
61 3.6 4.3 6.5#
70 0.0 3.0 4.4#

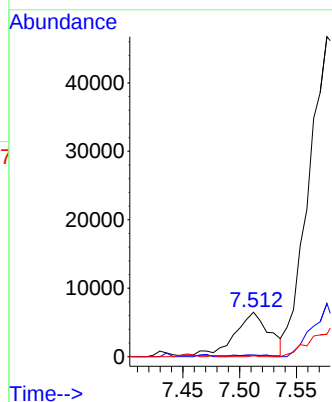

#38
Carbon Tetrachloride
Concen: 3.677 ug/l
RT: 8.241 min Scan# 1052
Delta R.T. -0.129 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25

Tgt Ion: 117 Resp: 41232
Ion Ratio Lower Upper
117 100
119 7.1 74.3 111.5#
121 0.0 25.0 37.4#


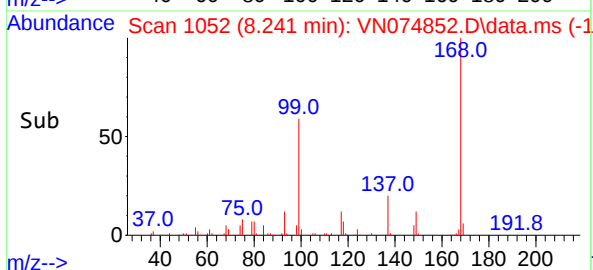

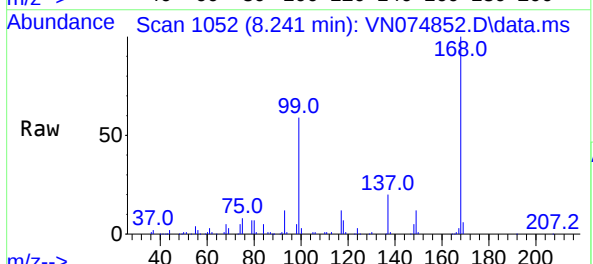




#43
Isopropyl Acetate
Concen: 16.958 ug/l
RT: 8.700 min Scan# 1130
Delta R.T. -0.000 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25




Instrument :
MSVOA_N
ClientSampleId :
PB148255ZHE#01


Tgt Ion: 43 Resp: 499791
Ion Ratio Lower Upper
43 100
61 17.9 19.4 29.0#
87 12.2 10.1 15.1

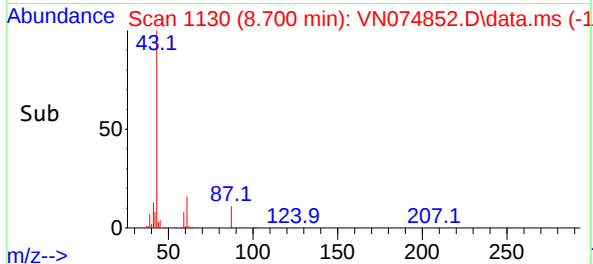

#48
Methyl methacrylate
Concen: 1.142 ug/l
RT: 9.671 min Scan# 1295
Delta R.T. 0.053 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25

Tgt Ion: 41 Resp: 13818
Ion Ratio Lower Upper
41 100
69 2.5 0.0 0.0#
39 59.7 54.4 81.6


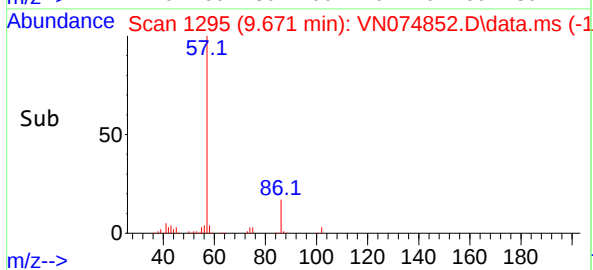

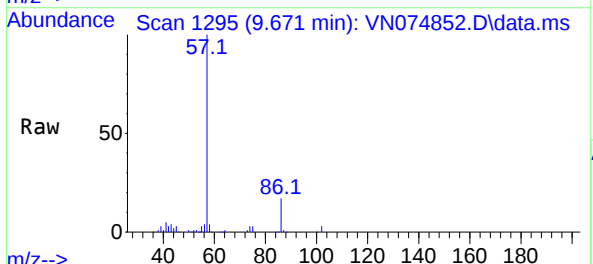




#49
1,4-Dioxane
Concen: 1.026 ug/l
RT: 9.706 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25




Instrument :
MSVOA_N
ClientSampleId :
PB148255ZHE#01


Tgt Ion: 88 Resp: 269
Ion Ratio Lower Upper
88 100
43 0.0 23.4 35.2#
58 0.0 54.9 82.3#

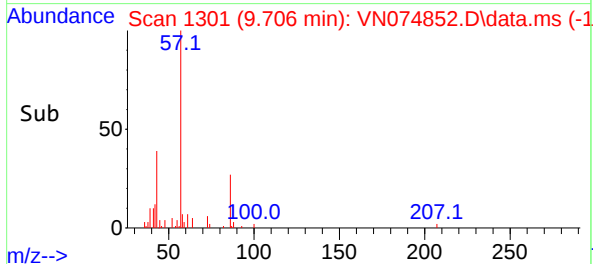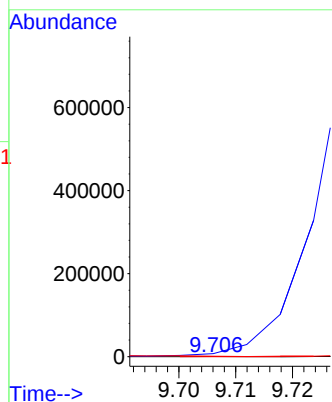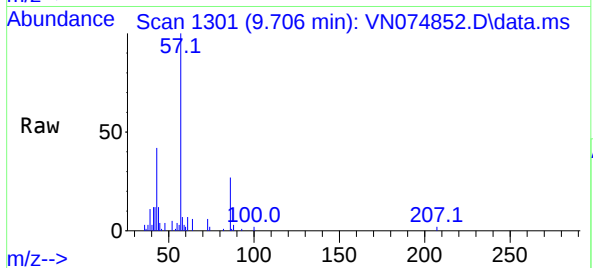

#50
Toluene-d8
Concen: 28.481 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25

Tgt Ion: 98 Resp: 897741
Ion Ratio Lower Upper
98 100
100 63.0 50.7 76.1


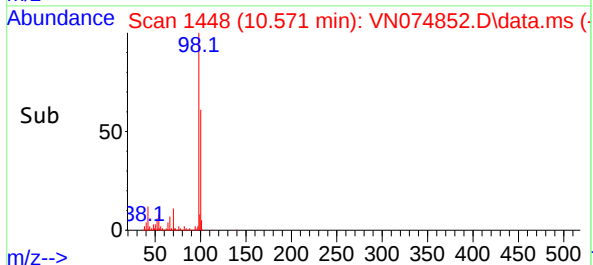

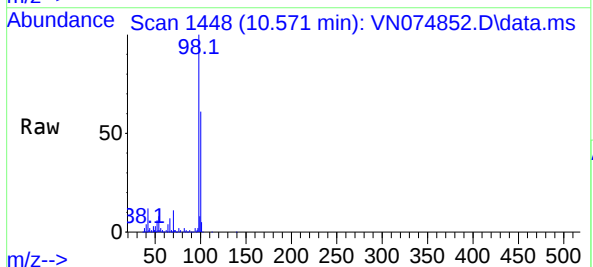




#51
4-Methyl-2-Pentanone
Concen: 2.262 ug/l
RT: 10.453 min Scan# 1413
Delta R.T. 0.006 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25




Instrument :
MSVOA_N
ClientSampleId :
PB148255ZHE#01


Tgt Ion: 43 Resp: 42937
Ion Ratio Lower Upper
43 100
58 22.6 30.6 45.8#

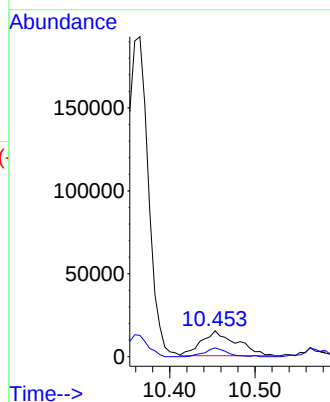

#54
cis-1,3-Dichloropropene
Concen: 9.758 ug/l
RT: 10.365 min Scan# 1413
Delta R.T. 0.053 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25

Tgt Ion: 75 Resp: 156852
Ion Ratio Lower Upper
75 100
77 0.3 24.4 36.6#
39 35.4 38.6 57.8#

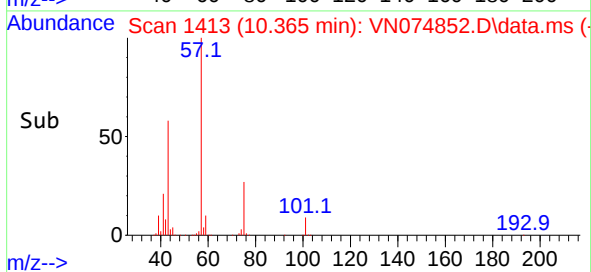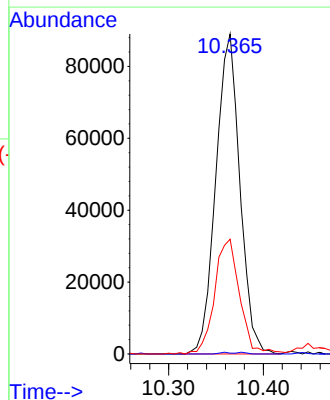



#57

1,3-Dichloropropane

Concen: 1.115 ug/l

RT: 11.212 min Scan# 1557

Delta R.T. 0.047 min

Lab File: VN074852.D

Acq: 11 Oct 2022 17:25

Instrument :

MSVOA_N

ClientSampleId :





PB148255ZHE#01

Tgt Ion: 76 Resp: 18686

Ion Ratio Lower Upper

76 100

78 2.3 26.2 39.2#

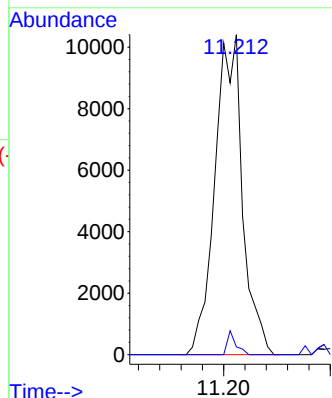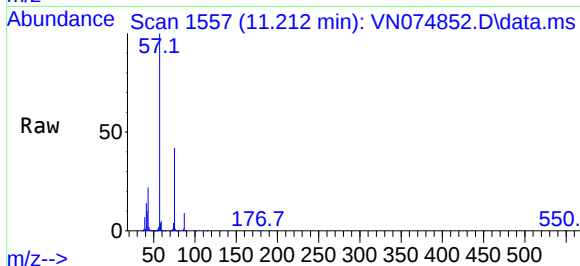

#59

2-Hexanone

Concen: 30.638 ug/l

RT: 11.177 min Scan# 1551

Delta R.T. -0.024 min

Lab File: VN074852.D




Acq: 11 Oct 2022 17:25


Tgt Ion: 43 Resp: 439836

Ion Ratio Lower Upper

43 100

58 0.0 27.3 81.9#


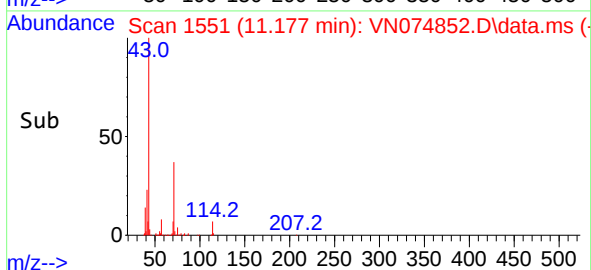

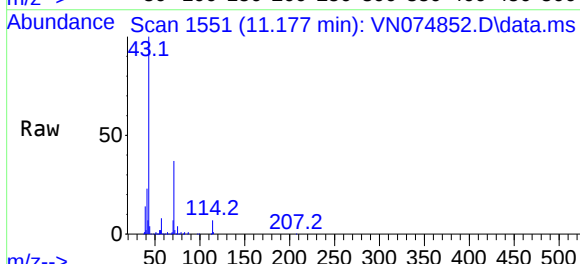


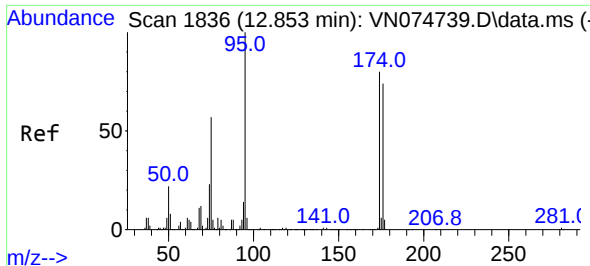

#62
4-Bromofluorobenzene
Concen: 33.338 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25




Instrument :
MSVOA_N
ClientSampleId :
PB148255ZHE#01


Tgt Ion: 95 Resp: 319437
Ion Ratio Lower Upper
95 100
174 82.1 0.0 149.4
176 74.5 0.0 142.0

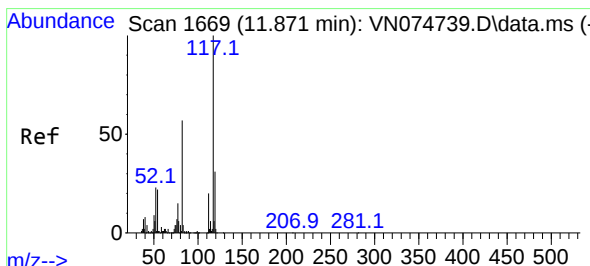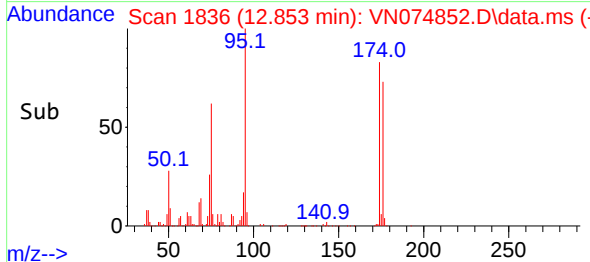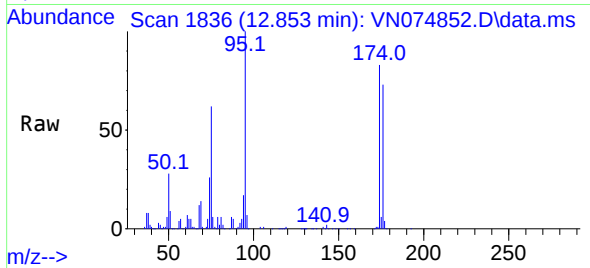

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1669
Delta R.T. -0.000 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25

Tgt Ion: 117 Resp: 761749
Ion Ratio Lower Upper
117 100
82 59.0 45.4 68.2
119 31.9 25.1 37.7


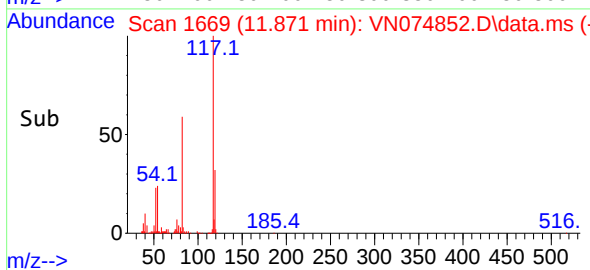

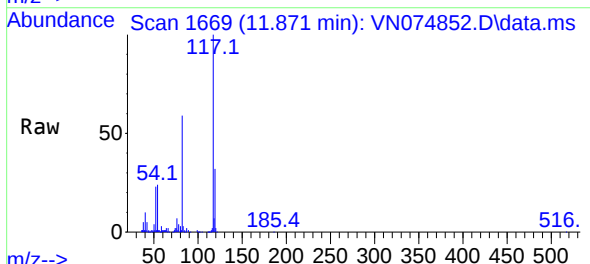


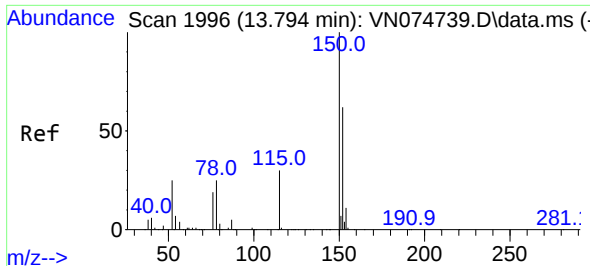

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25




Instrument :
MSVOA_N
ClientSampleId :
PB148255ZHE#01


Tgt Ion:152 Resp: 324590
Ion Ratio Lower Upper
152 100
115 59.2 30.0 90.0
150 158.2 0.0 356.4

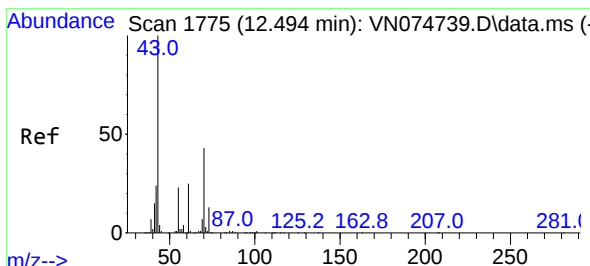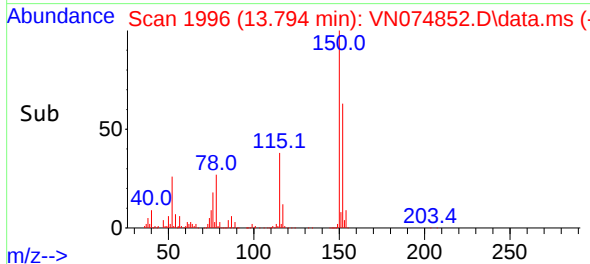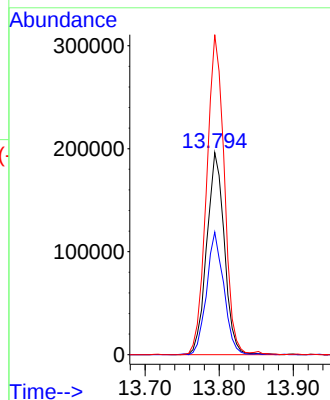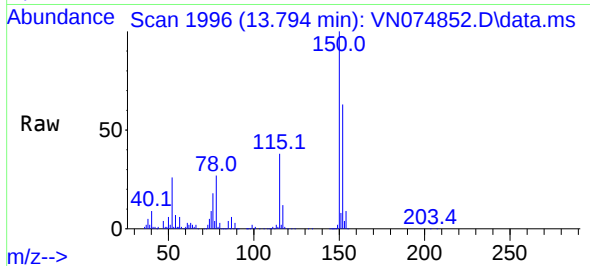

#74
N-ethyl acetate
Concen: 0.382 ug/l
RT: 12.494 min Scan# 1775
Delta R.T. -0.000 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25

Tgt Ion: 43 Resp: 7220
Ion Ratio Lower Upper
43 100
70 23.7 32.9 49.3#
55 6.6 17.8 26.6#
61 9.3 18.9 28.3#


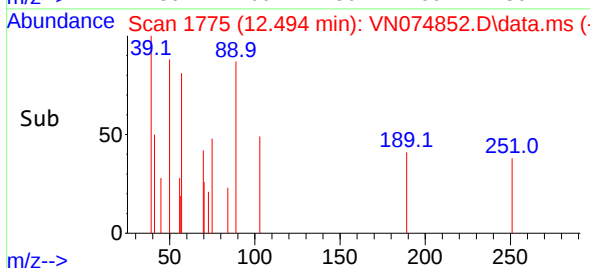
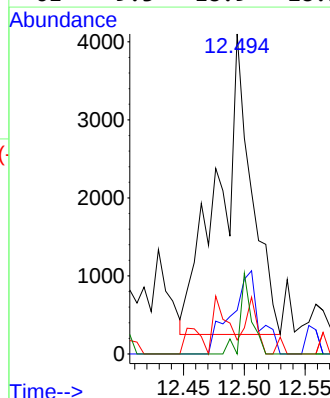
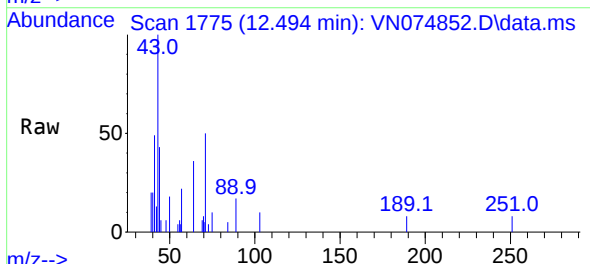




#75
1,1,2-Tetrachloroethane
Concen: Below Cal
RT: 12.941 min Scan# 1851
Delta R.T. 0.000 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25




Instrument :
MSVOA_N
ClientSampleId :
PB148255ZHE#01


Tgt Ion: 83 Resp: 1000
Ion Ratio Lower Upper
83 100
131 0.0 4.3 12.8#
85 0.0 32.9 98.6#

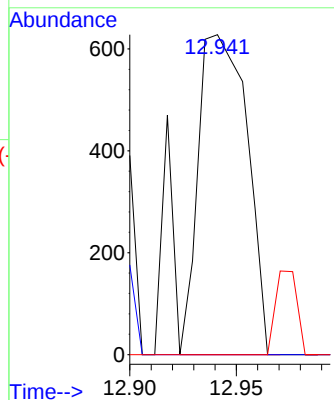

#76
1,2,3-Trichloropropane
Concen: 19.765 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.141 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25

Tgt Ion: 75 Resp: 191487
Ion Ratio Lower Upper
75 100
77 1.4 76.9 230.7#


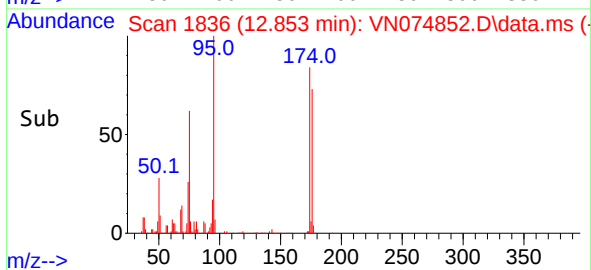
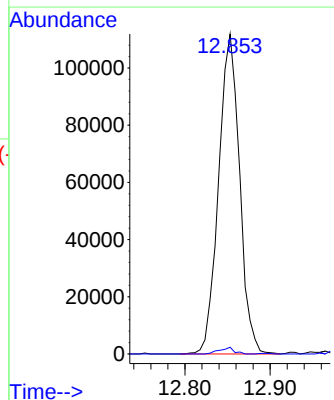





#77
Bromobenzene
Concen: Below Cal
RT: 12.976 min Scan# 1857
Delta R.T. -0.006 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25




Instrument :
MSVOA_N
ClientSampleId :
PB148255ZHE#01


Tgt Ion:156 Resp: 1366
Ion Ratio Lower Upper
156 100
77 154.4 124.7 374.1
158 62.0 48.3 144.9

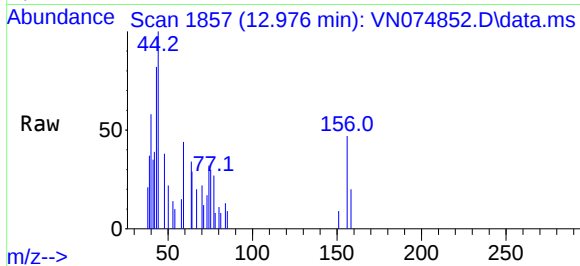

#81
trans-1,4-Dichloro-2-butene
Concen: 38.510 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.118 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25

Tgt Ion: 75 Resp: 191487
Ion Ratio Lower Upper
75 100
53 0.1 71.4 107.0#
89 0.0 32.1 48.1#


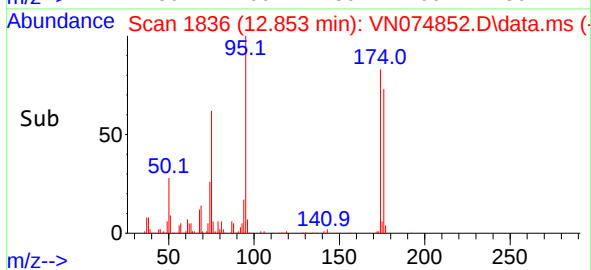

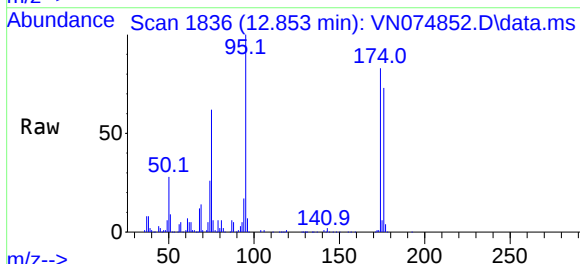


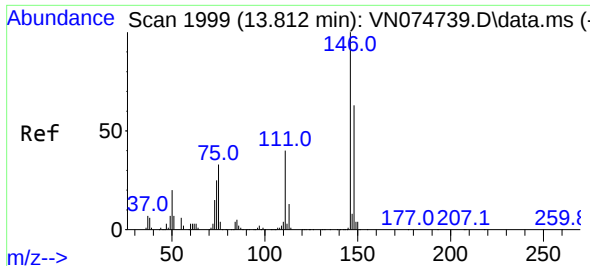

#88
 1,4-Dichlorobenzene
 Concen: 0.288 ug/l
 RT: 13.800 min Scan# 1999
 Delta R.T. -0.012 min
 Lab File: VN074852.D
 Acq: 11 Oct 2022 17:25




Instrument :
 MSVOA_N
 ClientSampleId :
 PB148255ZHE#01


Tgt Ion:146 Resp: 3366
 Ion Ratio Lower Upper
 146 100
 111 180.2 19.9 59.6#
 148 0.0 31.8 95.4#

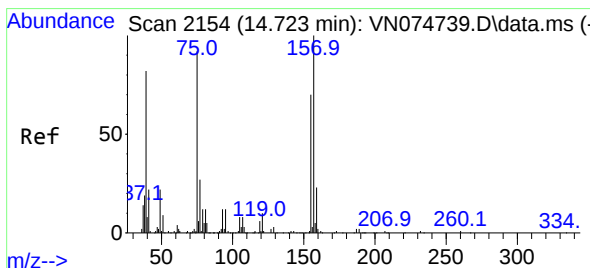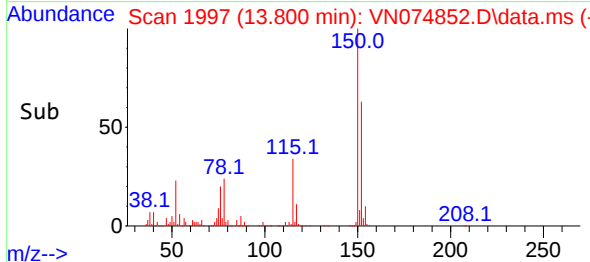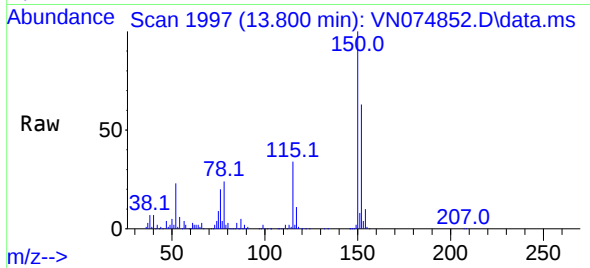

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.456 ug/l
 RT: 14.717 min Scan# 2153
 Delta R.T. -0.006 min
 Lab File: VN074852.D
 Acq: 11 Oct 2022 17:25

Tgt Ion: 75 Resp: 1180
 Ion Ratio Lower Upper
 75 100
 155 18.4 40.3 120.8#
 157 70.4 51.3 153.9


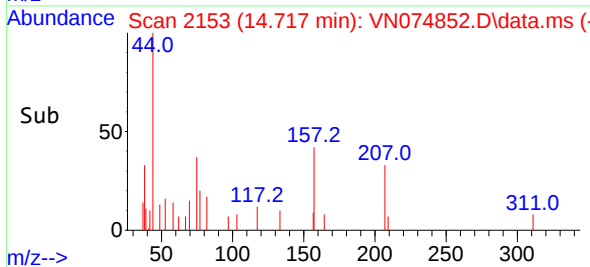

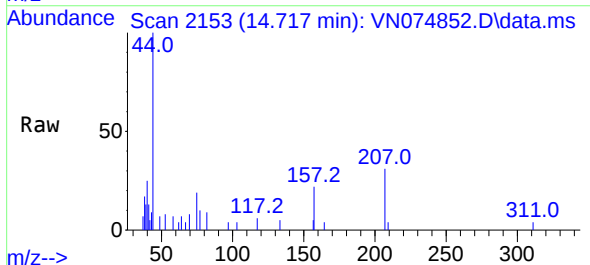


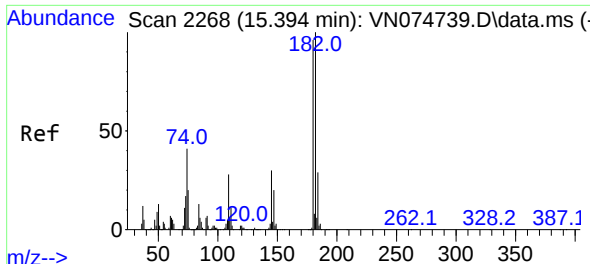

#93
1,2,4-Trichlorobenzene
Concen: 0.455 ug/l
RT: 15.406 min Scan# 21
Delta R.T. 0.012 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25




Instrument :
MSVOA_N
ClientSampleId :
PB148255ZHE#01


Tgt Ion:180 Resp: 2372
Ion Ratio Lower Upper
180 100
182 122.7 48.5 145.5
145 22.4 16.1 48.3

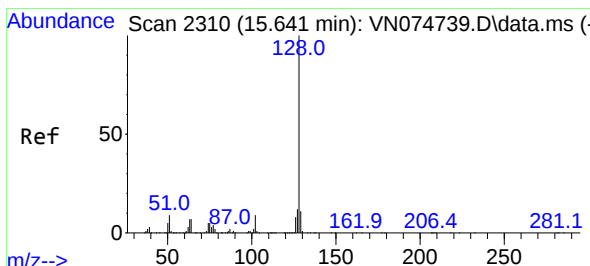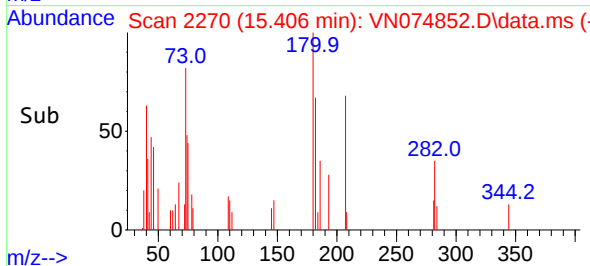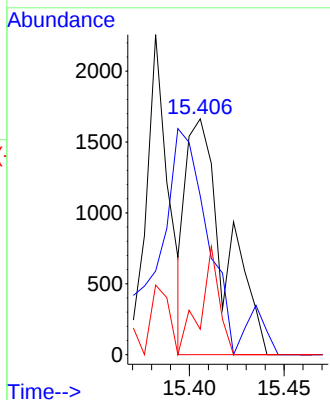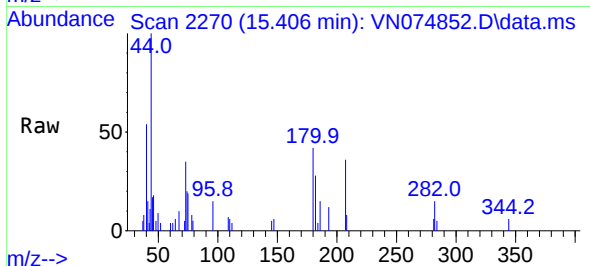

#95
Naphthalene
Concen: 1.069 ug/l
RT: 15.653 min Scan# 2312
Delta R.T. 0.012 min
Lab File: VN074852.D
Acq: 11 Oct 2022 17:25


Tgt Ion:128 Resp: 24118
Ion Ratio Lower Upper
128 100
127 10.2 10.2 15.2
129 0.0 9.0 13.4#

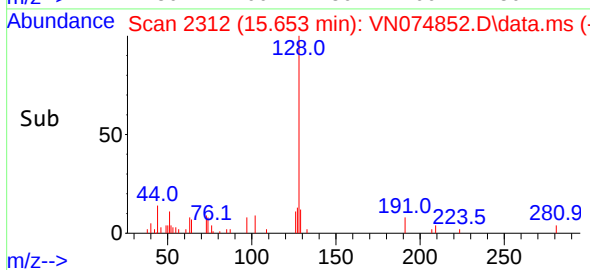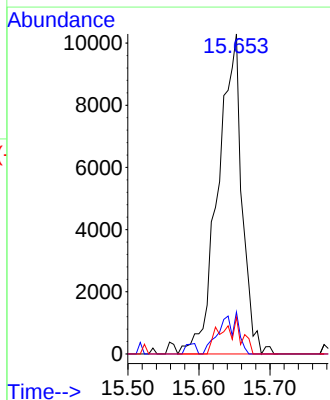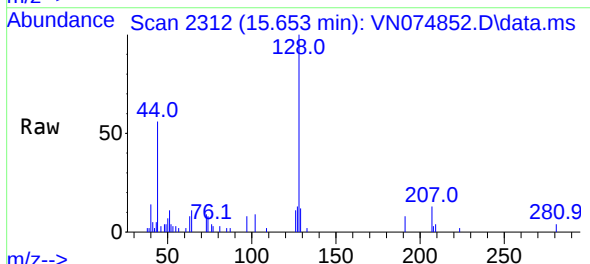



#96
 1,2,3-Trichlorobenzene
 Concen: Below Cal
 RT: 15.847 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VN074852.D
 Acq: 11 Oct 2022 17:25

Instrument :
 MSVOA_N
 ClientSampleId :
 PB148255ZHE#01

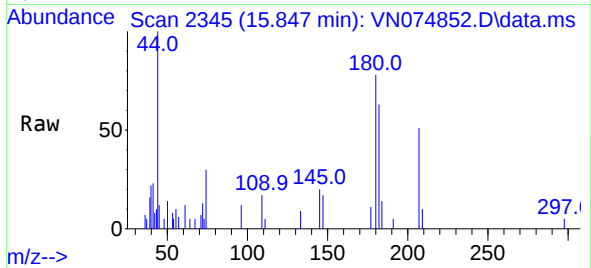

Tgt Ion:180 Resp: 2488
 Ion Ratio Lower Upper
 180 100
 182 212.4 47.3 142.0#
 145 82.8 17.1 51.2#

