
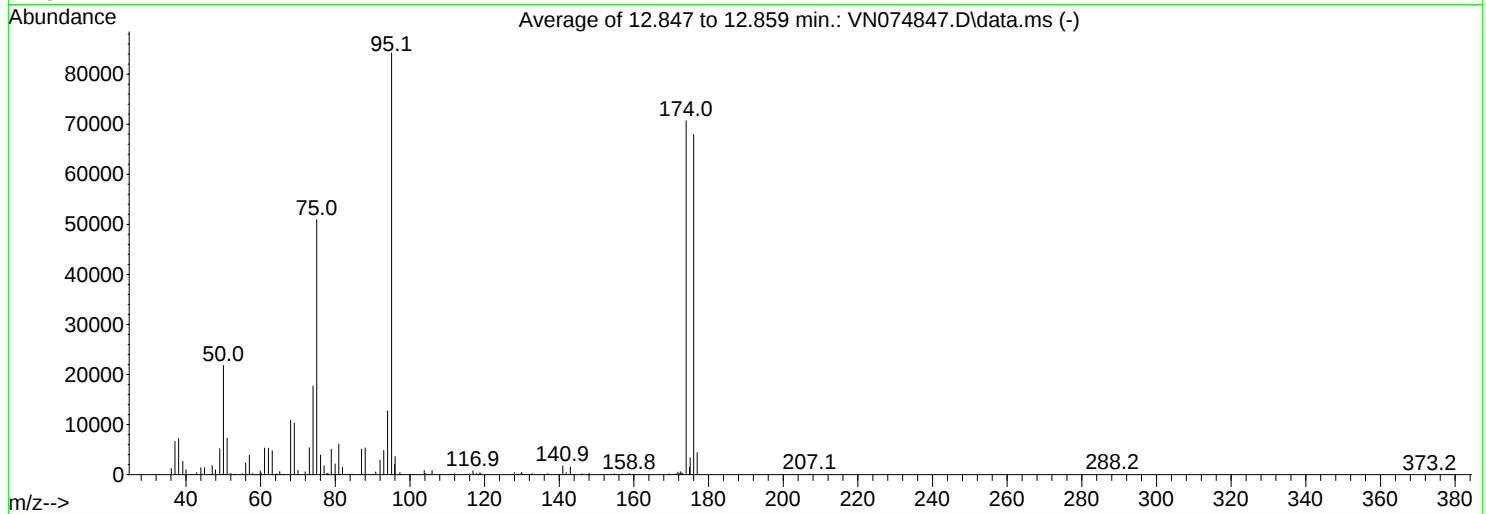


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101122\
Data File : VN074847.D
Acq On : 11 Oct 2022 14:45
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
Title : SW846 8260
Last Update : Thu Oct 06 05:37:50 2022

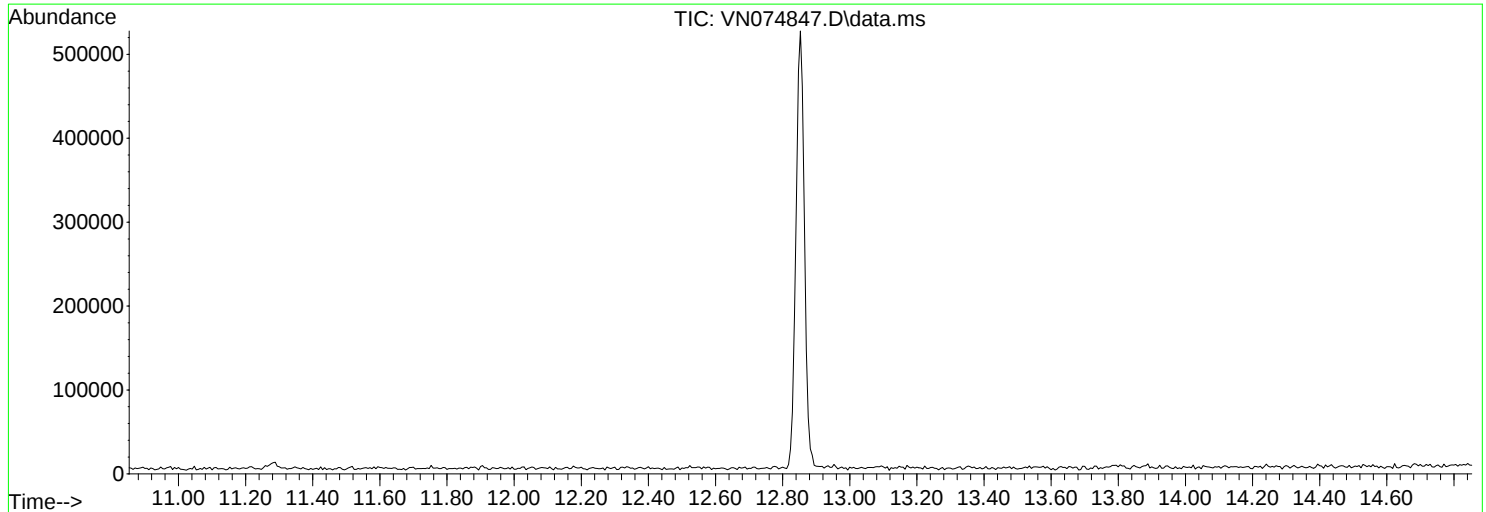

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.9	21800	PASS
75	95	30	60	60.5	50939	FAIL*
95	95	100	100	100.0	84256	PASS
96	95	5	9	4.3	3608	FAIL*
173	174	0.00	2	0.5	346	PASS
174	95	50	100	83.9	70693	PASS
175	174	5	9	4.8	3368	FAIL*
176	174	95	101	96.1	67960	PASS
177	176	5	9	6.5	4400	PASS