

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101123\
 Data File : VN079531.D
 Acq On : 11 Oct 2023 20:48
 Operator : JC\MD
 Sample : 04823-04DL 10X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Oct 12 06:15:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
 Quant Title : SW846 8260
 QLast Update : Fri Oct 06 03:34:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	319847	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	621401	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	632965	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	237400	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	255657	49.297	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	98.600%
35) Dibromofluoromethane	8.171	113	220316	49.336	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.680%
50) Toluene-d8	10.571	98	740740	45.844	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	91.680%
62) 4-Bromofluorobenzene	12.853	95	282971	54.571	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	109.140%
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	5.524	59	1000	1.281	ug/l #	89
12) 1,1-Dichloroethene	4.306	96	1343	0.355	ug/l #	58
13) Acrolein	4.201	56	49093	63.166	ug/l #	16
16) Acetone	4.430	43	384228	186.793	ug/l #	57
18) Methyl Acetate	5.036	43	9519	0.945	ug/l #	67
20) Methylene Chloride	5.277	84	1778	Below Cal	#	93
22) Diisopropyl ether	6.730	45	104180	7.618	ug/l #	1
23) Vinyl Acetate	6.730	43	253007	32.892	ug/l #	62
25) 2-Butanone	7.500	43	9087	2.976	ug/l #	76
31) Cyclohexane	8.236	56	9114	1.239	ug/l #	57
36) 1,1-Dichloropropene	8.230	75	28843	4.303	ug/l #	48
38) Carbon Tetrachloride	8.230	117	34757	5.180	ug/l #	17
40) Benzene	8.612	78	98133	4.930	ug/l	100
43) Isopropyl Acetate	8.724	43	11103	0.950	ug/l #	49
48) Methyl methacrylate	9.665	41	3318	0.663	ug/l #	32
52) Toluene	10.635	92	88825	7.581	ug/l	91
59) 2-Hexanone	11.200	43	3364	0.707	ug/l	69
67) Ethyl Benzene	11.971	91	21908	0.894	ug/l	95
68) m/p-Xylenes	12.076	106	28438	3.194	ug/l	95
69) o-Xylene	12.400	106	12843	1.467	ug/l	97
70) Styrene	12.412	104	8037	0.581	ug/l #	81
71) Bromoform	12.847	173	1696	0.449	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	12.800	83	37606	4.161	ug/l #	32
76) 1,2,3-Trichloropropane	12.853	75	160559	23.457	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.176	105	3570	0.205	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.853	75	160559	68.061	ug/l #	15
84) 1,2,4-Trimethylbenzene	13.488	105	11308	0.680	ug/l	96
85) sec-Butylbenzene	13.488	105	11308	0.568	ug/l #	57
90) Hexachloroethane	14.318	117	54	Below Cal	#	21
95) Naphthalene	15.647	128	100265	12.654	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101123\
Data File : VN079531.D
Acq On : 11 Oct 2023 20:48
Operator : JC\MD
Sample : 04823-04DL 10X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Oct 12 06:15:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
Quant Title : SW846 8260
QLast Update : Fri Oct 06 03:34:49 2023
Response via : Initial Calibration

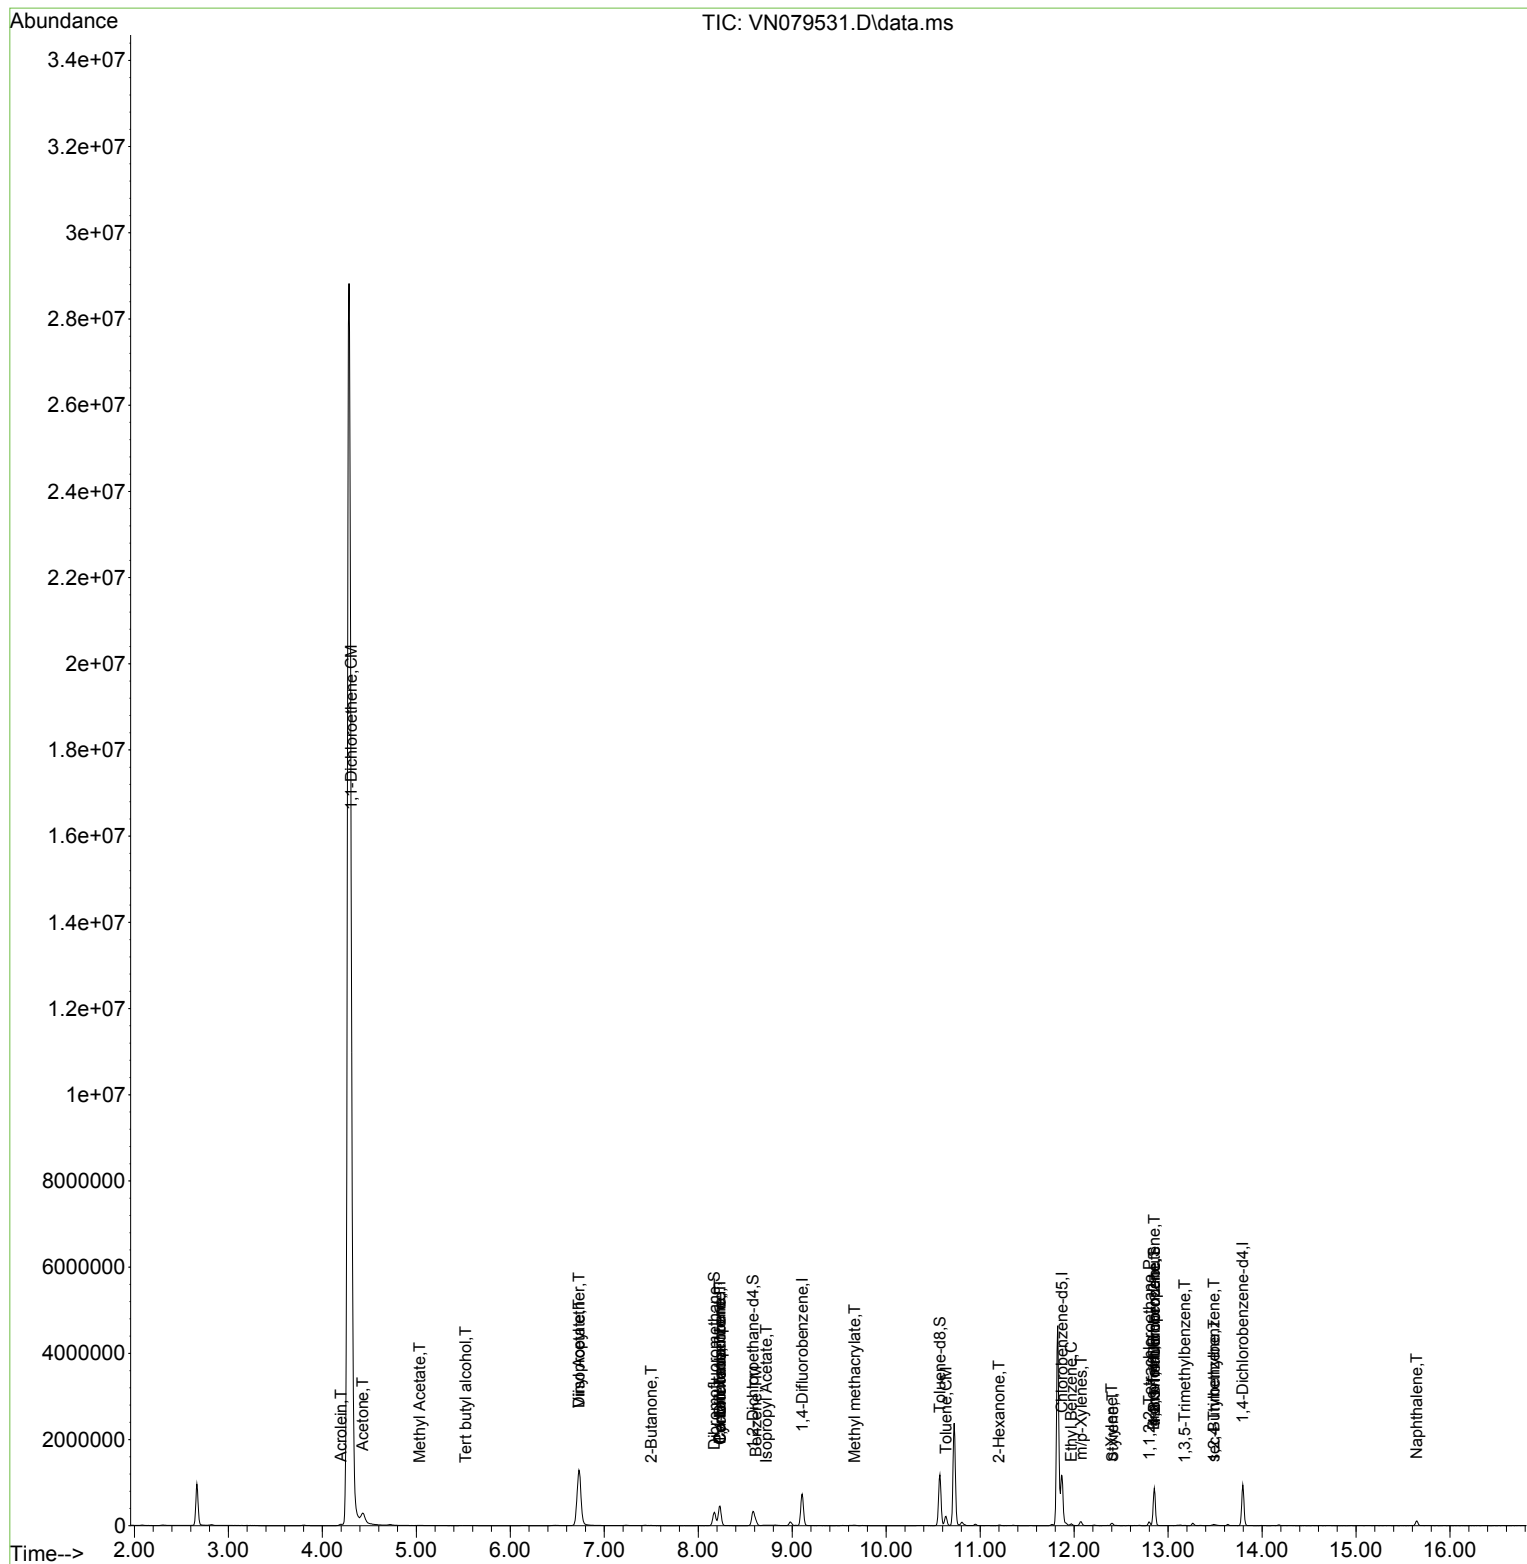






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.000 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48

Instrument :
MSVOA_N
ClientSampleId :



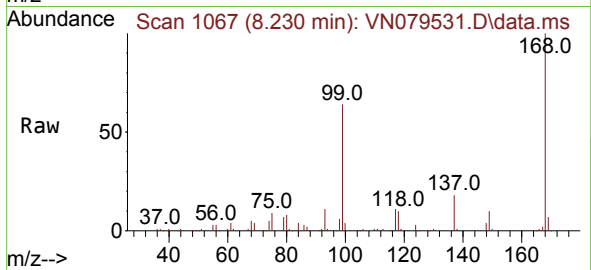



Tgt Ion:168 Resp: 319847
Ion Ratio Lower Upper
168 100
99 64.3 53.0 79.6

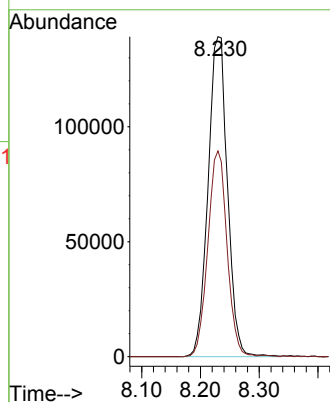

#11
Tert butyl alcohol
Concen: 1.281 ug/l
RT: 5.524 min Scan# 607
Delta R.T. -0.006 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48

Tgt Ion: 59 Resp: 1000
Ion Ratio Lower Upper
59 100
57 14.4 8.2 12.4#



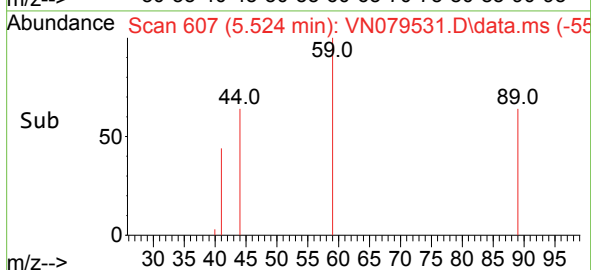





#12
1,1-Dichloroethene
Concen: 0.355 ug/l
RT: 4.306 min Scan# 407
Delta R.T. -0.041 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 96 Resp: 1343
Ion Ratio Lower Upper
96 100
61 113.2 112.7 169.1
98 129.1 51.2 76.8#

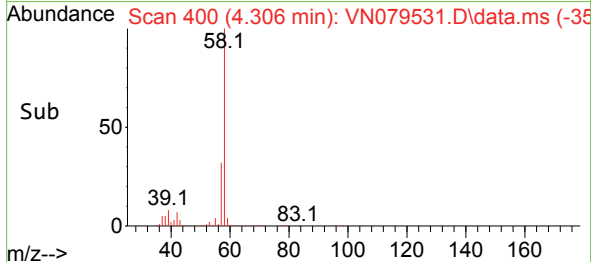

#13
Acrolein
Concen: 63.166 ug/l
RT: 4.201 min Scan# 382
Delta R.T. 0.018 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48

Tgt Ion: 56 Resp: 49093
Ion Ratio Lower Upper
56 100
55 0.0 54.5 81.7#


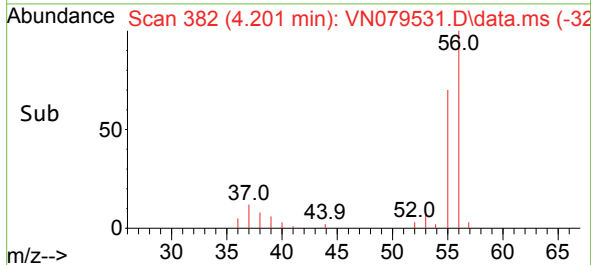

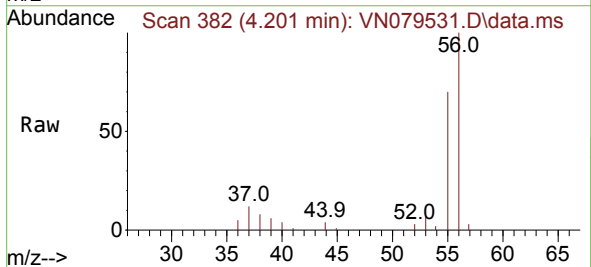




#16
Acetone
Concen: 186.793 ug/l
RT: 4.430 min Scan# 41
Delta R.T. -0.000 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 384228
Ion Ratio Lower Upper
43 100
58 60.2 28.0 42.0#

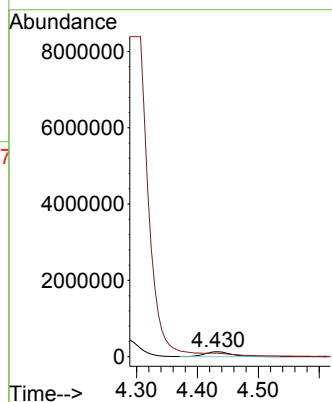

#18
Methyl Acetate
Concen: 0.945 ug/l
RT: 5.036 min Scan# 524
Delta R.T. 0.006 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48


Tgt Ion: 43 Resp: 9519
Ion Ratio Lower Upper
43 100
74 14.1 26.2 39.4#

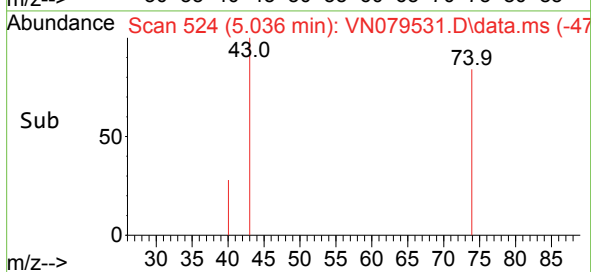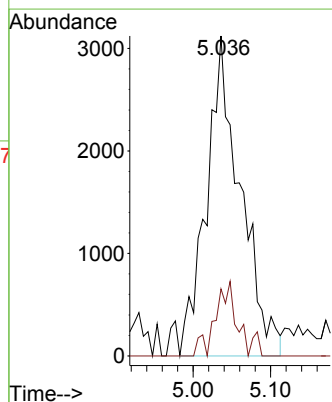






#20
Methylene Chloride
Concen: Below Cal
RT: 5.277 min Scan# 51
Delta R.T. -0.006 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:	84	Resp:	1778
Ion	Ratio	Lower	Upper
84	100		
49	97.2	79.7	119.5
51	39.3	25.2	37.8#
86	57.1	53.3	79.9




#22
Diisopropyl ether
Concen: 7.618 ug/l
RT: 6.730 min Scan# 812
Delta R.T. 0.053 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48



Tgt Ion:	45	Resp:	104180
Ion	Ratio	Lower	Upper
45	100		
43	232.4	45.5	68.3#
87	0.0	31.8	47.8#
59	852.3	11.6	17.4#



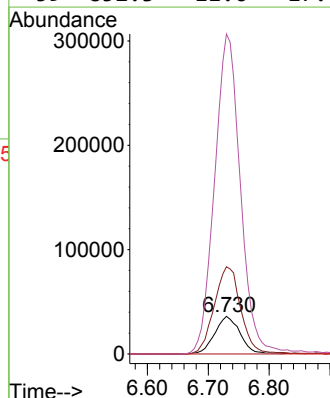





#23
 Vinyl Acetate
 Concen: 32.892 ug/l
 RT: 6.730 min Scan# 812
 Delta R.T. 0.124 min
 Lab File: VN079531.D
 Acq: 11 Oct 2023 20:48




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 43 Resp: 253007
 Ion Ratio Lower Upper
 43 100
 86 0.0 13.0 19.6#

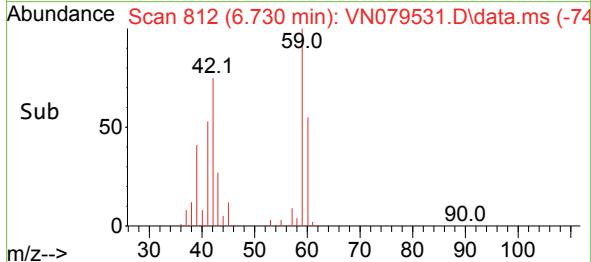

#25
 2-Butanone
 Concen: 2.976 ug/l
 RT: 7.500 min Scan# 943
 Delta R.T. 0.012 min
 Lab File: VN079531.D
 Acq: 11 Oct 2023 20:48


Tgt Ion: 43 Resp: 9087
 Ion Ratio Lower Upper
 43 100
 72 23.1 30.2 45.2#

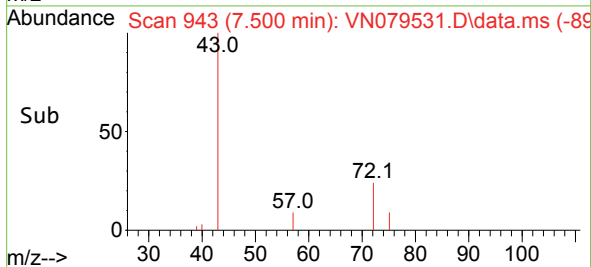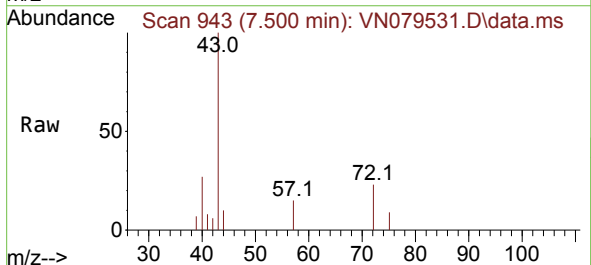






#31
Cyclohexane
Concen: 1.239 ug/l
RT: 8.236 min Scan# 1068
Delta R.T. -0.029 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48

Instrument :
MSVOA_N
ClientSampleId :



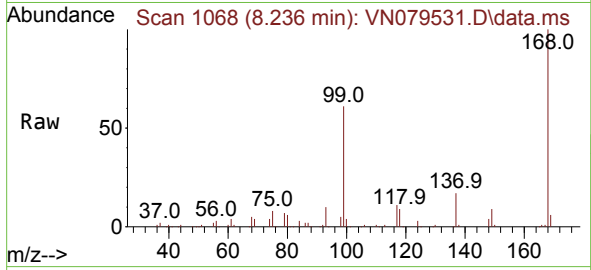



Tgt Ion: 56 Resp: 9114
Ion Ratio Lower Upper
56 100
69 132.0 26.8 40.2#
84 101.3 81.8 122.6

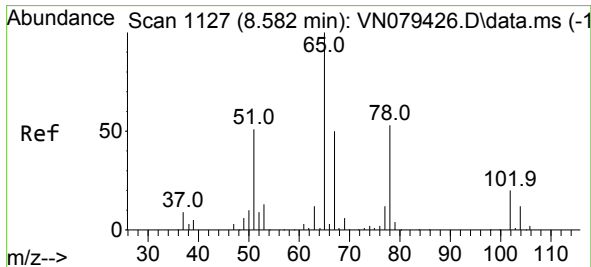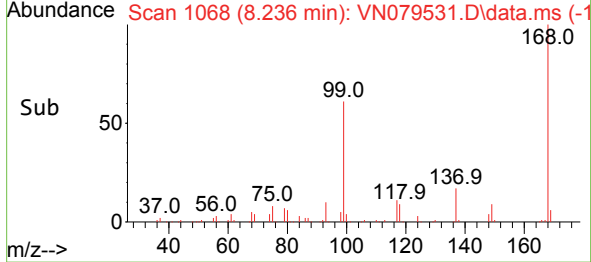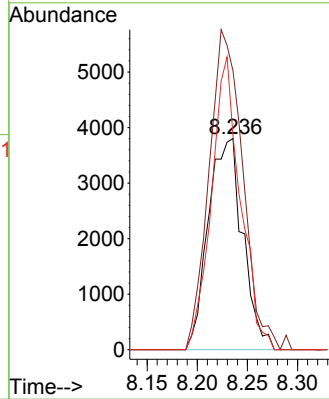

#33
1,2-Dichloroethane-d4
Concen: 49.297 ug/l
RT: 8.583 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48


Tgt Ion: 65 Resp: 255657
Ion Ratio Lower Upper
65 100
67 51.3 0.0 106.6

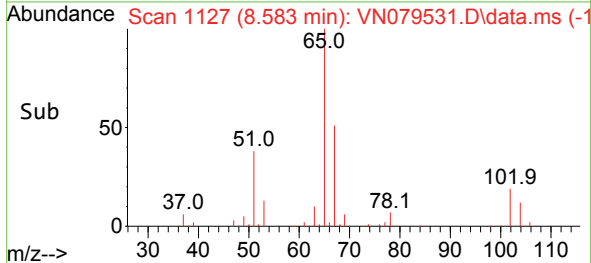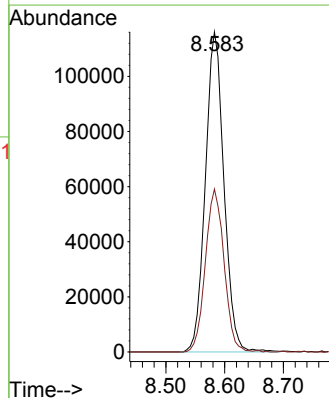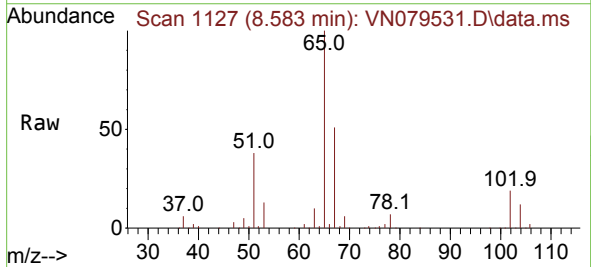






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:114 Resp: 621401
Ion Ratio Lower Upper
114 100
63 21.6 0.0 36.4
88 15.6 0.0 30.6



#35
Dibromofluoromethane
Concen: 49.336 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. 0.000 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48

Tgt Ion:113 Resp: 220316
Ion Ratio Lower Upper
113 100
111 103.7 82.6 123.8
192 17.0 12.7 19.1

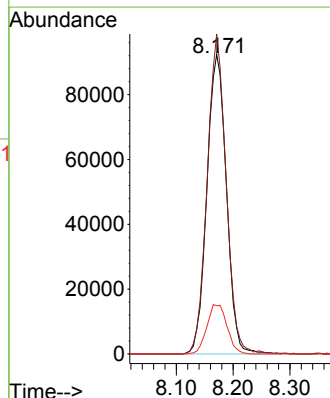



#36

1,1-Dichloropropene

Concen: 4.303 ug/l

RT: 8.230 min Scan# 1067

Delta R.T. -0.147 min


Lab File: VN079531.D

Acq: 11 Oct 2023 20:48

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 75 Resp: 28843

Ion Ratio Lower Upper

75 100

110 8.9 19.1 57.3#

77 0.0 25.0 37.4#

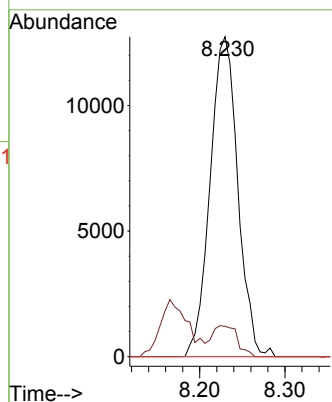

#38

Carbon Tetrachloride

Concen: 5.180 ug/l

RT: 8.230 min Scan# 1067

Delta R.T. -0.135 min

Lab File: VN079531.D

Acq: 11 Oct 2023 20:48




Tgt Ion: 117 Resp: 34757


Ion Ratio Lower Upper

117 100

119 6.4 77.3 115.9#

121 0.0 23.3 34.9#


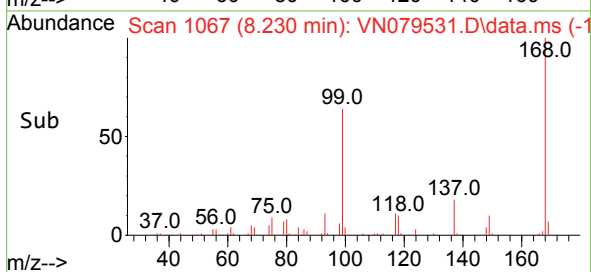

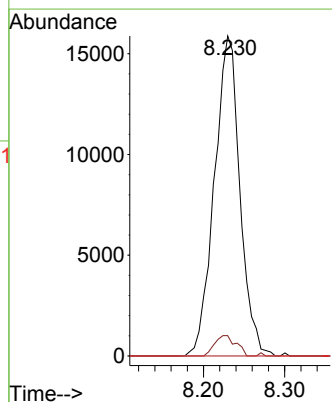




#40
Benzene
Concen: 4.930 ug/l
RT: 8.612 min Scan# 1132
Delta R.T. 0.000 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 78 Resp: 98133
Ion Ratio Lower Upper
78 100
77 23.6 19.0 28.6

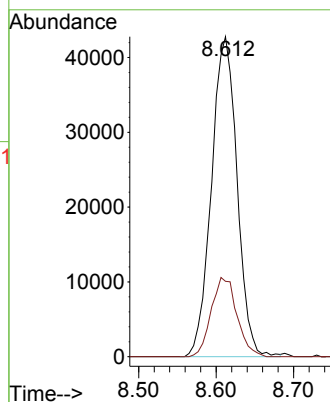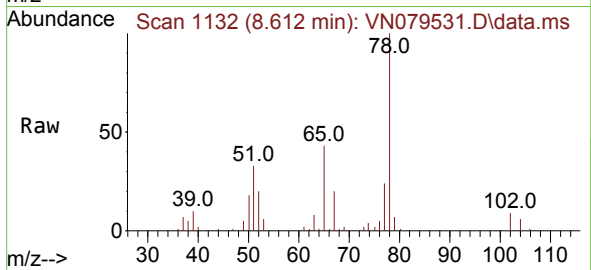

#43
Isopropyl Acetate
Concen: 0.950 ug/l
RT: 8.724 min Scan# 1151
Delta R.T. 0.030 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48


Tgt Ion: 43 Resp: 11103
Ion Ratio Lower Upper
43 100
61 0.0 24.7 37.1#
87 0.0 14.6 21.8#

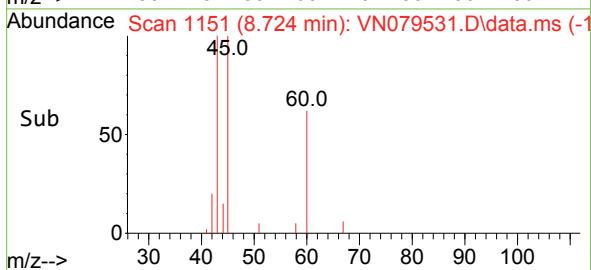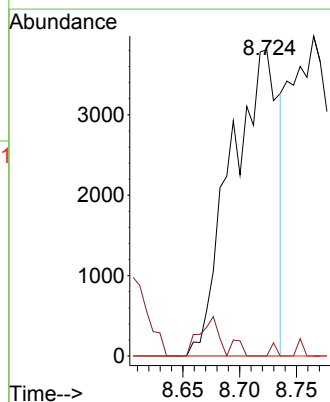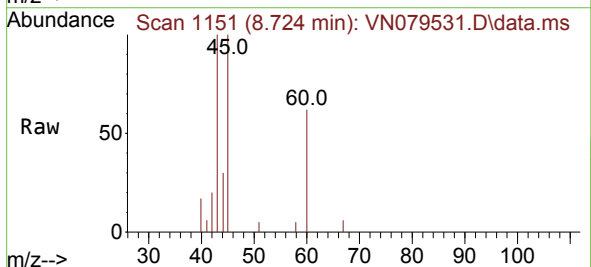






#48
Methyl methacrylate
Concen: 0.663 ug/l
RT: 9.665 min Scan# 11
Delta R.T. -0.023 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 41 Resp: 3318
Ion Ratio Lower Upper
41 100
69 0.0 90.4 135.6#
39 62.9 54.6 81.8



#50
Toluene-d8
Concen: 45.844 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48

Tgt Ion: 98 Resp: 740740
Ion Ratio Lower Upper
98 100
100 64.6 52.0 78.0

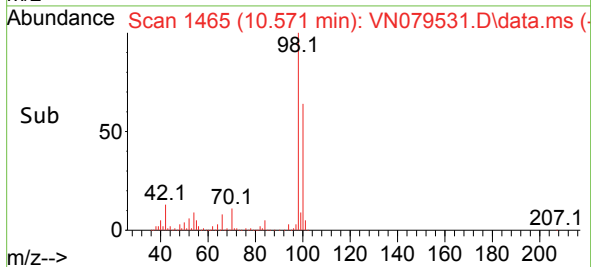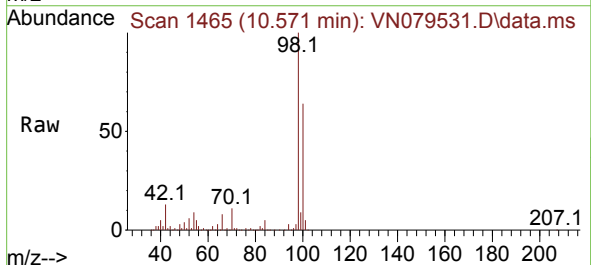

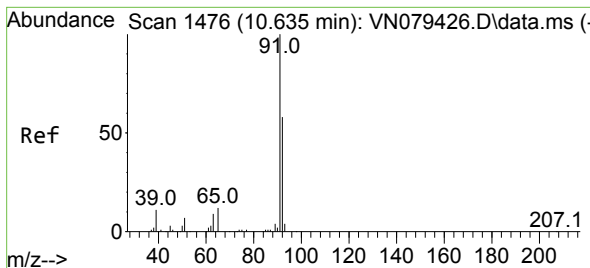

#52

Toluene

Concen: 7.581 ug/l

RT: 10.635 min Scan# 1476

Delta R.T. 0.000 min

Lab File: VN079531.D

Acq: 11 Oct 2023 20:48

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 92 Resp: 88825

Ion Ratio Lower Upper

92 100

91 184.3 137.4 206.0

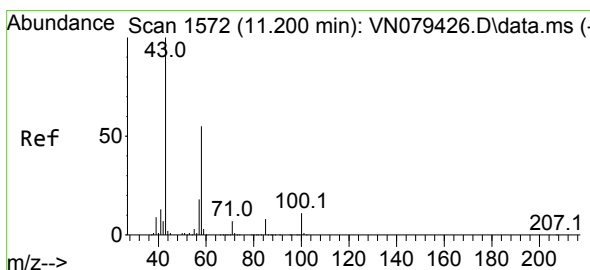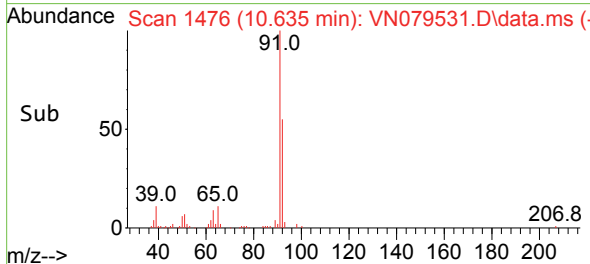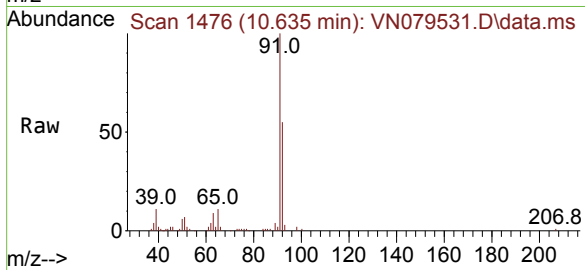

#59

2-Hexanone

Concen: 0.707 ug/l

RT: 11.200 min Scan# 1572

Delta R.T. 0.000 min

Lab File: VN079531.D




Acq: 11 Oct 2023 20:48


Tgt Ion: 43 Resp: 3364

Ion Ratio Lower Upper

43 100

58 39.4 31.7 95.1


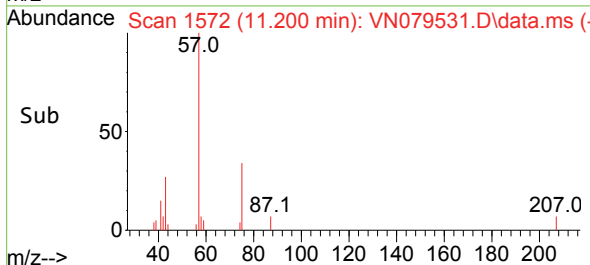

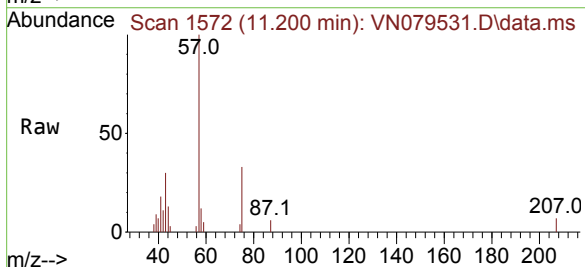




#62
4-Bromofluorobenzene
Concen: 54.571 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 282971
Ion Ratio Lower Upper
95 100
174 75.5 0.0 143.8
176 72.8 0.0 135.8

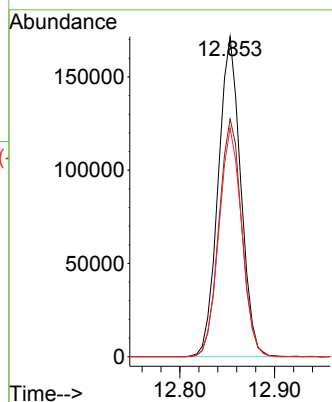

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1686
Delta R.T. 0.000 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48

Tgt Ion: 117 Resp: 632965
Ion Ratio Lower Upper
117 100
82 57.6 44.0 66.0
119 32.1 25.6 38.4


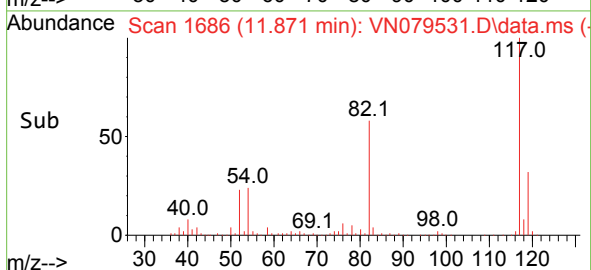




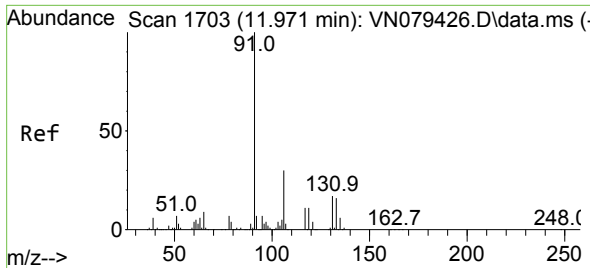

#67
Ethyl Benzene
Concen: 0.894 ug/l
RT: 11.971 min Scan# 1703
Delta R.T. 0.000 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 21908
Ion Ratio Lower Upper
91 100
106 29.1 25.6 38.4

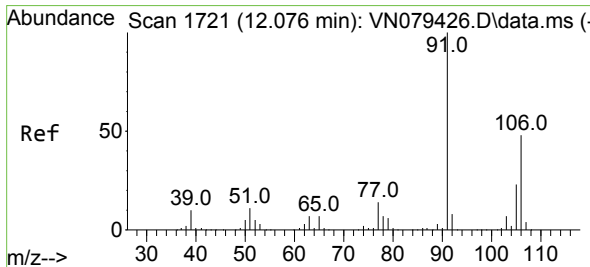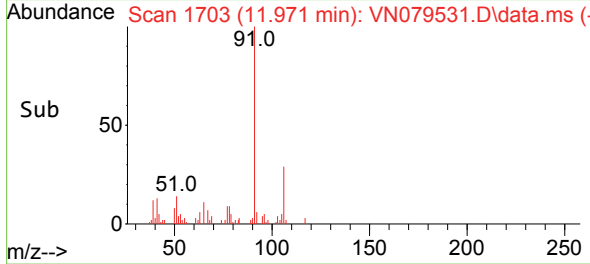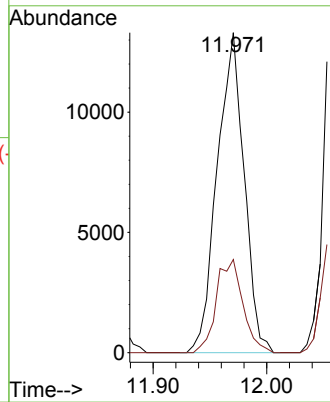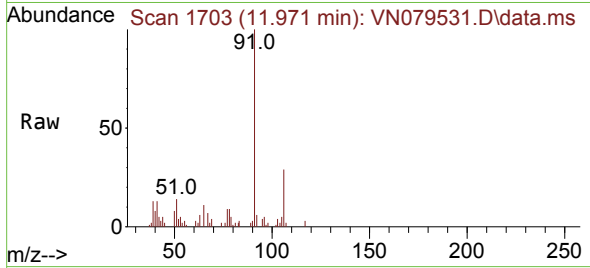

#68
m/p-Xylenes
Concen: 3.194 ug/l
RT: 12.076 min Scan# 1721
Delta R.T. 0.000 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48

Tgt Ion:106 Resp: 28438
Ion Ratio Lower Upper
106 100
91 207.7 159.6 239.4


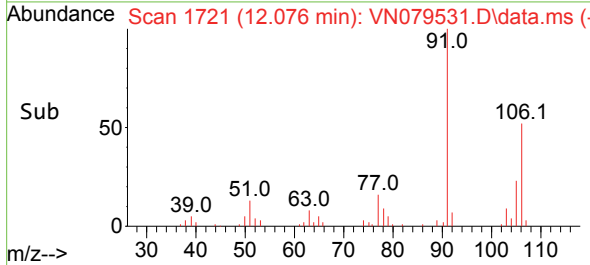

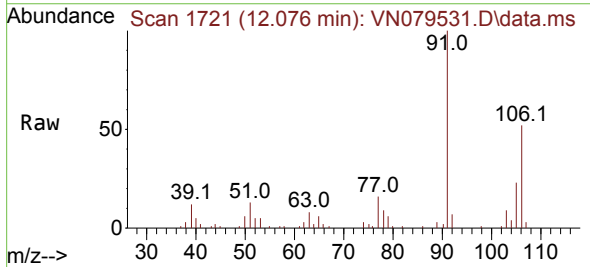




#69
o-Xylene
Concen: 1.467 ug/l
RT: 12.400 min Scan# 1777
Delta R.T. -0.006 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 12843
Ion Ratio Lower Upper
106 100
91 214.7 105.2 315.5

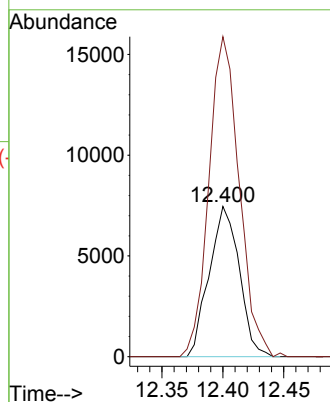

#70
Styrene
Concen: 0.581 ug/l
RT: 12.412 min Scan# 1778
Delta R.T. -0.006 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48

Tgt Ion:104 Resp: 8037
Ion Ratio Lower Upper
104 100
78 64.7 39.5 59.3#
103 64.9 43.2 64.8#

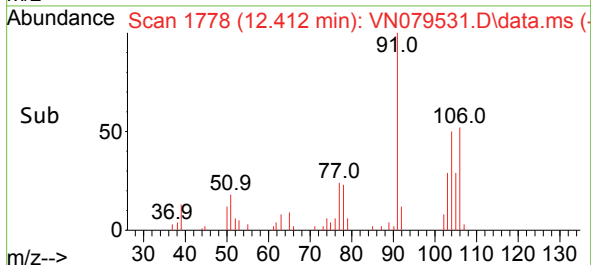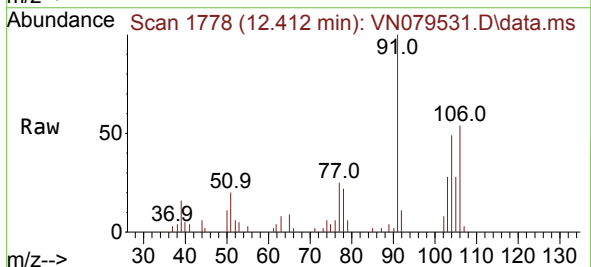



#71

Bromoform

Concen: 0.449 ug/l

RT: 12.847 min Scan# 1807

Delta R.T. 0.265 min

Lab File: VN079531.D

Acq: 11 Oct 2023 20:48

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:173 Resp: 1696

Ion Ratio Lower Upper

173 100

175 810.6 24.3 73.0#

254 0.0 0.0 0.0

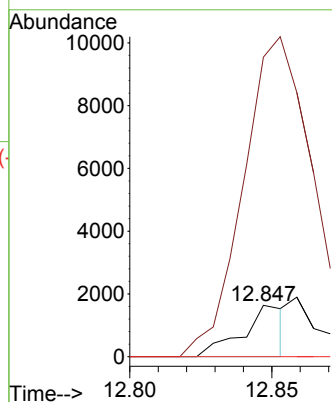

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. 0.000 min

Lab File: VN079531.D

Acq: 11 Oct 2023 20:48




Tgt Ion:152 Resp: 237400


Ion Ratio Lower Upper

152 100

115 63.1 32.3 96.8

150 160.8 0.0 355.8


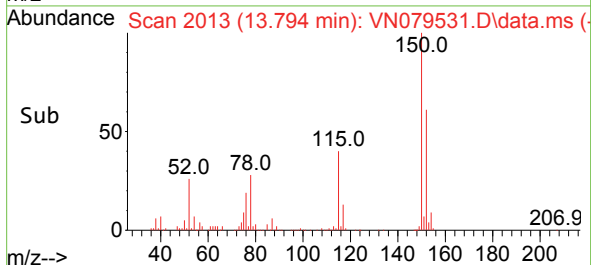

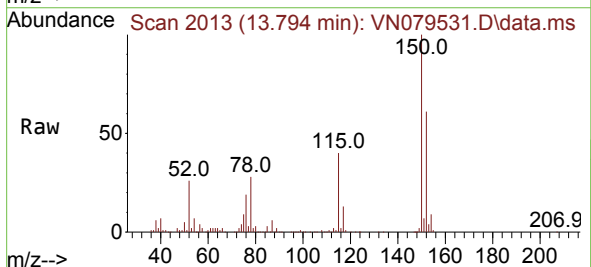




#75
 1,1,2,2-Tetrachloroethane
 Concen: 4.161 ug/l
 RT: 12.800 min Scan# 1853
 Delta R.T. -0.141 min
 Lab File: VN079531.D
 Acq: 11 Oct 2023 20:48




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 83 Resp: 37606
 Ion Ratio Lower Upper
 83 100
 131 0.0 5.0 15.0#
 85 5.7 31.9 95.7#

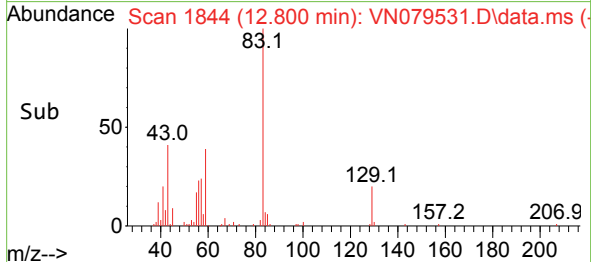

#76
 1,2,3-Trichloropropane
 Concen: 23.457 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. -0.147 min
 Lab File: VN079531.D
 Acq: 11 Oct 2023 20:48

Tgt Ion: 75 Resp: 160559
 Ion Ratio Lower Upper
 75 100
 77 1.3 84.5 253.5#

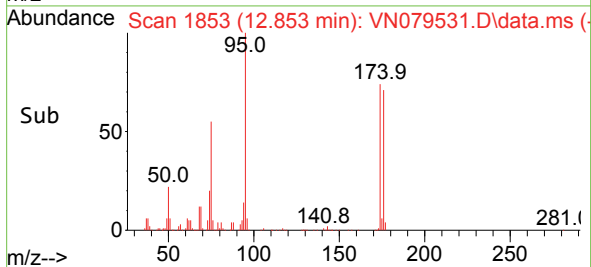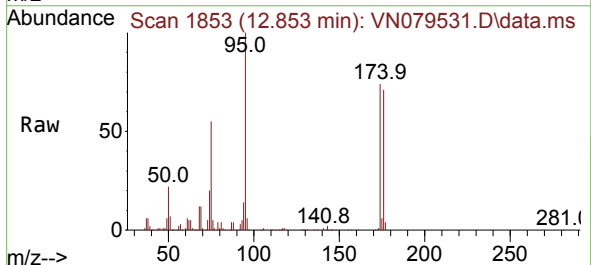



#80

1,3,5-Trimethylbenzene

Concen: 0.205 ug/l

RT: 13.176 min Scan# 1908

Delta R.T. 0.000 min

Lab File: VN079531.D

Acq: 11 Oct 2023 20:48

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:105 Resp: 3570

Ion Ratio Lower Upper

105 100

120 48.2 24.1 72.3



#81

trans-1,4-Dichloro-2-butene

Concen: 68.061 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. 0.112 min

Lab File: VN079531.D

Acq: 11 Oct 2023 20:48




Tgt Ion: 75 Resp: 160559


Ion Ratio Lower Upper

75 100

53 0.3 67.4 101.2#

89 0.0 38.8 58.2#

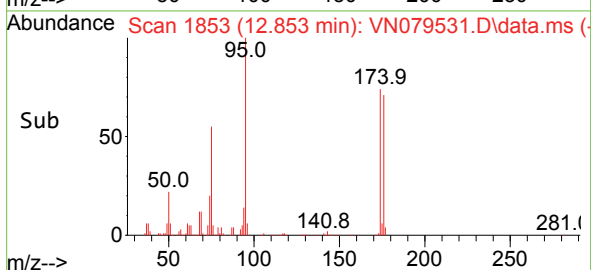



#84

1,2,4-Trimethylbenzene

Concen: 0.680 ug/l

RT: 13.488 min Scan# 1961

Delta R.T. 0.000 min

Lab File: VN079531.D

Acq: 11 Oct 2023 20:48

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:105 Resp: 11308

Ion Ratio Lower Upper

105 100

120 41.2 22.0 66.0

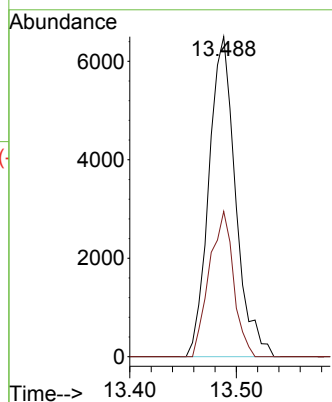

#85

sec-Butylbenzene

Concen: 0.568 ug/l

RT: 13.488 min Scan# 1961

Delta R.T. -0.135 min

Lab File: VN079531.D




Acq: 11 Oct 2023 20:48


Tgt Ion:105 Resp: 11308

Ion Ratio Lower Upper

105 100


134 0.0 9.8 29.3#

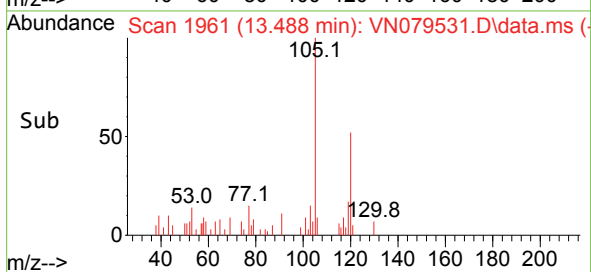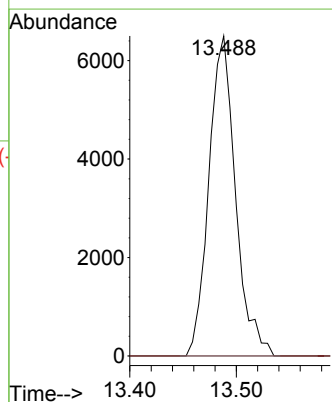






#90
Hexachloroethane
Concen: Below Cal
RT: 14.318 min Scan# 2105
Delta R.T. -0.017 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48

Instrument :
MSVOA_N
ClientSampleId :



Tgt Ion:117 Resp: 54
Ion Ratio Lower Upper
117 100
201 0.0 29.3 88.0#

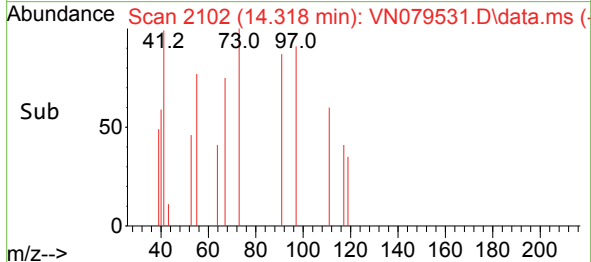

#95
Naphthalene
Concen: 12.654 ug/l
RT: 15.647 min Scan# 2328
Delta R.T. -0.000 min
Lab File: VN079531.D
Acq: 11 Oct 2023 20:48

Tgt Ion:128 Resp: 100265
Ion Ratio Lower Upper
128 100
127 11.9 10.0 15.0
129 11.2 8.7 13.1

