
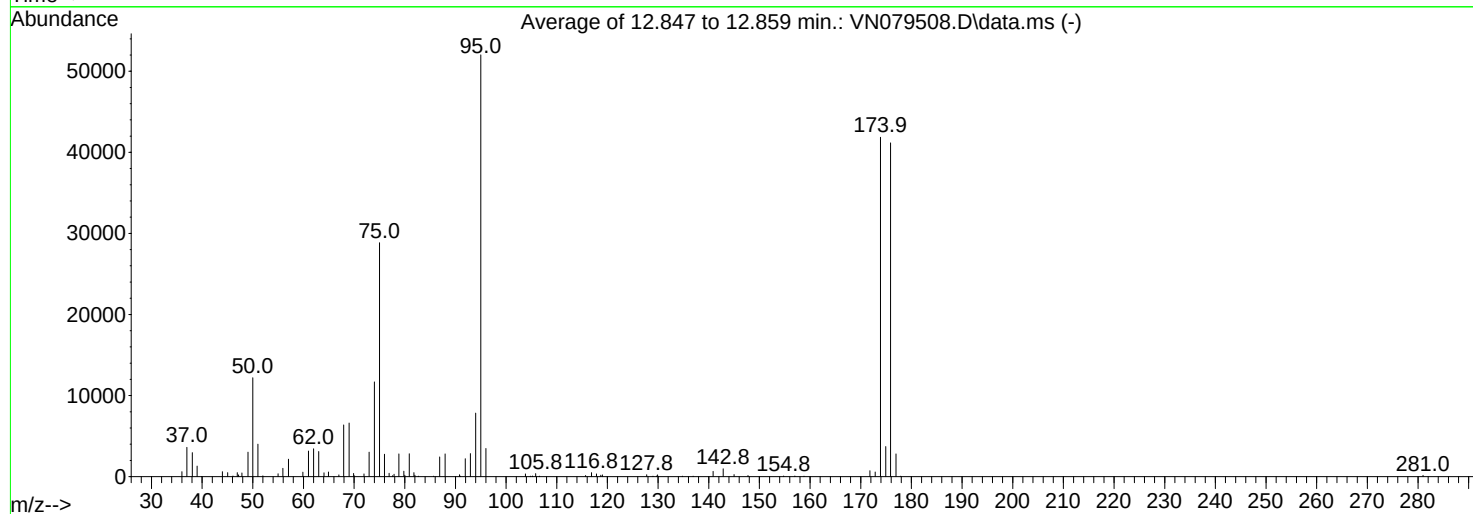


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN101123\  
Data File : VN079508.D  
Acq On : 11 Oct 2023 10:30  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N100523W.M  
Title : SW846 8260  
Last Update : Fri Oct 06 03:34:49 2023

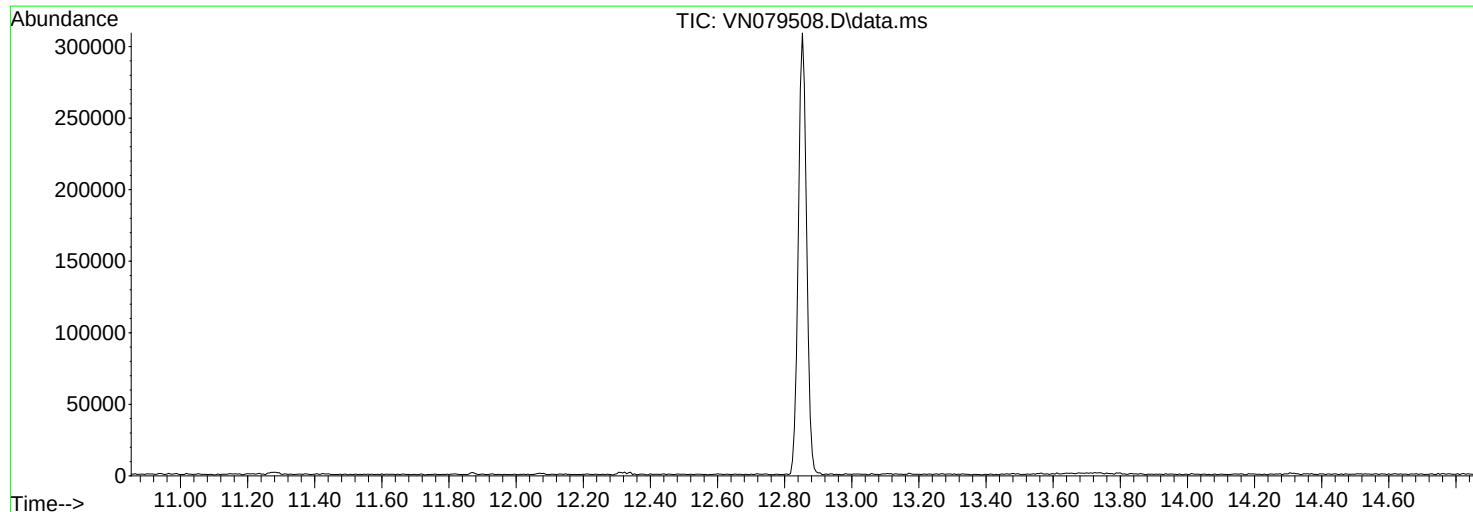

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 23.5         | 12204      | PASS                |
| 75             | 95              | 30              | 60              | 55.5         | 28853      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 52021      | PASS                |
| 96             | 95              | 5               | 9               | 6.7          | 3473       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.4          | 575        | PASS                |
| 174            | 95              | 50              | 100             | 80.5         | 41856      | PASS                |
| 175            | 174             | 5               | 9               | 8.8          | 3703       | PASS                |
| 176            | 174             | 95              | 101             | 98.3         | 41157      | PASS                |
| 177            | 176             | 5               | 9               | 6.8          | 2794       | PASS                |

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z   | abund. |
|-------|--------|-------|--------|-------|--------|-------|--------|
| 36.00 | 614    | 49.05 | 3018   | 64.05 | 477    | 76.00 | 275    |
| 37.00 | 3618   | 50.00 | 12204  | 64.95 | 582    | 76.90 | 421    |
| 38.05 | 2957   | 51.00 | 4001   | 67.00 | 215    | 77.60 | 12     |
| 39.00 | 1304   | 52.00 | 109    | 67.95 | 6366   | 77.90 | 28     |
| 39.90 | 24     | 55.00 | 352    | 69.00 | 6617   | 78.85 | 2801   |
| 44.00 | 607    | 55.95 | 1024   | 69.90 | 387    | 79.80 | 663    |
| 45.05 | 494    | 57.05 | 2146   | 70.10 | 109    | 80.00 | 178    |
| 46.10 | 73     | 59.90 | 550    | 71.95 | 342    | 80.90 | 2827   |
| 46.95 | 502    | 61.00 | 3167   | 72.95 | 3013   | 81.80 | 488    |
| 47.20 | 210    | 62.00 | 3435   | 74.00 | 11675  | 82.00 | 188    |
| 47.85 | 453    | 63.00 | 3090   | 75.00 | 28853  | 82.70 | 56     |

Average of 12.847 to 12.859 min.: VN079508.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z    | abund. | m/z    | abund. | m/z    | abund. |
|--------|--------|--------|--------|--------|--------|--------|--------|
| 85.70  | 58     | 104.80 | 66     | 129.70 | 88     | 171.80 | 736    |
| 86.90  | 2428   | 105.20 | 75     | 129.90 | 212    | 172.85 | 575    |
| 87.95  | 2801   | 105.85 | 375    | 134.80 | 53     | 173.90 | 41856  |
| 90.80  | 230    | 106.60 | 63     | 136.90 | 51     | 174.95 | 3703   |
| 91.00  | 64     | 115.70 | 135    | 140.85 | 649    | 175.90 | 41157  |
| 91.95  | 2204   | 116.85 | 494    | 142.85 | 971    | 176.95 | 2794   |
| 92.95  | 2846   | 117.85 | 336    | 145.00 | 258    | 177.90 | 50     |
| 94.00  | 7828   | 118.70 | 179    | 147.75 | 143    | 281.00 | 152    |
| 95.00  | 52021  | 119.00 | 222    | 154.80 | 81     |        |        |
| 96.00  | 3473   | 127.75 | 234    | 157.00 | 75     |        |        |
| 103.80 | 335    | 129.00 | 50     | 158.80 | 53     |        |        |

Instrument :

MSVOA\_N

ClientSampleId :

BFB