
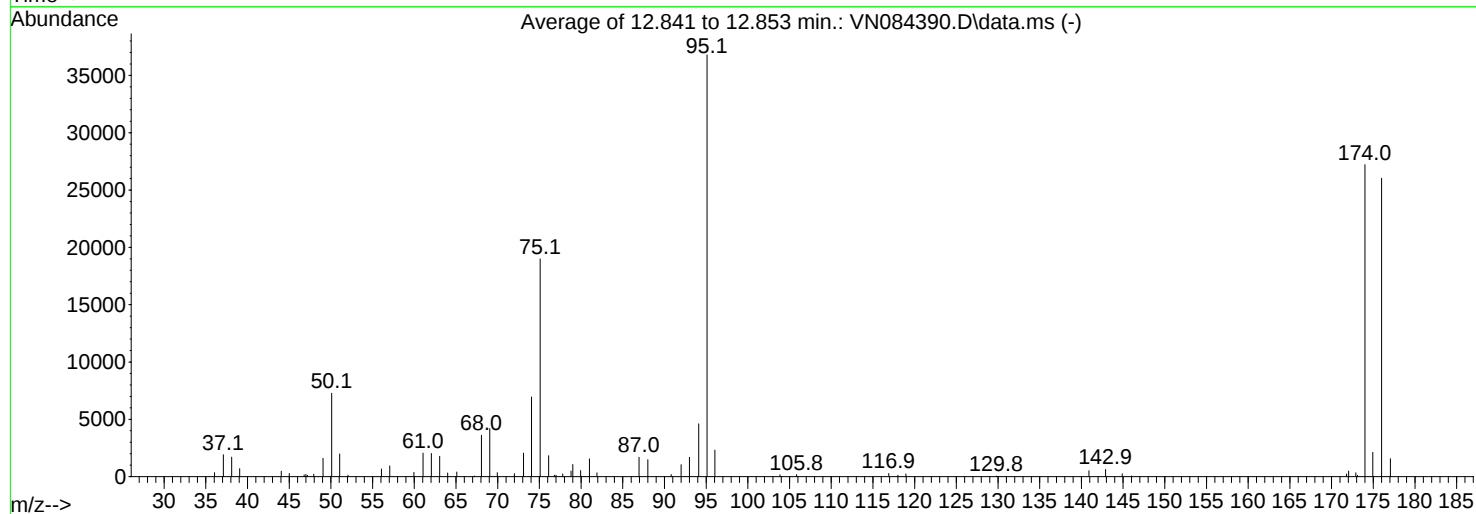


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101124\
Data File : VN084390.D
Acq On : 11 Oct 2024 08:36
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N093024W.M
Title : SW846 8260
Last Update : Tue Oct 01 07:11:01 2024

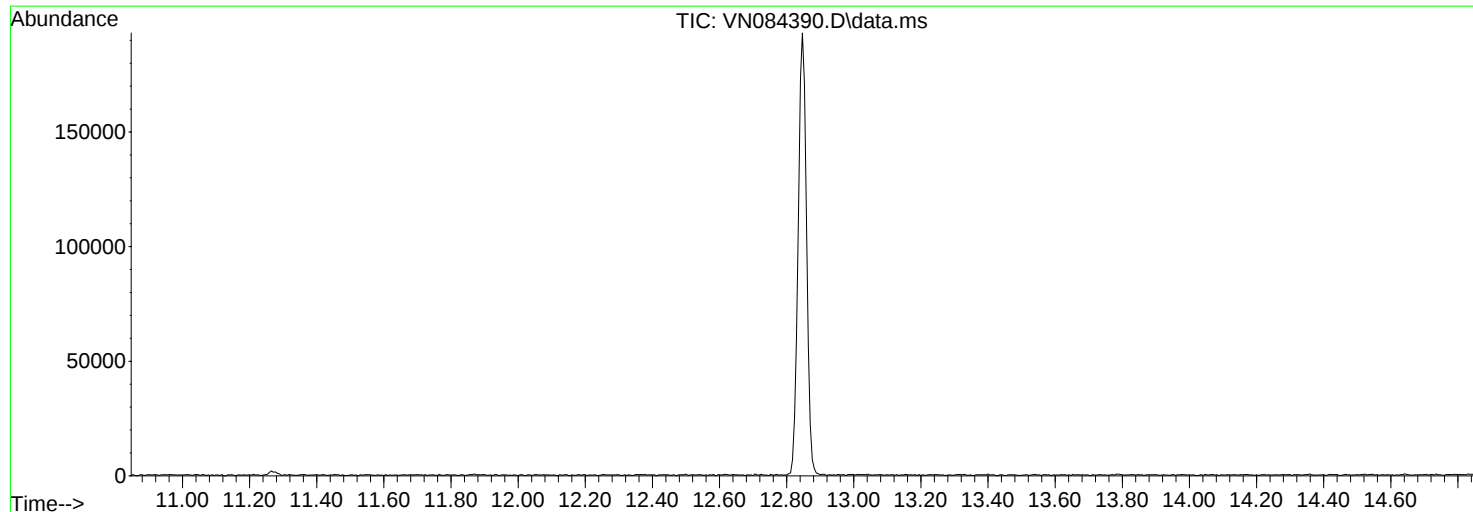

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	7271	PASS
75	95	30	60	51.6	18995	PASS
95	95	100	100	100.0	36795	PASS
96	95	5	9	6.3	2317	PASS
173	174	0.00	2	1.2	336	PASS
174	95	50	100	74.0	27216	PASS
175	174	5	9	7.8	2124	PASS
176	174	95	101	95.6	26024	PASS
177	176	5	9	6.0	1563	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	346	50.10	7271	67.20	54	77.80	231
37.10	1918	51.05	1976	68.05	3618	78.80	481
38.10	1699	52.05	131	69.05	4193	79.00	106
39.05	702	56.05	671	69.95	350	79.95	52
44.05	477	57.05	934	72.00	269	81.00	1545
45.00	287	59.95	382	73.10	2050	81.90	338
46.80	154	61.05	2052	74.05	6946	86.95	1685
47.00	199	62.05	2022	75.10	18995	88.00	1482
47.20	119	63.05	1772	76.10	1823	90.80	180
47.95	211	64.00	324	76.80	129	92.00	1042
49.05	1610	65.10	402	77.00	130	93.00	1689

Average of 12.841 to 12.853 min.: VN084390.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.10	4600	144.90	254				
95.10	36795	146.00	56				
96.05	2317	171.80	218				
103.85	170	172.05	490				
105.85	180	172.90	336				
116.90	287	173.10	114				
118.00	130	174.00	27216				
118.95	245	174.95	2124				
129.80	51	176.00	26024				
140.90	522	177.05	1563				
142.90	634						

Instrument :

MSVOA_N

ClientSampleId :

BFB