



1,2,4-Trichlorobenzene

Response Ratio

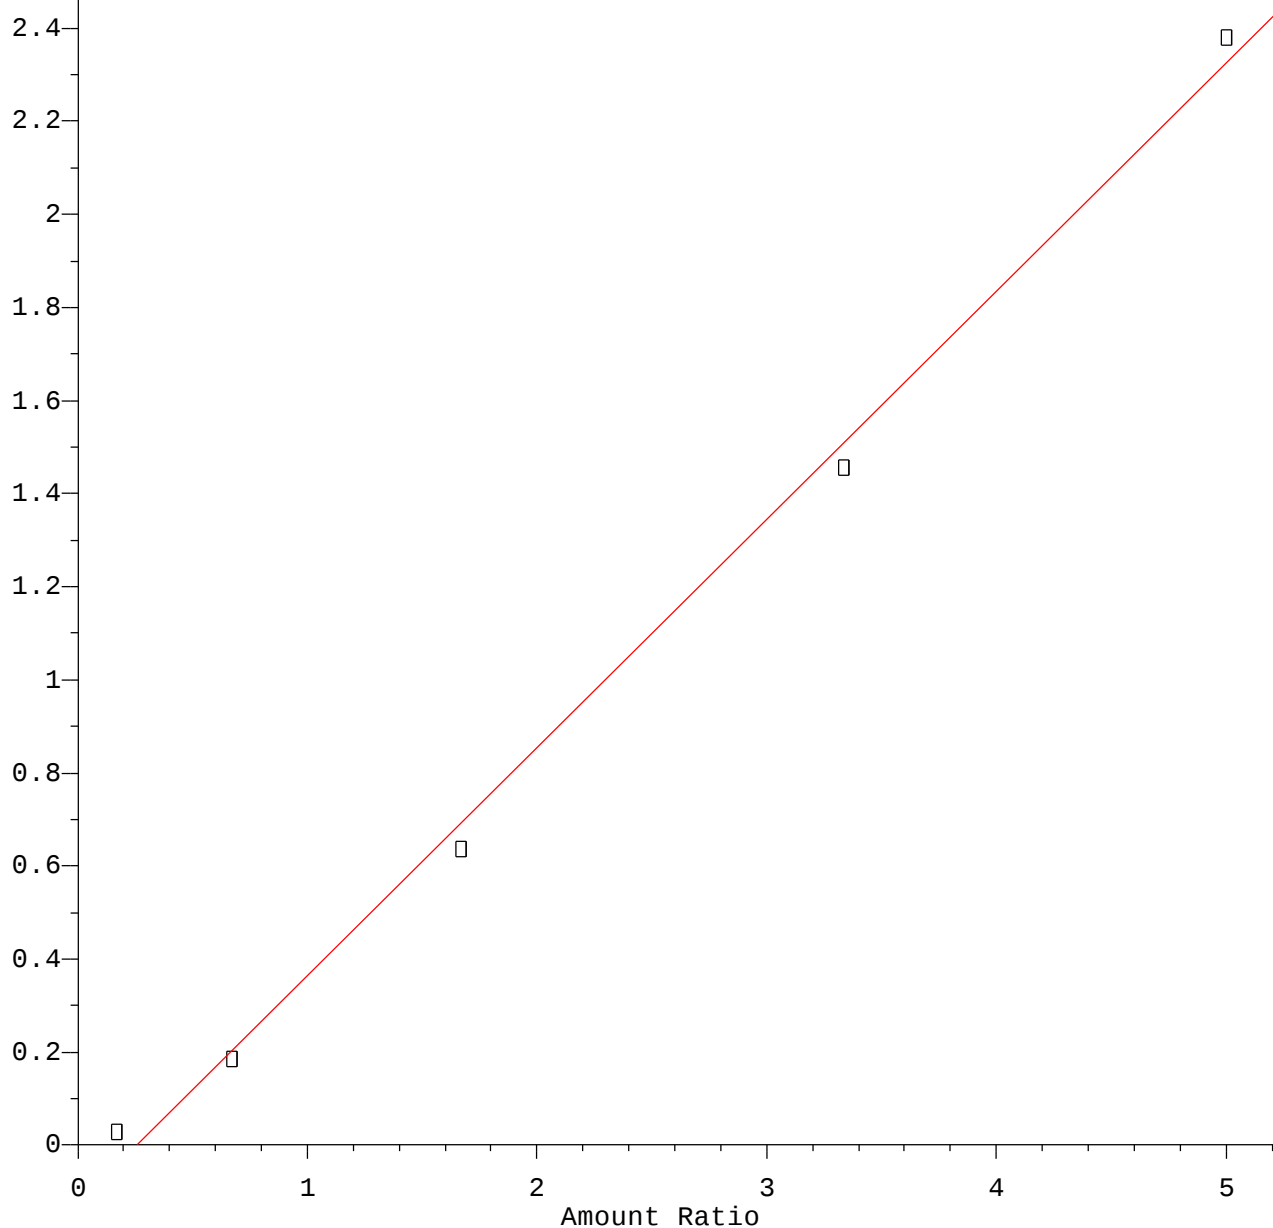

Resp Ratio = $4.90 \times 10^{-1} \times \text{Amt} - 1.26 \times 10^{-1}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N101218W.M
Calibration Table Last Updated: Fri Oct 12 10:23:44 2018

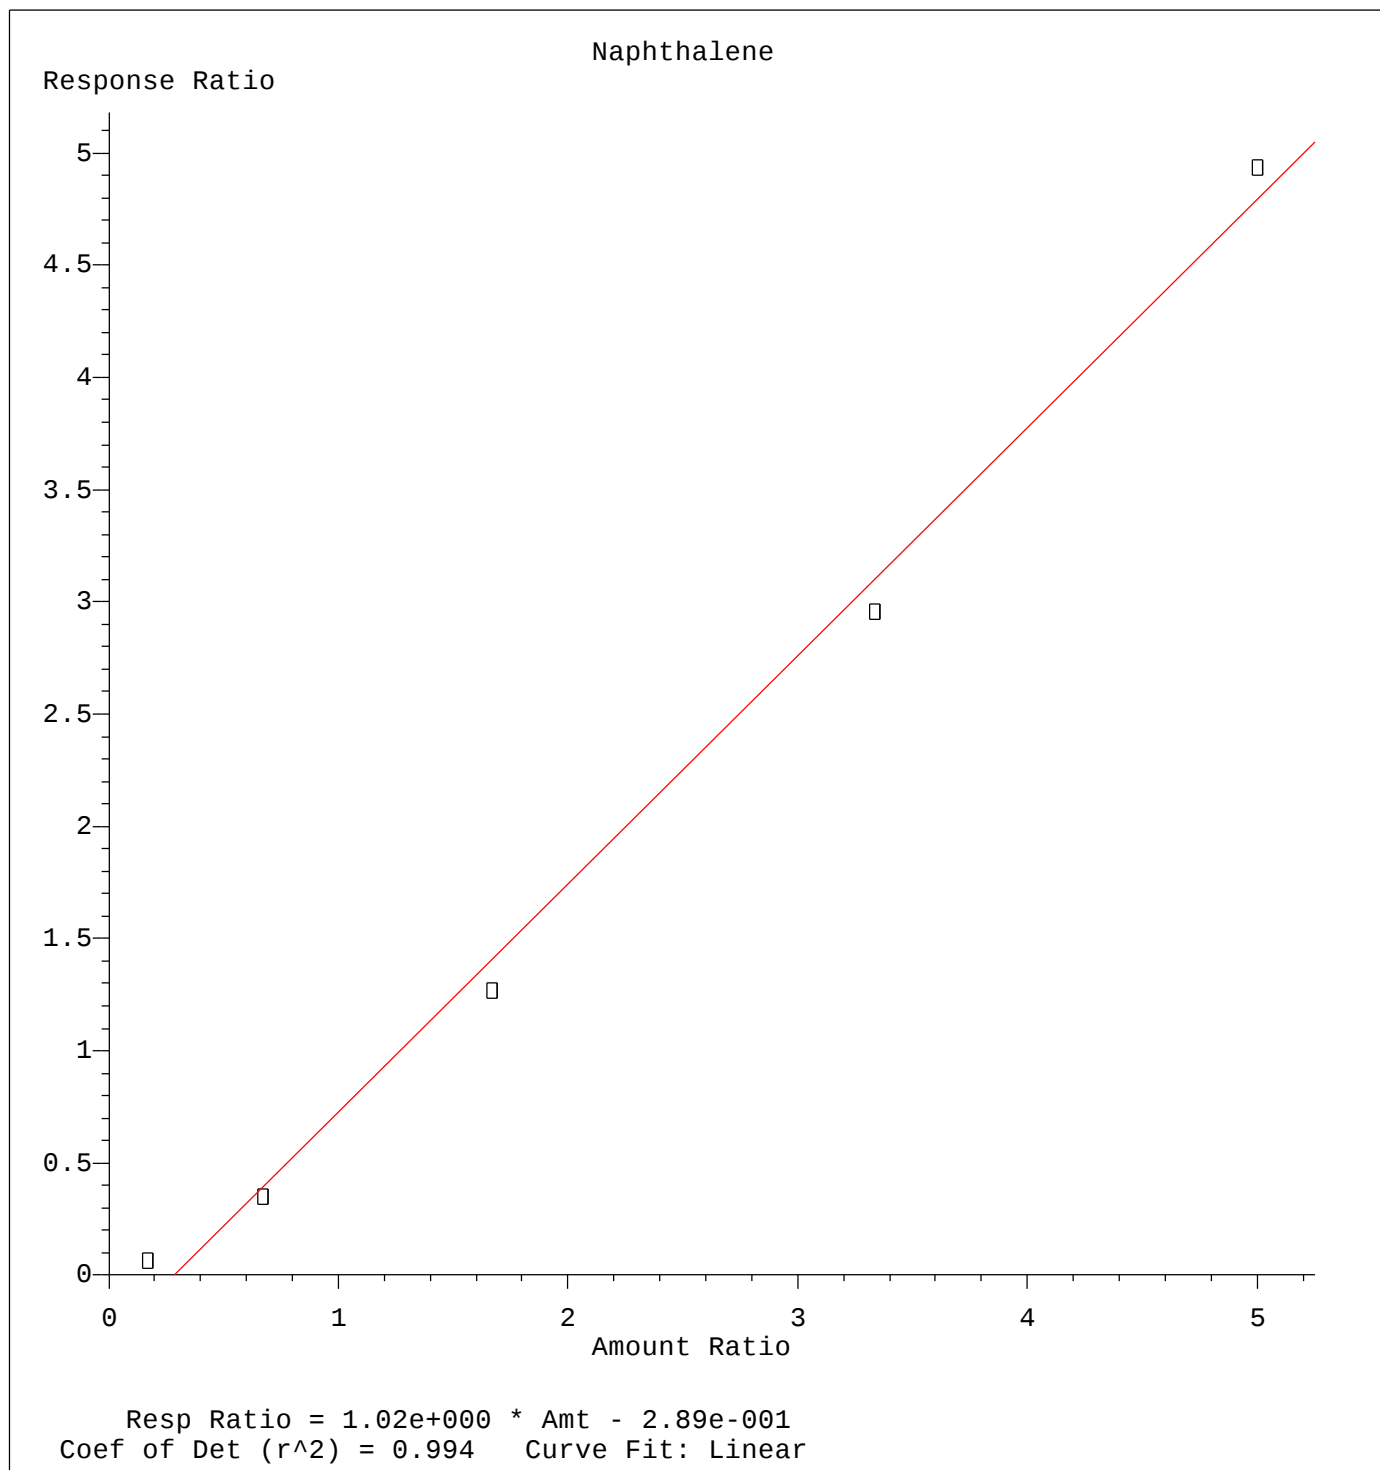

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N101218W.M
Calibration Table Last Updated: Fri Oct 12 10:23:44 2018

1,2,4-Trichlorobenzene

Response Ratio

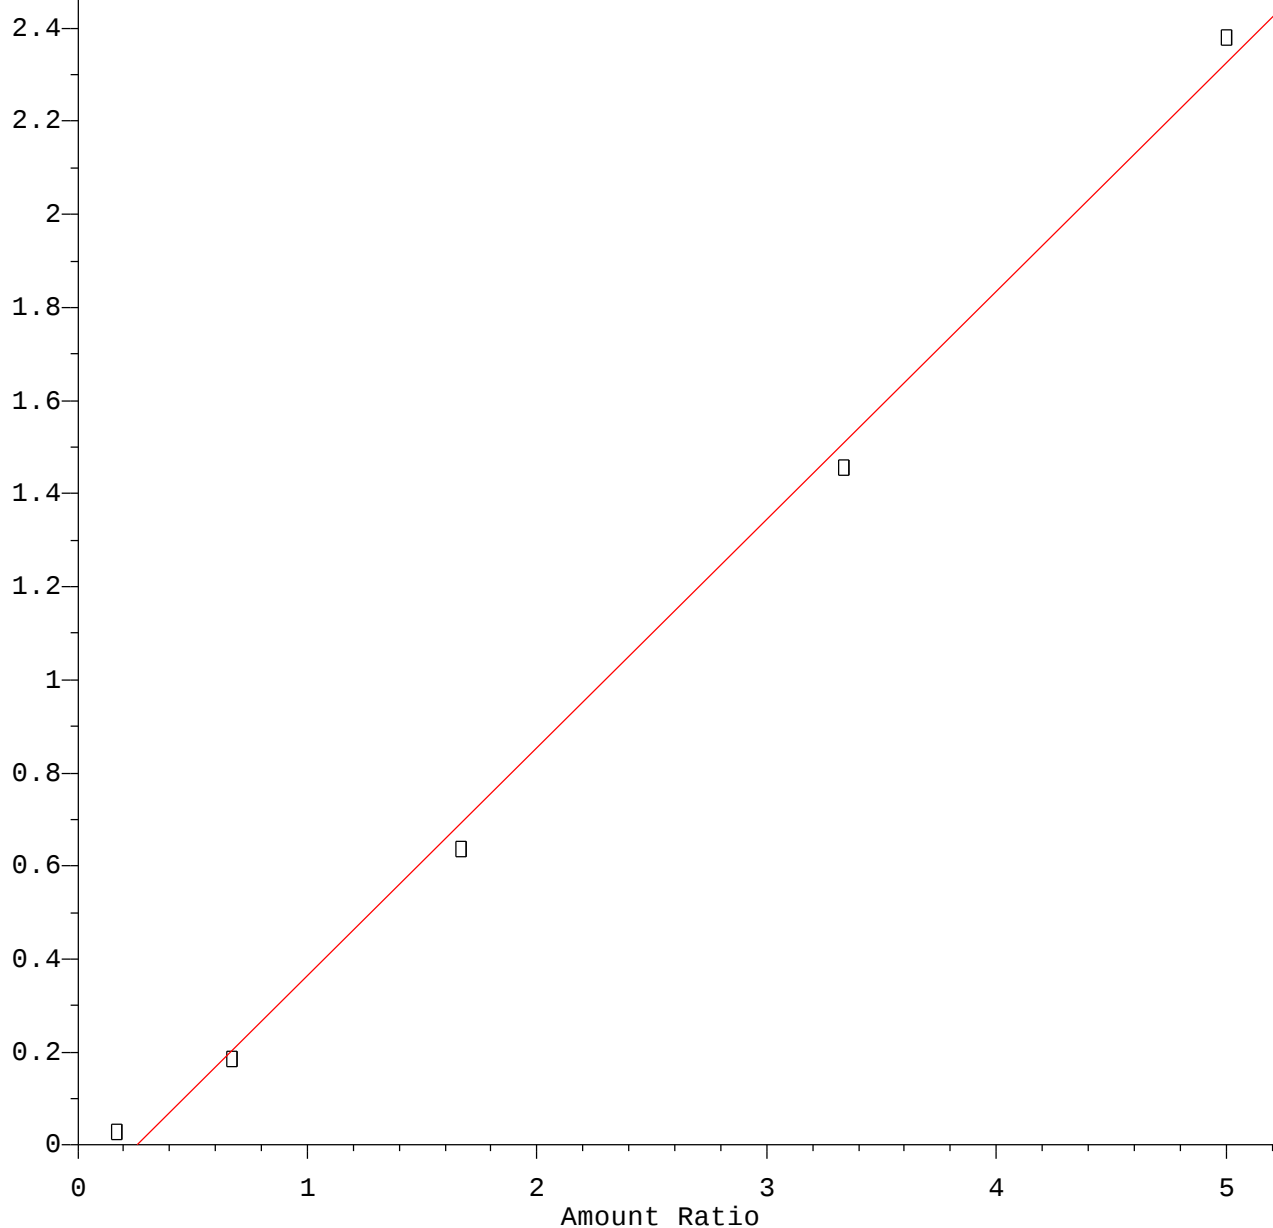

Resp Ratio = $4.90 \times 10^{-1} \times \text{Amt} - 1.26 \times 10^{-1}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N101218W.M
Calibration Table Last Updated: Fri Oct 12 10:23:44 2018