

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN101218\
 Data File : VN051844.D
 Acq On : 12 Oct 2018 20:46
 Operator : MD\SY
 Sample : J5459-02
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 25 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Quant Time: Oct 13 02:23:35 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101118W.M
 Quant Title : SW846 8260
 QLast Update : Fri Oct 12 09:51:20 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	806566	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1161440	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	999036	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	335350	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	433870	56.28	ug/l	0.00
Spiked Amount	50.000		Recovery	=	112.56%	
35) Dibromofluoromethane	7.59	113	439085	60.80	ug/l	0.00
Spiked Amount	50.000		Recovery	=	121.60%	
50) Toluene-d8	10.09	98	1582761	58.81	ug/l	0.00
Spiked Amount	50.000		Recovery	=	117.62%	
62) 4-Bromofluorobenzene	12.40	95	443653	47.76	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.52%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN101218\
Data File : VN051844.D
Acq On : 12 Oct 2018 20:46
Operator : MD\SY
Sample : J5459-02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 25 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Time: Oct 13 02:23:35 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N101118W.M
Quant Title : SW846 8260
QLast Update : Fri Oct 12 09:51:20 2018
Response via : Initial Calibration

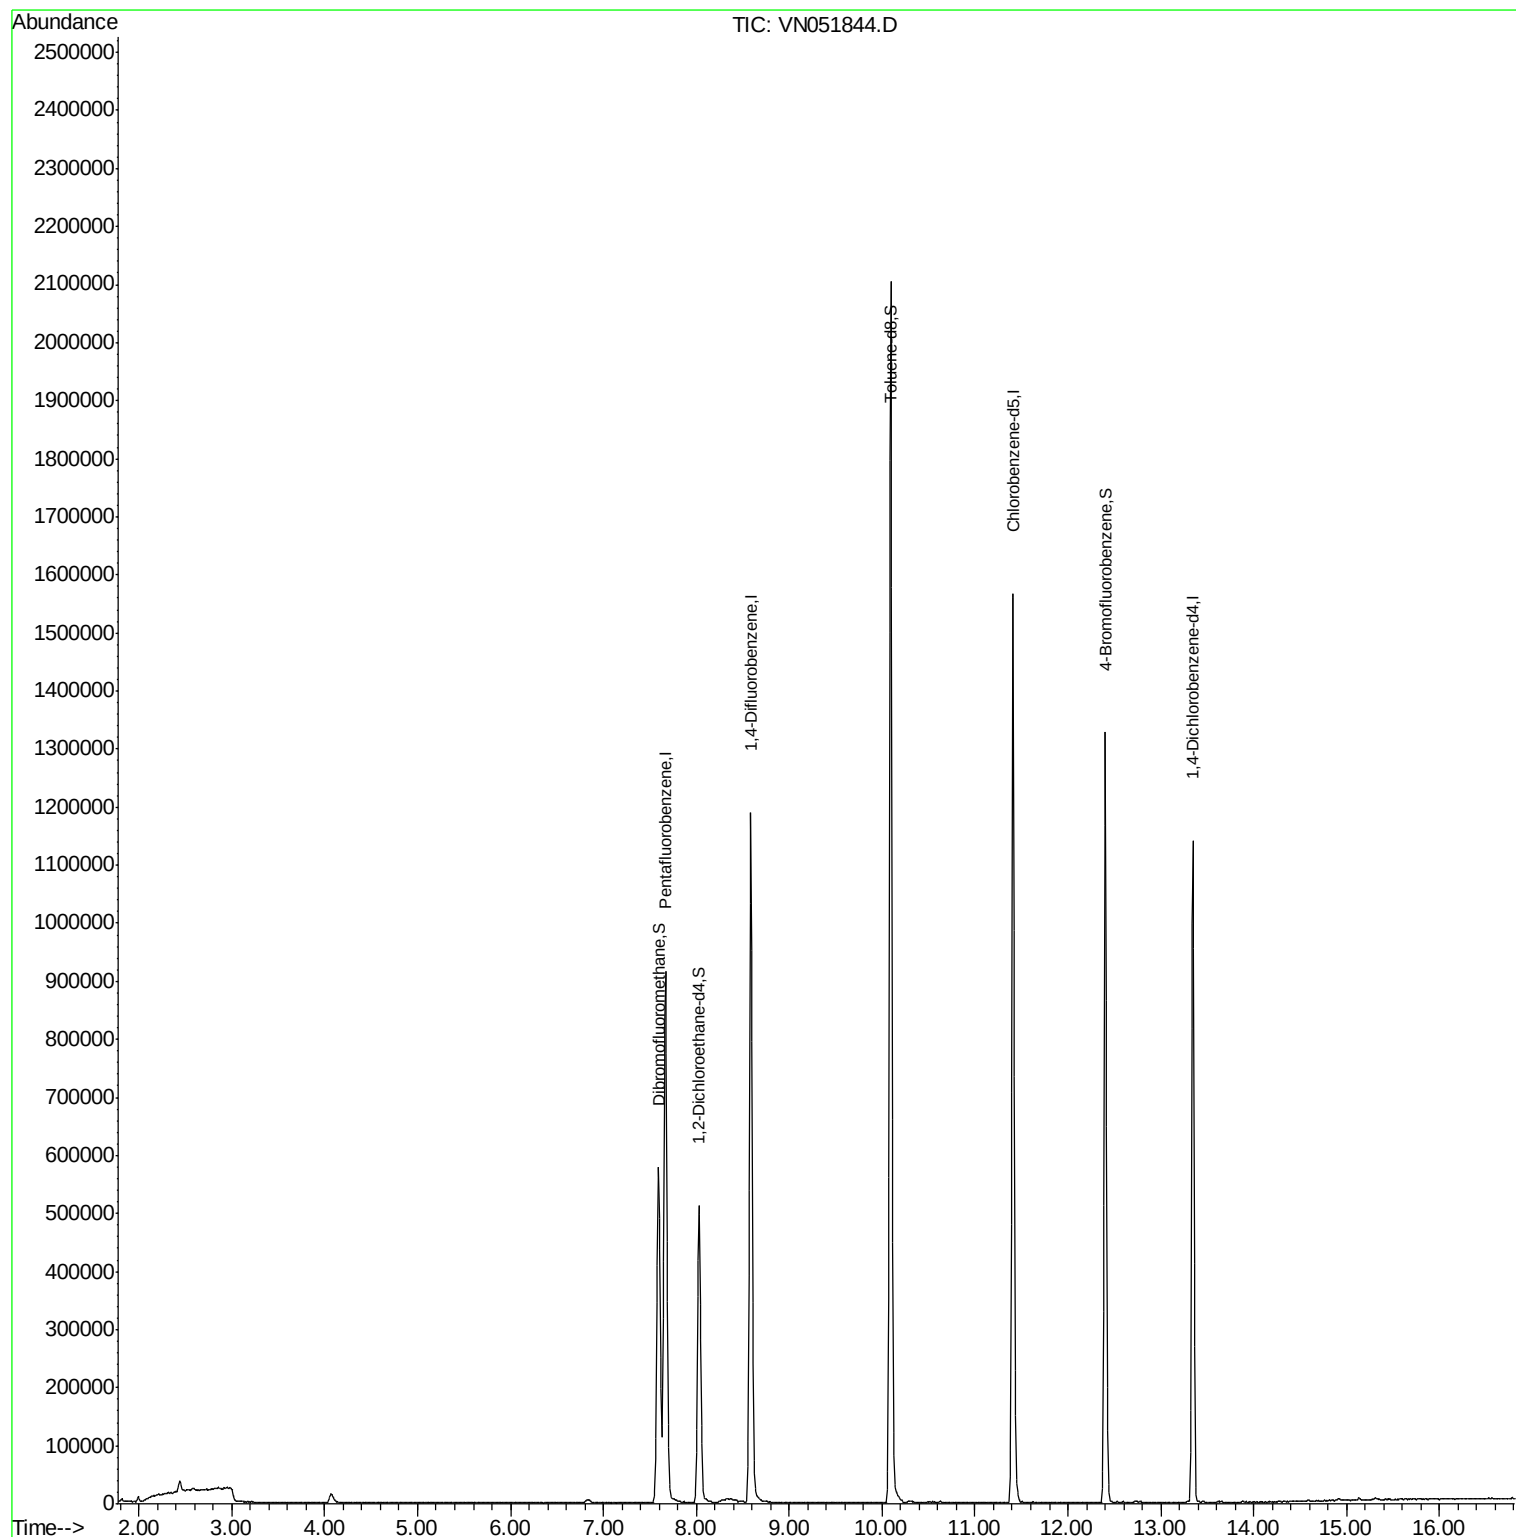

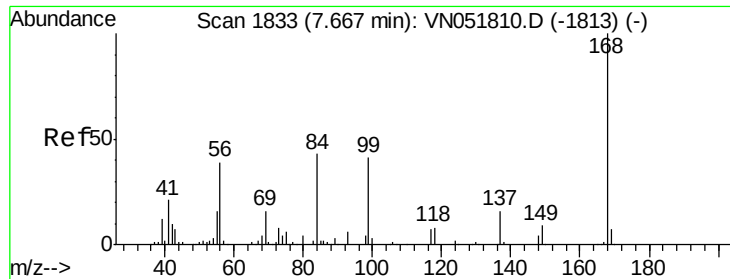

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. 0.00 min

Lab File: VN051844.D

Acq: 12 Oct 2018 20:46

Instrument :

MSVOA_N

ClientSampleId :


STORAGE-BLANK-WATER-REF-5

Tgt Ion:168 Resp: 806566

Ion Ratio Lower Upper

168 100

99 49.7 39.6 59.4

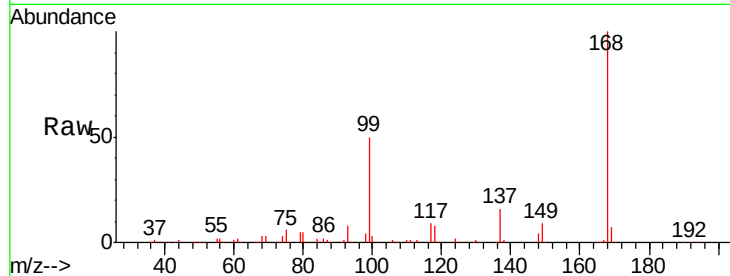

Abundance Ion 167.90 (167.60 to 168.60): VN051810.D (-1813) (-)

Ion 98.90 (98.60 to 99.60): VN051810.D (-1813) (-)

7.67



300000

200000

100000

0

Time-->

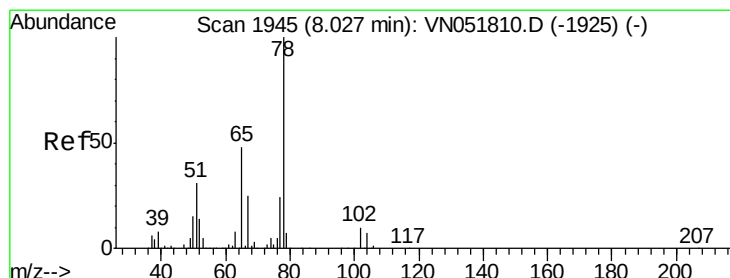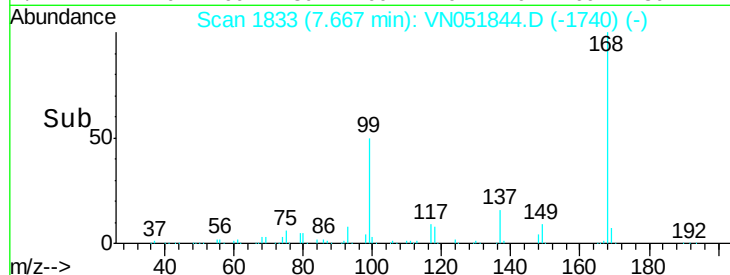

#33

1,2-Dichloroethane-d4

Concen: Below ug/l

RT: 8.03 min Scan# 1946

Delta R.T. 0.00 min

Lab File: VN051844.D


Acq: 12 Oct 2018 20:46

Tgt Ion: 65 Resp: 433870

Ion Ratio Lower Upper

65 100

67 52.1 0.0 110.4

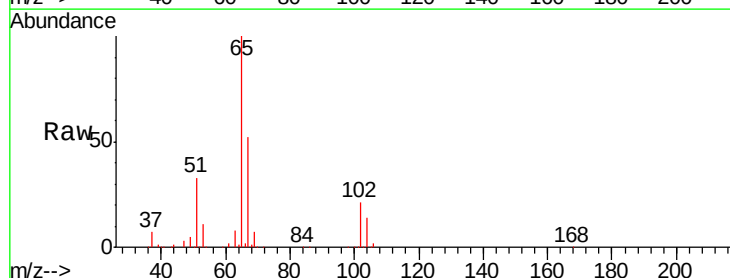

Abundance Ion 64.90 (64.60 to 65.60): VN051810.D (-1925) (-)

Ion 66.90 (66.60 to 67.60): VN051810.D (-1925) (-)

8.03

200000


150000


100000

50000

0

Time-->

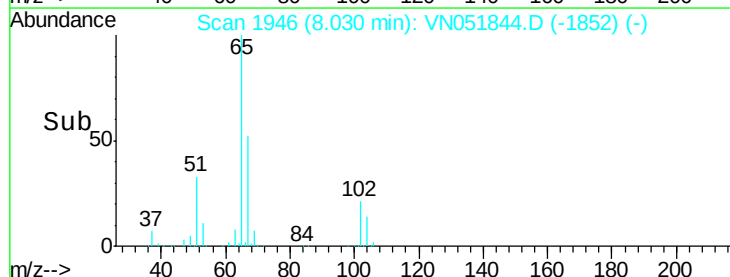

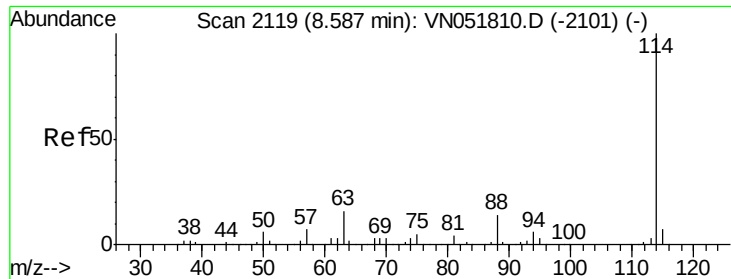

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 8.59 min Scan# 2119

Delta R.T. 0.00 min

Lab File: VN051844.D

Acq: 12 Oct 2018 20:46

Instrument :

MSVOA_N

ClientSampleId :

STORAGE-BLANK-WATER-REF-5


Tgt Ion:114 Resp: 1161440

Ion Ratio Lower Upper

114 100

63 16.6 0.0 38.6




88 14.3 0.0 30.6

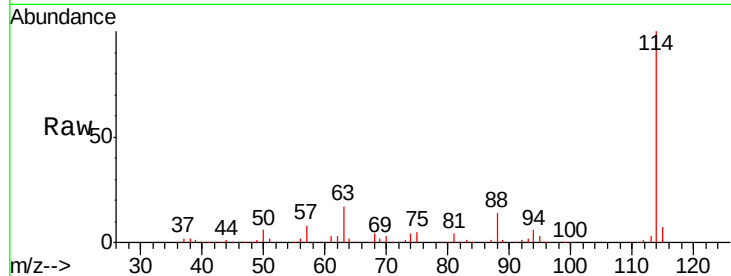

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN0

Ion 87.90 (87.60 to 88.60): VN0

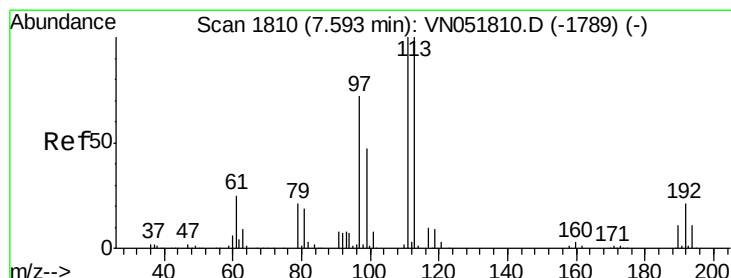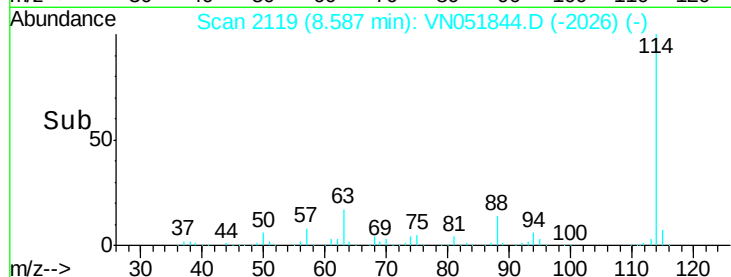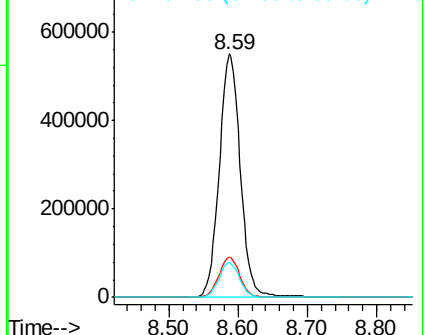

#35

Dibromofluoromethane

Concen: 50.00 ug/l

RT: 7.59 min Scan# 1810

Delta R.T. 0.00 min

Lab File: VN051844.D

Acq: 12 Oct 2018 20:46


Tgt Ion:113 Resp: 439085

Ion Ratio Lower Upper

113 100

111 101.5 82.6 123.8



192 21.1 18.0 27.0

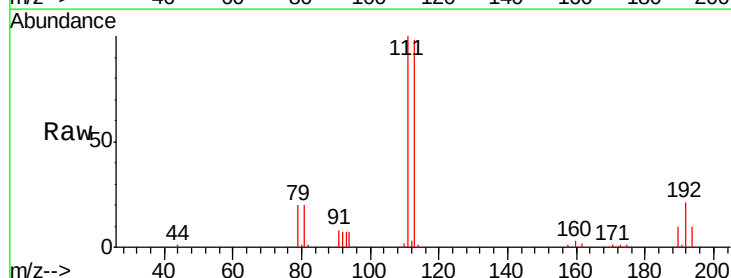


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



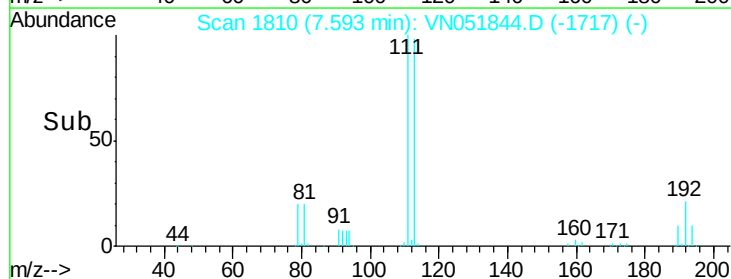
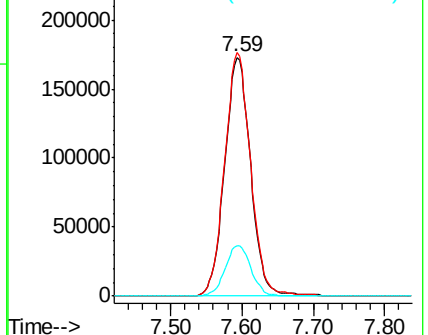


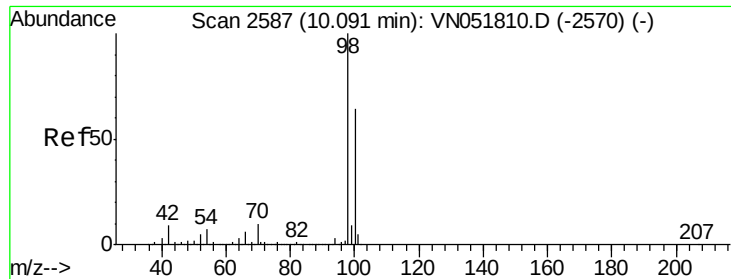

#50
Toluene-d8
Concen: N.D. ug/l
RT: 10.09 min Scan# 2587
Delta R.T. 0.00 min
Lab File: VN051844.D
Acq: 12 Oct 2018 20:46




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion: 98 Resp: 1582761
Ion Ratio Lower Upper
98 100
100 63.6 51.5 77.3

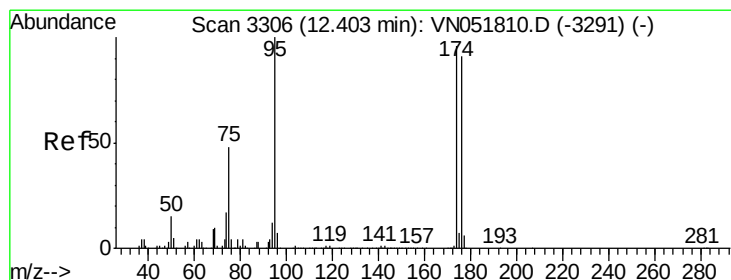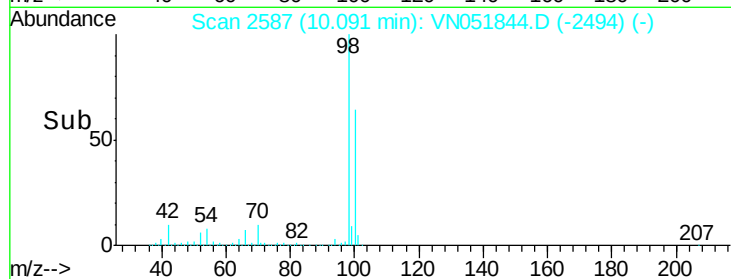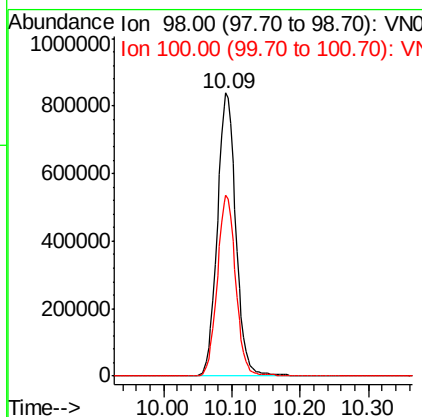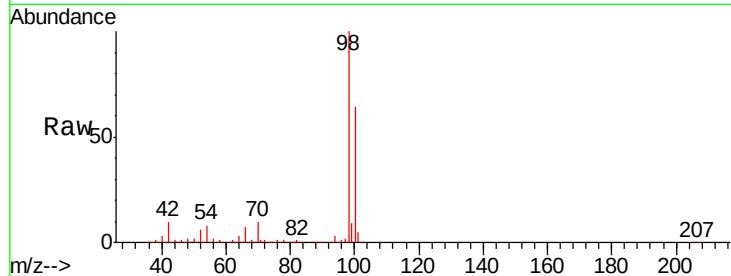

#62
4-Bromofluorobenzene
Concen: N.D. ug/l
RT: 12.40 min Scan# 3306
Delta R.T. 0.00 min
Lab File: VN051844.D
Acq: 12 Oct 2018 20:46

Tgt Ion: 95 Resp: 443653
Ion Ratio Lower Upper
95 100
174 94.5 0.0 183.0
176 92.0 0.0 178.8

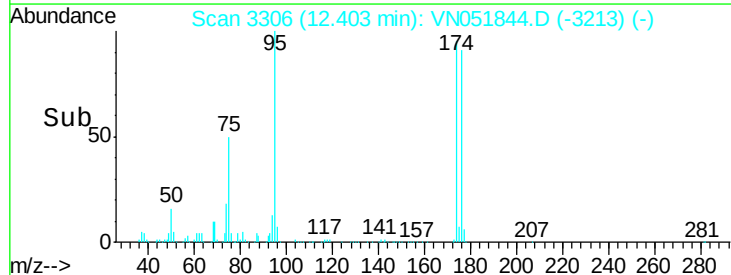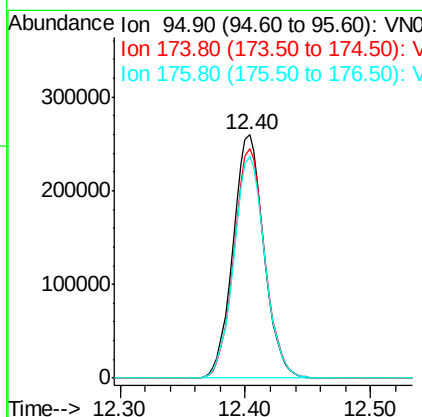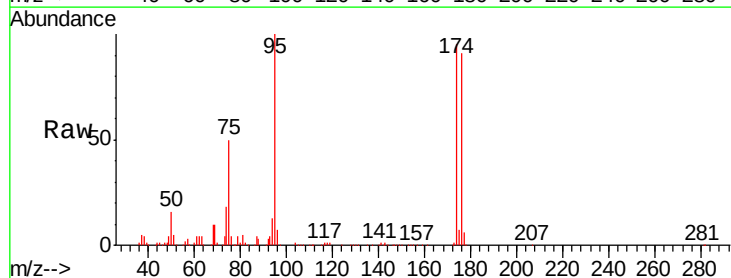


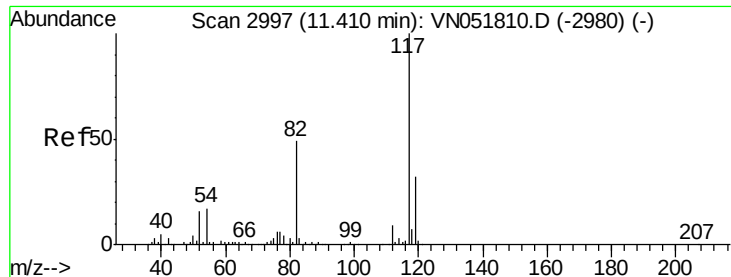




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.41 min Scan# 2997
Delta R.T. 0.00 min
Lab File: VN051844.D
Acq: 12 Oct 2018 20:46

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Tgt Ion:117 Resp: 999036
Ion Ratio Lower Upper
117 100
82 49.1 42.6 64.0
119 32.4 25.8 38.6

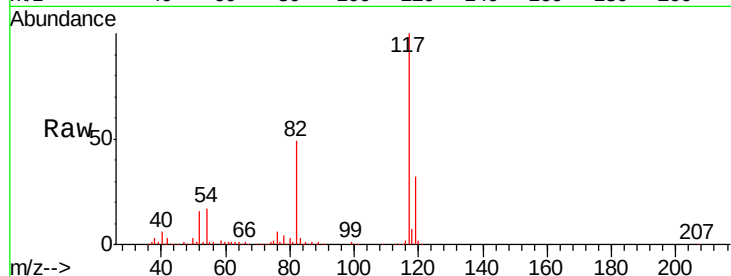


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

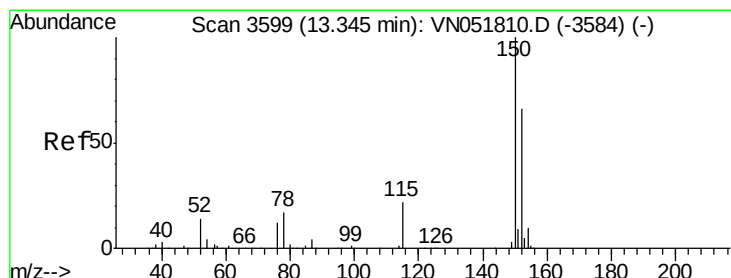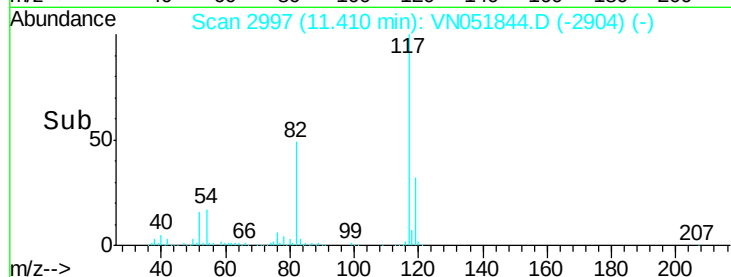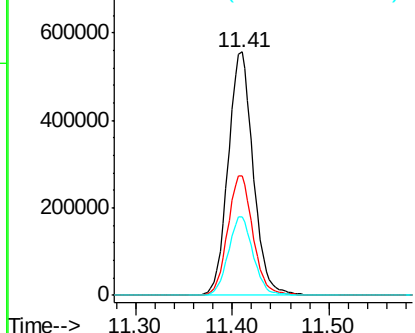

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.35 min Scan# 3599
Delta R.T. 0.00 min
Lab File: VN051844.D
Acq: 12 Oct 2018 20:46

Tgt Ion:152 Resp: 335350
Ion Ratio Lower Upper
152 100
115 55.5 27.8 83.4
150 158.4 0.0 351.4

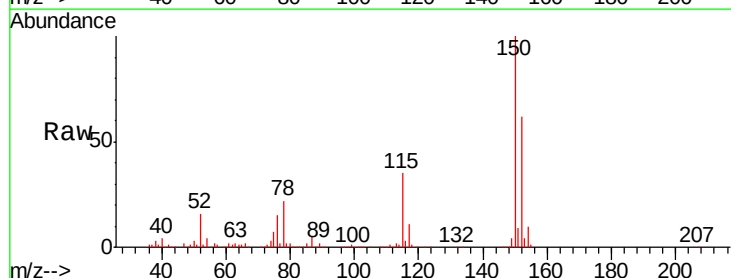

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

