


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101218\
 Data File : VN051822.D
 Acq On : 12 Oct 2018 7:40
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N101218W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Oct 12 10:23:44 2018

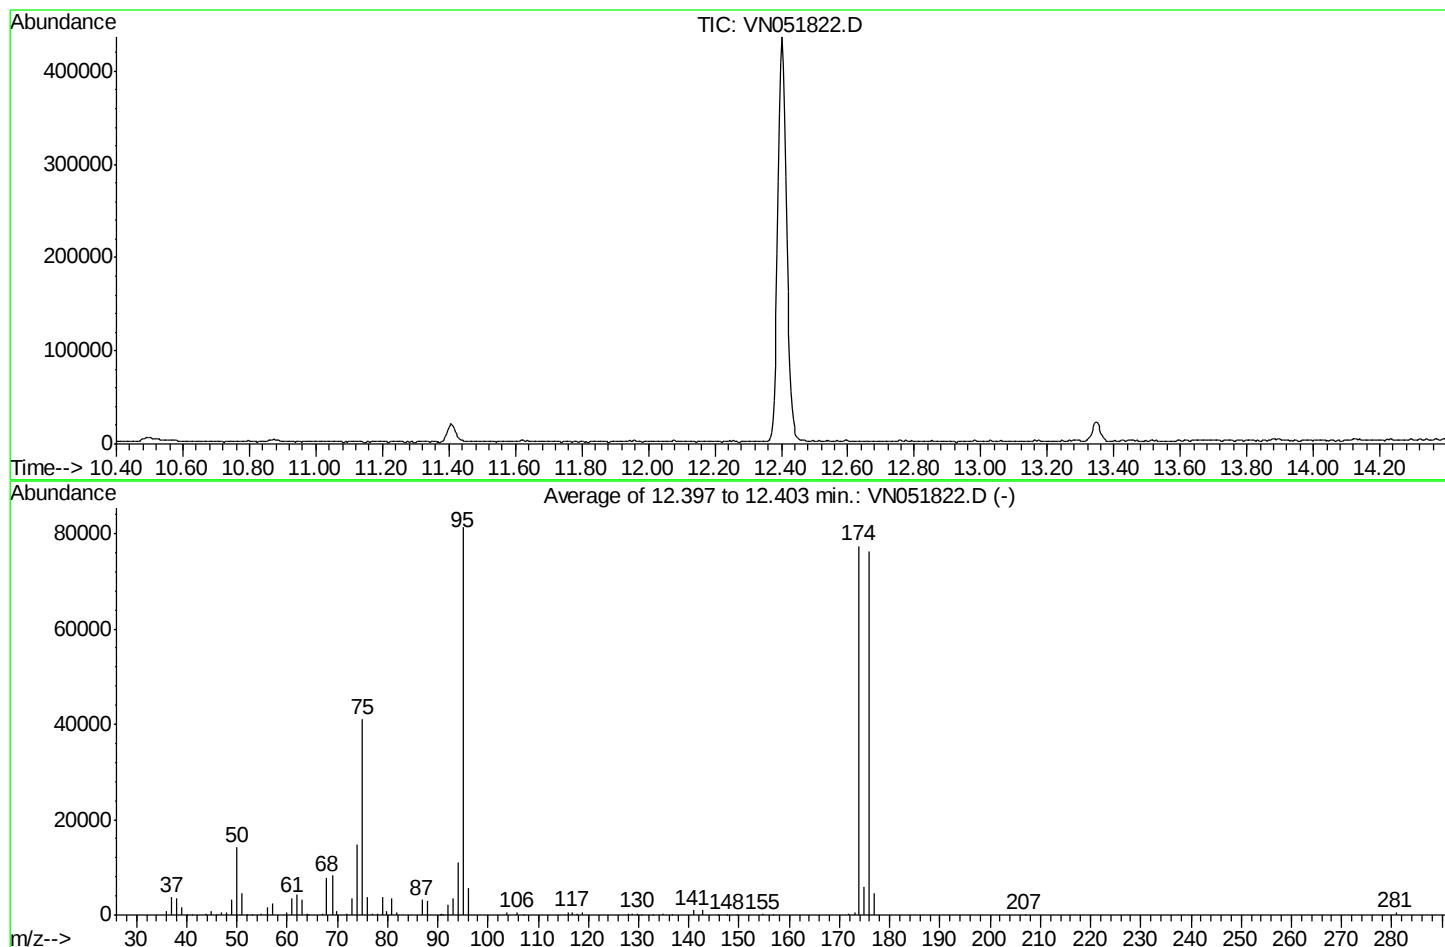

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	14172	PASS
75	95	30	60	50.4	40997	PASS
95	95	100	100	100.0	81322	PASS
96	95	5	9	6.9	5572	PASS
173	174	0.00	2	0.8	639	PASS
174	95	50	100	95.1	77336	PASS
175	174	5	9	7.7	5939	PASS
176	174	95	101	98.6	76216	PASS
177	176	5	9	6.0	4584	PASS