


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN101218\
Data File : VN051838.D
Acq On : 12 Oct 2018 17:29
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101118W.M
Title : SW846 8260
Last Update : Fri Oct 12 09:51:20 2018

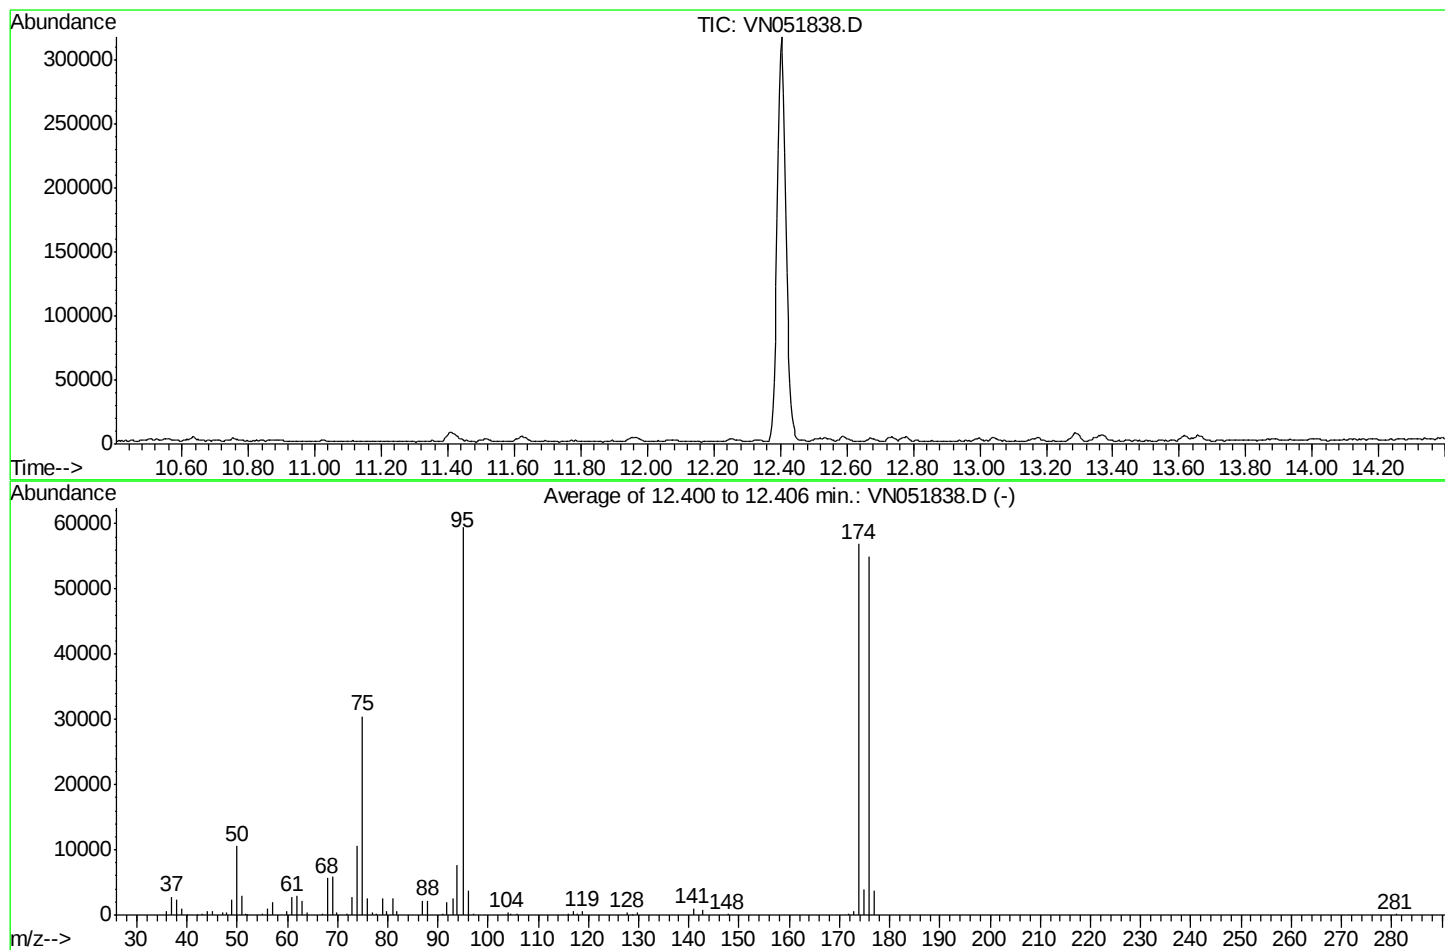

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	10520	PASS
75	95	30	60	51.3	30488	PASS
95	95	100	100	100.0	59448	PASS
96	95	5	9	6.2	3693	PASS
173	174	0.00	2	1.0	564	PASS
174	95	50	100	95.7	56909	PASS
175	174	5	9	7.0	3988	PASS
176	174	95	101	96.6	54965	PASS
177	176	5	9	6.9	3775	PASS