

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN101220\
 Data File : VN064093.D
 Acq On : 12 Oct 2020 21:26
 Operator : JC/MD
 Sample : L4356-01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 RECLAMATION-TANK

Quant Time: Oct 13 01:10:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 01 01:46:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	230632	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	420807	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	447246	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	192901	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	186687	49.00	ug/l	0.00
Spiked Amount			Recovery	=	98.00%	
35) Dibromofluoromethane	7.55	113	143234	49.05	ug/l	0.00
Spiked Amount			Recovery	=	98.10%	
50) Toluene-d8	10.06	98	554086	50.06	ug/l	0.00
Spiked Amount			Recovery	=	100.12%	
62) 4-Bromofluorobenzene	12.38	95	220298	52.94	ug/l	0.00
Spiked Amount			Recovery	=	105.88%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	4.71	59	545	1.296	ug/l #	71
14) Allyl chloride	4.02	41	14835	3.438	ug/l #	81
16) Acetone	3.77	43	288850	246.269	ug/l	100
17) Carbon Disulfide	4.01	76	391	0.762	ug/l #	76
18) Methyl Acetate	4.28	43	7154	2.349	ug/l #	76
20) Methylene Chloride	4.51	84	10072	3.840	ug/l	96
23) Vinyl Acetate	5.97	43	6250	0.850	ug/l #	75
25) 2-Butanone	6.79	43	75565	45.442	ug/l	93
29) Tetrahydrofuran	7.17	42	779	0.698	ug/l #	68
30) Chloroform	7.33	83	1765	0.334	ug/l	99
31) Cyclohexane	7.62	56	6382	1.443	ug/l #	4
36) 1,1-Dichloropropene	7.62	75	19695	4.620	ug/l #	52
37) Ethyl Acetate	6.89	43	7490	1.768	ug/l #	82
38) Carbon Tetrachloride	7.62	117	25625	5.360	ug/l #	14
40) Benzene	8.00	78	2765	0.227	ug/l	94
41) Methacrylonitrile	7.14	41	1509	0.802	ug/l #	39
48) Methyl methacrylate	9.14	41	5896	1.708	ug/l #	12
51) 4-Methyl-2-Pentanone	9.95	43	308730	75.302	ug/l	99
52) Toluene	10.12	92	1874	0.249	ug/l	95
54) cis-1,3-Dichloropropene	9.88	75	6151	1.174	ug/l #	67
56) Ethyl methacrylate	10.32	69	17881	4.176	ug/l #	70
59) 2-Hexanone	10.69	43	71793	23.572	ug/l #	28
74) N-ethyl acetate	12.07	43	205	2.246	ug/l #	14
76) 1,2,3-Trichloropropane	12.38	75	118103	27.774	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.38	75	118103	79.993	ug/l #	6
95) Naphthalene	15.10	128	1921	2.102	ug/l #	8


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN101220\
Data File : VN064093.D
Acq On : 12 Oct 2020 21:26
Operator : JC/MD
Sample : L4356-01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
RECLAMATION-TANK

Quant Time: Oct 13 01:10:34 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 01 01:46:38 2020
Response via : Initial Calibration

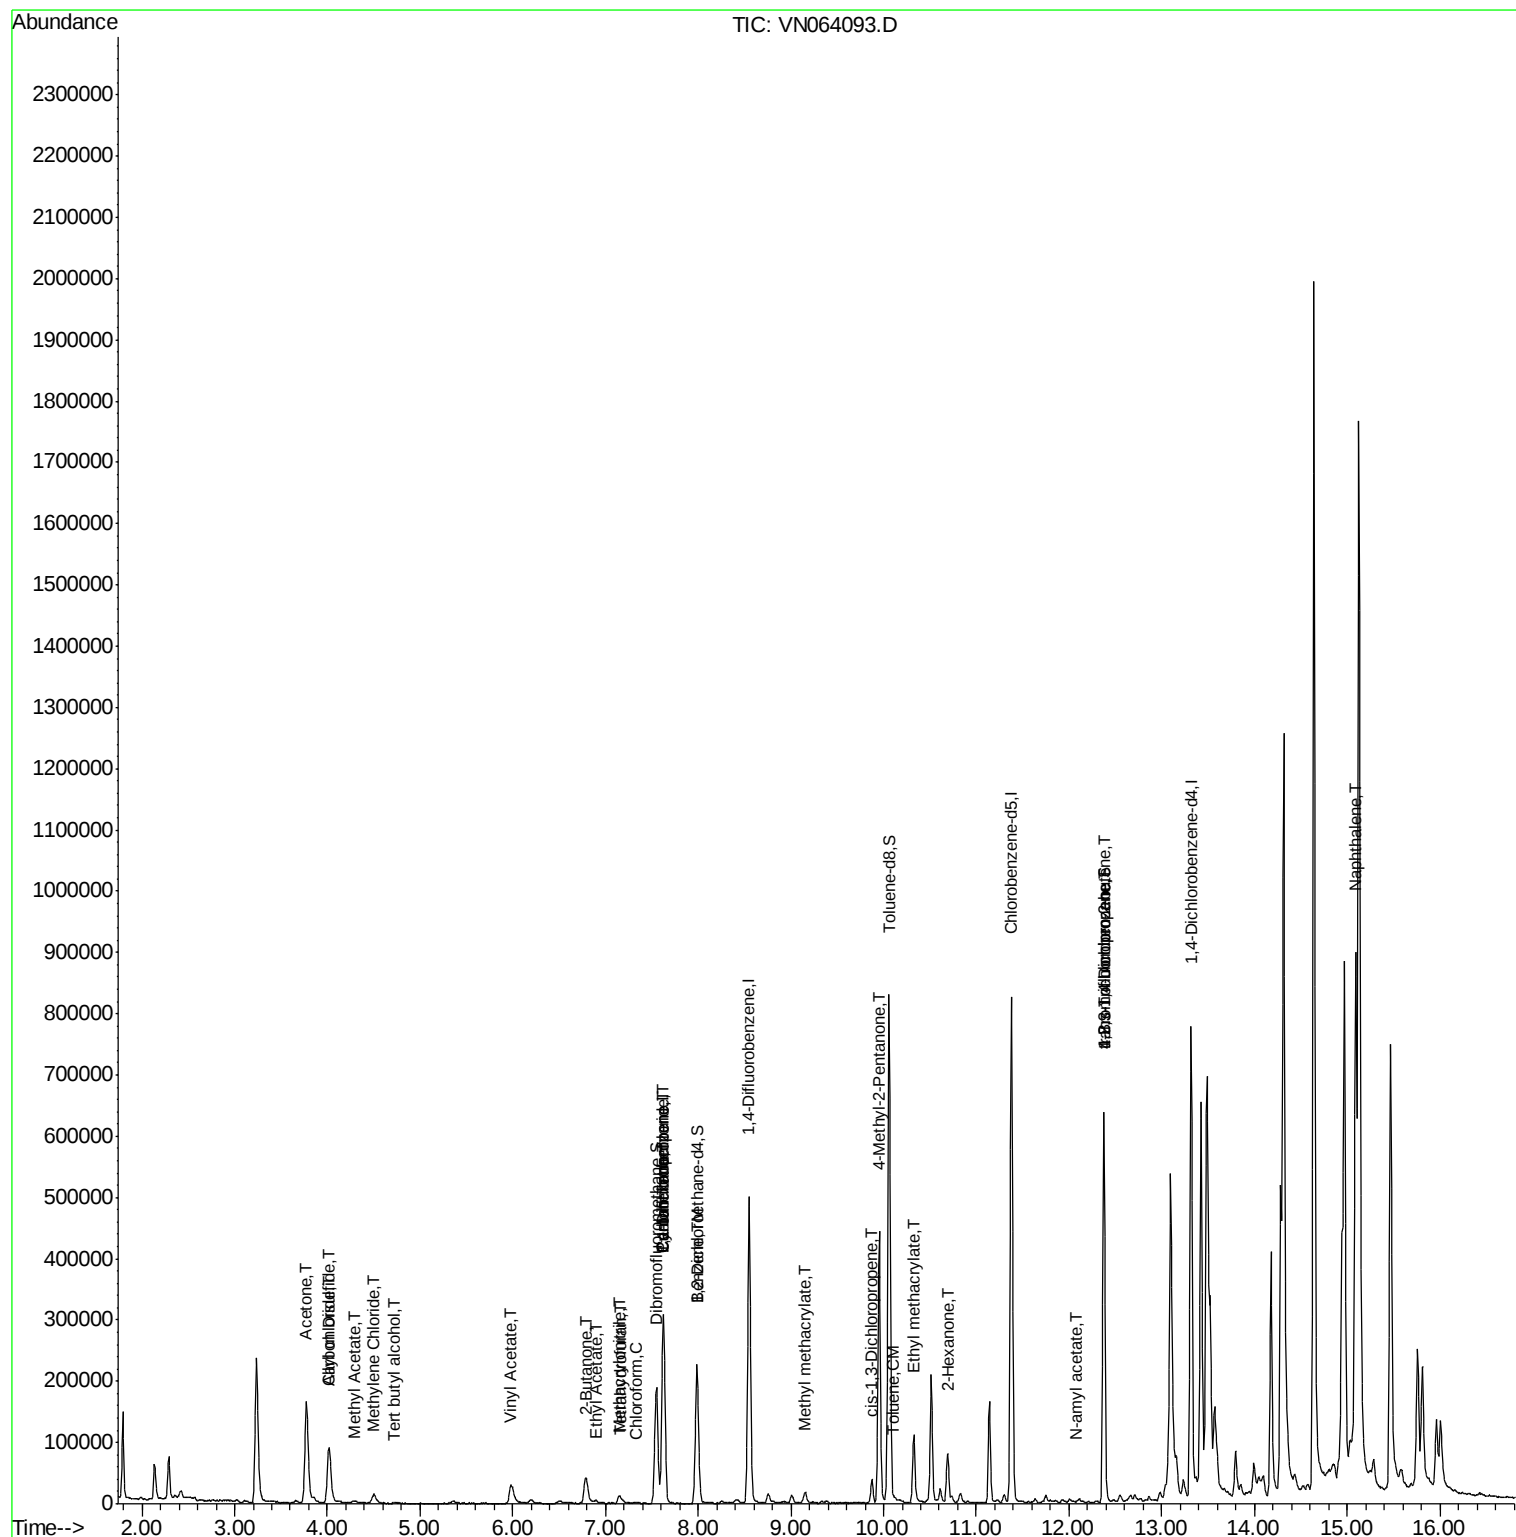

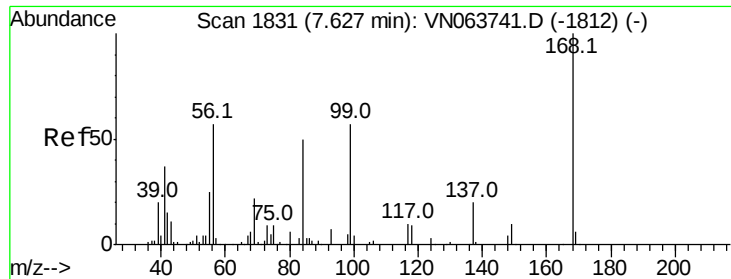

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN064093.D

Acq: 12 Oct 2020 21:26

Instrument :

MSVOA_N

ClientSampleId :


RECLAMATION-TANK

Tot Ion:168 Resp: 230632

Ion Ratio Lower Upper

168 100

99 61.1 51.8 77.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.63

100000

80000



60000

40000

20000

0

Time-->



#11

Tert butyl alcohol

Concen: 1.296 ug/l

RT: 4.71 min Scan# 925

Delta R.T. -0.01 min

Lab File: VN064093.D


Acq: 12 Oct 2020 21:26

Tgt Ion: 59 Resp: 545

Ion Ratio Lower Upper

59 100

57 0.0 8.7 13.1#



Abundance Ion 59.00 (58.70 to 59.70): VN

Ion 57.00 (56.70 to 57.70): VN

4.71

600

500

400


300


200

100

0

Time-->









#14
Allvl chloride
Concen: 3.438 ug/l
RT: 4.02 min Scan# 709
Delta R.T. -0.26 min
Lab File: VN064093.D
Acq: 12 Oct 2020 21:26




Instrument :
MSVOA_N
ClientSampleId :
RECLAMATION-TANK


Tot Ion: 41 Resp: 14835
Ion Ratio Lower Upper
41 100
39 75.9 64.5 96.7
76 2.6 25.9 38.9#

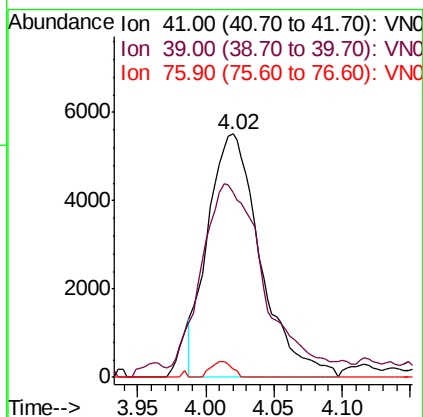

#16
Acetone
Concen: 246.269 ug/l
RT: 3.77 min Scan# 632
Delta R.T. 0.00 min
Lab File: VN064093.D
Acq: 12 Oct 2020 21:26

Tgt Ion: 43 Resp: 288850
Ion Ratio Lower Upper
43 100
58 27.7 22.3 33.5



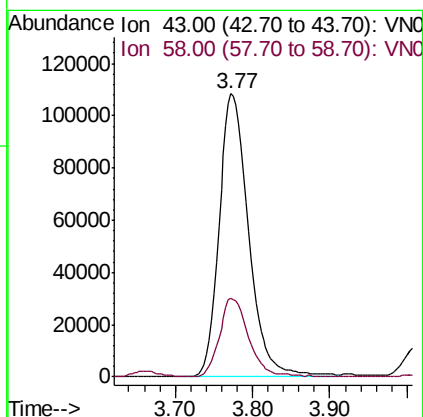





#17
Carbon Disulfide
Concen: 0.762 ug/l
RT: 4.01 min Scan# 707
Delta R.T. 0.00 min
Lab File: VN064093.D
Acq: 12 Oct 2020 21:26




Instrument :
MSVOA_N
ClientSampleId :
RECLAMATION-TANK


Tot Ion: 76 Resp: 391
Ion Ratio Lower Upper
76 100
78 0.0 7.0 10.4#

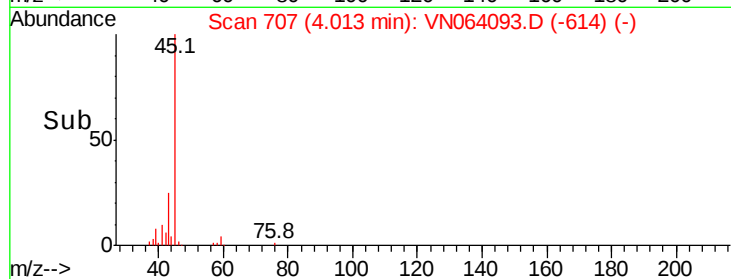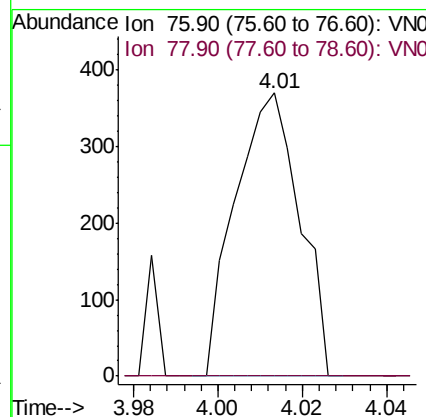

#18
Methyl Acetate
Concen: 2.349 ug/l
RT: 4.28 min Scan# 791
Delta R.T. 0.01 min
Lab File: VN064093.D
Acq: 12 Oct 2020 21:26

Tgt Ion: 43 Resp: 7154
Ion Ratio Lower Upper
43 100
74 10.4 17.4 26.2#

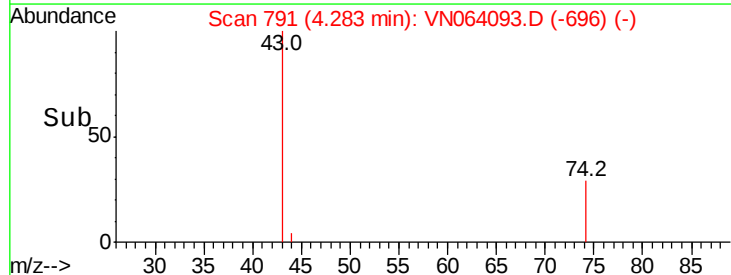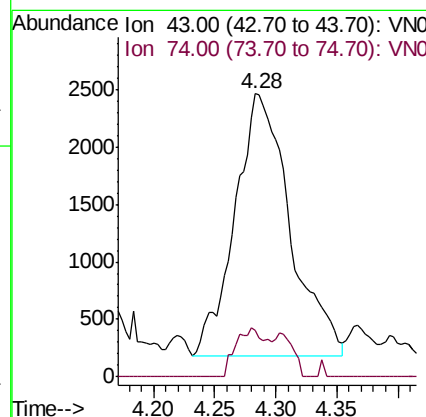


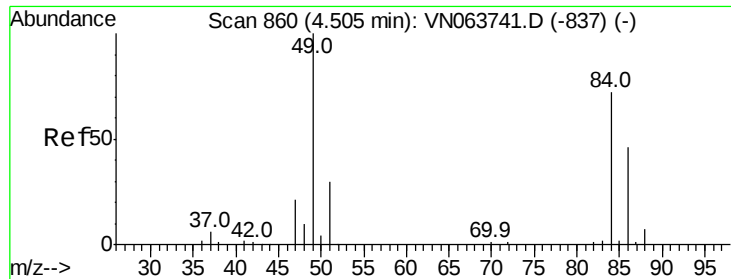




#20
Methvlene Chloride
Concen: 3.840 ug/l
RT: 4.51 min Scan# 860
Delta R.T. 0.00 min
Lab File: VN064093.D
Acq: 12 Oct 2020 21:26

Instrument :
MSVOA_N
ClientSampleId :
RECLAMATION-TANK

Tot Ion: 84 Resp: 10072
Ion Ratio Lower Upper
84 100
49 143.0 110.4 165.6
51 47.2 33.3 49.9
86 64.3 50.7 76.1




Abundance Ion 83.90 (83.60 to 84.60): VNO
Ion 48.90 (48.60 to 49.60): VNO
Ion 50.90 (50.60 to 51.60): VNO
Ion 85.90 (85.60 to 86.60): VNO

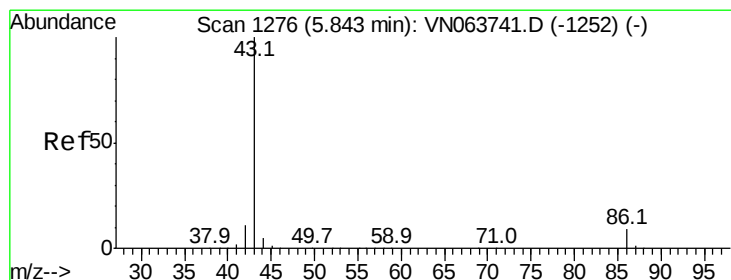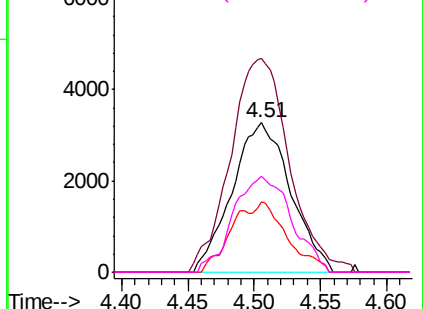




#23
Vinyl Acetate
Concen: 0.850 ug/l
RT: 5.97 min Scan# 1317
Delta R.T. 0.13 min
Lab File: VN064093.D
Acq: 12 Oct 2020 21:26

Tgt Ion: 43 Resp: 6250
Ion Ratio Lower Upper
43 100
86 0.0 7.3 10.9#



Abundance Ion 43.00 (42.70 to 43.70): VNO
Ion 86.00 (85.70 to 86.70): VNO

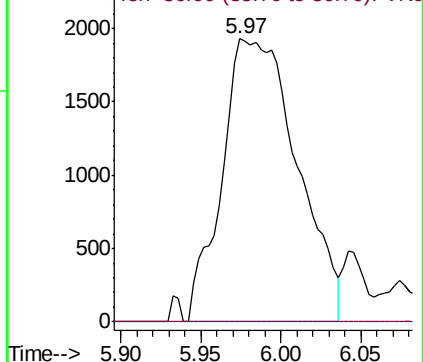

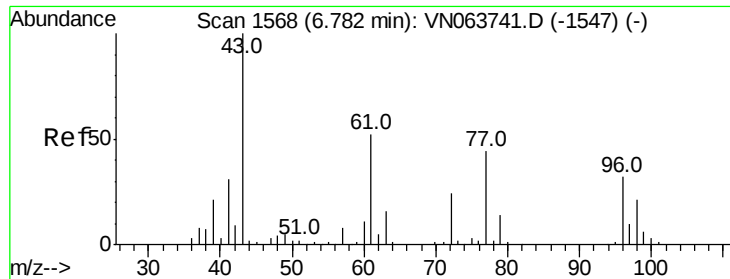

#25

2-Butanone

Concen: 45.442 ug/l

RT: 6.79 min Scan# 1570

Delta R.T. 0.01 min

Lab File: VN064093.D

Acq: 12 Oct 2020 21:26

Instrument :

MSVOA_N

ClientSampleId :


RECLAMATION-TANK

Tot Ion: 43 Resp: 75565

Ion Ratio Lower Upper




43 100

72 20.7 19.3 28.9

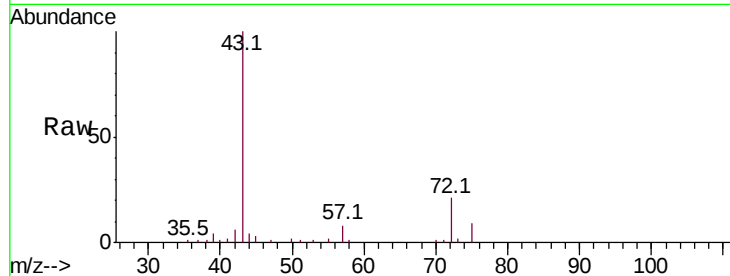

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 72.00 (71.70 to 72.70): VN0

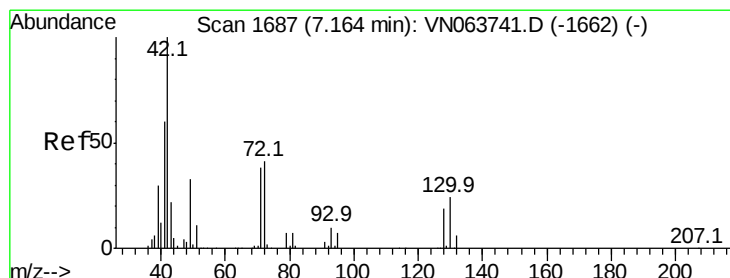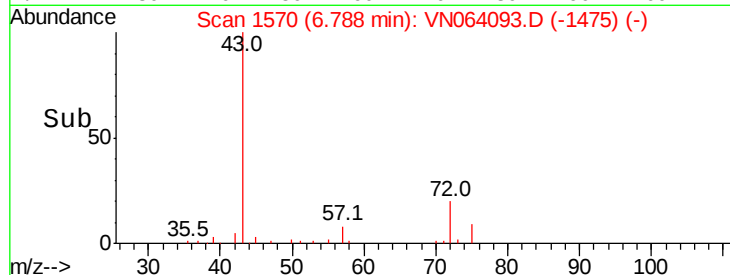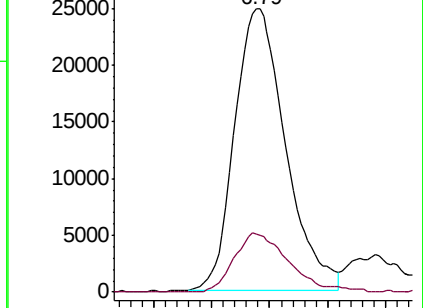

#29

Tetrahydrofuran

Concen: 0.698 ug/l

RT: 7.17 min Scan# 1688

Delta R.T. 0.00 min

Lab File: VN064093.D

Acq: 12 Oct 2020 21:26


Tgt Ion: 42 Resp: 779

Ion Ratio Lower Upper

42 100

72 42.4 32.8 49.2



71 0.0 30.6 45.8#

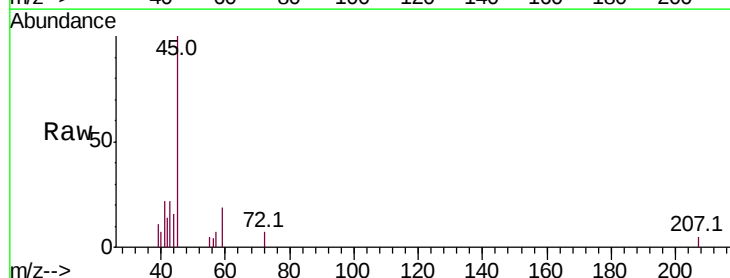


Abundance Ion 42.00 (41.70 to 42.70): VN0

Ion 72.00 (71.70 to 72.70): VN0

Ion 71.00 (70.70 to 71.70): VN0



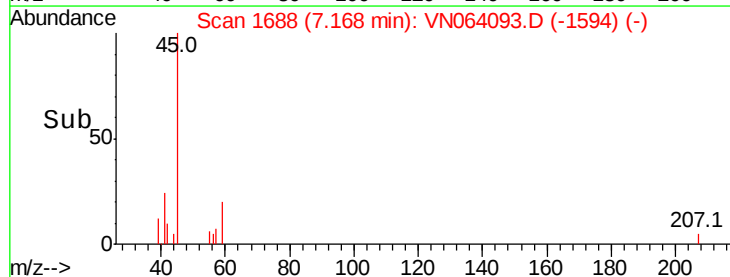
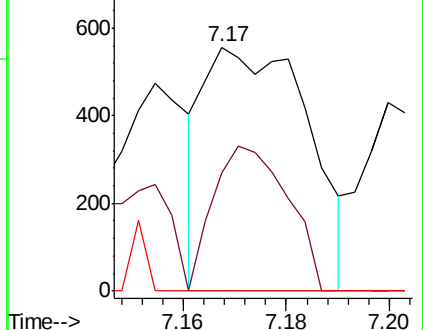




#30
Chloroform
Concen: 0.334 ug/l
RT: 7.33 min Scan# 1739
Delta R.T. 0.00 min
Lab File: VN064093.D
Acq: 12 Oct 2020 21:26




Instrument :
MSVOA_N
ClientSampleId :
RECLAMATION-TANK


Tot Ion: 83 Resp: 1765
Ion Ratio Lower Upper
83 100
85 67.2 54.6 82.0

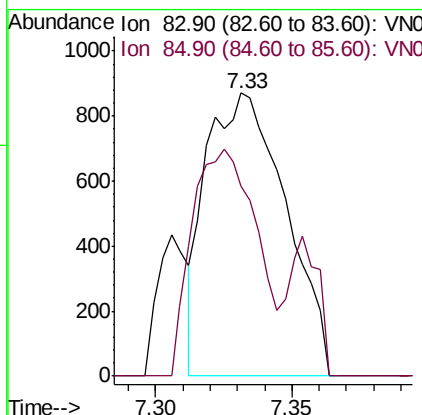

#31
Cyclohexane
Concen: 1.443 ug/l
RT: 7.62 min Scan# 1829
Delta R.T. 0.01 min
Lab File: VN064093.D
Acq: 12 Oct 2020 21:26

Tgt Ion: 56 Resp: 6382
Ion Ratio Lower Upper
56 100
69 174.9 25.4 38.2#
84 107.0 63.3 94.9#



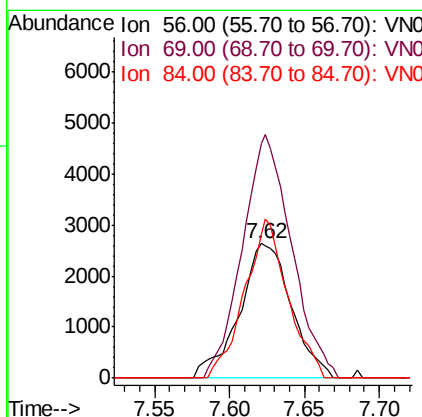



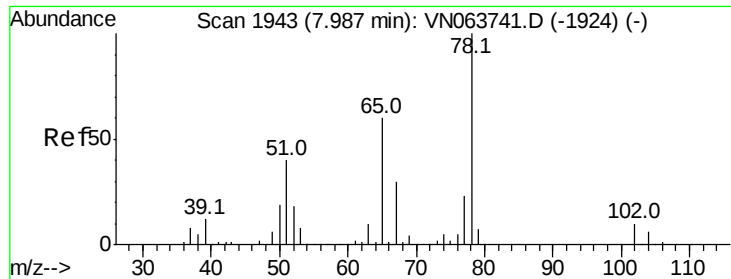

#33
 1,2-Dichloroethane-d4
 Concen: 48.997 ug/l
 RT: 7.99 min Scan# 1943
 Delta R.T. 0.00 min
 Lab File: VN064093.D
 Acq: 12 Oct 2020 21:26




Instrument :
 MSVOA_N
 ClientSampleId :
 RECLAMATION-TANK


Tot Ion: 65 Resp: 186687
 Ion Ratio Lower Upper
 65 100
 67 51.7 0.0 99.6

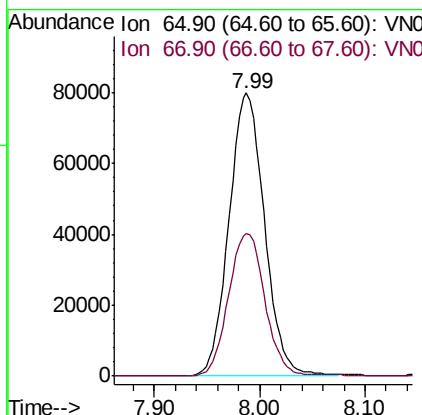

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2118
 Delta R.T. 0.00 min
 Lab File: VN064093.D
 Acq: 12 Oct 2020 21:26

Tgt Ion: 114 Resp: 420807
 Ion Ratio Lower Upper
 114 100
 63 23.7 0.0 45.0
 88 16.8 0.0 34.0

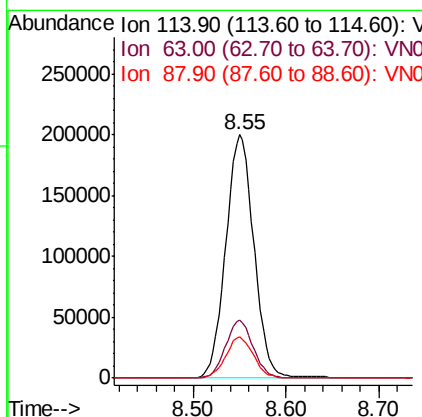


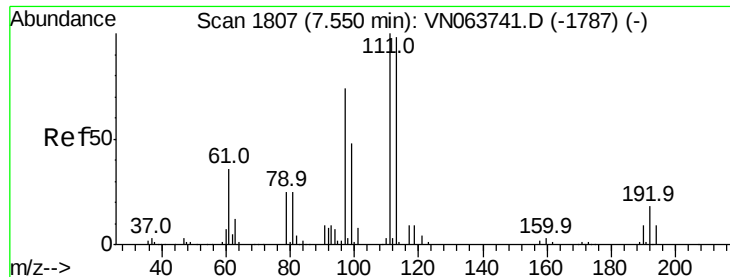




#35
Dibromofluoromethane
Concen: 49.055 ug/l
RT: 7.55 min Scan# 1807
Delta R.T. 0.00 min
Lab File: VN064093.D
Acq: 12 Oct 2020 21:26

Instrument :
MSVOA_N
ClientSampleId :
RECLAMATION-TANK

Tot Ion:113 Resp: 143234
Ion Ratio Lower Upper
113 100
111 102.3 81.8 122.8
192 18.0 14.2 21.2

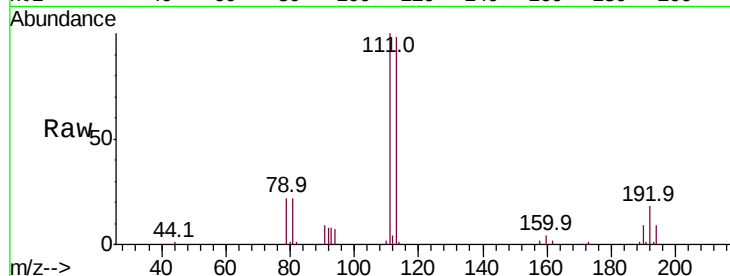


Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

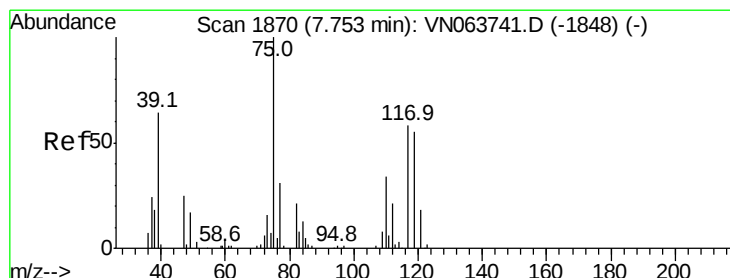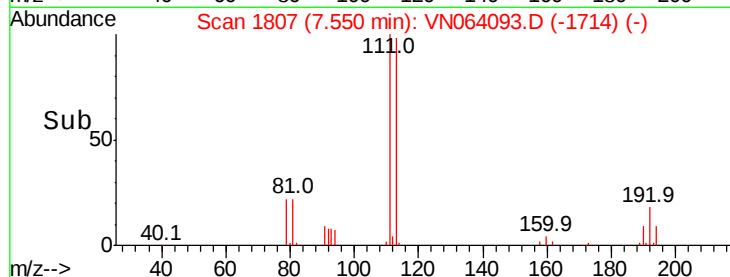
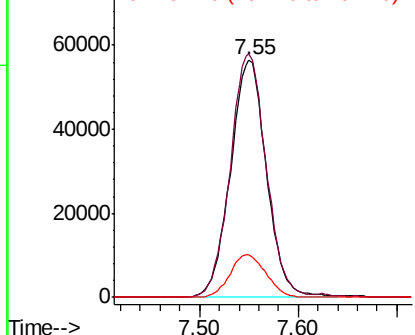



#36
1,1-Dichloropropene
Concen: 4.620 ug/l
RT: 7.62 min Scan# 1829
Delta R.T. -0.13 min
Lab File: VN064093.D
Acq: 12 Oct 2020 21:26

Tgt Ion: 75 Resp: 19695
Ion Ratio Lower Upper
75 100
110 10.2 16.9 50.6#
77 0.0 24.5 36.7#

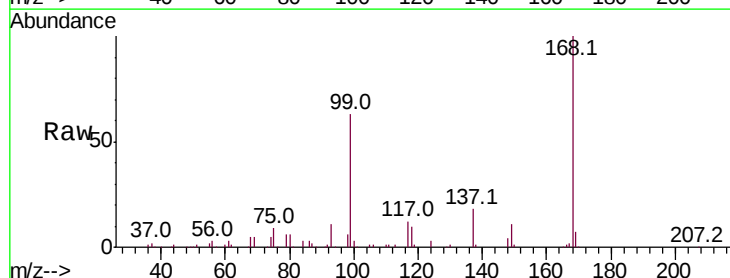

Abundance Ion 74.90 (74.60 to 75.60): V
Ion 109.90 (109.60 to 110.60): V
Ion 76.90 (76.60 to 77.60): V



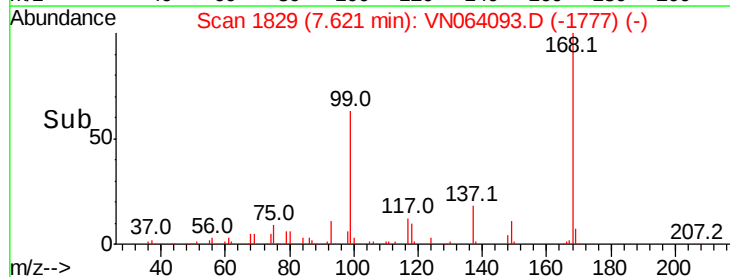
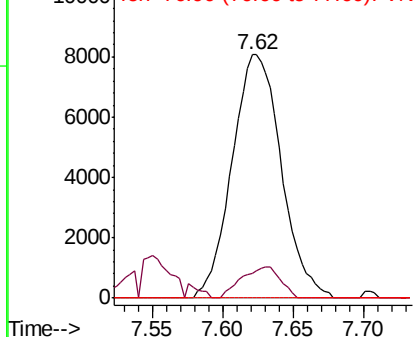




#37
Ethyl Acetate
Concen: 1.768 ug/l
RT: 6.89 min Scan# 1602
Delta R.T. 0.01 min
Lab File: VN064093.D
Acq: 12 Oct 2020 21:26




Instrument :
MSVOA_N
ClientSampleId :
RECLAMATION-TANK


Tot Ion: 43 Resp: 7490
Ion Ratio Lower Upper
43 100
61 4.2 10.4 15.6#
70 5.0 7.3 10.9#

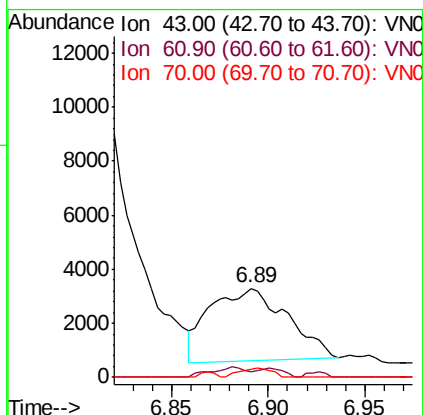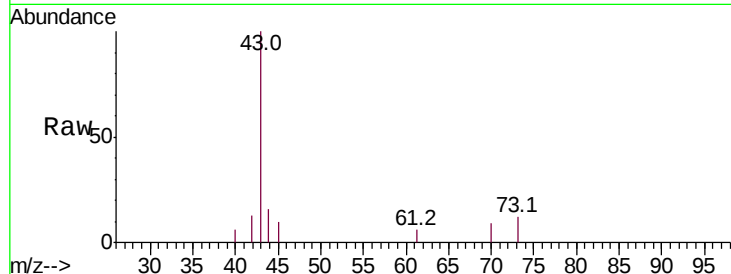

#38
Carbon Tetrachloride
Concen: 5.360 ug/l
RT: 7.62 min Scan# 1829
Delta R.T. -0.11 min
Lab File: VN064093.D
Acq: 12 Oct 2020 21:26

Tgt Ion: 117 Resp: 25625
Ion Ratio Lower Upper
117 100
119 5.3 80.1 120.1#
121 0.0 25.7 38.5#

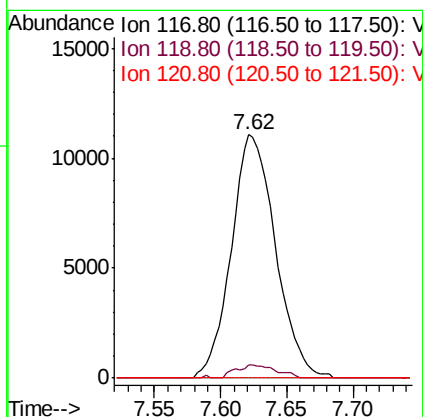



#40

Benzene

Concen: 0.227 ug/l

RT: 8.00 min Scan# 1946

Delta R.T. -0.01 min

Lab File: VN064093.D

Acq: 12 Oct 2020 21:26





Instrument :
MSVOA_N
ClientSampleId :
RECLAMATION-TANK

Tot Ion: 78 Resp: 2765

Ion Ratio Lower Upper

78 100

77 20.6 18.7 28.1

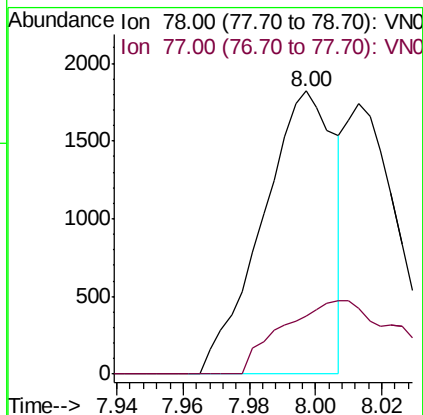

#41

Methacrylonitrile

Concen: 0.802 ug/l

RT: 7.14 min Scan# 1680

Delta R.T. 0.01 min

Lab File: VN064093.D

Acq: 12 Oct 2020 21:26

Tgt Ion: 41 Resp: 1509




Ion Ratio Lower Upper


41 100

39 73.5 42.5 63.7#

67 0.0 57.4 86.2#

52 0.0 26.9 40.3#


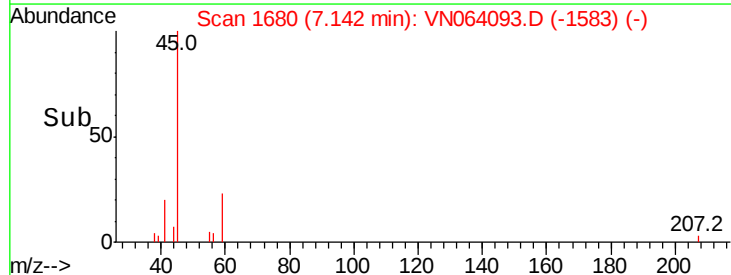
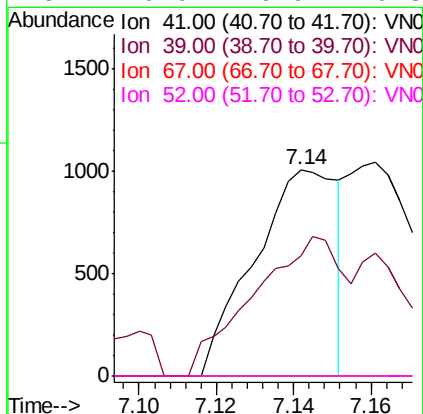



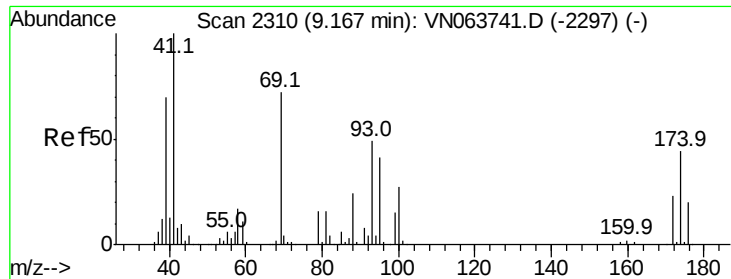

#48
Methvl methacrylate
Concen: 1.708 ug/l
RT: 9.14 min Scan# 2302
Delta R.T. -0.03 min
Lab File: VN064093.D
Acq: 12 Oct 2020 21:26




Instrument :
MSVOA_N
ClientSampleId :
RECLAMATION-TANK


Tot Ion: 41 Resp: 5896
Ion Ratio Lower Upper
41 100
69 0.0 60.9 91.3#
39 0.0 57.5 86.3#

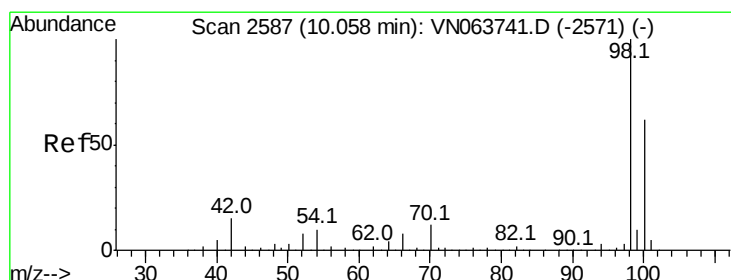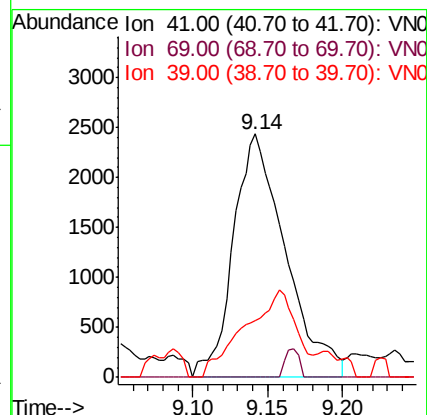

#50
Toluene-d8
Concen: 50.058 ug/l
RT: 10.06 min Scan# 2587
Delta R.T. 0.00 min
Lab File: VN064093.D
Acq: 12 Oct 2020 21:26

Tgt Ion: 98 Resp: 554086
Ion Ratio Lower Upper
98 100
100 64.7 49.8 74.6

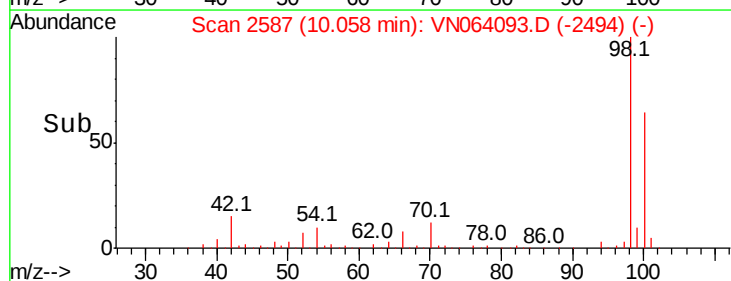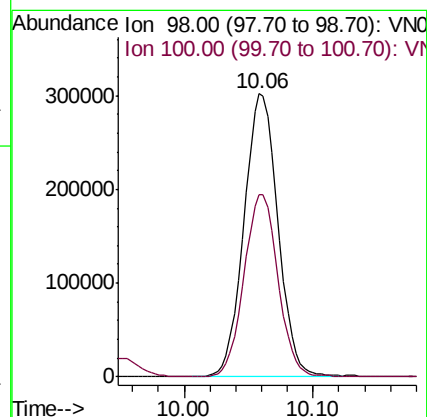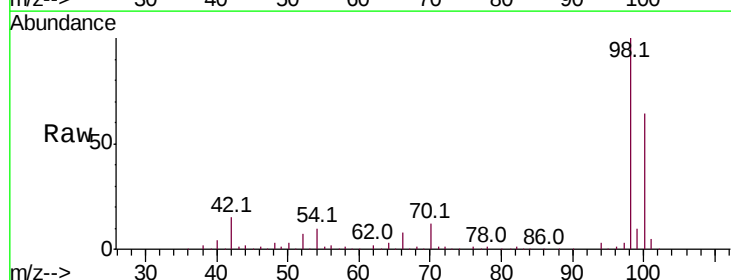



#51

4-Methyl-2-Pentanone

Concen: 75.302 ug/l

RT: 9.95 min Scan# 2554

Delta R.T. 0.00 min

Lab File: VN064093.D

Acq: 12 Oct 2020 21:26

Instrument :

MSVOA_N

ClientSampleId :


RECLAMATION-TANK

Tot Ion: 43 Resp: 308730

Ion Ratio Lower Upper

43 100

58 34.8 28.4 42.6



Abundance Ion 43.00 (42.70 to 43.70): VN063741.D (-2537) (-)

Ion 58.00 (57.70 to 58.70): VN063741.D (-2537) (-)

200000

150000



100000

50000

0

9.90 9.95 10.00

Time-->



#52

Toluene

Concen: 0.249 ug/l

RT: 10.12 min Scan# 2606

Delta R.T. -0.01 min

Lab File: VN064093.D


Acq: 12 Oct 2020 21:26

Tgt Ion: 92 Resp: 1874

Ion Ratio Lower Upper

92 100

91 182.7 140.6 210.8



Abundance Ion 92.00 (91.70 to 92.70): VN063741.D (-2592) (-)

Ion 91.00 (90.70 to 91.70): VN063741.D (-2592) (-)

2000

1500


1000


500

0

10.10 10.12 10.15

Time-->






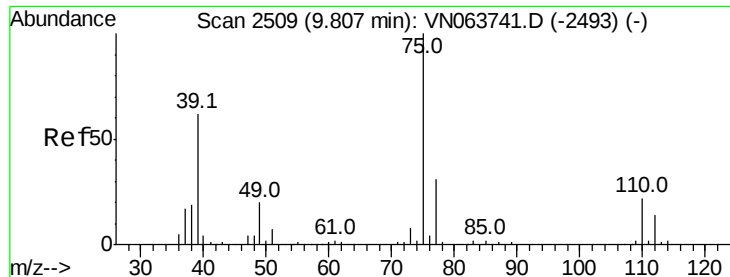


#54

cis-1,3-Dichloropropene
 Concen: 1.174 ug/l
 RT: 9.88 min Scan# 2531
 Delta R.T. 0.07 min
 Lab File: VN064093.D
 Acq: 12 Oct 2020 21:26

Instrument :
 MSVOA_N
 ClientSampleId :
 RECLAMATION-TANK




Tot Ion: 75 Resp: 6151
 Ion Ratio Lower Upper
 75 100
 77 0.0 24.6 36.8#
 39 45.4 49.7 74.5#

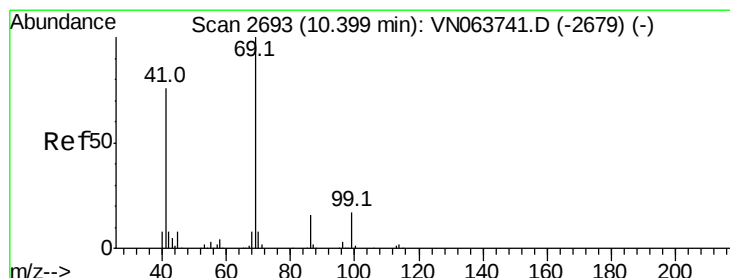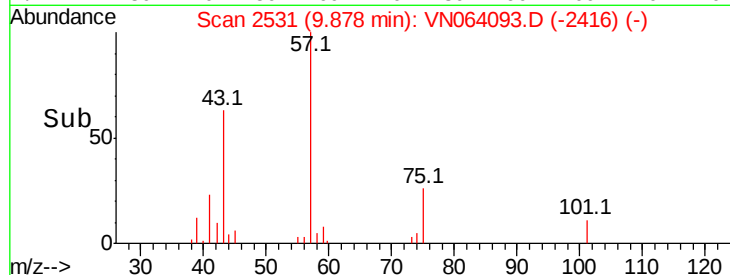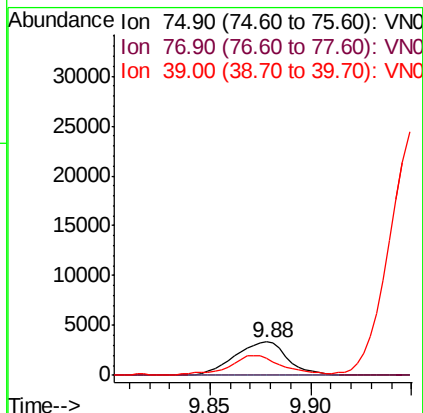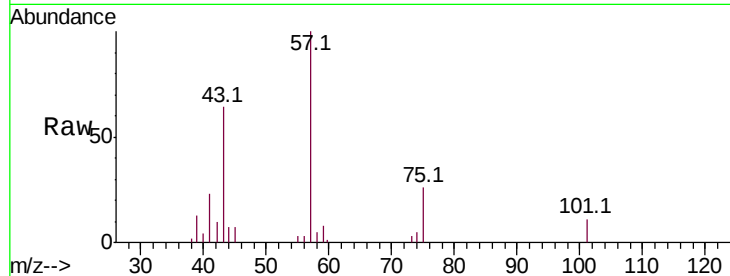


#56

Ethyl methacrylate
 Concen: 4.176 ug/l
 RT: 10.32 min Scan# 2670
 Delta R.T. -0.07 min
 Lab File: VN064093.D
 Acq: 12 Oct 2020 21:26

Tgt Ion: 69 Resp: 17881
 Ion Ratio Lower Upper
 69 100
 41 118.7 61.1 91.7#
 39 54.4 42.2 63.4

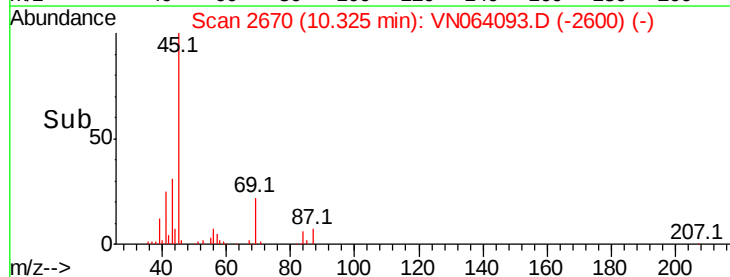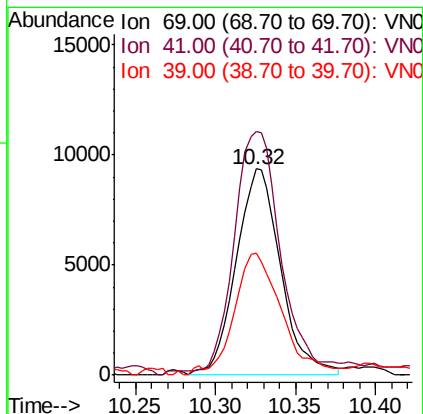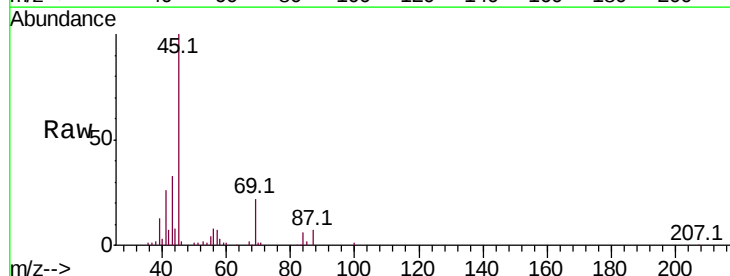



#59

2-Hexanone

Concen: 23.572 ug/l

RT: 10.69 min Scan# 2783

Delta R.T. -0.03 min

Lab File: VN064093.D

Acq: 12 Oct 2020 21:26

Instrument :

MSVOA_N

ClientSampleId :





RECLAMATION-TANK

Tot Ion: 43 Resp: 71793

Ion Ratio Lower Upper

43 100

58 0.0 24.6 73.8#

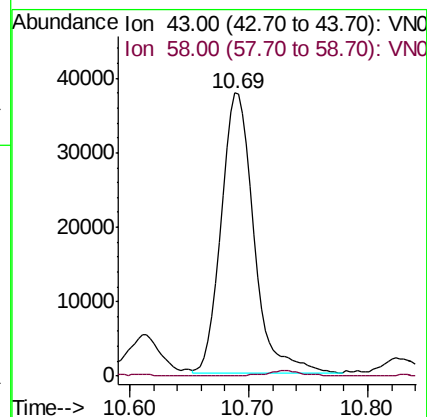

#62

4-Bromofluorobenzene

Concen: 52.944 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.00 min

Lab File: VN064093.D

Acq: 12 Oct 2020 21:26




Tgt Ion: 95 Resp: 220298


Ion Ratio Lower Upper

95 100

174 73.0 0.0 150.6

176 69.8 0.0 145.4



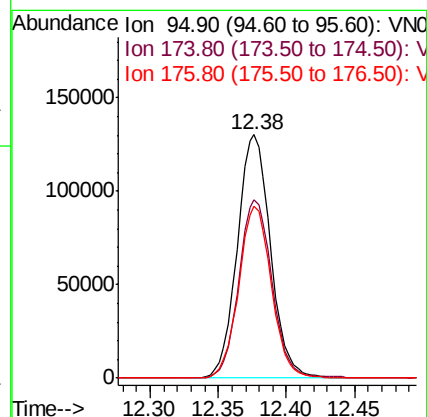



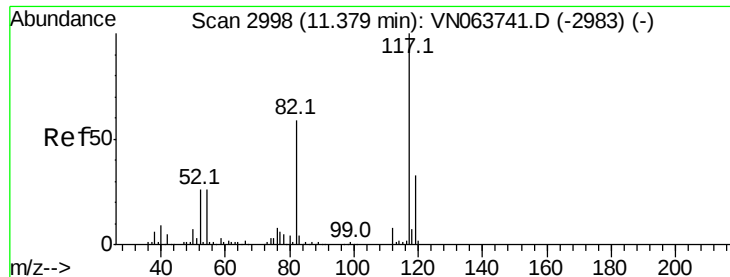

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN064093.D
Acq: 12 Oct 2020 21:26




Instrument :
MSVOA_N
ClientSampleId :
RECLAMATION-TANK


Tot Ion:117 Resp: 447246
Ion Ratio Lower Upper
117 100
82 59.4 47.4 71.2
119 32.0 26.4 39.6

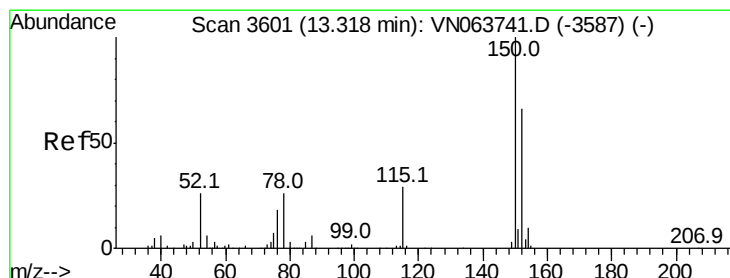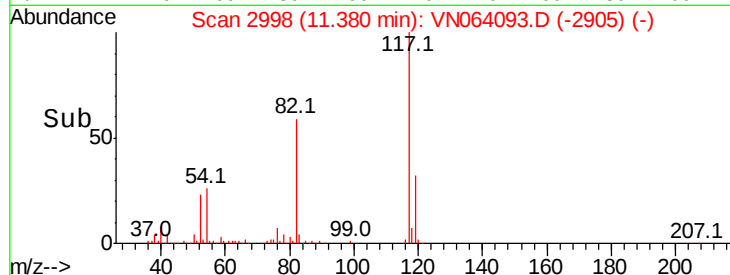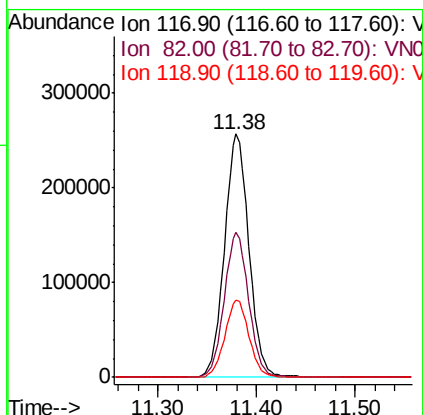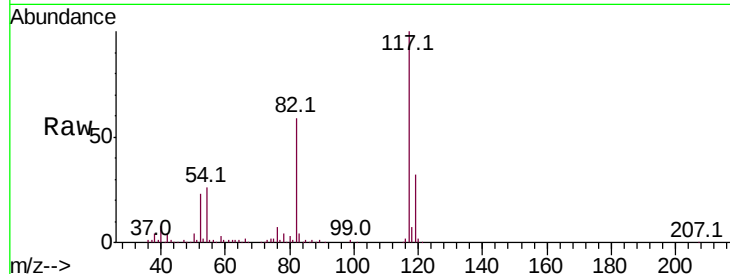

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3601
Delta R.T. 0.00 min
Lab File: VN064093.D
Acq: 12 Oct 2020 21:26

Tgt Ion:152 Resp: 192901
Ion Ratio Lower Upper
152 100
115 64.0 31.3 93.8
150 160.6 0.0 341.8

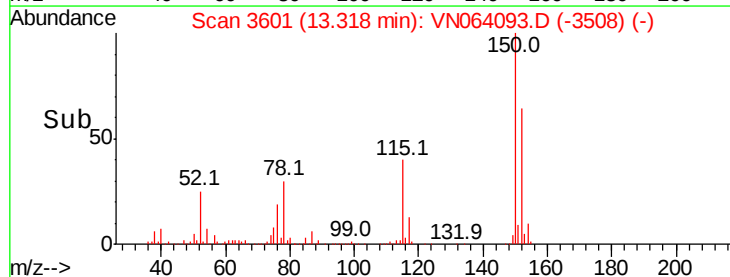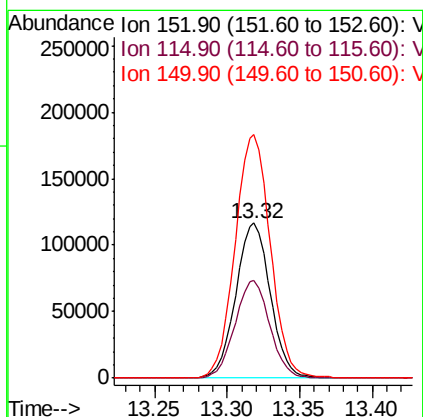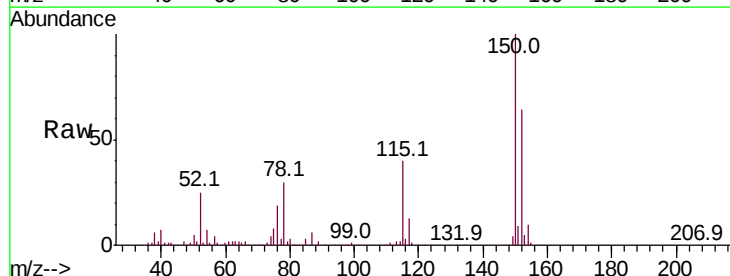

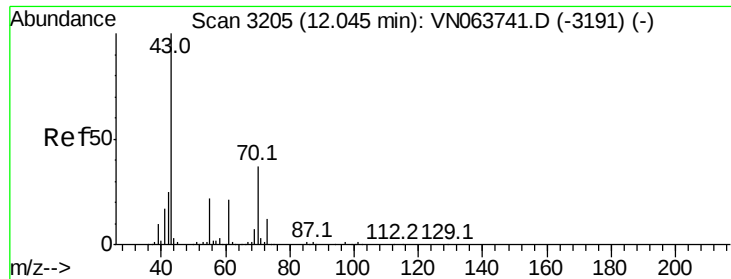

#74

N-amvl acetate

Concen: 2.246 ug/l

RT: 12.07 min Scan# 3213

Delta R.T. 0.03 min

Lab File: VN064093.D

Acq: 12 Oct 2020 21:26

Instrument :

MSVOA_N

ClientSampleId :

RECLAMATION-TANK

Tot Ion: 43 Resp: 205





Ion Ratio Lower Upper

43 100

70 0.0 29.8 44.8#

55 100.5 17.9 26.9#

61 0.0 17.0 25.4#

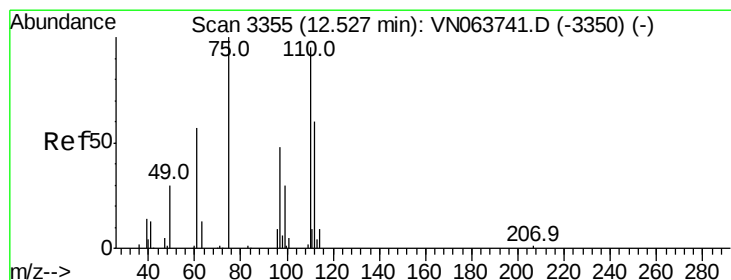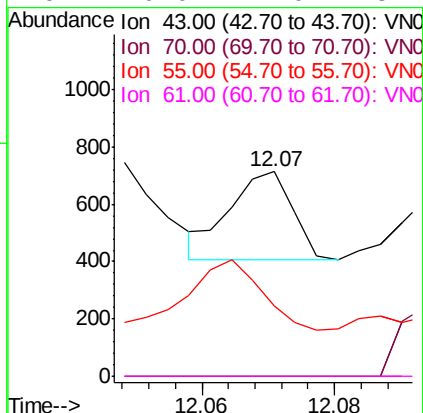

#76

1,2,3-Trichloropropane

Concen: 27.774 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. -0.15 min

Lab File: VN064093.D




Acq: 12 Oct 2020 21:26


Tgt Ion: 75 Resp: 118103

Ion Ratio Lower Upper

75 100

77 1.0 0.0 0.0#

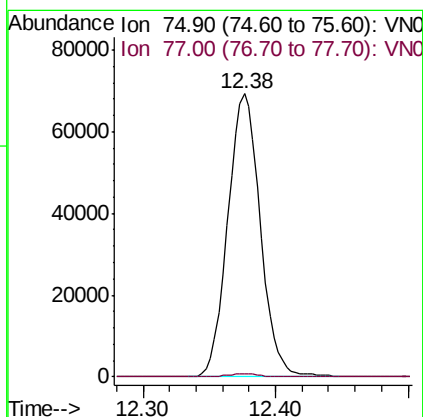

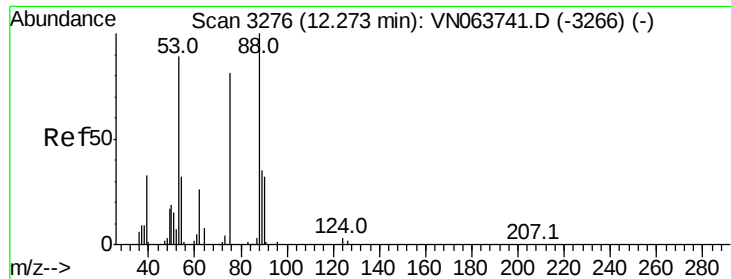

#81

trans-1,4-Dichloro-2-butene

Concen: 79.993 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.10 min

Lab File: VN064093.D

Acq: 12 Oct 2020 21:26

Instrument :

MSVOA_N

ClientSampleId :

RECLAMATION-TANK


Tot Ion: 75 Resp: 118103

Ion Ratio Lower Upper

75 100

53 0.1 88.2 132.2#




89 0.0 36.0 54.0#



Abundance Ion 74.90 (74.60 to 75.60): VN064093.D (-3308) (-)

Ion 53.00 (52.70 to 53.70): VN064093.D (-3308) (-)

Ion 88.90 (88.60 to 89.60): VN064093.D (-3308) (-)

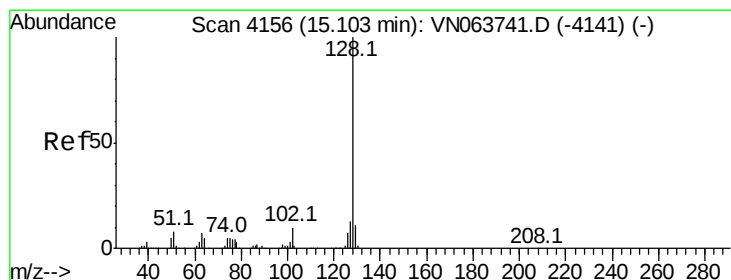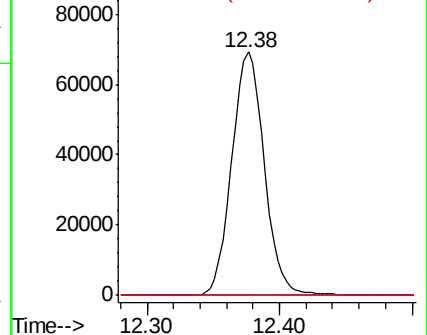

#95

Naphthalene

Concen: 2.102 ug/l

RT: 15.10 min Scan# 4155

Delta R.T. -0.00 min

Lab File: VN064093.D

Acq: 12 Oct 2020 21:26


Tgt Ion: 128 Resp: 1921

Ion Ratio Lower Upper

128 100

127 80.1 10.5 15.7#

129 11.4 8.7 13.1



Abundance Ion 128.00 (127.70 to 128.70): VN064093.D (-4155) (-)

Ion 127.00 (126.70 to 127.70): VN064093.D (-4155) (-)

Ion 129.00 (128.70 to 129.70): VN064093.D (-4155) (-)

