


Dichlorodifluoromethane

Response Ratio

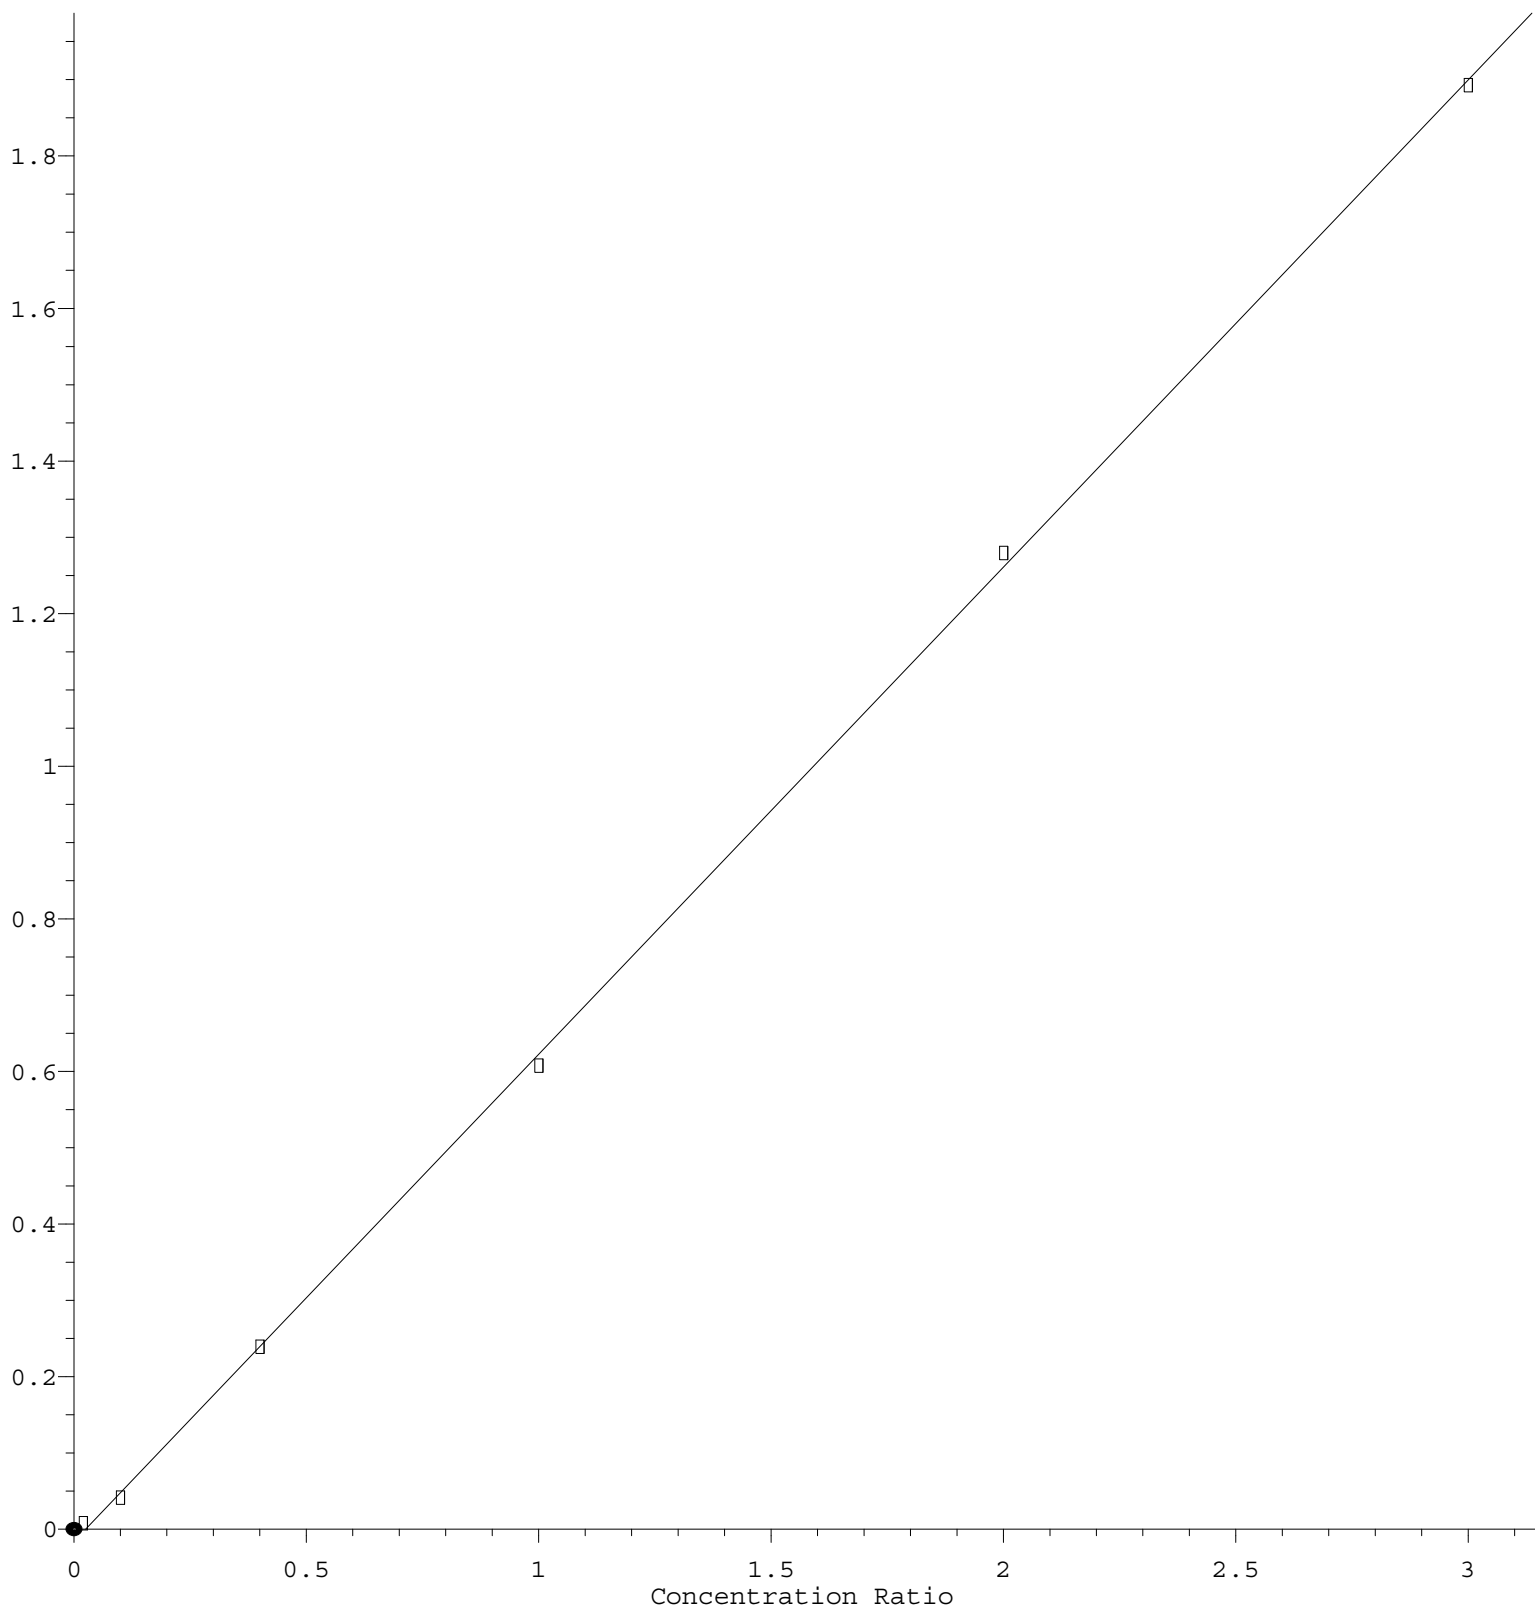

$$\text{Response} = 6.385\text{e-}001 * \text{Amt} - 1.588\text{e-}002$$


Coef of Det (r^2) = 0.999729 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N101221W.M

Calibration Table Last Updated: Wed Oct 13 05:44:40 2021

Naphthalene


Response Ratio

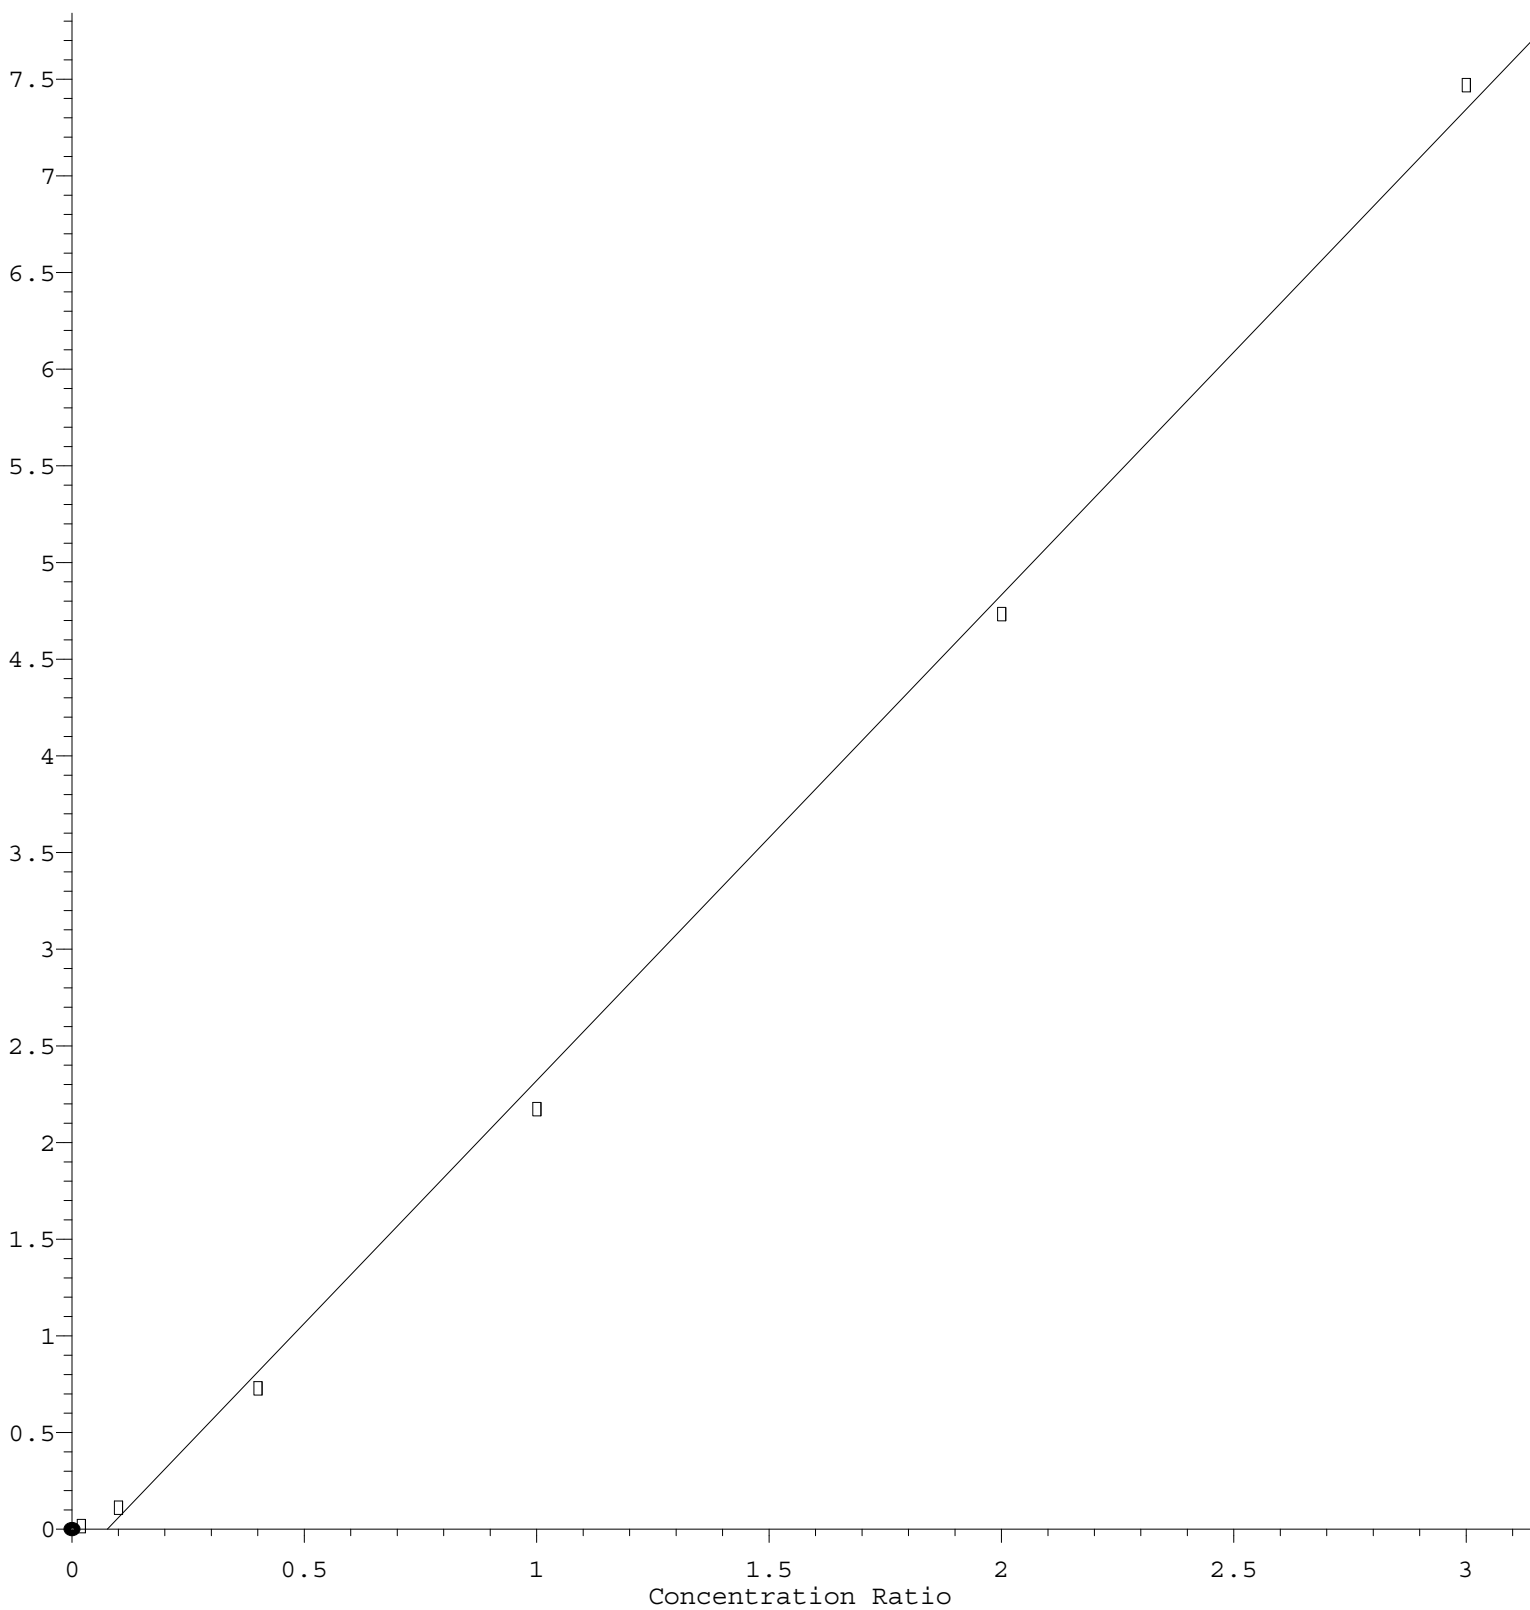

$\text{Response} = 2.512\text{e}+000 * \text{Amt} - 1.915\text{e}-001$
 Coef of Det (r^2) = 0.998175 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N101221W.M
 Calibration Table Last Updated: Wed Oct 13 05:44:40 2021

1,2,3-Trichlorobenzene

Response Ratio

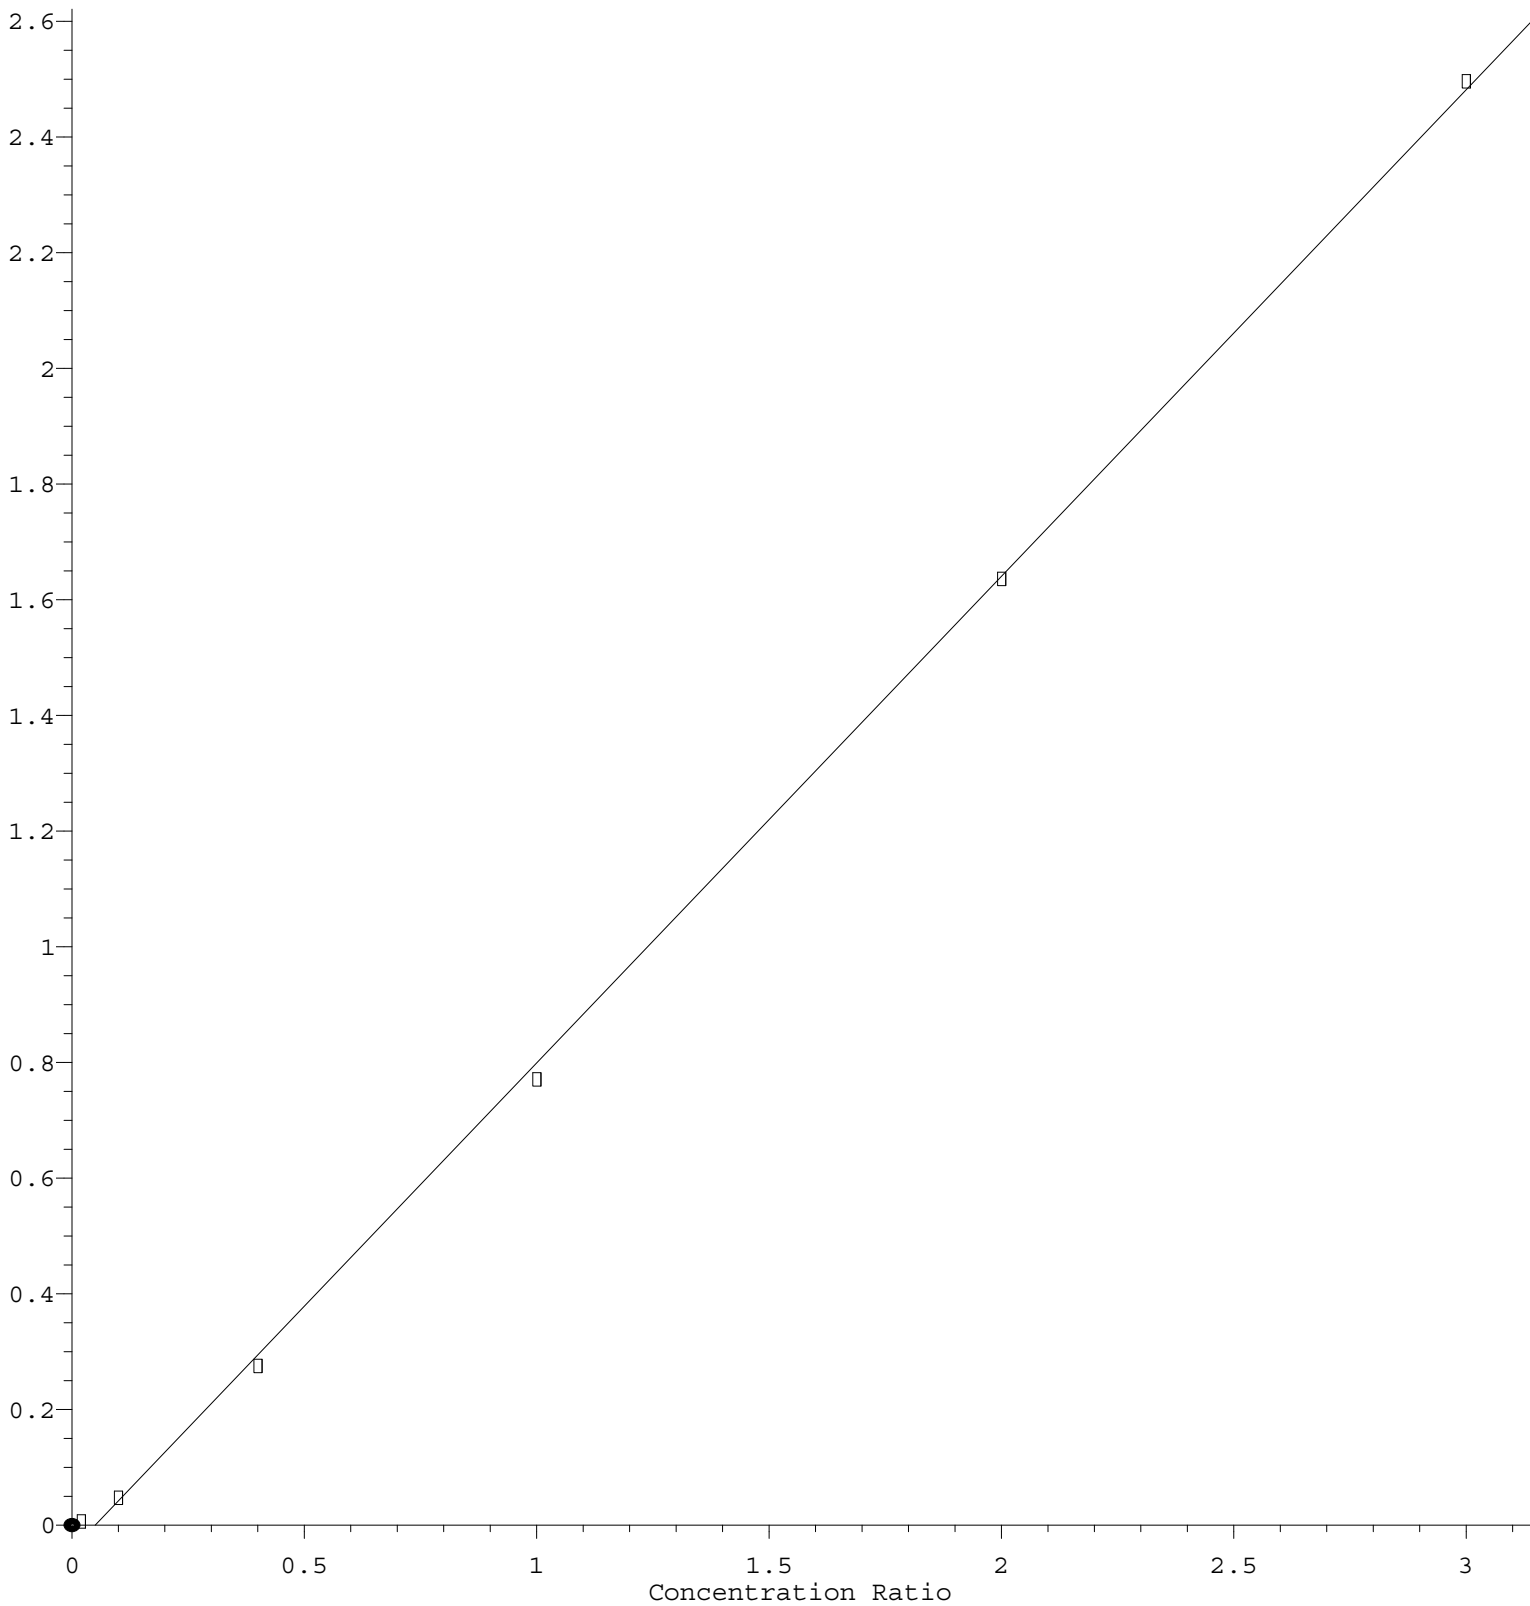


$$\text{Response} = 8.413\text{e-}001 * \text{Amt} - 4.230\text{e-}002$$

Coef of Det (r^2) = 0.999512 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N101221W.M

Calibration Table Last Updated: Wed Oct 13 05:44:40 2021


1,4-Dioxane

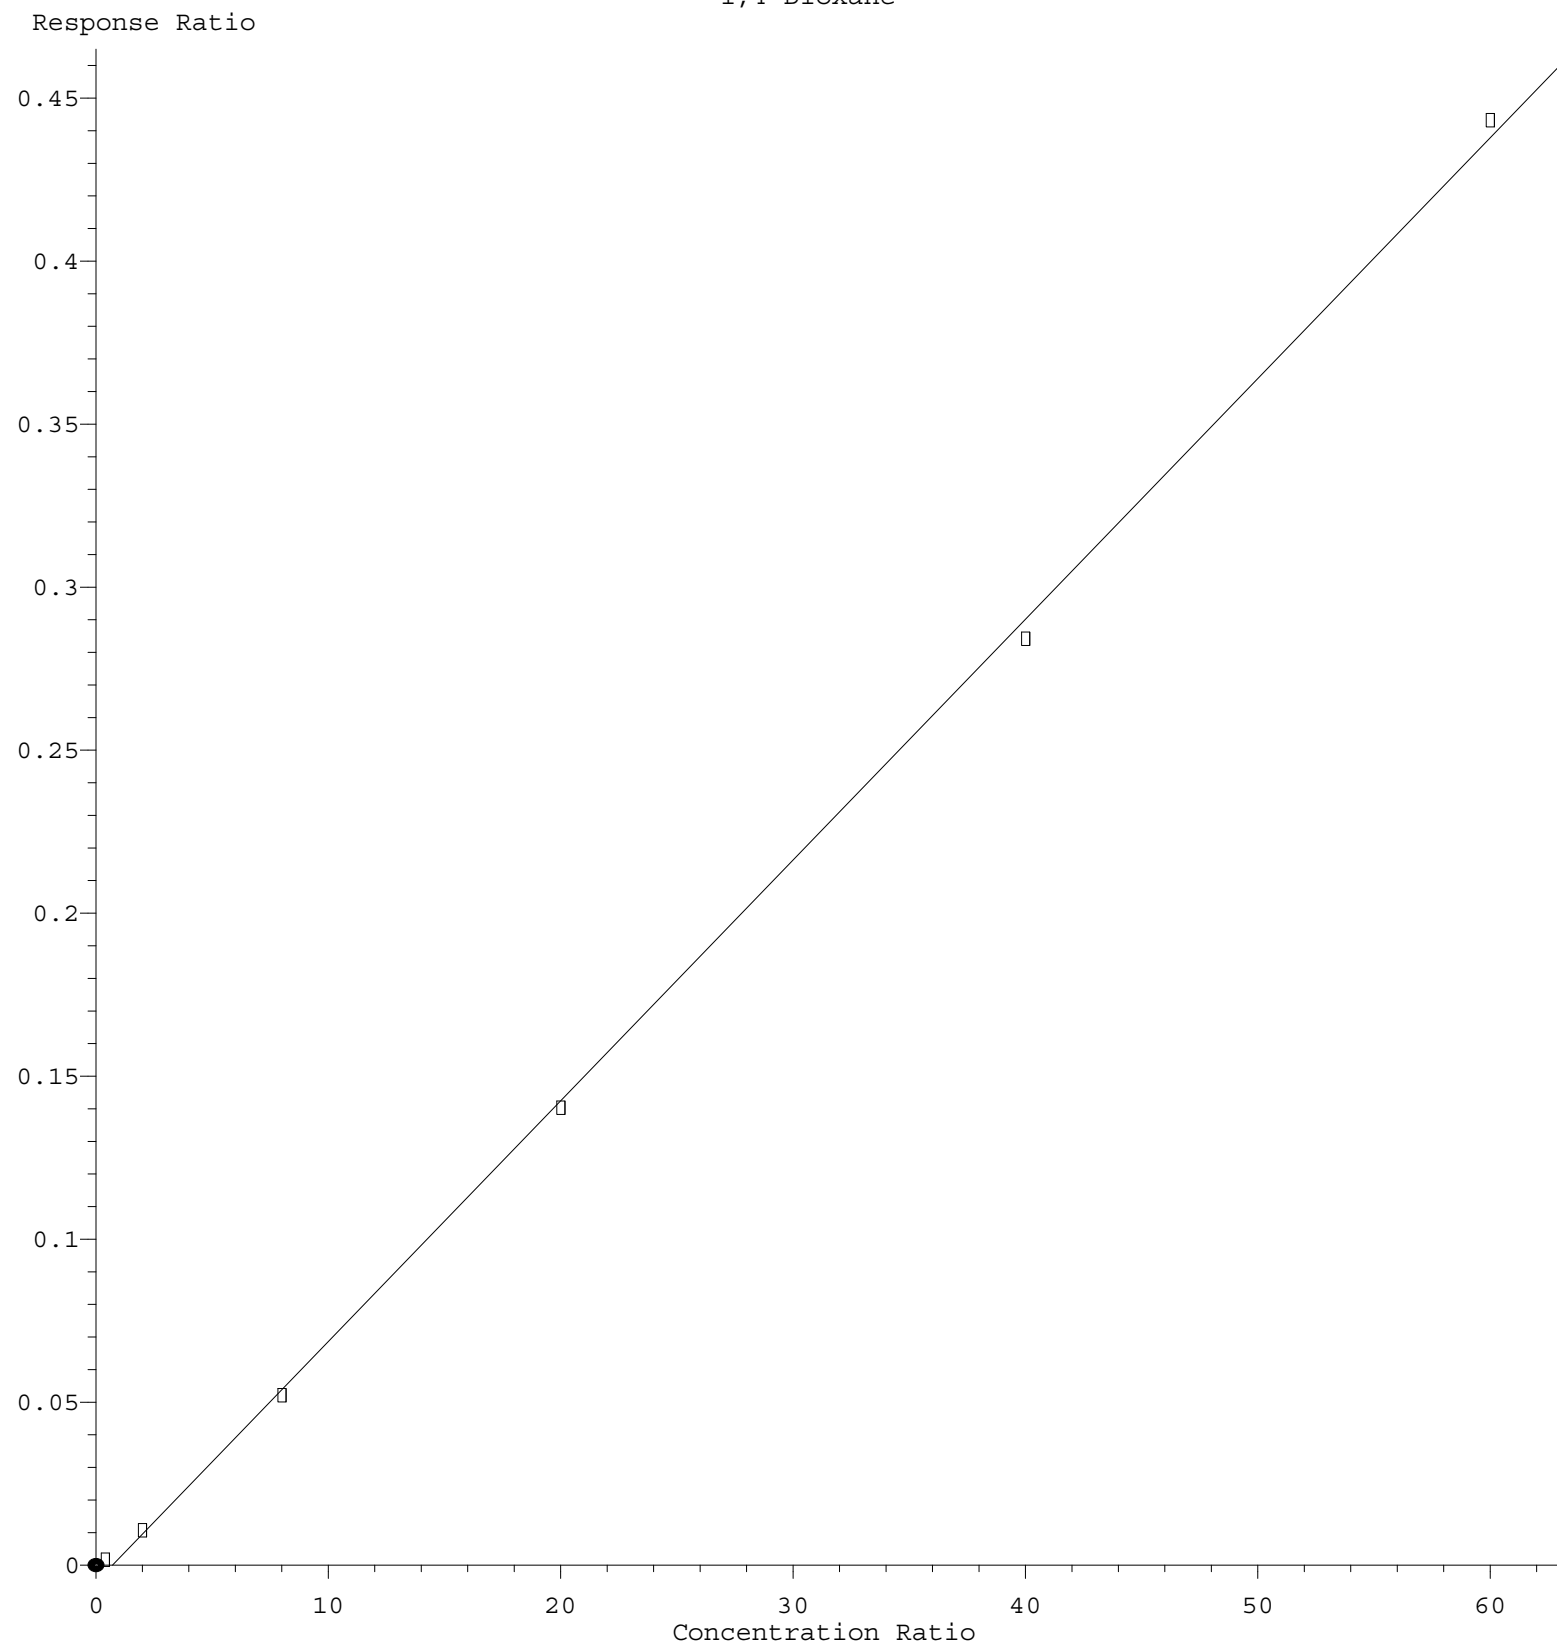

Response = $7.390 \times 10^{-3} \times \text{Amt} - 5.267 \times 10^{-3}$
 Coef of Det (r^2) = 0.999424 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N101221W.M
 Calibration Table Last Updated: Wed Oct 13 05:44:40 2021

2-Chloroethyl Vinyl ether


Response Ratio

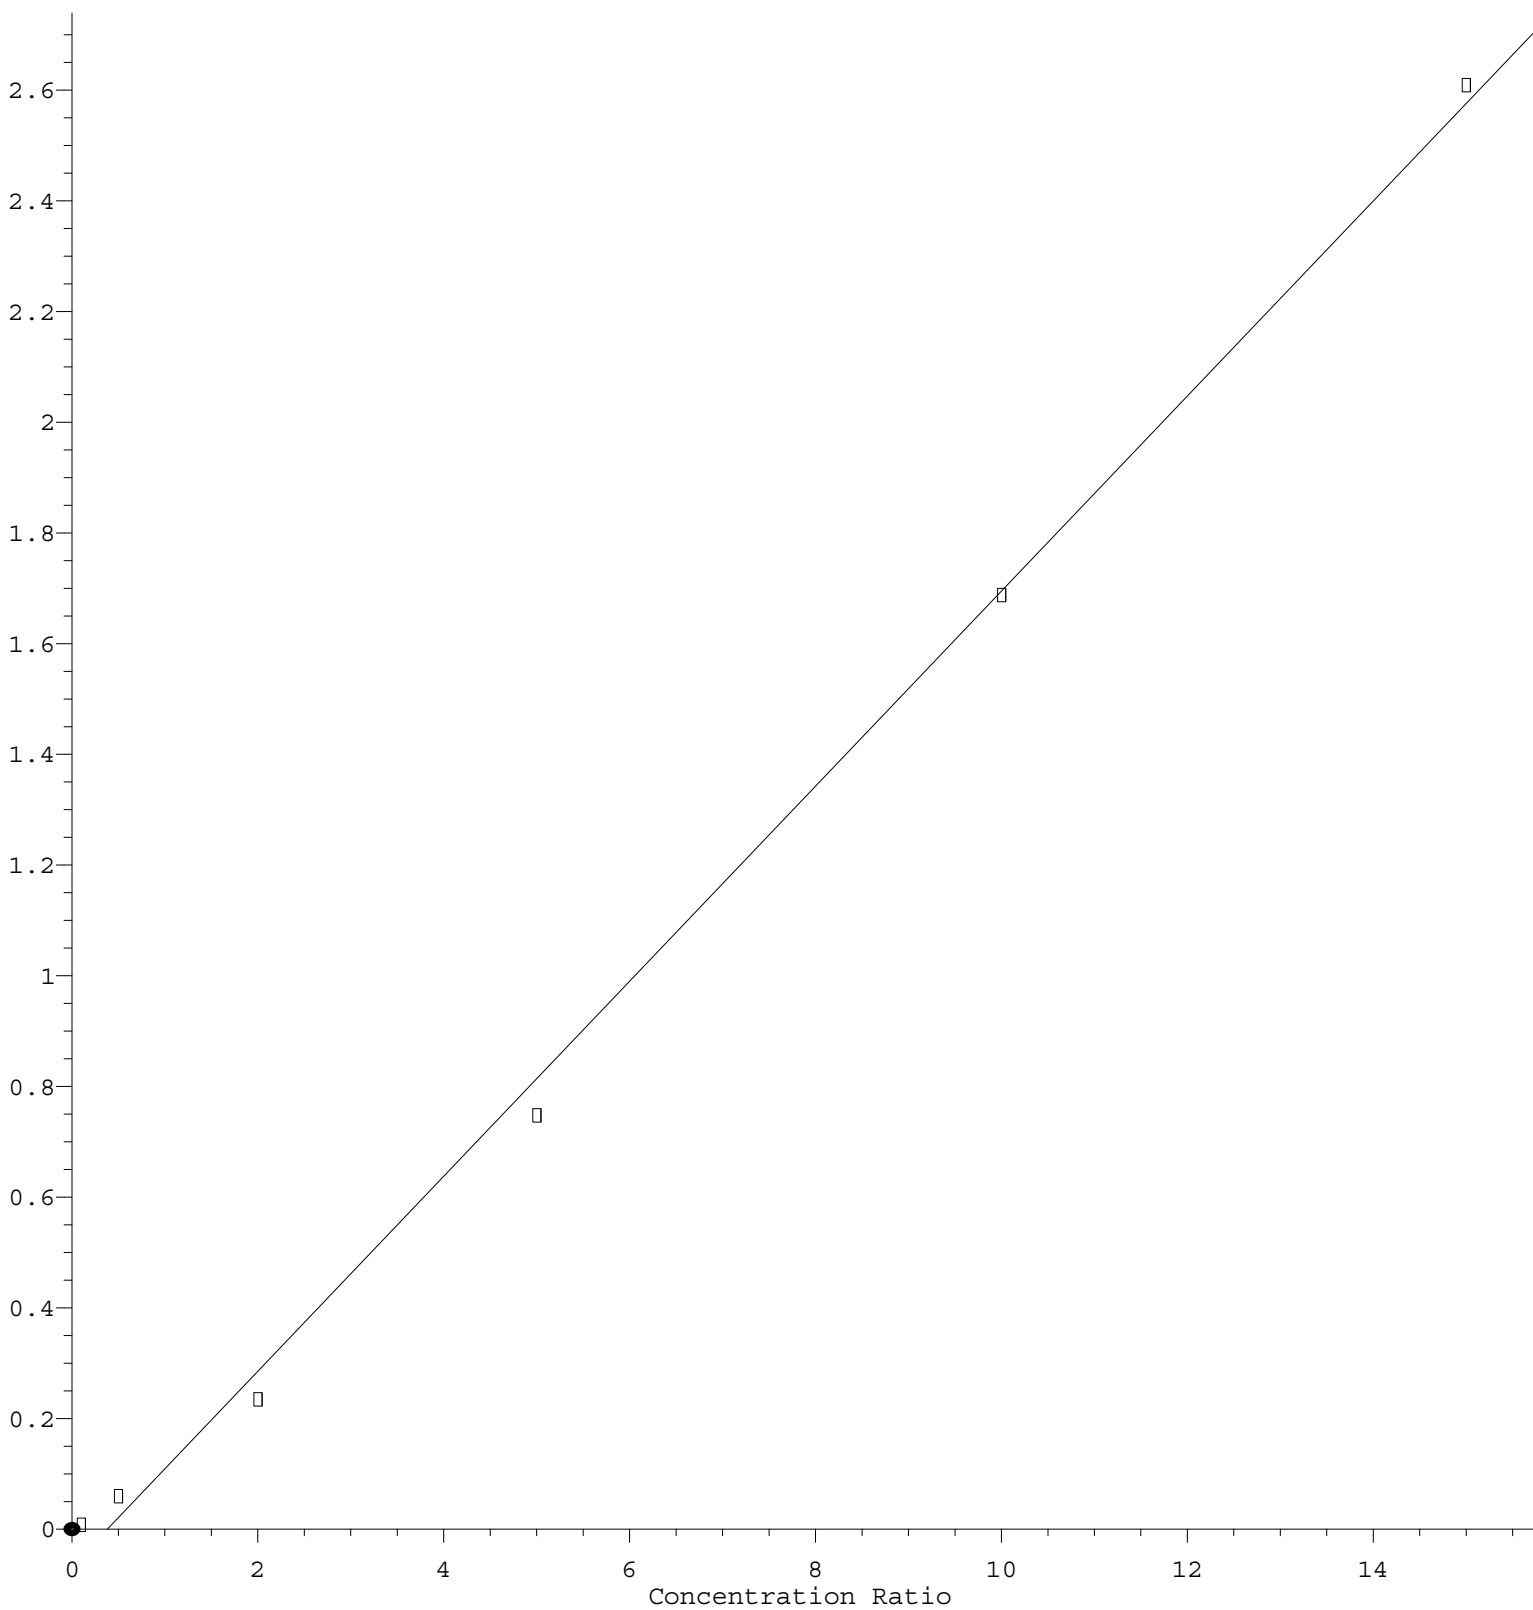

Response = 1.761e-001 * Amt - 6.608e-002
 Coef of Det (r^2) = 0.997659 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N101221W.M
 Calibration Table Last Updated: Wed Oct 13 05:44:40 2021

1,2,4-Trichlorobenzene

Response Ratio

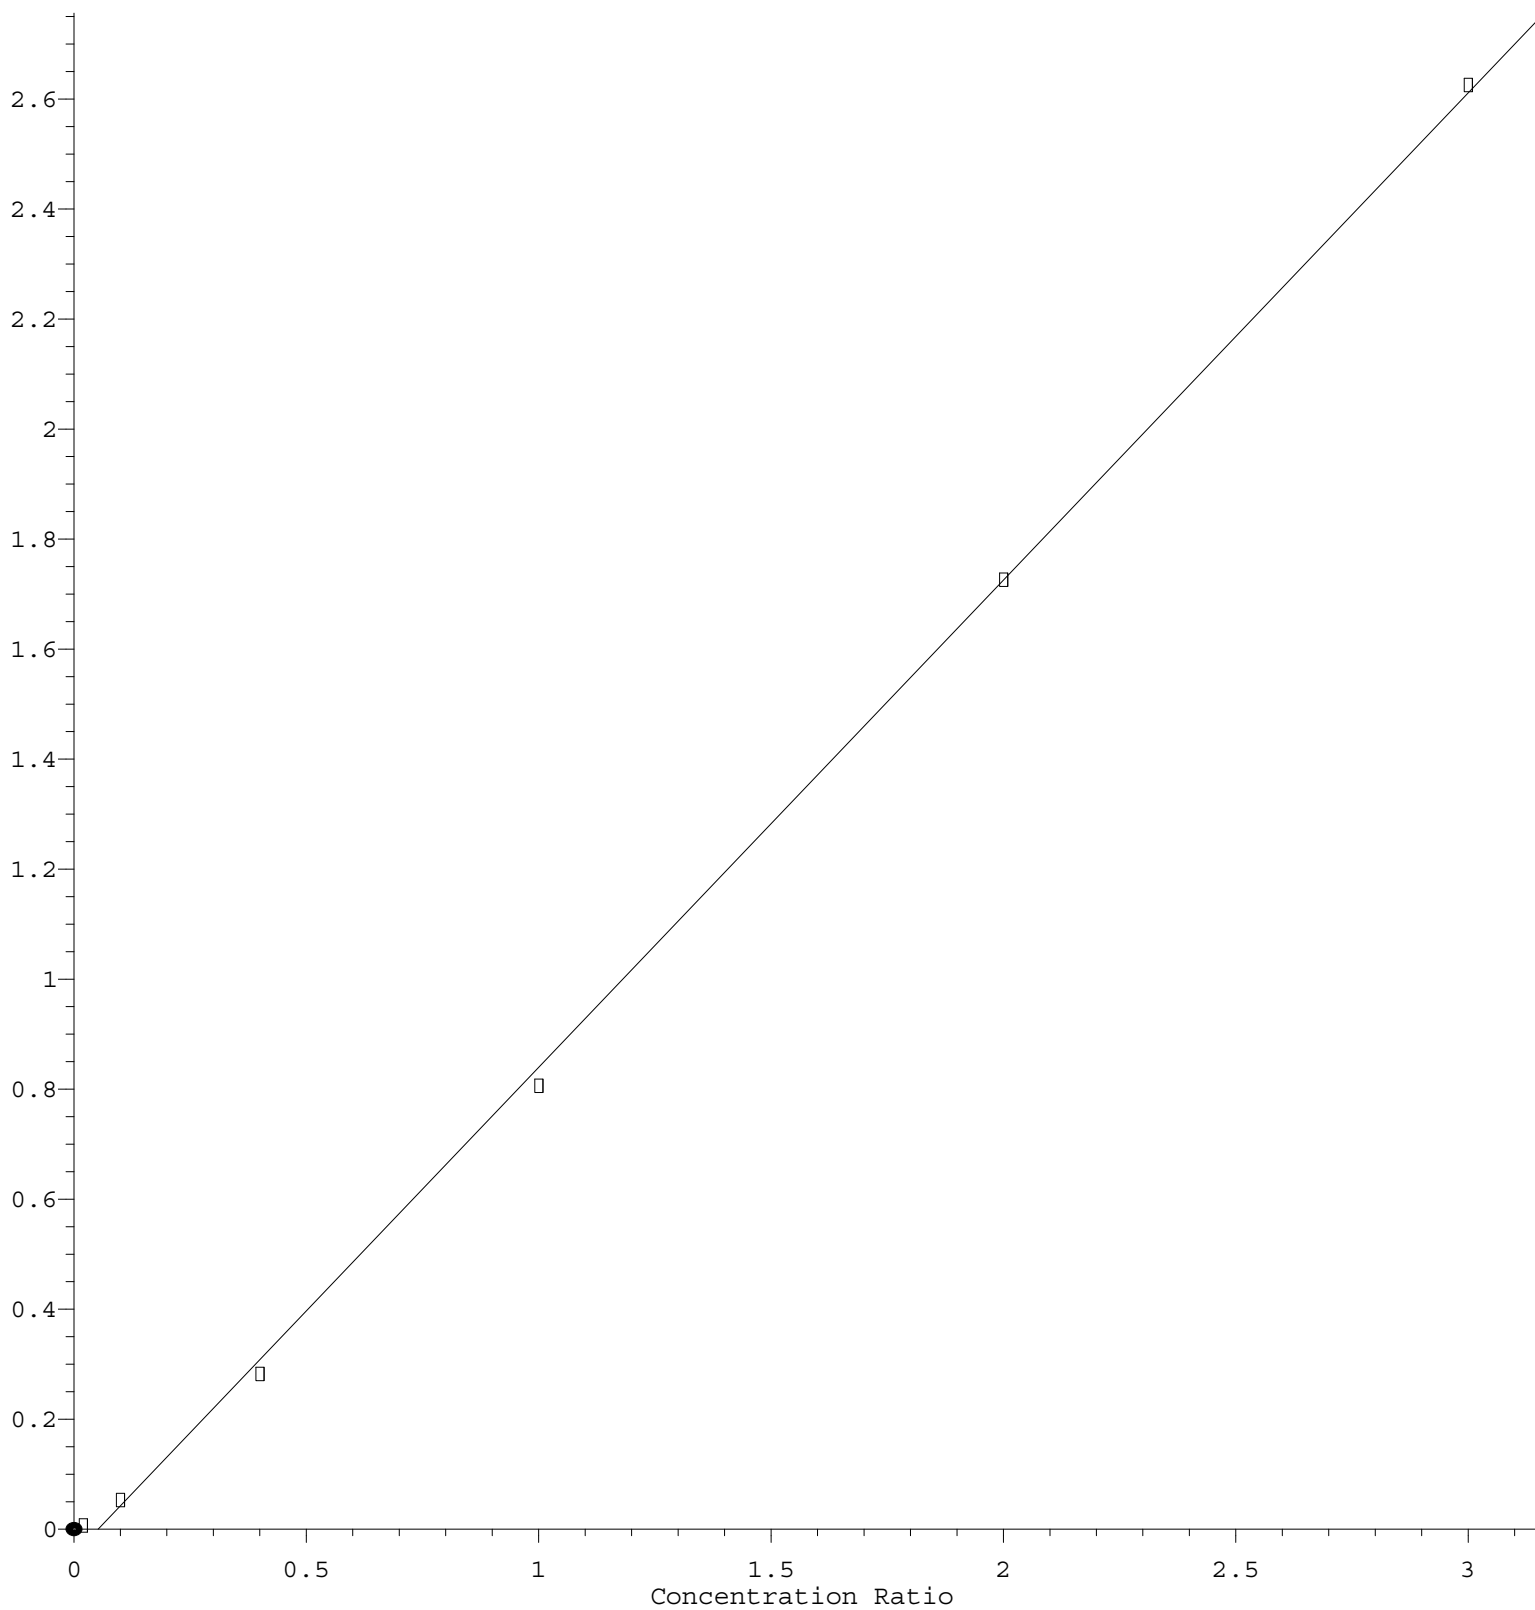

$$\text{Response} = 8.858\text{e-}001 * \text{Amt} - 4.609\text{e-}002$$

Coef of Det (r^2) = 0.999396 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N101221W.M

Calibration Table Last Updated: Wed Oct 13 05:44:40 2021