


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101221\
Data File : VN068857.D
Acq On : 12 Oct 2021 9:19
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Title : SW846 8260
Last Update : Wed Oct 13 05:44:40 2021

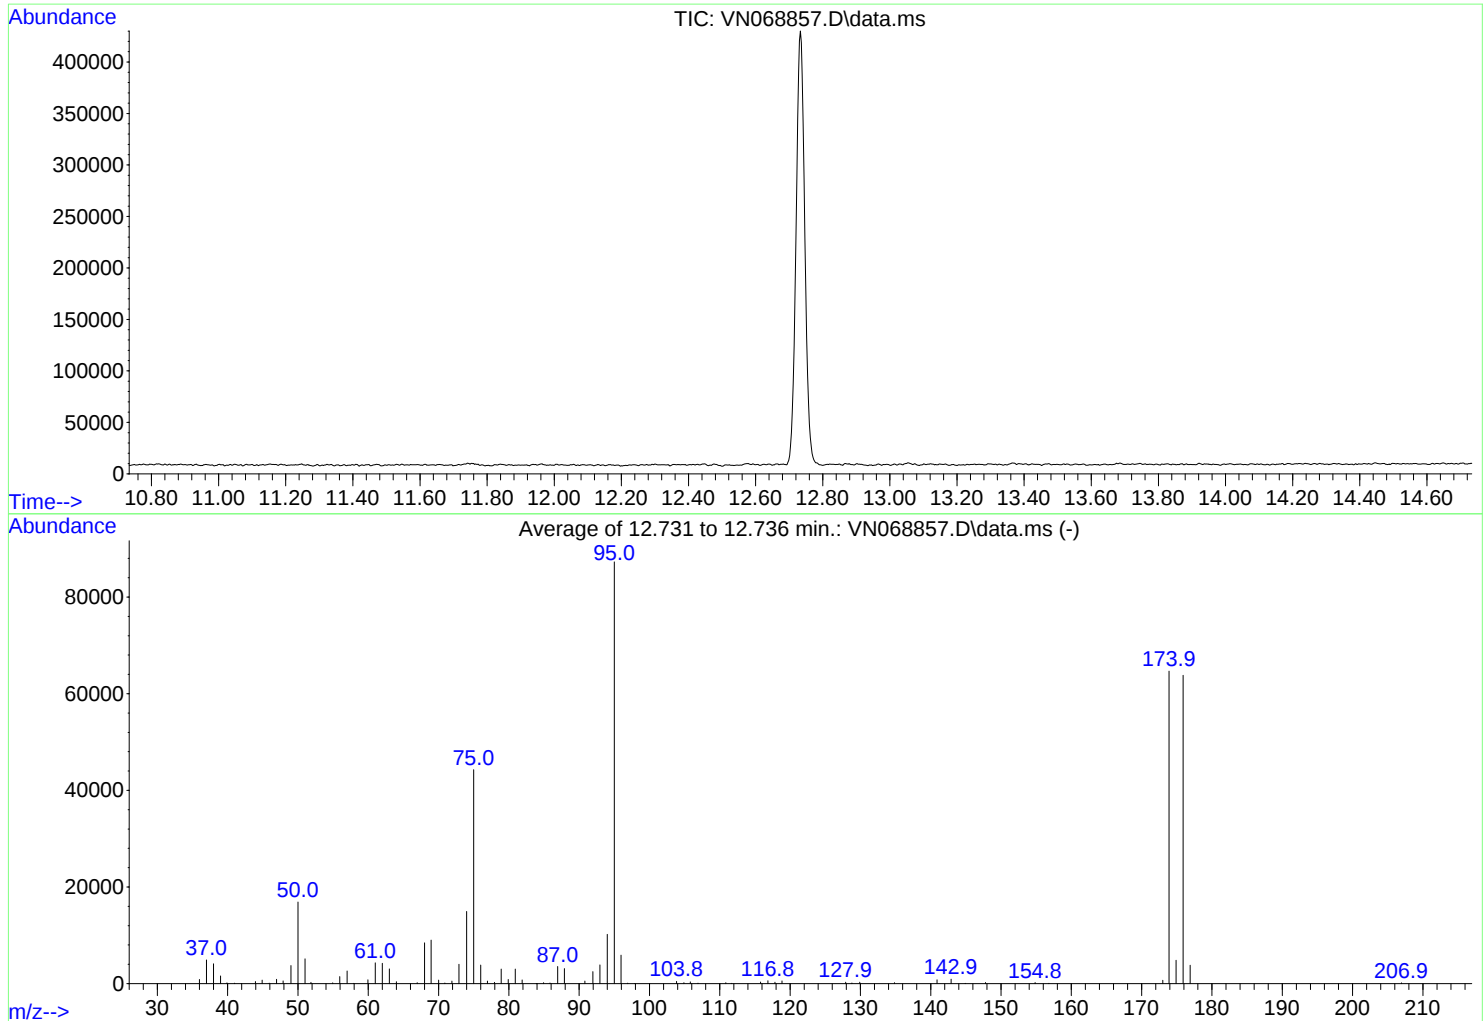

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3984

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	16904	PASS
75	95	30	60	50.7	44280	PASS
95	95	100	100	100.0	87293	PASS
96	95	5	9	6.8	5895	PASS
173	174	0.00	2	1.1	714	PASS
174	95	50	100	74.1	64683	PASS
175	174	5	9	7.5	4855	PASS
176	174	95	101	98.6	63800	PASS
177	176	5	9	6.0	3807	PASS