
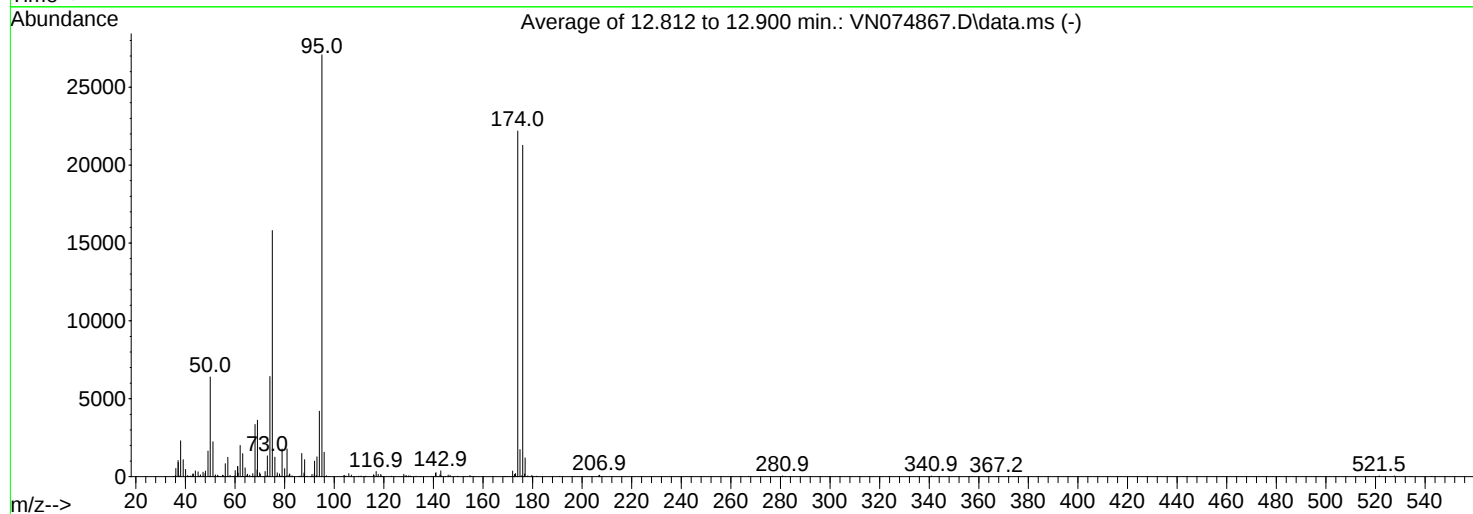


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101222\
Data File : VN074867.D
Acq On : 12 Oct 2022 09:26
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N101222W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Oct 13 07:52:24 2022

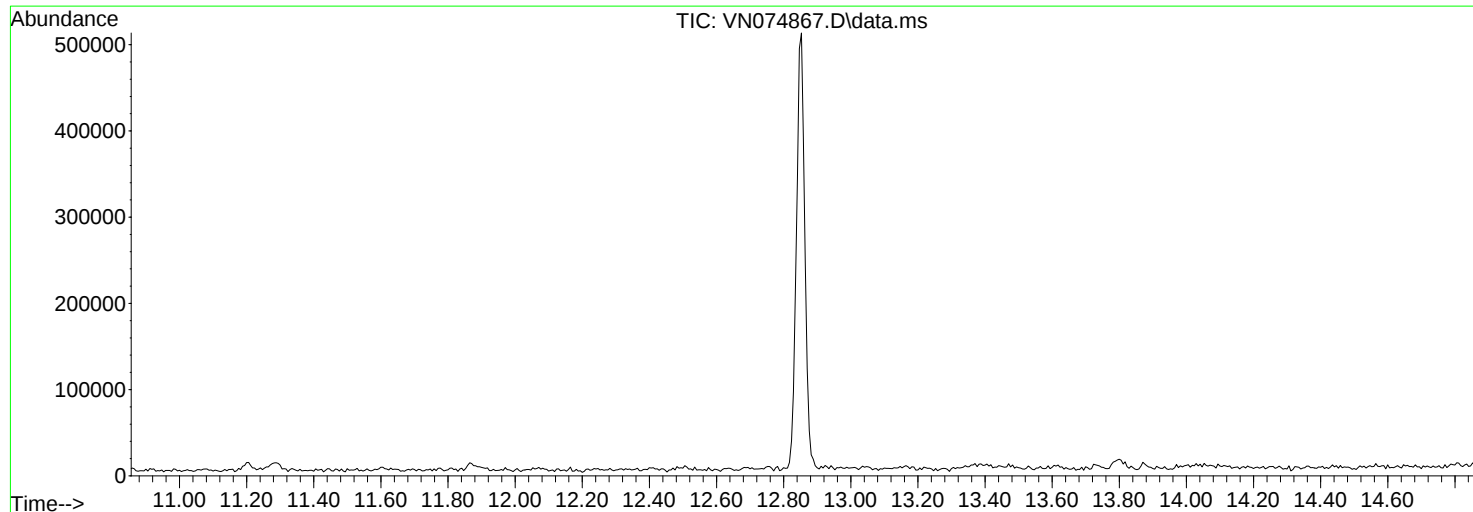

AutoFind: Averaged scan 1829 to 1844; Bkg corrected with scan 1828

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.6	6399	PASS
75	95	30	60	58.4	15801	PASS
95	95	100	100	100.0	27076	PASS
96	95	5	9	5.8	1567	PASS
173	174	0.00	2	0.9	194	PASS
174	95	50	100	81.9	22185	PASS
175	174	5	9	7.8	1738	PASS
176	174	95	101	95.9	21271	PASS
177	176	5	9	5.6	1201	PASS