

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101223\
 Data File : VN079538.D
 Acq On : 12 Oct 2023 12:13
 Operator : JC\MD
 Sample : VN1012WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Oct 13 01:16:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
 Quant Title : SW846 8260
 QLast Update : Fri Oct 06 03:34:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.229	168	239955	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	467914	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	449228	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	139511	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	206080	52.968	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 105.940%	
35) Dibromofluoromethane	8.171	113	179611	53.414	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 106.820%	
50) Toluene-d8	10.570	98	557423	45.815	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 91.620%	
62) 4-Bromofluorobenzene	12.853	95	180171	46.143	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 92.280%	
Target Compounds						
					Qvalue	
5) Bromomethane	2.947	94	644	0.241	ug/l #	45
11) Tert butyl alcohol	5.536	59	120	0.205	ug/l #	72
13) Acrolein	4.189	56	165	0.283	ug/l #	68
15) Acrylonitrile	5.718	53	387	0.228	ug/l #	69
16) Acetone	4.447	43	793	0.514	ug/l #	40
17) Carbon Disulfide	4.712	76	3149	0.356	ug/l #	90
18) Methyl Acetate	5.053	43	2149	0.285	ug/l #	63
20) Methylene Chloride	5.288	84	453	Below Cal	#	61
25) 2-Butanone	7.506	43	777	0.339	ug/l #	37
31) Cyclohexane	8.229	56	6996	1.268	ug/l #	47
36) 1,1-Dichloropropene	8.229	75	22641	4.486	ug/l #	47
38) Carbon Tetrachloride	8.235	117	26133	5.172	ug/l #	17
43) Isopropyl Acetate	8.724	43	2942	0.334	ug/l #	49
51) 4-Methyl-2-Pentanone	10.447	43	1505	0.303	ug/l #	71
59) 2-Hexanone	11.200	43	2947	0.822	ug/l	69
74) N-amyl acetate	12.500	43	1235	0.232	ug/l #	74
75) 1,1,2,2-Tetrachloroethane	12.941	83	640	Below Cal	#	96
76) 1,2,3-Trichloropropane	12.853	75	101742	25.293	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	101742	73.390	ug/l #	15
82) 4-Chlorotoluene	13.229	91	2069	0.231	ug/l	90
87) 1,3-Dichlorobenzene	13.735	146	1334	0.264	ug/l	87
88) 1,4-Dichlorobenzene	13.735	146	1334	0.256	ug/l	87
89) n-Butylbenzene	14.058	91	2285	0.319	ug/l	90
90) Hexachloroethane	14.341	117	249	Below Cal	#	21
91) 1,2-Dichlorobenzene	14.111	146	1639	0.333	ug/l	93
92) 1,2-Dibromo-3-Chloropr...	14.723	75	363	0.484	ug/l #	64
93) 1,2,4-Trichlorobenzene	15.400	180	1501	0.984	ug/l	96
94) Hexachlorobutadiene	15.505	225	1280	1.078	ug/l	86
95) Naphthalene	15.647	128	5975	1.283	ug/l #	95
96) 1,2,3-Trichlorobenzene	15.858	180	2042	1.122	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101223\
Data File : VN079538.D
Acq On : 12 Oct 2023 12:13
Operator : JC\MD
Sample : VN1012WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Oct 13 01:16:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
Quant Title : SW846 8260
QLast Update : Fri Oct 06 03:34:49 2023
Response via : Initial Calibration

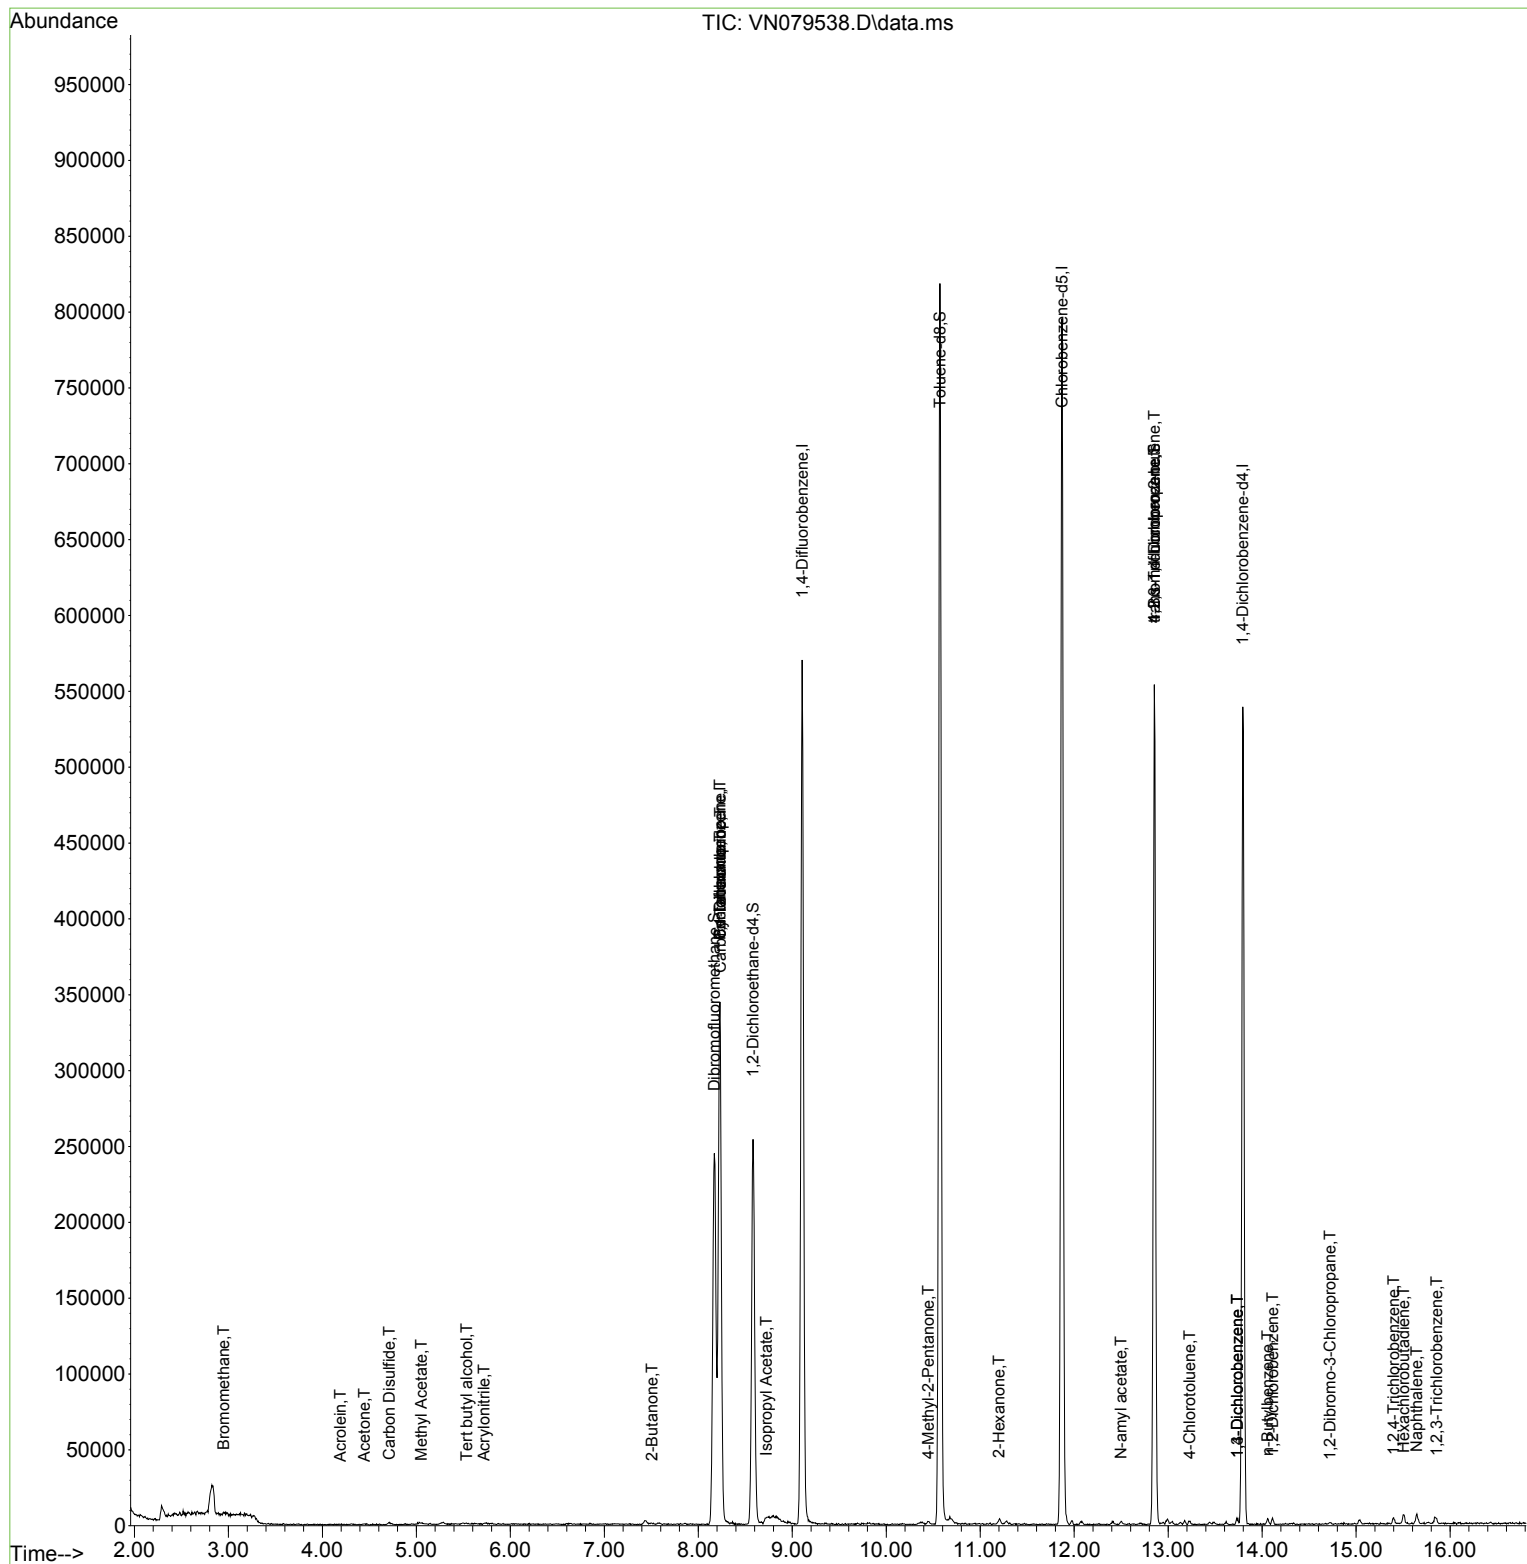



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.229 min Scan# 1

Delta R.T. -0.001 min


Lab File: VN079538.D

Acq: 12 Oct 2023 12:13

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion:168 Resp: 239955

Ion Ratio Lower Upper

168 100

99 63.5 53.0 79.6



#5

Bromomethane

Concen: 0.241 ug/l

RT: 2.947 min Scan# 169

Delta R.T. 0.012 min

Lab File: VN079538.D




Acq: 12 Oct 2023 12:13


Tgt Ion: 94 Resp: 644

Ion Ratio Lower Upper

94 100


96 39.2 73.1 109.7#

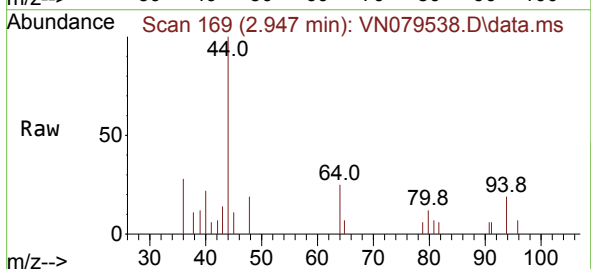






#11
Tert butyl alcohol
Concen: 0.205 ug/l
RT: 5.536 min Scan# 608
Delta R.T. 0.006 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 59 Resp: 120
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

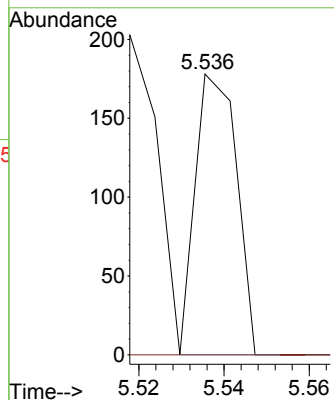

#13
Acrolein
Concen: 0.283 ug/l
RT: 4.189 min Scan# 380
Delta R.T. 0.006 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13


Tgt Ion: 56 Resp: 165
Ion Ratio Lower Upper
56 100
55 93.9 54.5 81.7#

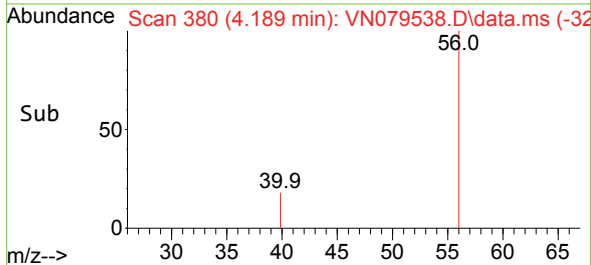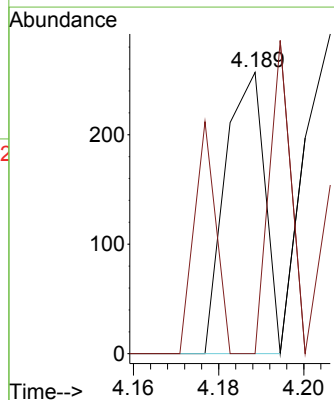






#15
Acrylonitrile
Concen: 0.228 ug/l
RT: 5.718 min Scan# 641
Delta R.T. -0.006 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 53 Resp: 387
Ion Ratio Lower Upper
53 100
52 96.9 65.3 97.9
51 0.0 28.9 43.3#



#16
Acetone
Concen: 0.514 ug/l
RT: 4.447 min Scan# 424
Delta R.T. 0.017 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13


Tgt Ion: 43 Resp: 793
Ion Ratio Lower Upper
43 100
58 0.0 28.0 42.0#

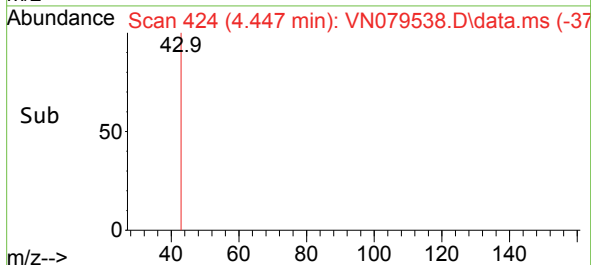






#17
Carbon Disulfide
Concen: 0.356 ug/l
RT: 4.712 min Scan# 41
Delta R.T. -0.000 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 76 Resp: 3149
Ion Ratio Lower Upper
76 100
78 13.0 7.4 11.0#

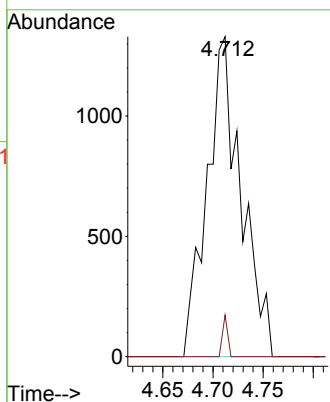


#18
Methyl Acetate
Concen: 0.285 ug/l
RT: 5.053 min Scan# 527
Delta R.T. 0.023 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13




Tgt Ion: 43 Resp: 2149
Ion Ratio Lower Upper
43 100
74 11.8 26.2 39.4#

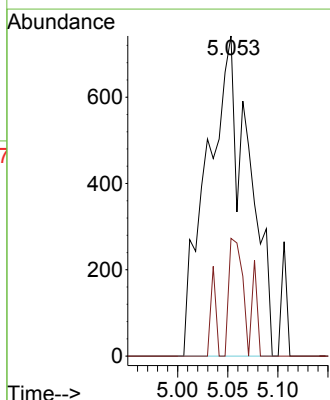






#20
Methylene Chloride
Concen: Below Cal
RT: 5.288 min Scan# 50
Delta R.T. 0.005 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 84 Resp: 453
Ion Ratio Lower Upper
84 100
49 52.2 79.7 119.5#
51 0.0 25.2 37.8#
86 52.5 53.3 79.9#

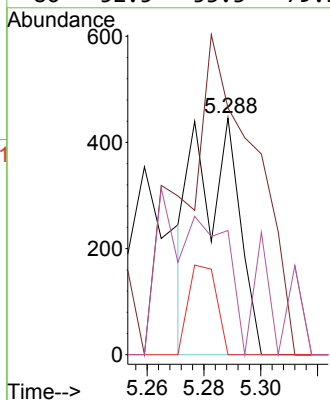

#25
2-Butanone
Concen: 0.339 ug/l
RT: 7.506 min Scan# 944
Delta R.T. 0.018 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13


Tgt Ion: 43 Resp: 777
Ion Ratio Lower Upper
43 100
72 0.0 30.2 45.2#

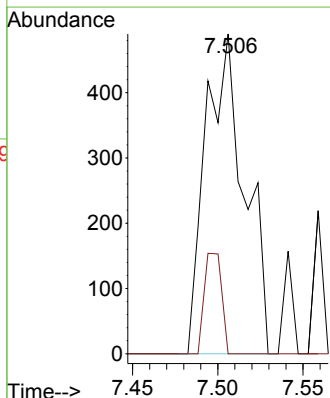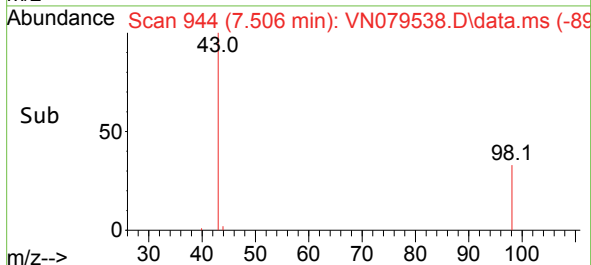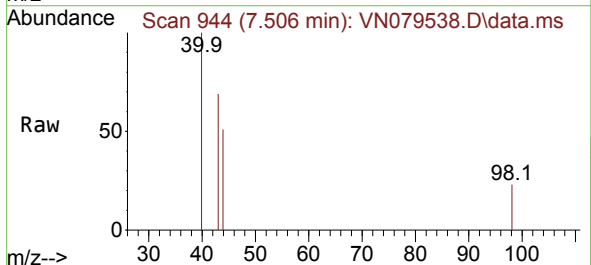






#31
Cyclohexane
Concen: 1.268 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.035 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 6996
Ion Ratio Lower Upper
56 100
69 111.5 26.8 40.2#
84 128.5 81.8 122.6#



#33
1,2-Dichloroethane-d4
Concen: 52.968 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. -0.000 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13

Tgt Ion: 65 Resp: 206080
Ion Ratio Lower Upper
65 100
67 51.5 0.0 106.6

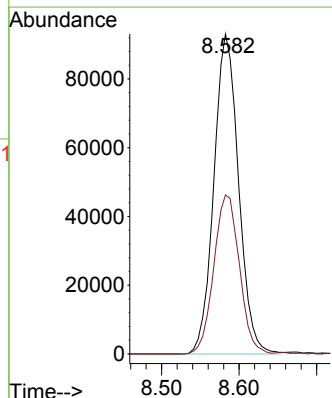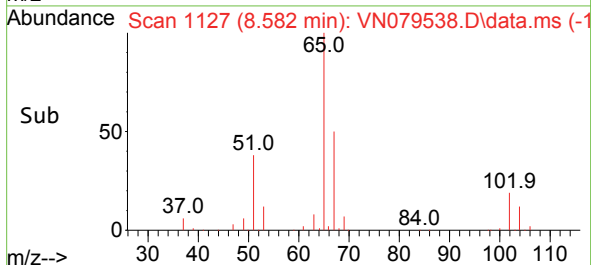



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN079538.D

Acq: 12 Oct 2023 12:13

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:114 Resp: 467914

Ion Ratio Lower Upper

114 100

63 21.5 0.0 36.4

88 16.1 0.0 30.6



#35

Dibromofluoromethane

Concen: 53.414 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VN079538.D

Acq: 12 Oct 2023 12:13




Tgt Ion:113 Resp: 179611


Ion Ratio Lower Upper

113 100

111 102.1 82.6 123.8

192 17.4 12.7 19.1

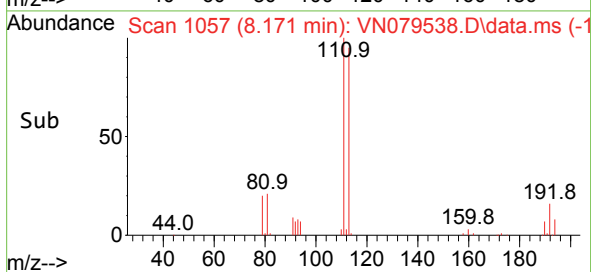



#36

1,1-Dichloropropene

Concen: 4.486 ug/l

RT: 8.229 min Scan# 1067

Delta R.T. -0.147 min


Lab File: VN079538.D

Acq: 12 Oct 2023 12:13

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 75 Resp: 22641

Ion Ratio Lower Upper

75 100

110 7.9 19.1 57.3#

77 0.0 25.0 37.4#



#38

Carbon Tetrachloride

Concen: 5.172 ug/l

RT: 8.235 min Scan# 1068

Delta R.T. -0.130 min

Lab File: VN079538.D

Acq: 12 Oct 2023 12:13




Tgt Ion: 117 Resp: 26133


Ion Ratio Lower Upper

117 100

119 6.2 77.3 115.9#

121 0.0 23.3 34.9#


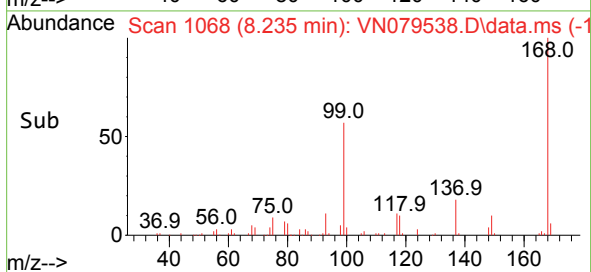

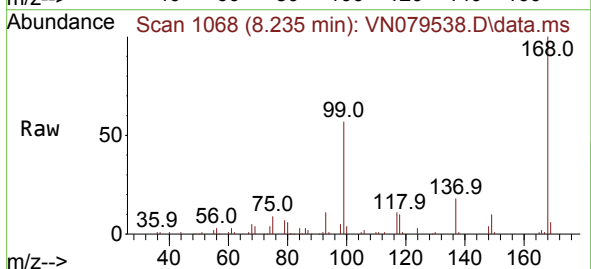




#43
Isopropyl Acetate
Concen: 0.334 ug/l
RT: 8.724 min Scan# 1151
Delta R.T. 0.029 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 2942
Ion Ratio Lower Upper
43 100
61 0.0 24.7 37.1#
87 0.0 14.6 21.8#

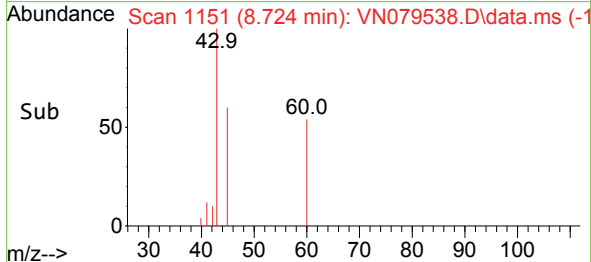

#50
Toluene-d8
Concen: 45.815 ug/l
RT: 10.570 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13


Tgt Ion: 98 Resp: 557423
Ion Ratio Lower Upper
98 100
100 63.5 52.0 78.0








#51
4-Methyl-2-Pentanone
Concen: 0.303 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. -0.000 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 1505
Ion Ratio Lower Upper
43 100
58 26.4 36.6 54.8#

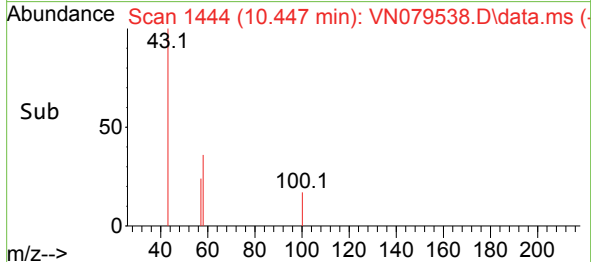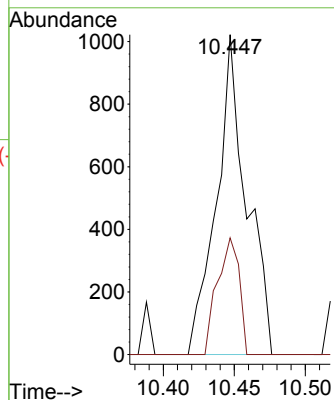

#59
2-Hexanone
Concen: 0.822 ug/l
RT: 11.200 min Scan# 1572
Delta R.T. -0.000 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13

Tgt Ion: 43 Resp: 2947
Ion Ratio Lower Upper
43 100
58 39.2 31.7 95.1


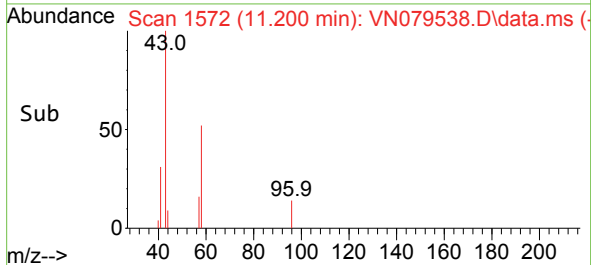
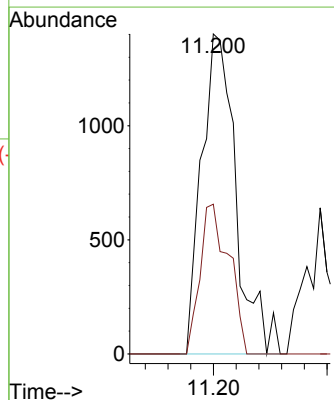





#62
4-Bromofluorobenzene
Concen: 46.143 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 180171
Ion Ratio Lower Upper
95 100
174 77.4 0.0 143.8
176 73.9 0.0 135.8



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1686
Delta R.T. -0.000 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13

Tgt Ion: 117 Resp: 449228
Ion Ratio Lower Upper
117 100
82 58.9 44.0 66.0
119 33.8 25.6 38.4







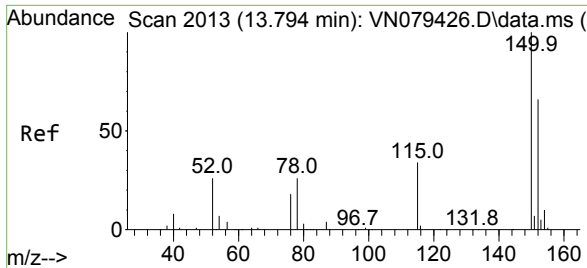

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 20
Delta R.T. -0.000 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:152 Resp: 139511
Ion Ratio Lower Upper
152 100
115 62.1 32.3 96.8
150 156.8 0.0 355.8

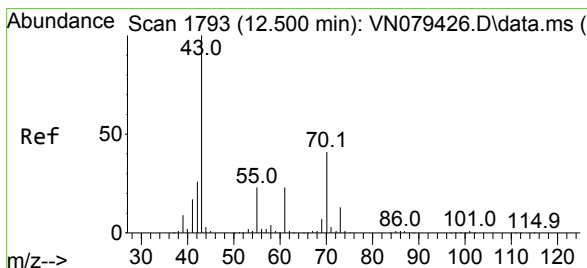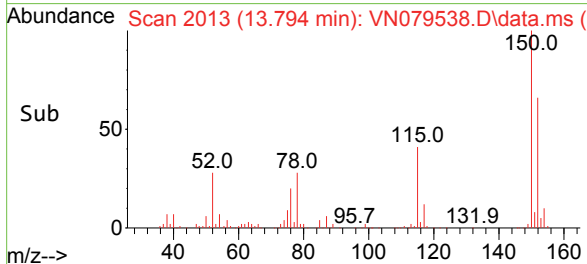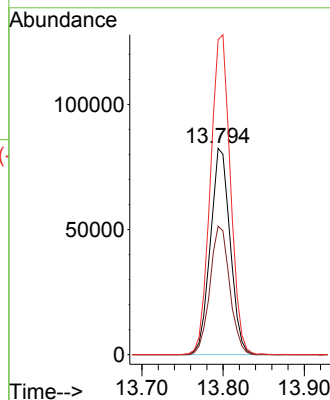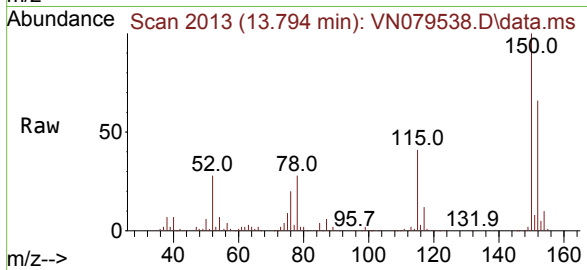

#74
N-ethyl acetate
Concen: 0.232 ug/l
RT: 12.500 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13

Tgt Ion: 43 Resp: 1235
Ion Ratio Lower Upper
43 100
70 27.0 43.4 65.2#
55 33.3 21.4 32.0#
61 20.2 22.8 34.2#

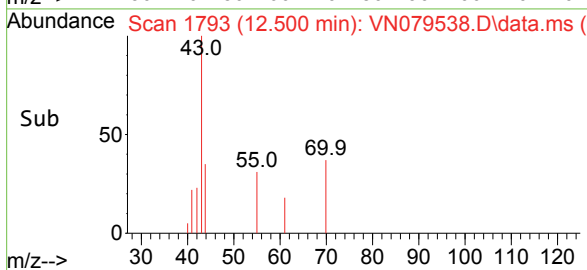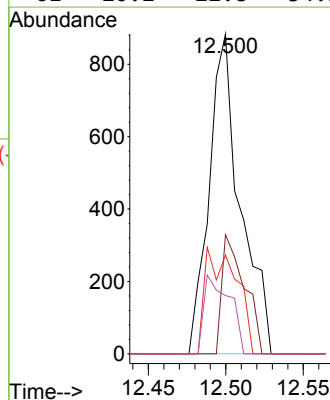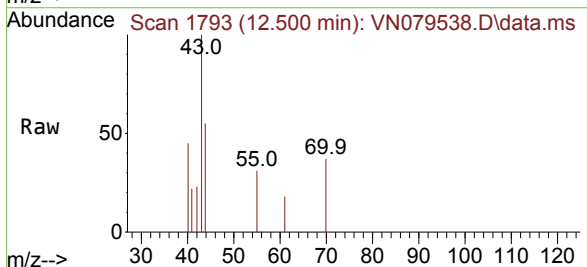



#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 12.941 min Scan# 1868

Delta R.T. -0.000 min


Lab File: VN079538.D

Acq: 12 Oct 2023 12:13

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 83 Resp: 640

Ion Ratio Lower Upper

83 100

131 0.0 5.0 15.0#

85 63.3 31.9 95.7

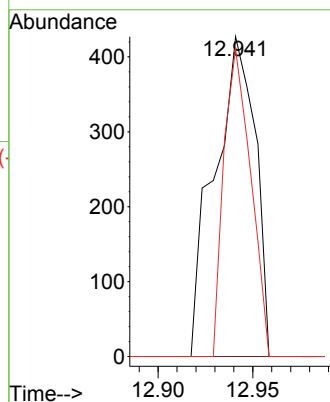

#76

1,2,3-Trichloropropane

Concen: 25.293 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.147 min

Lab File: VN079538.D




Acq: 12 Oct 2023 12:13


Tgt Ion: 75 Resp: 101742

Ion Ratio Lower Upper

75 100

77 1.1 84.5 253.5#


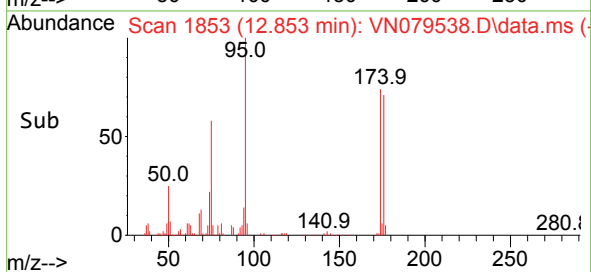

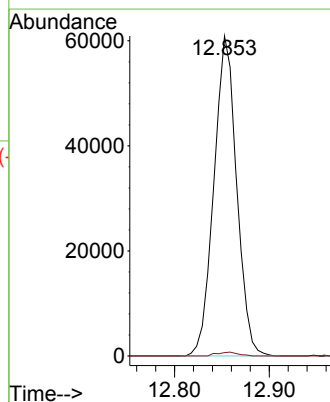




#81
trans-1,4-Dichloro-2-butene
Concen: 73.390 ug/l
RT: 12.853 min Scan# 11
Delta R.T. 0.112 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 101742
Ion Ratio Lower Upper
75 100
53 0.1 67.4 101.2#
89 0.0 38.8 58.2#



#82
4-Chlorotoluene
Concen: 0.231 ug/l
RT: 13.229 min Scan# 1917
Delta R.T. 0.006 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13

Tgt Ion: 91 Resp: 2069
Ion Ratio Lower Upper
91 100
126 27.5 16.7 50.0





#87

1,3-Dichlorobenzene

Concen: 0.264 ug/l

RT: 13.735 min Scan# 2003

Delta R.T. -0.000 min

Lab File: VN079538.D

Acq: 12 Oct 2023 12:13

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:146 Resp: 1334

Ion Ratio Lower Upper

146 100

111 42.8 22.1 66.3

148 48.4 32.0 96.0



#88

1,4-Dichlorobenzene

Concen: 0.256 ug/l

RT: 13.735 min Scan# 2003

Delta R.T. -0.082 min

Lab File: VN079538.D

Acq: 12 Oct 2023 12:13




Tgt Ion:146 Resp: 1334


Ion Ratio Lower Upper

146 100

111 42.8 20.6 61.8

148 48.4 31.6 94.8

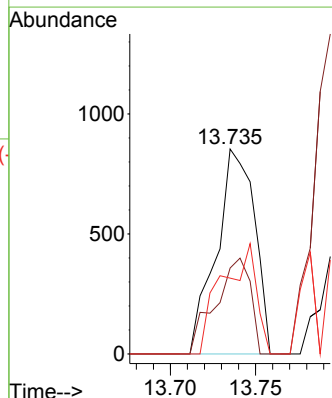



#89

n-Butylbenzene

Concen: 0.319 ug/l

RT: 14.058 min Scan# 2058

Delta R.T. -0.000 min

Lab File: VN079538.D

Acq: 12 Oct 2023 12:13

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 91 Resp: 2285

Ion Ratio Lower Upper

91 100

92 58.8 26.4 79.0

134 31.6 12.6 37.6



#90

Hexachloroethane

Concen: Below Cal

RT: 14.341 min Scan# 2106

Delta R.T. 0.006 min

Lab File: VN079538.D




Acq: 12 Oct 2023 12:13


Tgt Ion: 117 Resp: 249

Ion Ratio Lower Upper

117 100


201 0.0 29.3 88.0#

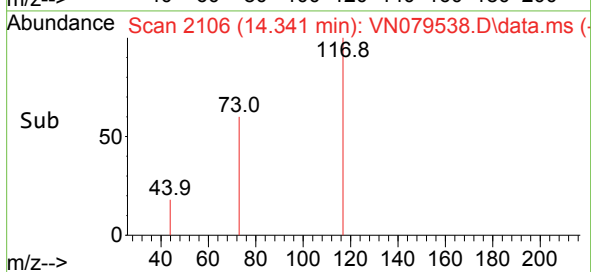






#91
1,2-Dichlorobenzene
Concen: 0.333 ug/l
RT: 14.111 min Scan# 2067
Delta R.T. -0.000 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:146 Resp: 1639
Ion Ratio Lower Upper
146 100
111 40.0 22.0 66.0
148 58.1 31.8 95.3




#92
1,2-Dibromo-3-Chloropropane
Concen: 0.484 ug/l
RT: 14.723 min Scan# 2171
Delta R.T. -0.000 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13



Tgt Ion: 75 Resp: 363
Ion Ratio Lower Upper
75 100
155 18.7 39.1 117.2#
157 89.3 50.3 150.9





#93

1,2,4-Trichlorobenzene

Concen: 0.984 ug/l

RT: 15.400 min Scan# 2286

Delta R.T. -0.000 min

Lab File: VN079538.D





Acq: 12 Oct 2023 12:13

Instrument :

MSVOA_N

ClientSampleId :

Tgt Ion:180	Resp:	1501
Ion Ratio	Lower	Upper
180	100	
182	89.5	46.1 138.2
145	36.9	16.6 49.8



#94

Hexachlorobutadiene

Concen: 1.078 ug/l




RT: 15.505 min Scan# 2304


Delta R.T. -0.000 min

Lab File: VN079538.D

Acq: 12 Oct 2023 12:13

Tgt Ion:225	Resp:	1280
Ion Ratio	Lower	Upper
225	100	
223	67.2	31.3 93.8
227	81.5	31.9 95.9









#95
Naphthalene
Concen: 1.283 ug/l
RT: 15.647 min Scan# 2328
Delta R.T. -0.000 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion:128 Resp: 5975
Ion Ratio Lower Upper
128 100
127 12.0 10.0 15.0
129 7.1 8.7 13.1#

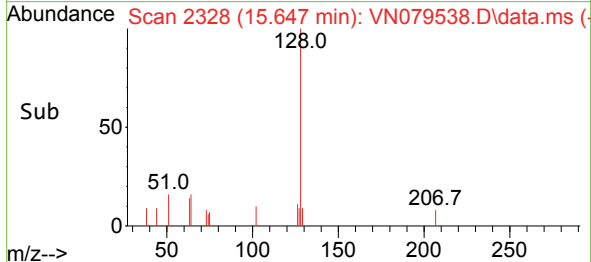

#96
1,2,3-Trichlorobenzene
Concen: 1.122 ug/l
RT: 15.858 min Scan# 2364
Delta R.T. 0.018 min
Lab File: VN079538.D
Acq: 12 Oct 2023 12:13

Tgt Ion:180 Resp: 2042
Ion Ratio Lower Upper
180 100
182 90.3 46.2 138.6
145 36.2 17.5 52.6

