
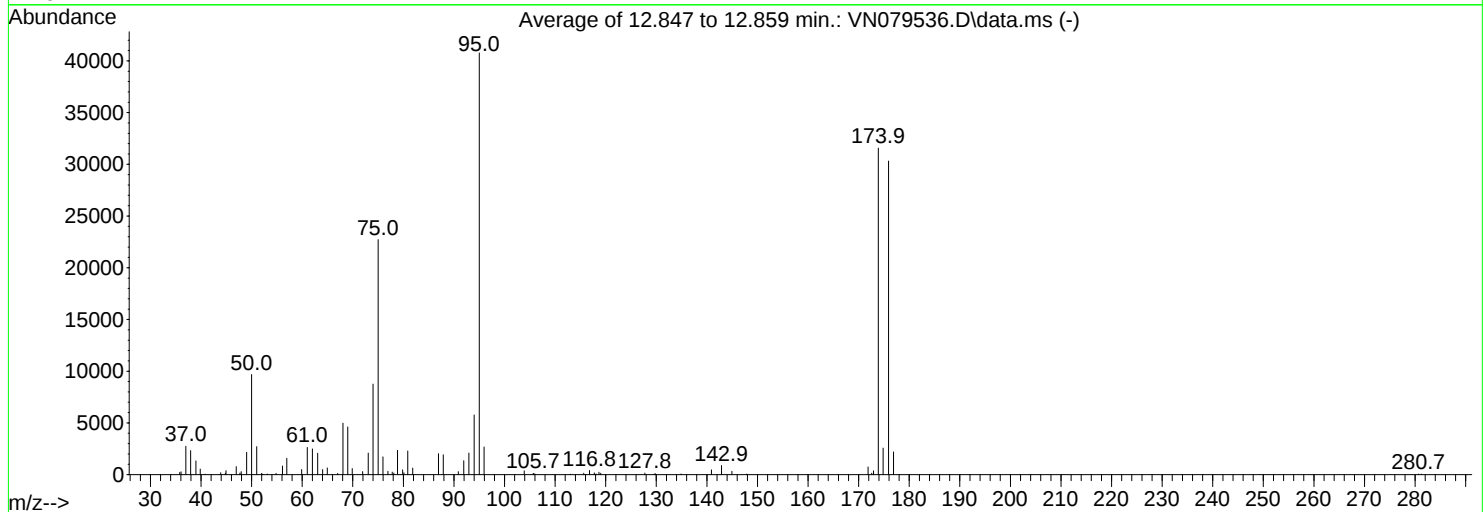


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101223\
Data File : VN079536.D
Acq On : 12 Oct 2023 10:51
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
Title : SW846 8260
Last Update : Fri Oct 06 03:34:49 2023

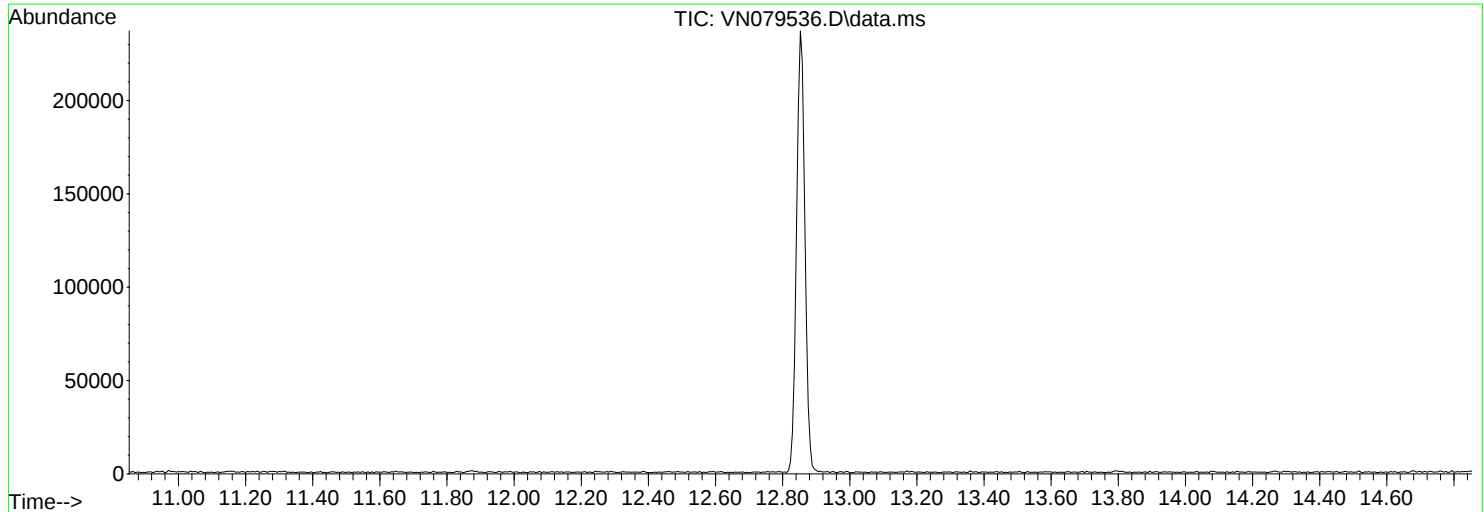

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	9683	PASS
75	95	30	60	55.7	22723	PASS
95	95	100	100	100.0	40776	PASS
96	95	5	9	6.6	2679	PASS
173	174	0.00	2	1.2	377	PASS
174	95	50	100	77.4	31573	PASS
175	174	5	9	8.1	2564	PASS
176	174	95	101	96.0	30320	PASS
177	176	5	9	7.2	2195	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	214	47.70	148	59.90	493	73.05	209
36.05	287	47.95	295	61.00	2632	74.00	875
37.00	2743	49.00	2171	62.00	2484	75.00	2272
37.95	2329	50.00	9683	63.05	2079	75.95	172
39.00	1331	51.00	2704	64.05	498	76.95	330
39.85	537	52.00	129	64.95	648	77.80	250
40.80	52	52.20	50	67.00	128	78.10	153
43.90	187	53.10	57	68.05	4979	78.85	2345
44.80	144	54.85	123	69.00	4610	79.85	471
44.95	380	56.10	839	69.90	590	80.10	185
46.95	780	56.95	1580	71.95	303	80.85	2292

Average of 12.847 to 12.859 min.: VN079536.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.85	629	105.80	108	129.80	87	175.90	30320
86.95	2027	106.00	69	134.90	70	176.90	2195
87.90	1922	113.00	55	140.90	472	280.70	59
90.85	289	115.65	147	142.90	884	281.20	51
91.95	1352	116.80	399	144.95	320		
92.95	2089	117.75	177	147.90	68		
94.00	5765	118.10	70	171.85	744		
95.00	40776	118.65	239	172.60	137		
95.95	2679	119.00	142	172.95	377		
103.90	375	127.75	156	173.90	31573		
105.65	127	129.60	63	174.85	2564		

Instrument :

MSVOA_N

ClientSampleId :

BFB