


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN101319\
Data File : VN058693.D
Acq On : 11 Oct 2019 11:09
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101319W.M
Title : SW846 8260
Last Update : Sat Oct 12 00:00:30 2019

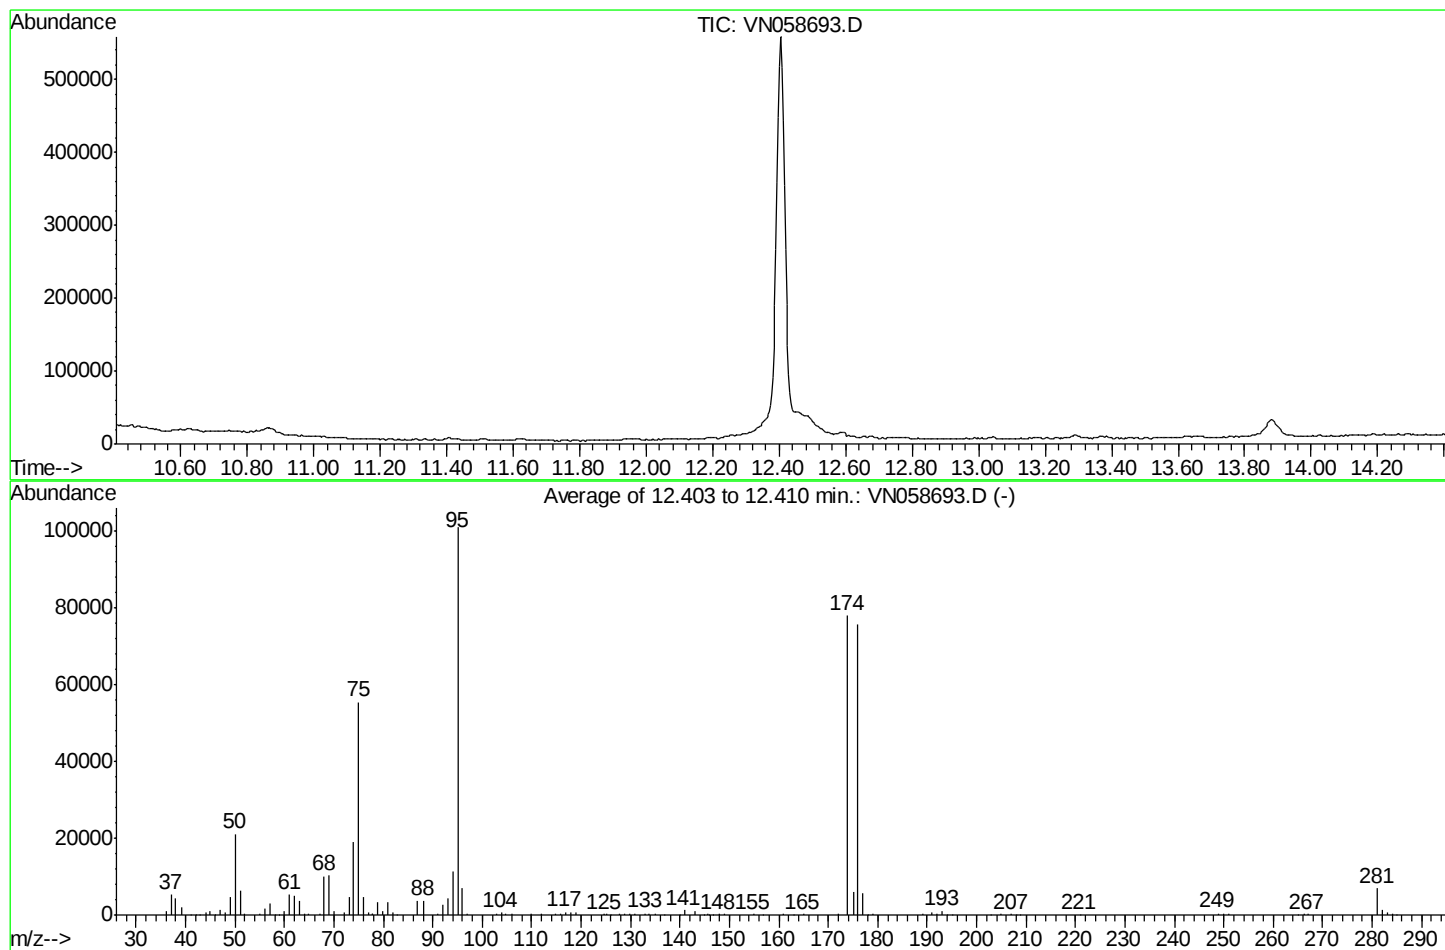

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	21010	PASS
75	95	30	60	54.9	55408	PASS
95	95	100	100	100.0	100930	PASS
96	95	5	9	7.0	7090	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	77.3	77978	PASS
175	174	5	9	7.8	6114	PASS
176	174	95	101	96.9	75545	PASS
177	176	5	9	7.4	5595	PASS