

Data File : VN064108.D  
Acq On : 13 Oct 2020 17:58  
Operator : JC/MD  
Sample : PB132303TB  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
PB132303TB

Quant Time: Oct 14 03:02:12 2020  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N093020W.M  
Quant Title : SW846 8260  
QLast Update : Thu Oct 01 01:46:38 2020  
Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|----------------------------|-------|------|----------|-------|-------|----------|
| 1) Pentafluorobenzene      | 7.63  | 168  | 216188   | 50.00 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.55  | 114  | 402667   | 50.00 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.38 | 117  | 435160   | 50.00 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.32 | 152  | 156684   | 50.00 | ug/l  | 0.00     |

#### System Monitoring Compounds

|                           |        |     |          |       |         |      |
|---------------------------|--------|-----|----------|-------|---------|------|
| 33) 1,2-Dichloroethane-d4 | 7.99   | 65  | 182950   | 51.22 | ug/l    | 0.00 |
| Spiked Amount             | 50.000 |     | Recovery | =     | 102.44% |      |
| 35) Dibromofluoromethane  | 7.55   | 113 | 138419   | 49.54 | ug/l    | 0.00 |
| Spiked Amount             | 50.000 |     | Recovery | =     | 99.08%  |      |
| 50) Toluene-d8            | 10.06  | 98  | 542924   | 51.26 | ug/l    | 0.00 |
| Spiked Amount             | 50.000 |     | Recovery | =     | 102.52% |      |
| 62) 4-Bromofluorobenzene  | 12.38  | 95  | 205289   | 51.56 | ug/l    | 0.00 |
| Spiked Amount             | 50.000 |     | Recovery | =     | 103.12% |      |

#### Target Compounds


|                                |       |     |        |        |        | Qvalue |
|--------------------------------|-------|-----|--------|--------|--------|--------|
| 16) Acetone                    | 3.78  | 43  | 10554  | 9.599  | ug/l   | 97     |
| 17) Carbon Disulfide           | 4.01  | 76  | 106    | 0.718  | ug/l # | 76     |
| 18) Methyl Acetate             | 4.29  | 43  | 3119   | 1.093  | ug/l   | 92     |
| 20) Methylene Chloride         | 4.51  | 84  | 7781   | 3.182  | ug/l   | 92     |
| 25) 2-Butanone                 | 6.80  | 43  | 1065   | 0.683  | ug/l # | 51     |
| 29) Tetrahydrofuran            | 7.18  | 42  | 359    | 0.343  | ug/l # | 36     |
| 31) Cyclohexane                | 7.63  | 56  | 5662   | 1.366  | ug/l # | 1      |
| 36) 1,1-Dichloropropene        | 7.62  | 75  | 19493  | 4.778  | ug/l # | 50     |
| 38) Carbon Tetrachloride       | 7.63  | 117 | 23773  | 5.197  | ug/l # | 14     |
| 43) Isopropyl Acetate          | 8.13  | 43  | 88901  | 13.298 | ug/l   | 99     |
| 45) 1,2-Dichloropropane        | 9.23  | 63  | 1746   | 0.555  | ug/l # | 44     |
| 48) Methyl methacrylate        | 9.15  | 41  | 4860   | 1.471  | ug/l # | 12     |
| 51) 4-Methyl-2-Pentanone       | 9.96  | 43  | 6755   | 1.722  | ug/l   | 88     |
| 54) cis-1,3-Dichloropropene    | 9.87  | 75  | 35051  | 6.988  | ug/l # | 60     |
| 57) 1,3-Dichloropropane        | 10.73 | 76  | 5884   | 1.203  | ug/l # | 43     |
| 59) 2-Hexanone                 | 10.74 | 43  | 101033 | 34.667 | ug/l # | 53     |
| 71) Bromoform                  | 12.38 | 173 | 1813   | 0.693  | ug/l # | 1      |
| 74) N-amyl acetate             | 12.01 | 43  | 1478   | 2.482  | ug/l # | 56     |
| 76) 1,2,3-Trichloropropane     | 12.38 | 75  | 108655 | 31.458 | ug/l # | 100    |
| 80) 1,3,5-Trimethylbenzene     | 12.71 | 105 | 7717   | 0.805  | ug/l   | 99     |
| 81) trans-1,4-Dichloro-2-buten | 12.38 | 75  | 108655 | 90.605 | ug/l # | 6      |
| 95) Naphthalene                | 15.11 | 128 | 186    | 1.946  | ug/l # | 69     |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VN064108.D  
Acq On : 13 Oct 2020 17:58  
Operator : JC/MD  
Sample : PB132303TB  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
Client Sample ID :  
PB132303TB

Quant Time: Oct 14 03:02:12 2020  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N093020W.M  
Quant Title : SW846 8260  
QLast Update : Thu Oct 01 01:46:38 2020  
Response via : Initial Calibration





#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN064108.D

Acq: 13 Oct 2020 17:58

Instrument :

MSVOA\_N

ClientSampleId :


PB132303TB

Tgt Ion: 168 Resp: 216188

Ion Ratio Lower Upper

168 100

99 64.9 51.8 77.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.63

100000

80000



60000

40000

20000

0

Time-->



#16

Acetone

Concen: 9.599 ug/l

RT: 3.78 min Scan# 634

Delta R.T. 0.01 min

Lab File: VN064108.D


Acq: 13 Oct 2020 17:58

Tgt Ion: 43 Resp: 10554

Ion Ratio Lower Upper

43 100

58 26.3 22.3 33.5



Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 58.00 (57.70 to 58.70): VNO

3.78

4000


3000


2000

1000

0

Time-->





#17

Carbon Disulfide

Concen: 0.718 ug/l

RT: 4.01 min Scan# 705

Delta R.T. -0.01 min

Lab File: VN064108.D

Acq: 13 Oct 2020 17:58

Instrument :

MSVOA\_N

ClientSampleId :


PB132303TB

Tgt Ion: 76 Resp: 106

Ion Ratio Lower Upper

76 100

78 0.0 7.0 10.4#



Abundance Ion 75.90 (75.60 to 76.60): VN0

Ion 77.90 (77.60 to 78.60): VN0

4.01



150

100

50

0

Time-->



#18

Methyl Acetate

Concen: 1.093 ug/l

RT: 4.29 min Scan# 792

Delta R.T. 0.01 min

Lab File: VN064108.D


Acq: 13 Oct 2020 17:58

Tgt Ion: 43 Resp: 3119

Ion Ratio Lower Upper

43 100

74 18.0 17.4 26.2



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 74.00 (73.70 to 74.70): VN0

4.29


1500


1000

500

0

Time-->







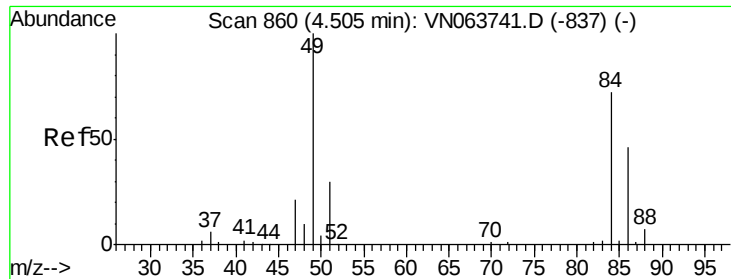

#20  
Methylene Chloride  
Concen: 3.182 ug/l  
RT: 4.51 min Scan# 861  
Delta R.T. 0.00 min  
Lab File: VN064108.D  
Acq: 13 Oct 2020 17:58




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB132303TB


Tgt Ion: 84 Resp: 7781  
Ion Ratio Lower Upper  
84 100  
49 127.7 110.4 165.6  
51 41.1 33.3 49.9  
86 72.6 50.7 76.1



#25  
2-Butanone  
Concen: 0.683 ug/l  
RT: 6.80 min Scan# 1575  
Delta R.T. 0.02 min  
Lab File: VN064108.D  
Acq: 13 Oct 2020 17:58

Tgt Ion: 43 Resp: 1065  
Ion Ratio Lower Upper  
43 100  
72 0.0 19.3 28.9#









#29  
Tetrahydrofuran  
Concen: 0.343 ug/l  
RT: 7.18 min Scan# 1691  
Delta R.T. 0.01 min  
Lab File: VN064108.D  
Acq: 13 Oct 2020 17:58




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB132303TB


Tgt Ion: 42 Resp: 359  
Ion Ratio Lower Upper  
42 100  
72 0.0 32.8 49.2#  
71 0.0 30.6 45.8#



#31  
Cyclohexane  
Concen: 1.366 ug/l  
RT: 7.63 min Scan# 1831  
Delta R.T. 0.01 min  
Lab File: VN064108.D  
Acq: 13 Oct 2020 17:58

Tgt Ion: 56 Resp: 5662  
Ion Ratio Lower Upper  
56 100  
69 180.6 25.4 38.2#  
84 136.1 63.3 94.9#









#33  
 1,2-Dichloroethane-d4  
 Concen: 51.224 ug/l  
 RT: 7.99 min Scan# 1943  
 Delta R.T. 0.00 min  
 Lab File: VN064108.D  
 Acq: 13 Oct 2020 17:58




Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 PB132303TB


Tgt Ion: 65 Resp: 182950  
 Ion Ratio Lower Upper  
 65 100  
 67 50.5 0.0 99.6



#34  
 1,4-Difluorobenzene  
 Concen: 50.000 ug/l  
 RT: 8.55 min Scan# 2118  
 Delta R.T. 0.00 min  
 Lab File: VN064108.D  
 Acq: 13 Oct 2020 17:58

Tgt Ion: 114 Resp: 402667  
 Ion Ratio Lower Upper  
 114 100  
 63 23.8 0.0 45.0  
 88 16.4 0.0 34.0









#35  
Dibromofluoromethane  
Concen: 49.541 ug/l  
RT: 7.55 min Scan# 1806  
Delta R.T. -0.00 min  
Lab File: VN064108.D  
Acq: 13 Oct 2020 17:58

Instrument :  
MSVOA\_N  
ClientSampleId :  
PB132303TB

Tgt Ion:113 Resp: 138419  
Ion Ratio Lower Upper  
113 100  
111 100.1 81.8 122.8  
192 18.1 14.2 21.2




Abundance Ion 112.80 (112.50 to 113.50): V  
Ion 110.80 (110.50 to 111.50): V  
Ion 191.70 (191.40 to 192.40): V






#36  
1,1-Dichloropropene  
Concen: 4.778 ug/l  
RT: 7.62 min Scan# 1830  
Delta R.T. -0.13 min  
Lab File: VN064108.D  
Acq: 13 Oct 2020 17:58

Tgt Ion: 75 Resp: 19493  
Ion Ratio Lower Upper  
75 100  
110 8.3 16.9 50.6#  
77 0.0 24.5 36.7#



Abundance Ion 74.90 (74.60 to 75.60): V  
Ion 109.90 (109.60 to 110.60): V  
Ion 76.90 (76.60 to 77.60): V









#38  
Carbon Tetrachloride  
Concen: 5.197 ug/l  
RT: 7.63 min Scan# 1832  
Delta R.T. -0.10 min  
Lab File: VN064108.D  
Acq: 13 Oct 2020 17:58

Instrument :  
MSVOA\_N  
ClientSampled :  
PB132303TB

Tgt Ion:117 Resp: 23773  
Ion Ratio Lower Upper  
117 100  
119 5.3 80.1 120.1#  
121 0.0 25.7 38.5#




Abundance Ion 116.80 (116.50 to 117.50): V  
Ion 118.80 (118.50 to 119.50): V  
Ion 120.80 (120.50 to 121.50): V






#43  
Isopropyl Acetate  
Concen: 13.298 ug/l  
RT: 8.13 min Scan# 1987  
Delta R.T. 0.00 min  
Lab File: VN064108.D  
Acq: 13 Oct 2020 17:58

Tgt Ion: 43 Resp: 88901  
Ion Ratio Lower Upper  
43 100  
61 17.5 14.2 21.4  
87 10.9 9.0 13.6



Abundance Ion 43.00 (42.70 to 43.70): VNO  
Ion 61.00 (60.70 to 61.70): VNO  
Ion 87.00 (86.70 to 87.70): VNO









#45  
 1,2-Dichloropropane  
 Concen: 0.555 ug/l  
 RT: 9.23 min Scan# 2331  
 Delta R.T. 0.15 min  
 Lab File: VN064108.D  
 Acq: 13 Oct 2020 17:58




Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 PB132303TB


Tgt Ion: 63 Resp: 1746  
 Ion Ratio Lower Upper  
 63 100  
 65 0.0 24.7 37.1#



#48  
 Methyl methacrylate  
 Concen: 1.471 ug/l  
 RT: 9.15 min Scan# 2304  
 Delta R.T. -0.02 min  
 Lab File: VN064108.D  
 Acq: 13 Oct 2020 17:58

Tgt Ion: 41 Resp: 4860  
 Ion Ratio Lower Upper  
 41 100  
 69 0.0 60.9 91.3#  
 39 0.0 57.5 86.3#





#50

Toluene-d8

Concen: 51.259 ug/l

RT: 10.06 min Scan# 2588

Delta R.T. 0.00 min

Lab File: VN064108.D

Acq: 13 Oct 2020 17:58

Instrument :

MSVOA\_N

ClientSampled :


PB132303TB

Tgt Ion: 98 Resp: 542924




Ion Ratio Lower Upper

98 100

100 63.2 49.8 74.6



Abundance Ion 98.00 (97.70 to 98.70): VN063741.D (-2571) (-)



#51

4-Methyl-2-Pentanone

Concen: 1.722 ug/l

RT: 9.96 min Scan# 2555

Delta R.T. 0.00 min

Lab File: VN064108.D


Acq: 13 Oct 2020 17:58

Tgt Ion: 43 Resp: 6755



Ion Ratio Lower Upper


43 100

58 42.3 28.4 42.6



Abundance Ion 43.00 (42.70 to 43.70): VN063741.D (-2537) (-)









#54

cis-1,3-Dichloropropene  
 Concen: 6.988 ug/l  
 RT: 9.87 min Scan# 2530  
 Delta R.T. 0.07 min  
 Lab File: VN064108.D  
 Acq: 13 Oct 2020 17:58

Instrument :  
 MSVOA\_N  
 ClientSampled :  
 PB132303TB




Tgt Ion: 75 Resp: 35051  
 Ion Ratio Lower Upper  
 75 100  
 77 0.0 24.6 36.8#  
 39 36.9 49.7 74.5#




#57

1,3-Dichloropropane  
 Concen: 1.203 ug/l  
 RT: 10.73 min Scan# 2797  
 Delta R.T. 0.05 min  
 Lab File: VN064108.D  
 Acq: 13 Oct 2020 17:58

Tgt Ion: 76 Resp: 5884  
 Ion Ratio Lower Upper  
 76 100  
 78 0.0 25.2 37.8#









#59  
2-Hexanone  
Concen: 34.667 ug/l  
RT: 10.74 min Scan# 2798  
Delta R.T. 0.02 min  
Lab File: VN064108.D  
Acq: 13 Oct 2020 17:58




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB132303TB


Tgt Ion: 43 Resp: 101033  
Ion Ratio Lower Upper  
43 100  
58 17.2 24.6 73.8#



#62  
4-Bromofluorobenzene  
Concen: 51.560 ug/l  
RT: 12.38 min Scan# 3308  
Delta R.T. 0.00 min  
Lab File: VN064108.D  
Acq: 13 Oct 2020 17:58

Tgt Ion: 95 Resp: 205289  
Ion Ratio Lower Upper  
95 100  
174 75.2 0.0 150.6  
176 71.7 0.0 145.4









#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.38 min Scan# 2998  
Delta R.T. 0.00 min  
Lab File: VN064108.D  
Acq: 13 Oct 2020 17:58




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB132303TB


Tgt Ion:117 Resp: 435160  
Ion Ratio Lower Upper  
117 100  
82 58.8 47.4 71.2  
119 31.5 26.4 39.6



#71  
Bromoform  
Concen: 0.693 ug/l  
RT: 12.38 min Scan# 3309  
Delta R.T. 0.28 min  
Lab File: VN064108.D  
Acq: 13 Oct 2020 17:58

Tgt Ion:173 Resp: 1813  
Ion Ratio Lower Upper  
173 100  
175 507.0 23.5 70.5#  
254 0.0 0.0 0.0





#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3601

Delta R.T. 0.00 min

Lab File: VN064108.D

Acq: 13 Oct 2020 17:58

Instrument :

MSVOA\_N

ClientSampleId :

PB132303TB


Tgt Ion:152 Resp: 156684

Ion Ratio Lower Upper

152 100

115 64.2 31.3 93.8




150 160.3 0.0 341.8



Abundance Ion 151.90 (151.60 to 152.60): V

200000 Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V



#74

N-ethyl acetate

Concen: 2.482 ug/l

RT: 12.01 min Scan# 3194

Delta R.T. -0.03 min

Lab File: VN064108.D

Acq: 13 Oct 2020 17:58

Tgt Ion: 43 Resp: 1478


Ion Ratio Lower Upper

43 100

70 0.0 29.8 44.8#

55 16.2 17.9 26.9#

61 0.0 17.0 25.4#






Abundance Ion 43.00 (42.70 to 43.70): V

2500 Ion 70.00 (69.70 to 70.70): V

Ion 55.00 (54.70 to 55.70): V

Ion 61.00 (60.70 to 61.70): V





#76

1,2,3-Trichloropropane

Concen: 31.458 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. -0.15 min

Lab File: VN064108.D

Acq: 13 Oct 2020 17:58

Instrument :

MSVOA\_N

ClientSampled :


PB132303TB

Tgt Ion: 75 Resp: 108655

Ion Ratio Lower Upper




75 100

77 1.1 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0



#80

1,3,5-Trimethylbenzene

Concen: 0.805 ug/l

RT: 12.71 min Scan# 3411

Delta R.T. 0.00 min

Lab File: VN064108.D


Acq: 13 Oct 2020 17:58

Tgt Ion: 105 Resp: 7717

Ion Ratio Lower Upper



105 100


120 47.1 23.3 69.9



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V





#81

trans-1,4-Dichloro-2-butene

Concen: 90.605 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.10 min

Lab File: VN064108.D

Acq: 13 Oct 2020 17:58

Instrument :

MSVOA\_N

ClientSampled :

PB132303TB


Tgt Ion: 75 Resp: 108655

Ion Ratio Lower Upper

75 100

53 0.1 88.2 132.2#




89 0.1 36.0 54.0#



Abundance Ion 74.90 (74.60 to 75.60): VN063741.D (-3266) (-)

Ion 53.00 (52.70 to 53.70): VN063741.D (-3266) (-)

Ion 88.90 (88.60 to 89.60): VN063741.D (-3266) (-)



#95

Naphthalene

Concen: 1.946 ug/l

RT: 15.11 min Scan# 4159

Delta R.T. 0.01 min

Lab File: VN064108.D

Acq: 13 Oct 2020 17:58


Tgt Ion: 128 Resp: 186

Ion Ratio Lower Upper

128 100

127 0.0 10.5 15.7#

129 0.0 8.7 13.1#



Abundance Ion 128.00 (127.70 to 128.70): VN063741.D (-4141) (-)

Ion 127.00 (126.70 to 127.70): VN063741.D (-4141) (-)

Ion 129.00 (128.70 to 129.70): VN063741.D (-4141) (-)

