


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN101320\
 Data File : VN064096.D
 Acq On : 13 Oct 2020 12:10
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N093020W.M
 Title : SW846 8260
 Last Update : Thu Oct 01 01:46:38 2020

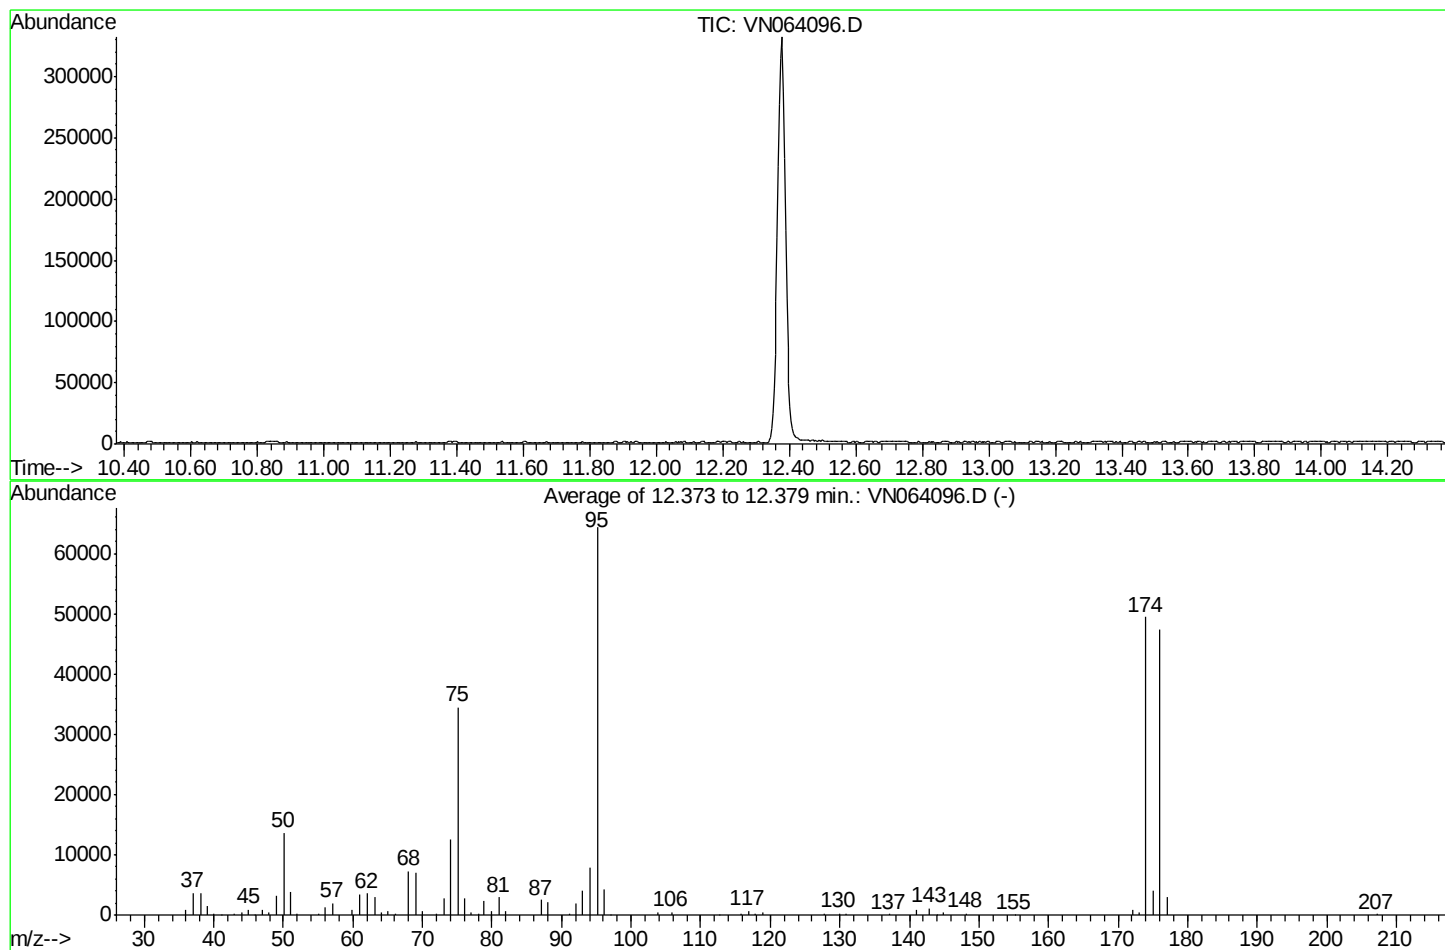

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	13695	PASS
75	95	30	60	53.6	34453	PASS
95	95	100	100	100.0	64330	PASS
96	95	5	9	6.7	4281	PASS
173	174	0.00	2	1.0	492	PASS
174	95	50	100	76.9	49474	PASS
175	174	5	9	8.2	4068	PASS
176	174	95	101	95.6	47277	PASS
177	176	5	9	6.5	3058	PASS