

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101321\
 Data File : VN068901.D
 Acq On : 13 Oct 2021 16:48
 Operator : JC/MD
 Sample : M4175-02
 Misc : 1.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 41173

Quant Time: Oct 14 06:43:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 13 05:44:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.080	168	419372	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.965	114	689730	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	602132	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	268717	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.432	65	253798	45.901	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	91.800%		
35) Dibromofluoromethane	8.019	113	203714	50.765	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	101.520%		
50) Toluene-d8	10.443	98	824255	51.335	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	102.680%		
62) 4-Bromofluorobenzene	12.733	95	289214	47.742	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	95.480%		
Target Compounds					Qvalue	
3) Chloromethane	2.295	50	1136	0.222	ug/l #	85
13) Acrolein	4.052	56	525	1.175	ug/l #	41
16) Acetone	4.315	43	5425	2.629	ug/l	89
18) Methyl Acetate	4.857	43	2566	0.328	ug/l #	41
20) Methylene Chloride	5.058	84	1347	0.284	ug/l	84
29) Tetrahydrofuran	7.702	42	2329	1.151	ug/l #	73
31) Cyclohexane	8.080	56	17973	2.091	ug/l #	40
36) 1,1-Dichloropropene	8.080	75	32773	5.563	ug/l #	50
38) Carbon Tetrachloride	8.080	117	41970	6.487	ug/l #	16
39) Methylcyclohexane	9.456	83	11247	1.483	ug/l	95
40) Benzene	8.453	78	3864	0.215	ug/l #	86
48) Methyl methacrylate	9.504	41	1397	0.277	ug/l #	29
52) Toluene	10.505	92	461838	40.014	ug/l	99
53) t-1,3-Dichloropropene	10.505	75	5585	0.749	ug/l #	1
55) 1,1,2-Trichloroethane	10.875	97	1415	0.311	ug/l #	28
67) Ethyl Benzene	11.846	91	33903	1.602	ug/l	94
68) m/p-Xylenes	11.953	106	46729	5.824	ug/l	100
69) o-Xylene	12.283	106	17213	2.143	ug/l	99
73) Isopropylbenzene	12.581	105	5025	0.225	ug/l	91
76) 1,2,3-Trichloropropane	12.733	75	148492	25.971	ug/l #	1
78) n-propylbenzene	12.921	91	18672	0.743	ug/l	96
79) 2-Chlorotoluene	12.986	91	4841	0.312	ug/l #	44
80) 1,3,5-Trimethylbenzene	13.063	105	18258	0.980	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.733	75	148492	62.135	ug/l #	12
83) tert-Butylbenzene	13.369	119	8614	0.531	ug/l #	62
84) 1,2,4-Trimethylbenzene	13.369	105	68229	3.801	ug/l	100
89) n-Butylbenzene	13.943	91	9594	0.640	ug/l #	73
90) Hexachloroethane	14.217	117	2613	0.690	ug/l #	12
93) 1,2,4-Trichlorobenzene	15.265	180	872	2.785	ug/l	90
95) Naphthalene	15.509	128	28734	5.940	ug/l #	91
96) 1,2,3-Trichlorobenzene	15.697	180	410	2.604	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101321\
Data File : VN068901.D
Acq On : 13 Oct 2021 16:48
Operator : JC/MD
Sample : M4175-02
Misc : 1.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
41173

Quant Time: Oct 14 06:43:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 13 05:44:40 2021
Response via : Initial Calibration




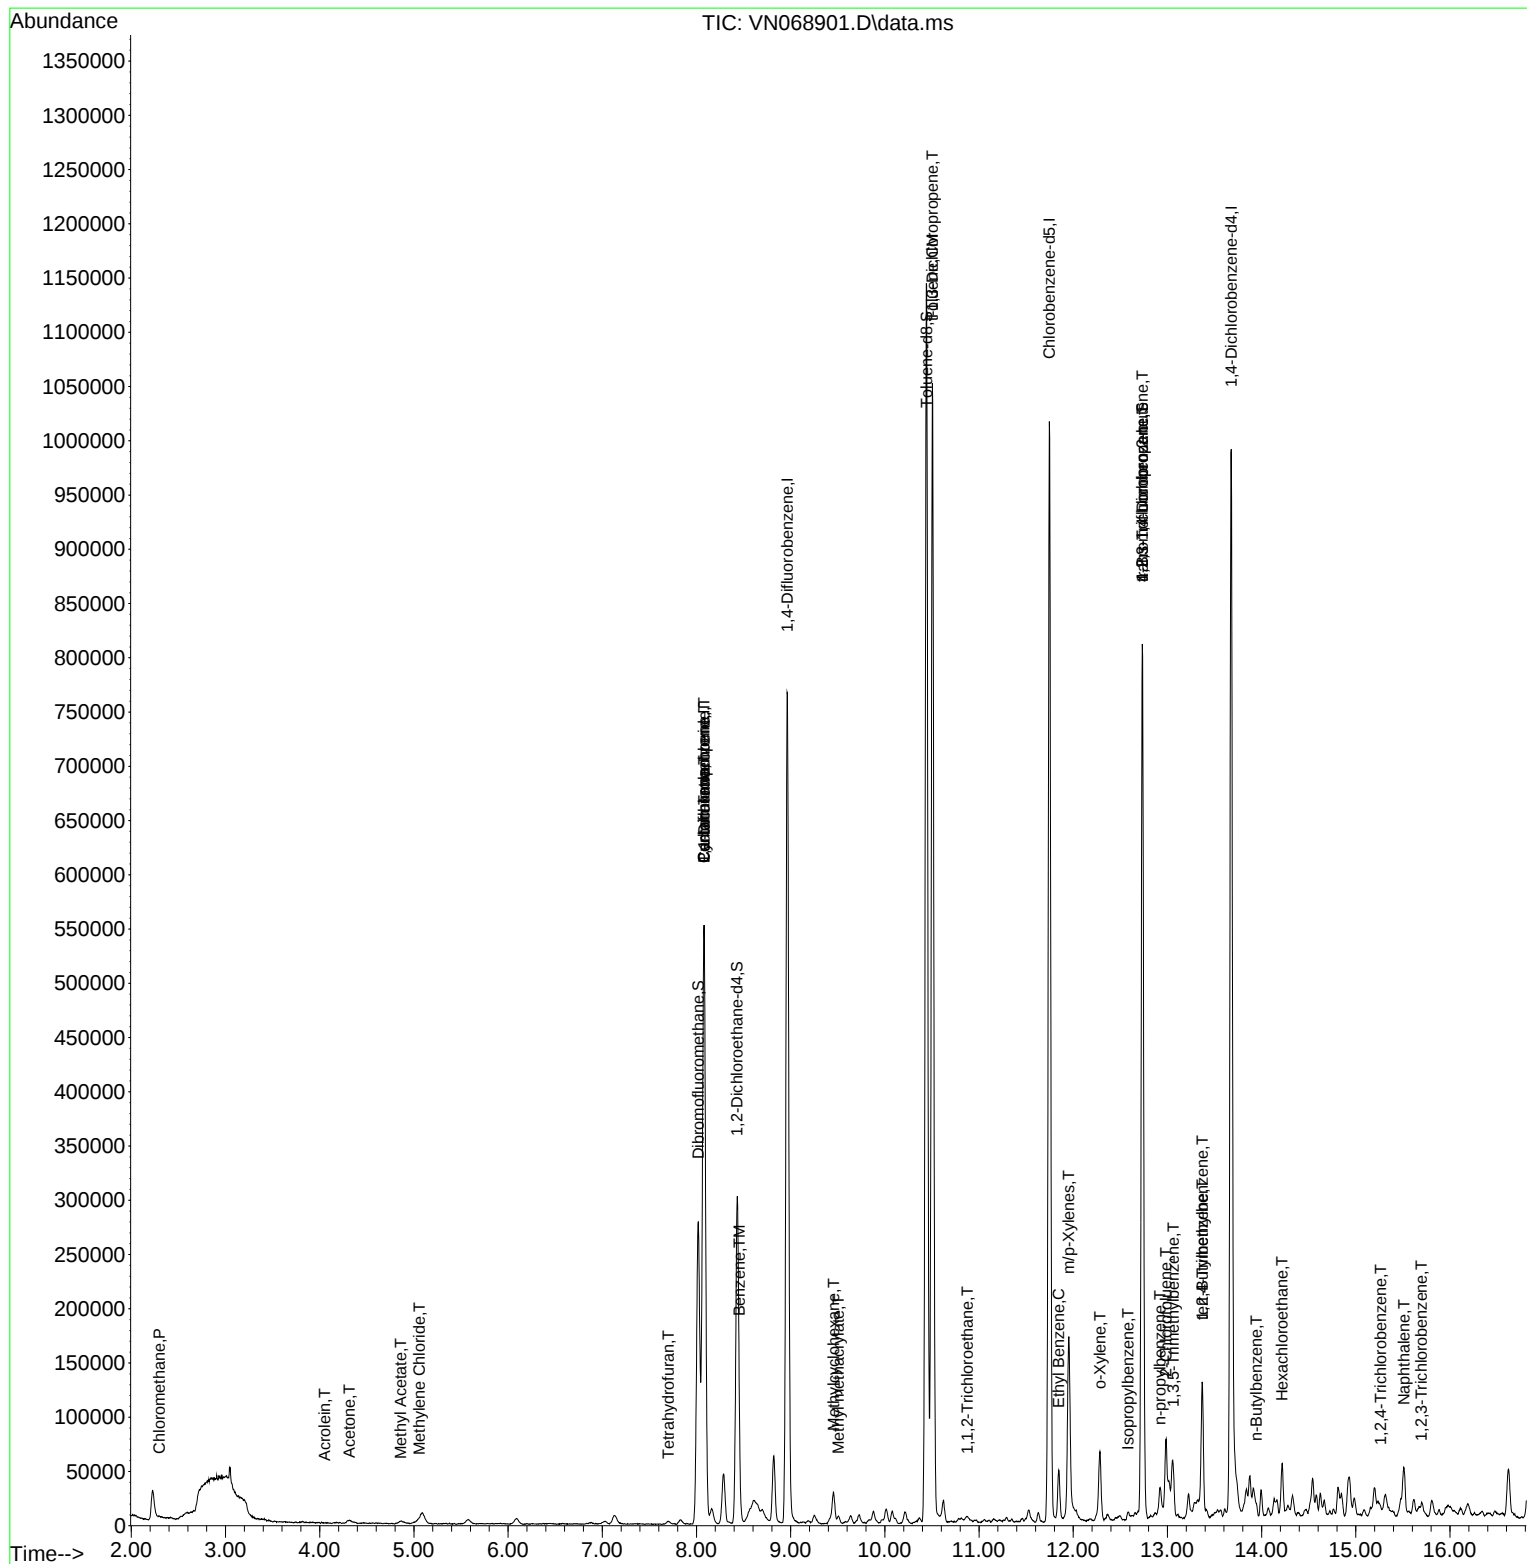




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.080 min Scan# 2271
Delta R.T. -0.006 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48




Instrument :
MSVOA_N
ClientSampled :
41173


Tgt Ion:168 Resp: 419372
Ion Ratio Lower Upper
168 100
99 59.0 48.9 73.3

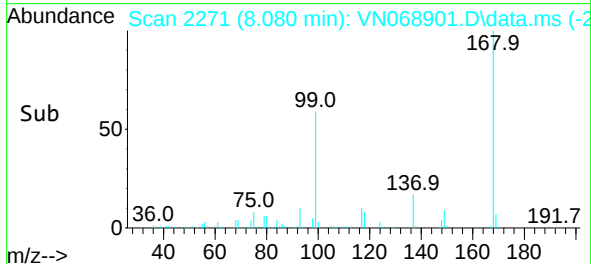

#3
Chloromethane
Concen: 0.222 ug/l
RT: 2.295 min Scan# 114
Delta R.T. -0.005 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48

Tgt Ion: 50 Resp: 1136
Ion Ratio Lower Upper
50 100
52 24.2 26.3 39.5#


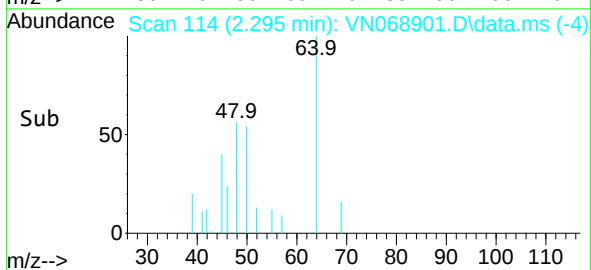

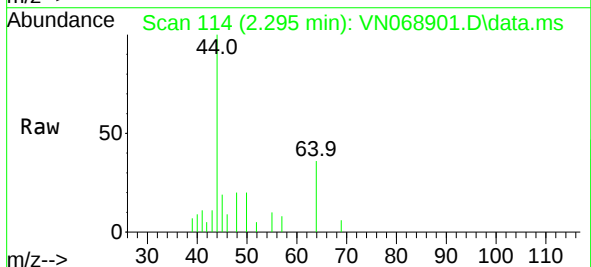




#13
Acrolein
Concen: 1.175 ug/l
RT: 4.052 min Scan# 769
Delta R.T. 0.011 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48




Instrument :
MSVOA_N
ClientSampleId :
41173


Tgt Ion: 56 Resp: 525
Ion Ratio Lower Upper
56 100
55 23.6 58.1 87.1#

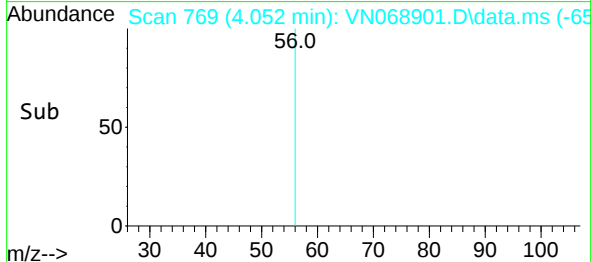

#16
Acetone
Concen: 2.629 ug/l
RT: 4.315 min Scan# 867
Delta R.T. 0.030 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48

Tgt Ion: 43 Resp: 5425
Ion Ratio Lower Upper
43 100
58 36.4 24.5 36.7


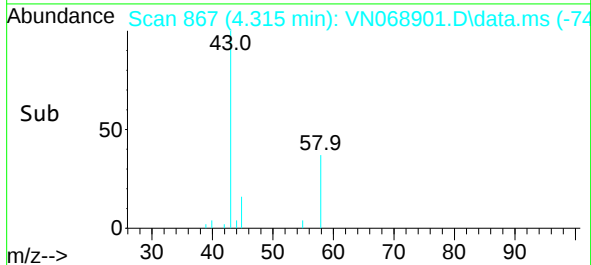

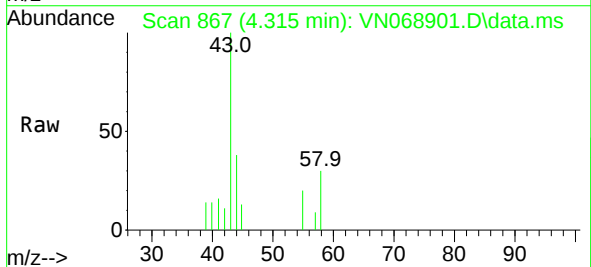


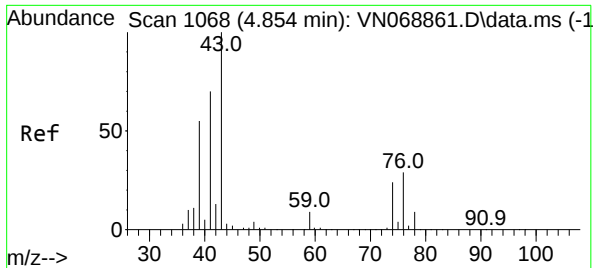

#18
Methyl Acetate
Concen: 0.328 ug/l
RT: 4.857 min Scan# 1069
Delta R.T. 0.003 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48




Instrument :
MSVOA_N
ClientSampled :
41173


Tgt Ion: 43 Resp: 2566
Ion Ratio Lower Upper
43 100
74 52.3 18.9 28.3#

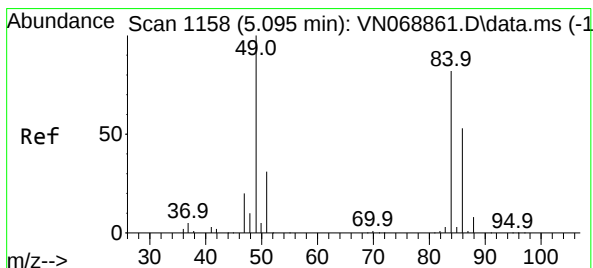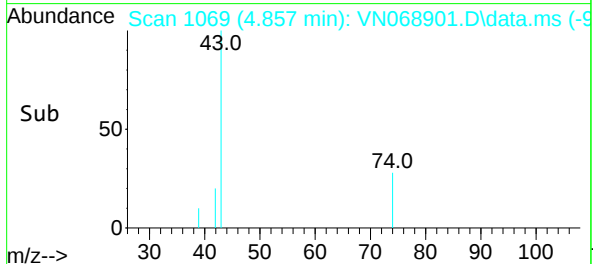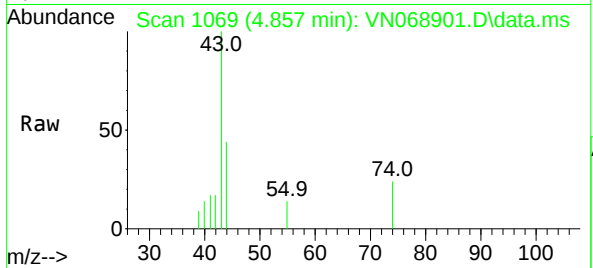

#20
Methylene Chloride
Concen: 0.284 ug/l
RT: 5.058 min Scan# 1144
Delta R.T. -0.038 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48

Tgt Ion: 84 Resp: 1347
Ion Ratio Lower Upper
84 100
49 98.7 97.6 146.4
51 33.7 30.3 45.5
86 55.0 51.8 77.6

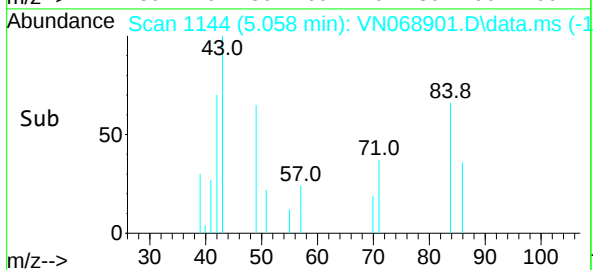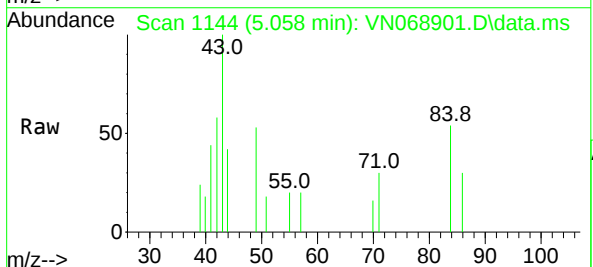



#29

Tetrahydrofuran

Concen: 1.151 ug/l

RT: 7.702 min Scan# 2130

Delta R.T. 0.019 min

Lab File: VN068901.D

Acq: 13 Oct 2021 16:48

Tgt Ion: 42 Resp: 2329

Ion Ratio Lower Upper

42 100

72 35.6 35.4 53.2





71 16.4 33.8 50.6#

Instrument :

MSVOA_N

ClientSampled :

41173



#31

Cyclohexane

Concen: 2.091 ug/l

RT: 8.080 min Scan# 2271

Delta R.T. -0.016 min

Lab File: VN068901.D

Acq: 13 Oct 2021 16:48




Tgt Ion: 56 Resp: 17973


Ion Ratio Lower Upper

56 100

69 121.4 26.9 40.3#

84 105.4 67.6 101.4#

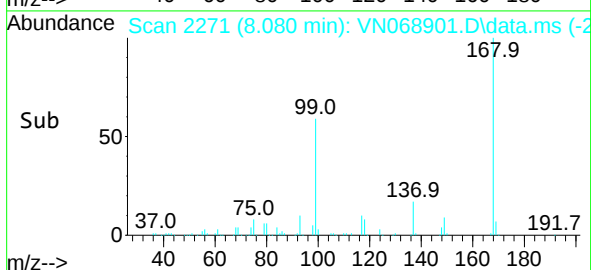







#33

1,2-Dichloroethane-d4
Concen: 45.901 ug/l
RT: 8.432 min Scan# 2402
Delta R.T. -0.008 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48

Instrument :
MSVOA_N
ClientSampleId :
41173




Tgt Ion: 65 Resp: 253798
Ion Ratio Lower Upper
65 100
67 52.2 0.0 103.8

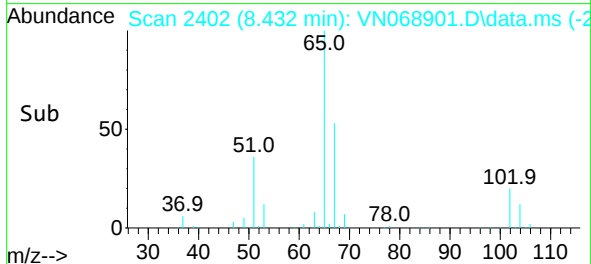


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.965 min Scan# 2601
Delta R.T. -0.003 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48

Tgt Ion: 114 Resp: 689730
Ion Ratio Lower Upper
114 100
63 20.6 0.0 42.6
88 16.1 0.0 32.0


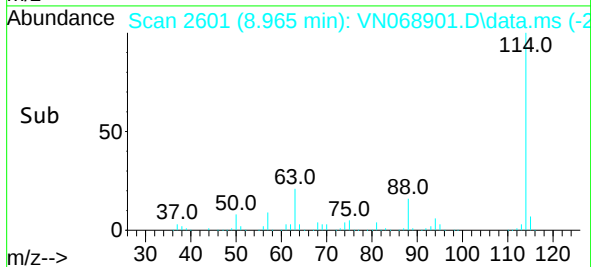

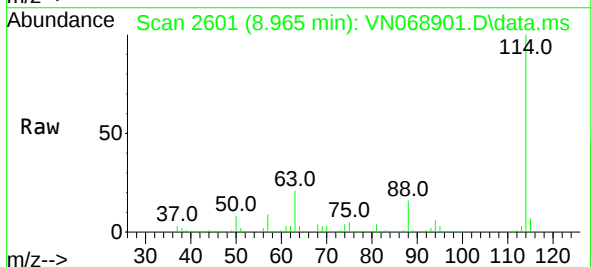




#35
Dibromofluoromethane
Concen: 50.765 ug/l
RT: 8.019 min Scan# 2248
Delta R.T. -0.003 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48




Instrument :
MSVOA_N
ClientSampled :
41173


Tgt Ion:113 Resp: 203714
Ion Ratio Lower Upper
113 100
111 103.5 83.2 124.8
192 19.4 15.0 22.4

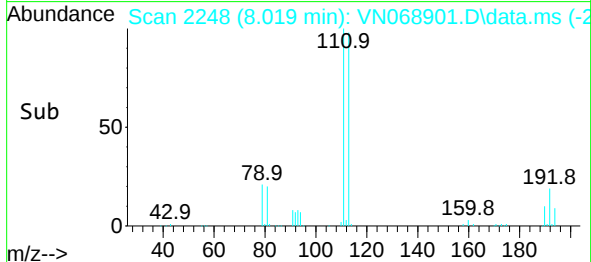

#36
1,1-Dichloropropene
Concen: 5.563 ug/l
RT: 8.080 min Scan# 2271
Delta R.T. -0.142 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48

Tgt Ion: 75 Resp: 32773
Ion Ratio Lower Upper
75 100
110 9.2 17.9 53.8#
77 0.0 24.7 37.1#


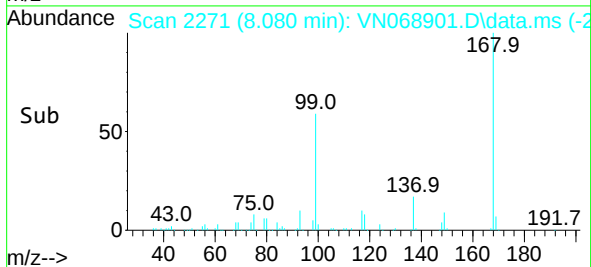

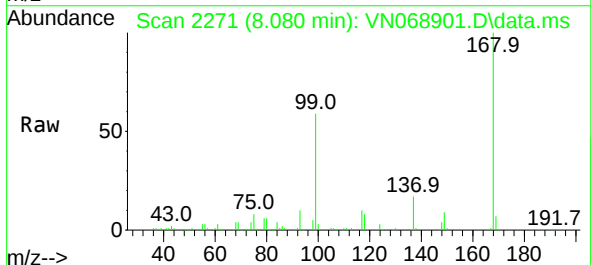




#38
Carbon Tetrachloride
Concen: 6.487 ug/l
RT: 8.080 min Scan# 2271
Delta R.T. -0.129 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48




Instrument :
MSVOA_N
ClientSampled :
41173


Tgt Ion:117 Resp: 41970
Ion Ratio Lower Upper
117 100
119 4.8 76.9 115.3#
121 0.0 24.6 37.0#

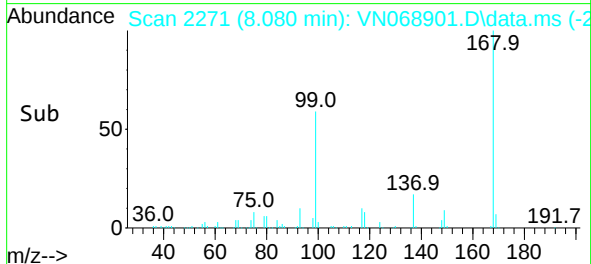

#39
Methylcyclohexane
Concen: 1.483 ug/l
RT: 9.456 min Scan# 2784
Delta R.T. -0.005 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48

Tgt Ion: 83 Resp: 11247
Ion Ratio Lower Upper
83 100
55 70.5 61.4 92.0
98 44.8 36.4 54.6


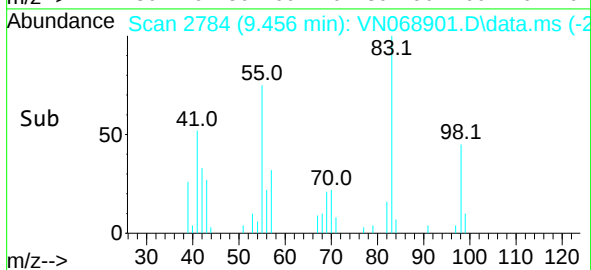

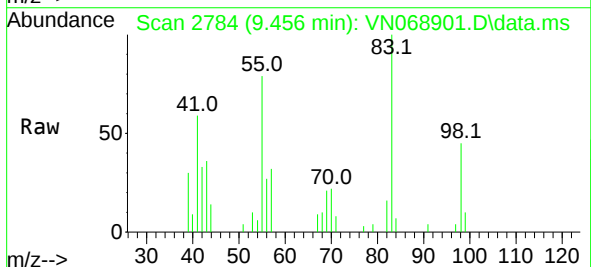




#40
Benzene
Concen: 0.215 ug/l
RT: 8.453 min Scan# 2410
Delta R.T. -0.008 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48




Instrument :
MSVOA_N
ClientSampled :
41173


Tgt Ion: 78 Resp: 3864
Ion Ratio Lower Upper
78 100
77 30.9 19.1 28.7#

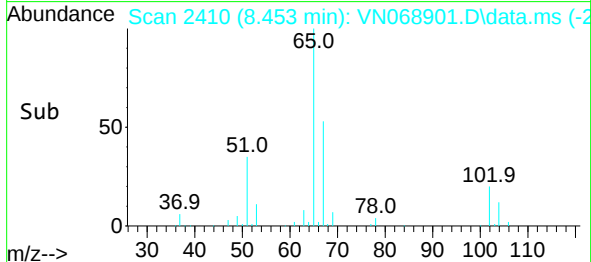

#48
Methyl methacrylate
Concen: 0.277 ug/l
RT: 9.504 min Scan# 2802
Delta R.T. -0.056 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48

Tgt Ion: 41 Resp: 1397
Ion Ratio Lower Upper
41 100
69 0.0 66.4 99.6#
39 29.3 50.2 75.2#


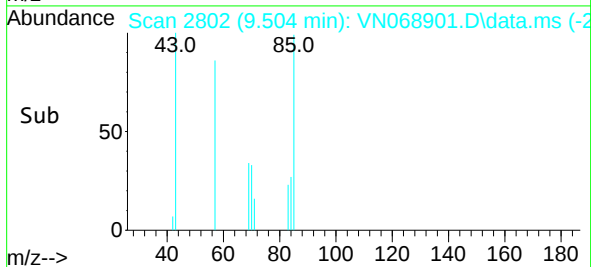

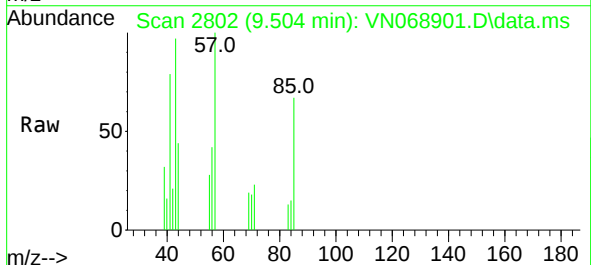




#50
Toluene-d8
Concen: 51.335 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48




Instrument :
MSVOA_N
ClientSampleId :
41173


Tgt Ion: 98 Resp: 824255
Ion Ratio Lower Upper
98 100
100 64.5 51.5 77.3

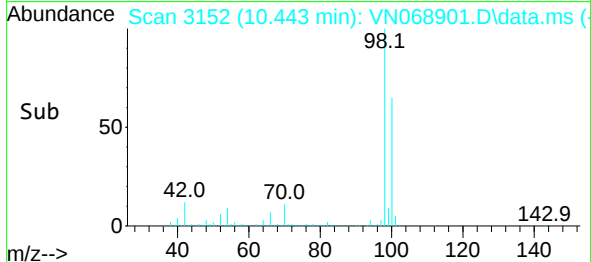

#52
Toluene
Concen: 40.014 ug/l
RT: 10.505 min Scan# 3175
Delta R.T. -0.003 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48

Tgt Ion: 92 Resp: 461838
Ion Ratio Lower Upper
92 100
91 174.0 138.5 207.7


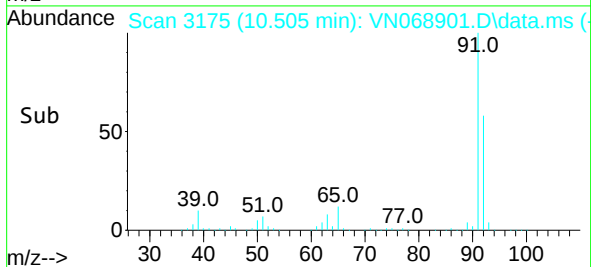

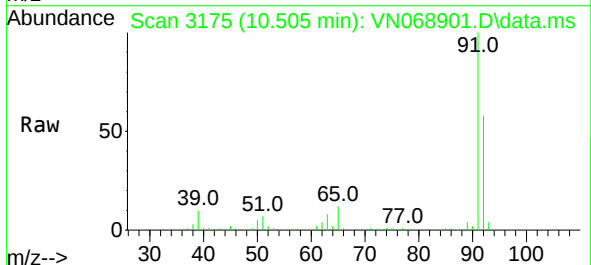




#53
t-1,3-Dichloropropene
Concen: 0.749 ug/l
RT: 10.505 min Scan# 3175
Delta R.T. -0.215 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48




Instrument :
MSVOA_N
ClientSampled :
41173


Tgt Ion: 75 Resp: 5585
Ion Ratio Lower Upper
75 100
77 141.4 25.4 38.2#

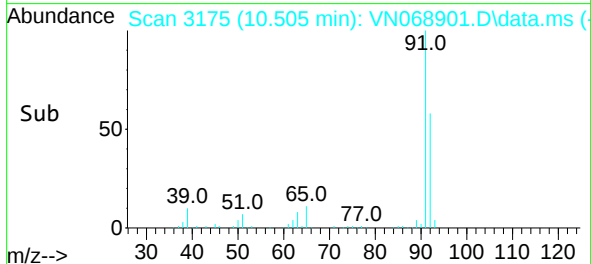

#55
1,1,2-Trichloroethane
Concen: 0.311 ug/l
RT: 10.875 min Scan# 3313
Delta R.T. -0.024 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48

Tgt Ion: 97 Resp: 1415
Ion Ratio Lower Upper
97 100
83 30.4 70.5 105.7#
85 0.0 45.3 67.9#
99 0.0 50.7 76.1#


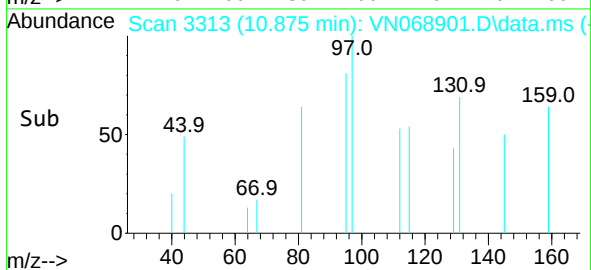

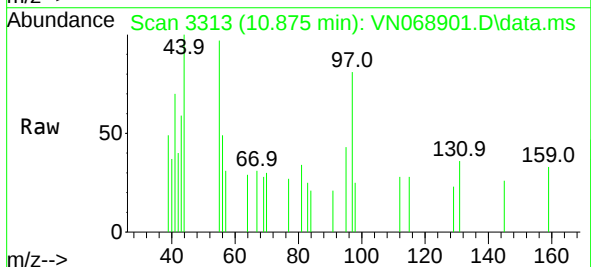




#62
4-Bromofluorobenzene
Concen: 47.742 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48




Instrument :
MSVOA_N
ClientSampleId :
41173


Tgt Ion: 95 Resp: 289214
Ion Ratio Lower Upper
95 100
174 76.6 0.0 144.8
176 73.5 0.0 140.0

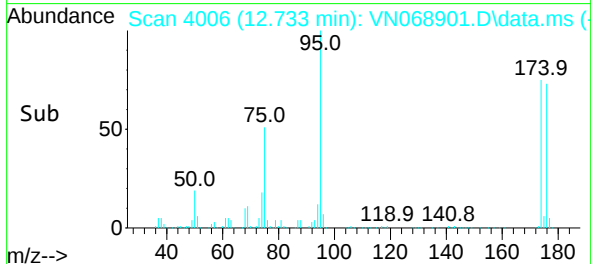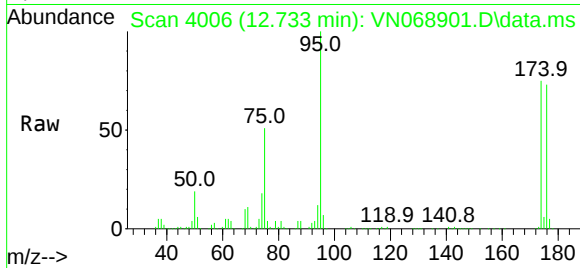

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48

Tgt Ion: 117 Resp: 602132
Ion Ratio Lower Upper
117 100
82 56.3 46.4 69.6
119 31.9 26.0 39.0


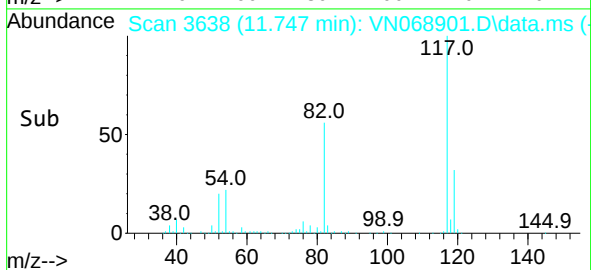

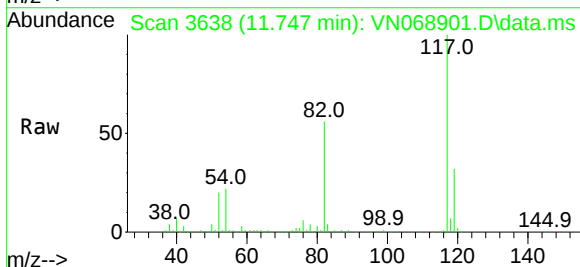


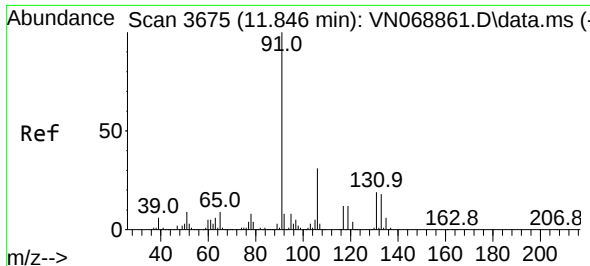

#67
Ethyl Benzene
Concen: 1.602 ug/l
RT: 11.846 min Scan# 3675
Delta R.T. 0.000 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48




Instrument :
MSVOA_N
ClientSampleId :
41173


Tgt Ion: 91 Resp: 33903
Ion Ratio Lower Upper
91 100
106 34.5 24.8 37.2

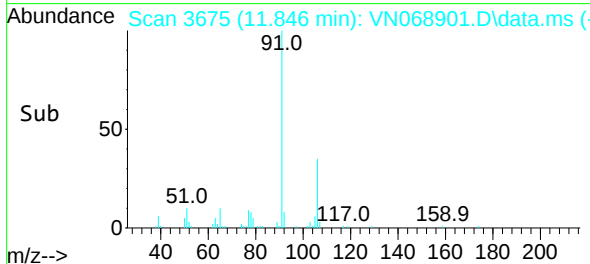

#68
m/p-Xylenes
Concen: 5.824 ug/l
RT: 11.953 min Scan# 3715
Delta R.T. 0.000 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48

Tgt Ion:106 Resp: 46729
Ion Ratio Lower Upper
106 100
91 208.8 166.8 250.2

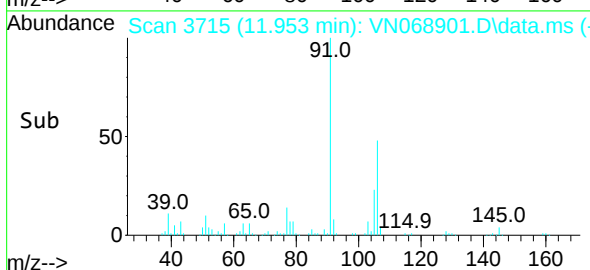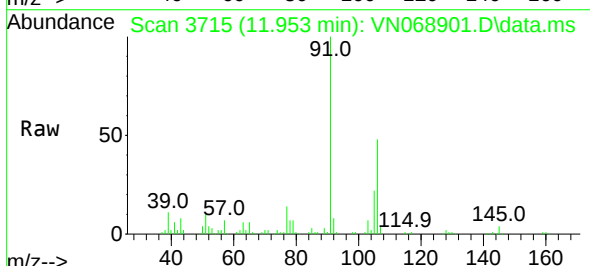



#69

o-Xylene

Concen: 2.143 ug/l

RT: 12.283 min Scan# 3838

Delta R.T. 0.000 min

Lab File: VN068901.D





Acq: 13 Oct 2021 16:48

Tgt Ion:106 Resp: 17213

Ion Ratio Lower Upper

106 100

91 218.0 109.6 328.6

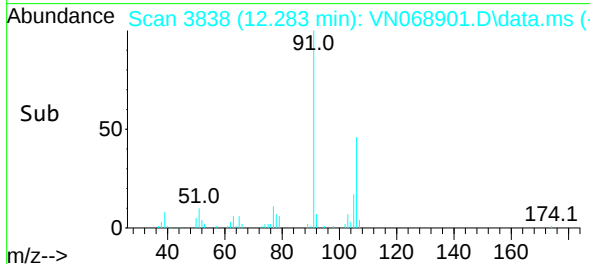

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.678 min Scan# 4358

Delta R.T. 0.003 min

Lab File: VN068901.D

Acq: 13 Oct 2021 16:48




Tgt Ion:152 Resp: 268717


Ion Ratio Lower Upper

152 100

115 63.5 31.4 94.3

150 156.4 0.0 351.0

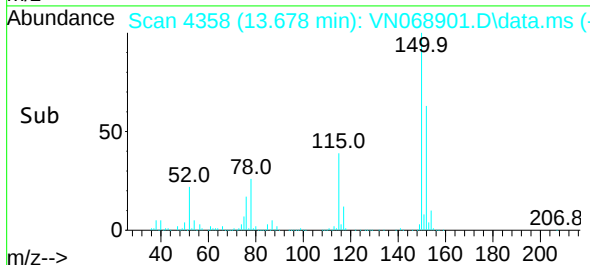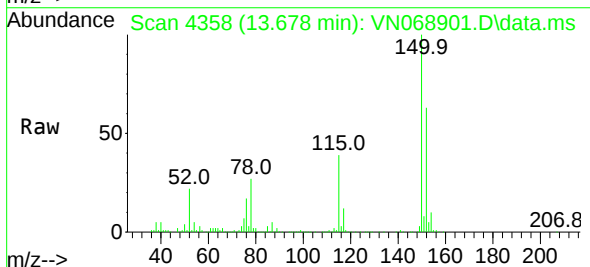



#73

Isopropylbenzene

Concen: 0.225 ug/l

RT: 12.581 min Scan# 3949

Delta R.T. 0.000 min

Lab File: VN068901.D





Acq: 13 Oct 2021 16:48

Tgt Ion:105 Resp: 5025

Ion Ratio Lower Upper

105 100

120 30.9 13.1 39.3

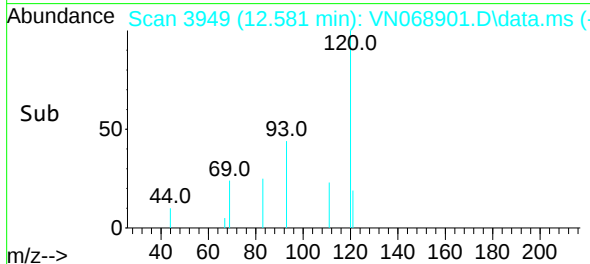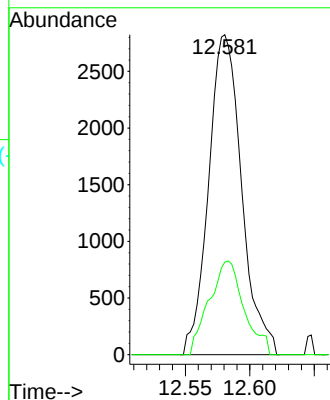

#76

1,2,3-Trichloropropane

Concen: 25.971 ug/l

RT: 12.733 min Scan# 4006

Delta R.T. -0.147 min

Lab File: VN068901.D




Acq: 13 Oct 2021 16:48


Tgt Ion: 75 Resp: 148492

Ion Ratio Lower Upper

75 100

77 1.3 96.2 288.4#


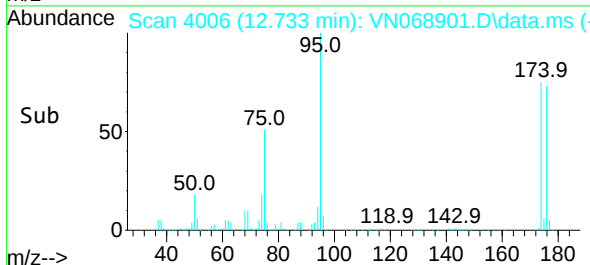
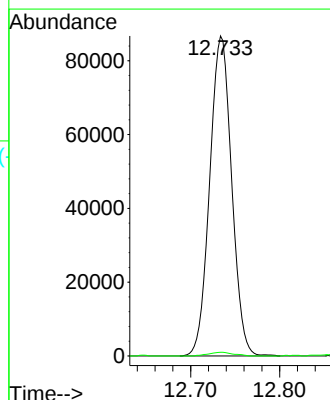
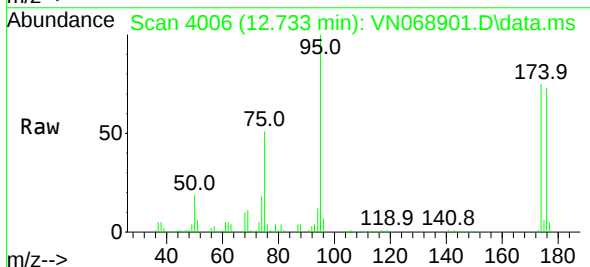




#78
n-propylbenzene
Concen: 0.743 ug/l
RT: 12.921 min Scan# 4076
Delta R.T. 0.000 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48




Instrument :
MSVOA_N
ClientSampled :
41173


Tgt Ion: 91 Resp: 18672
Ion Ratio Lower Upper
91 100
120 24.6 11.4 34.1

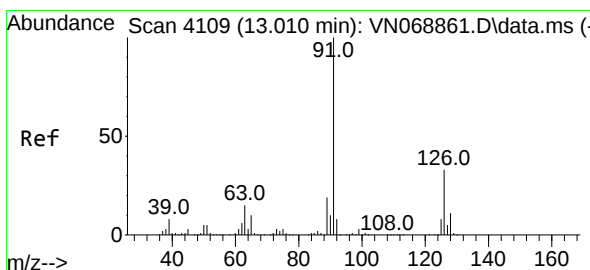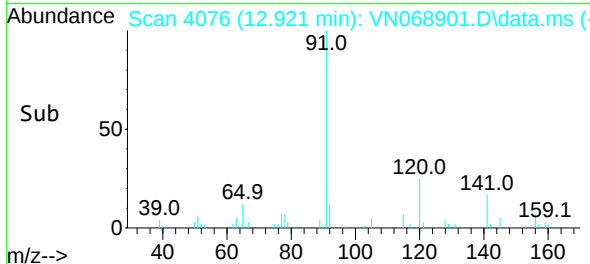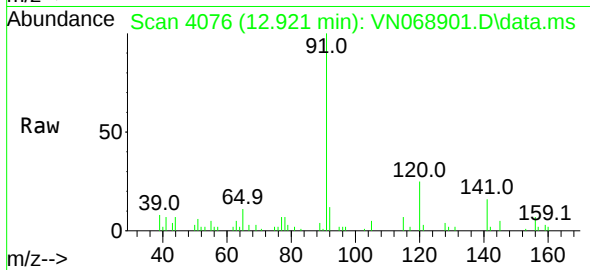

#79
2-Chlorotoluene
Concen: 0.312 ug/l
RT: 12.986 min Scan# 4100
Delta R.T. -0.024 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48

Tgt Ion: 91 Resp: 4841
Ion Ratio Lower Upper
91 100
126 1.0 16.4 49.4#


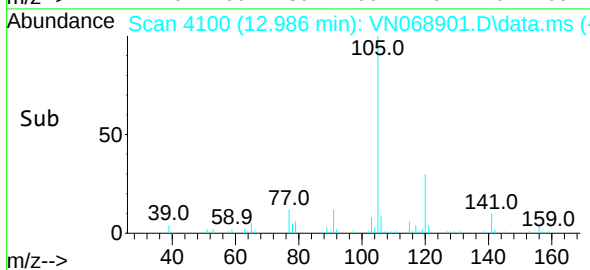

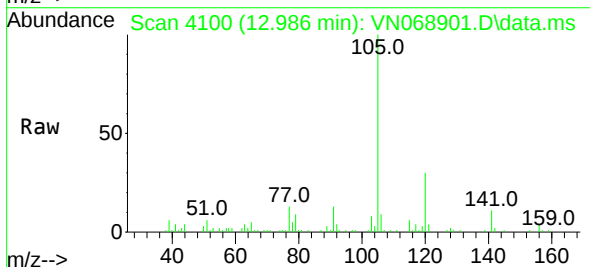




#80
1,3,5-Trimethylbenzene
Concen: 0.980 ug/l
RT: 13.063 min Scan# 4129
Delta R.T. 0.003 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48




Instrument :
MSVOA_N
ClientSampleId :
41173


Tgt Ion:105 Resp: 18258
Ion Ratio Lower Upper
105 100
120 45.0 23.4 70.2

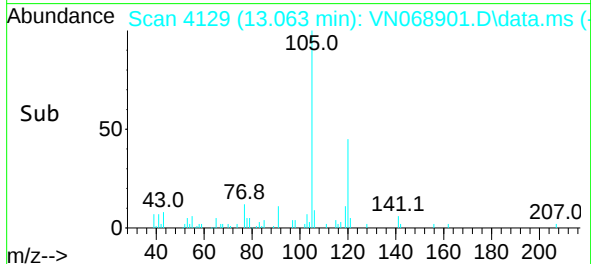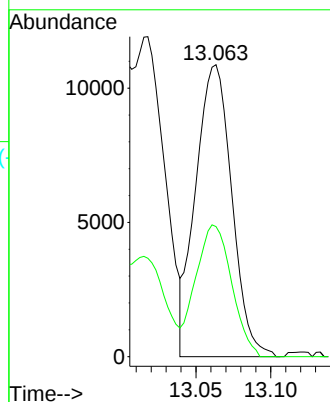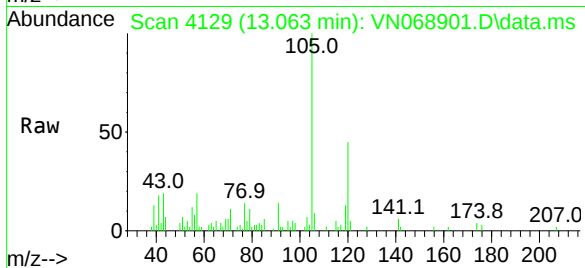

#81
trans-1,4-Dichloro-2-butene
Concen: 62.135 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.107 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48

Tgt Ion: 75 Resp: 148492
Ion Ratio Lower Upper
75 100
53 0.0 75.4 113.2#
89 0.0 36.9 55.3#


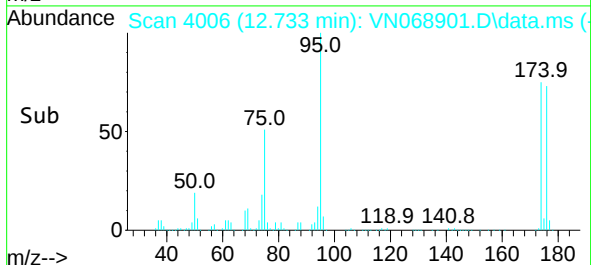
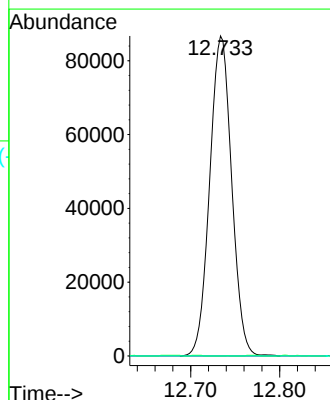
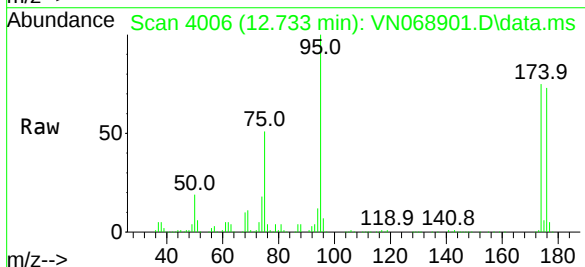




#83
tert-Butylbenzene
Concen: 0.531 ug/l
RT: 13.369 min Scan# 4243
Delta R.T. 0.043 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48




Instrument :
MSVOA_N
ClientSampled :
41173


Tgt Ion:119 Resp: 8614
Ion Ratio Lower Upper
119 100
91 96.6 34.6 103.9
134 0.0 12.6 37.6#

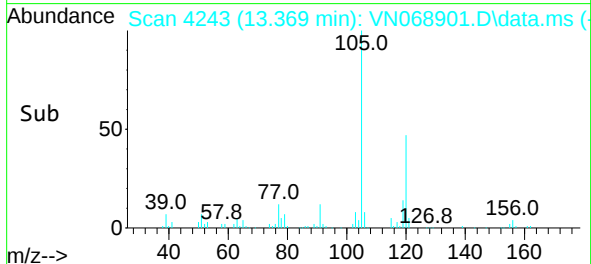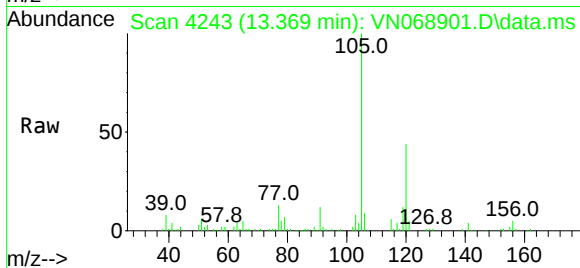

#84
1,2,4-Trimethylbenzene
Concen: 3.801 ug/l
RT: 13.369 min Scan# 4243
Delta R.T. 0.000 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48

Tgt Ion:105 Resp: 68229
Ion Ratio Lower Upper
105 100
120 44.0 21.9 65.5


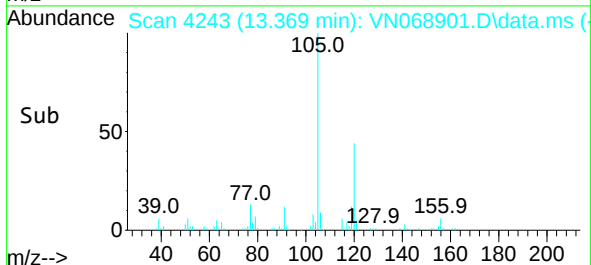

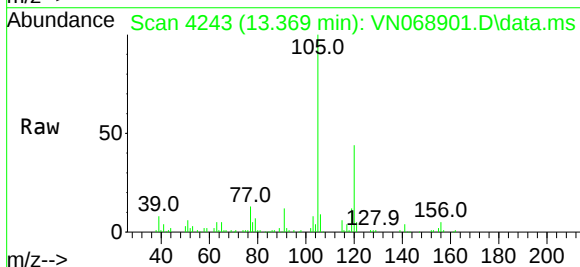


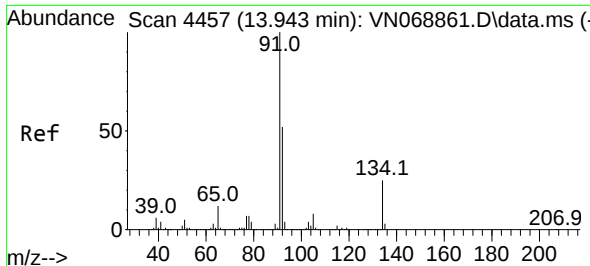

#89
n-Butylbenzene
Concen: 0.640 ug/l
RT: 13.943 min Scan# 4457
Delta R.T. 0.000 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48




Instrument :
MSVOA_N
ClientSampled :
41173


Tgt Ion: 91 Resp: 9594
Ion Ratio Lower Upper
91 100
92 41.2 26.0 78.0
134 0.0 12.5 37.5#

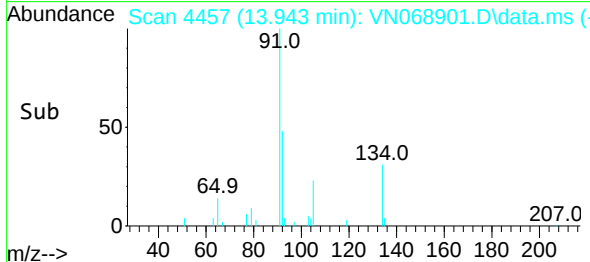

#90
Hexachloroethane
Concen: 0.690 ug/l
RT: 14.217 min Scan# 4559
Delta R.T. 0.003 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48

Tgt Ion: 117 Resp: 2613
Ion Ratio Lower Upper
117 100
201 0.0 37.1 111.5#


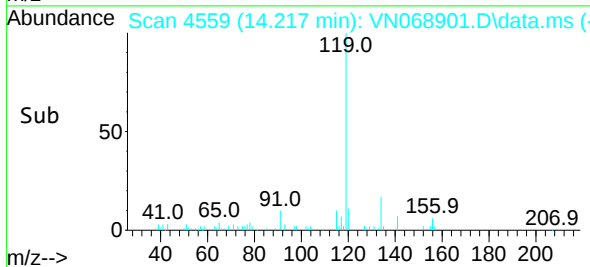

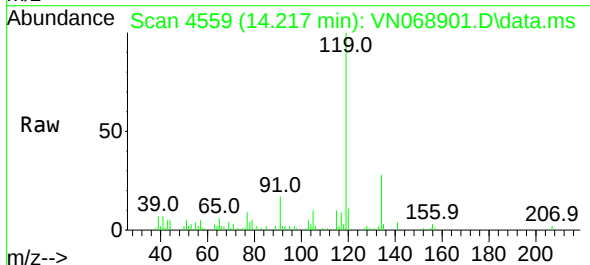




#93
1,2,4-Trichlorobenzene
Concen: 2.785 ug/l
RT: 15.265 min Scan# 4950
Delta R.T. 0.000 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48




Instrument :
MSVOA_N
ClientSampled :
41173


Tgt Ion:180 Resp: 872
Ion Ratio Lower Upper
180 100
182 92.8 47.9 143.7
145 49.2 16.4 49.2

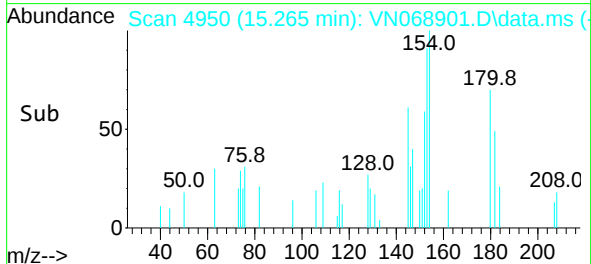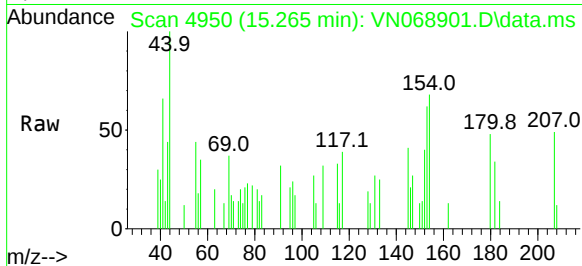

#95
Naphthalene
Concen: 5.940 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.002 min
Lab File: VN068901.D
Acq: 13 Oct 2021 16:48


Tgt Ion:128 Resp: 28734
Ion Ratio Lower Upper
128 100
127 7.5 10.5 15.7#
129 12.5 8.9 13.3

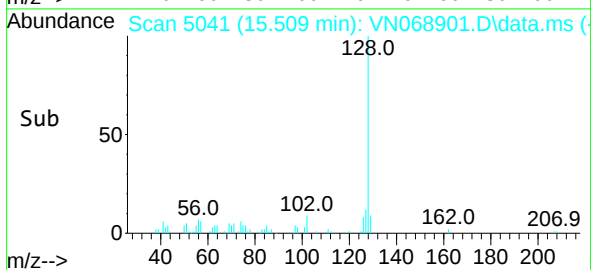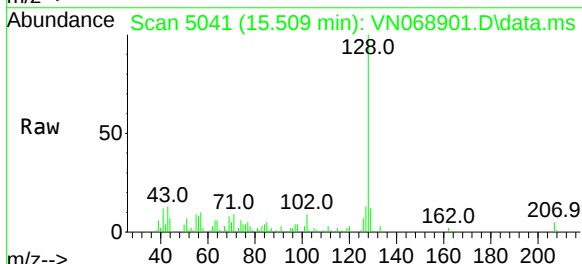



#96
 1,2,3-Trichlorobenzene
 Concen: 2.604 ug/l
 RT: 15.697 min Scan# 5111
 Delta R.T. -0.005 min
 Lab File: VN068901.D
 Acq: 13 Oct 2021 16:48

Instrument :
 MSVOA_N
 ClientSampleId :
 41173

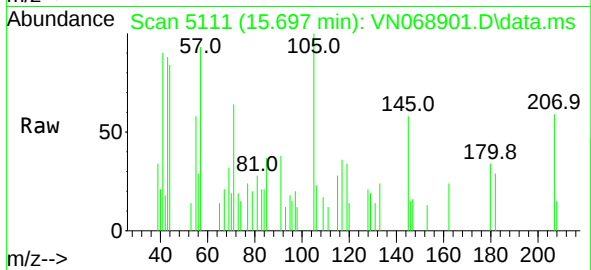

Tgt Ion:180 Resp: 410
 Ion Ratio Lower Upper
 180 100
 182 205.1 48.1 144.3#
 145 323.4 17.4 52.2#

