


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN101321\  
Data File : VN068887.D  
Acq On : 13 Oct 2021 10:15  
Operator : JC/MD  
Sample : BFB  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N101221W.M  
Title : SW846 8260  
Last Update : Wed Oct 13 05:44:40 2021

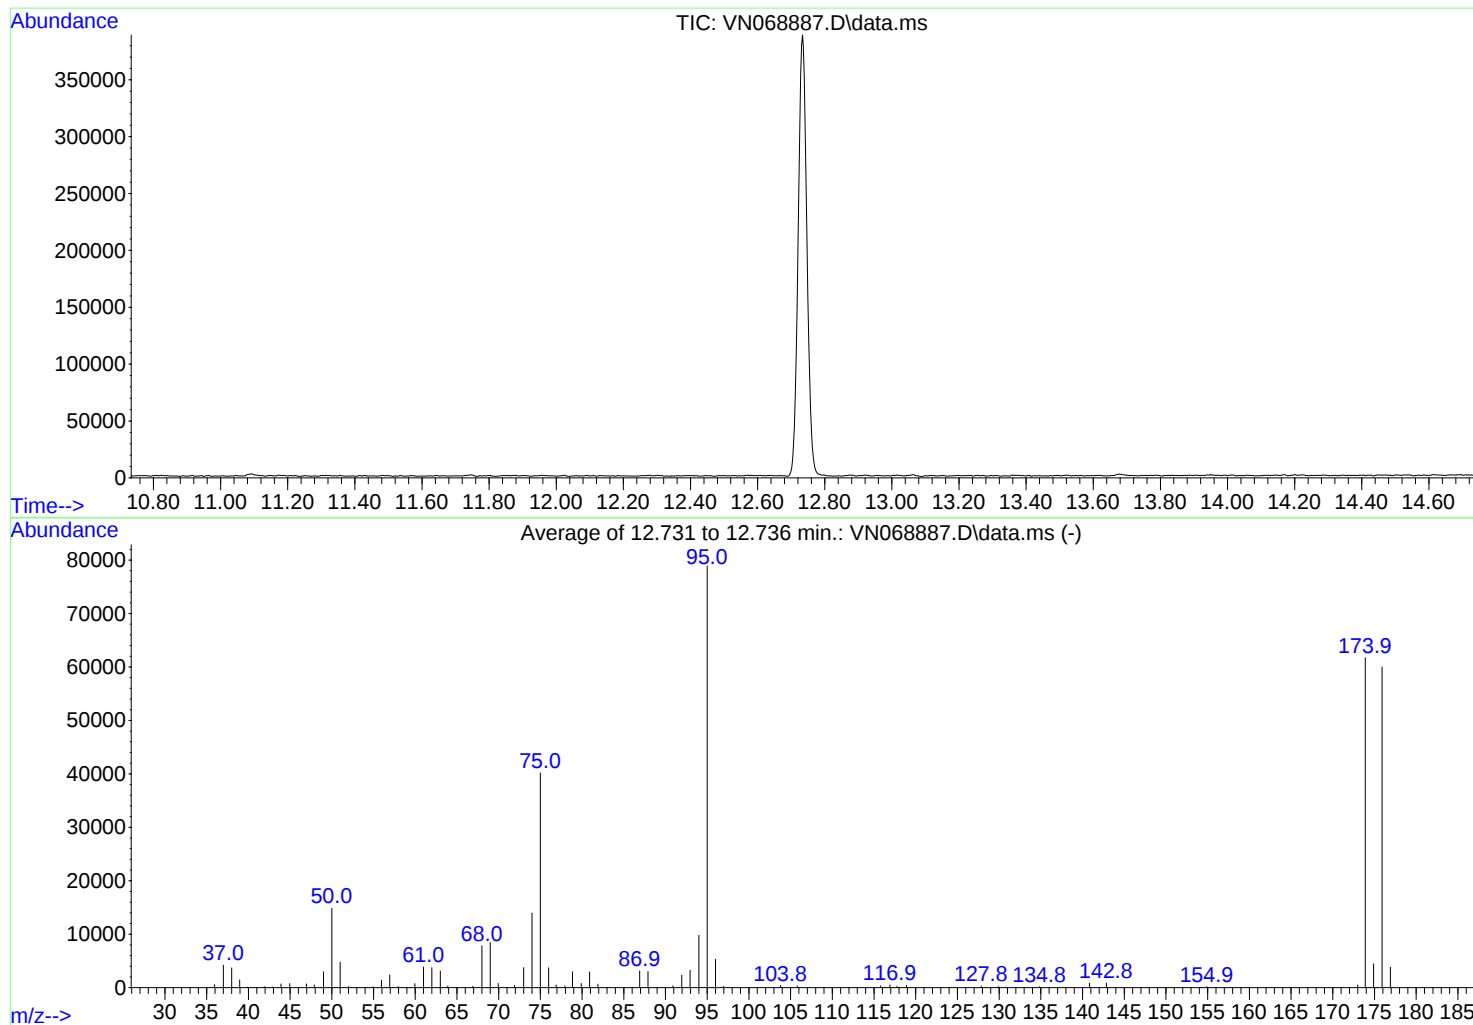

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3988

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 18.8  | 14854 | PASS      |
| 75     | 95      | 30     | 60     | 50.9  | 40173 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 78915 | PASS      |
| 96     | 95      | 5      | 9      | 6.8   | 5331  | PASS      |
| 173    | 174     | 0.00   | 2      | 0.8   | 512   | PASS      |
| 174    | 95      | 50     | 100    | 78.2  | 61715 | PASS      |
| 175    | 174     | 5      | 9      | 7.2   | 4466  | PASS      |
| 176    | 174     | 95     | 101    | 97.2  | 60003 | PASS      |
| 177    | 176     | 5      | 9      | 6.4   | 3845  | PASS      |