


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101322\
Data File : VN074890.D
Acq On : 13 Oct 2022 11:30
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N101222W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Oct 13 07:52:24 2022

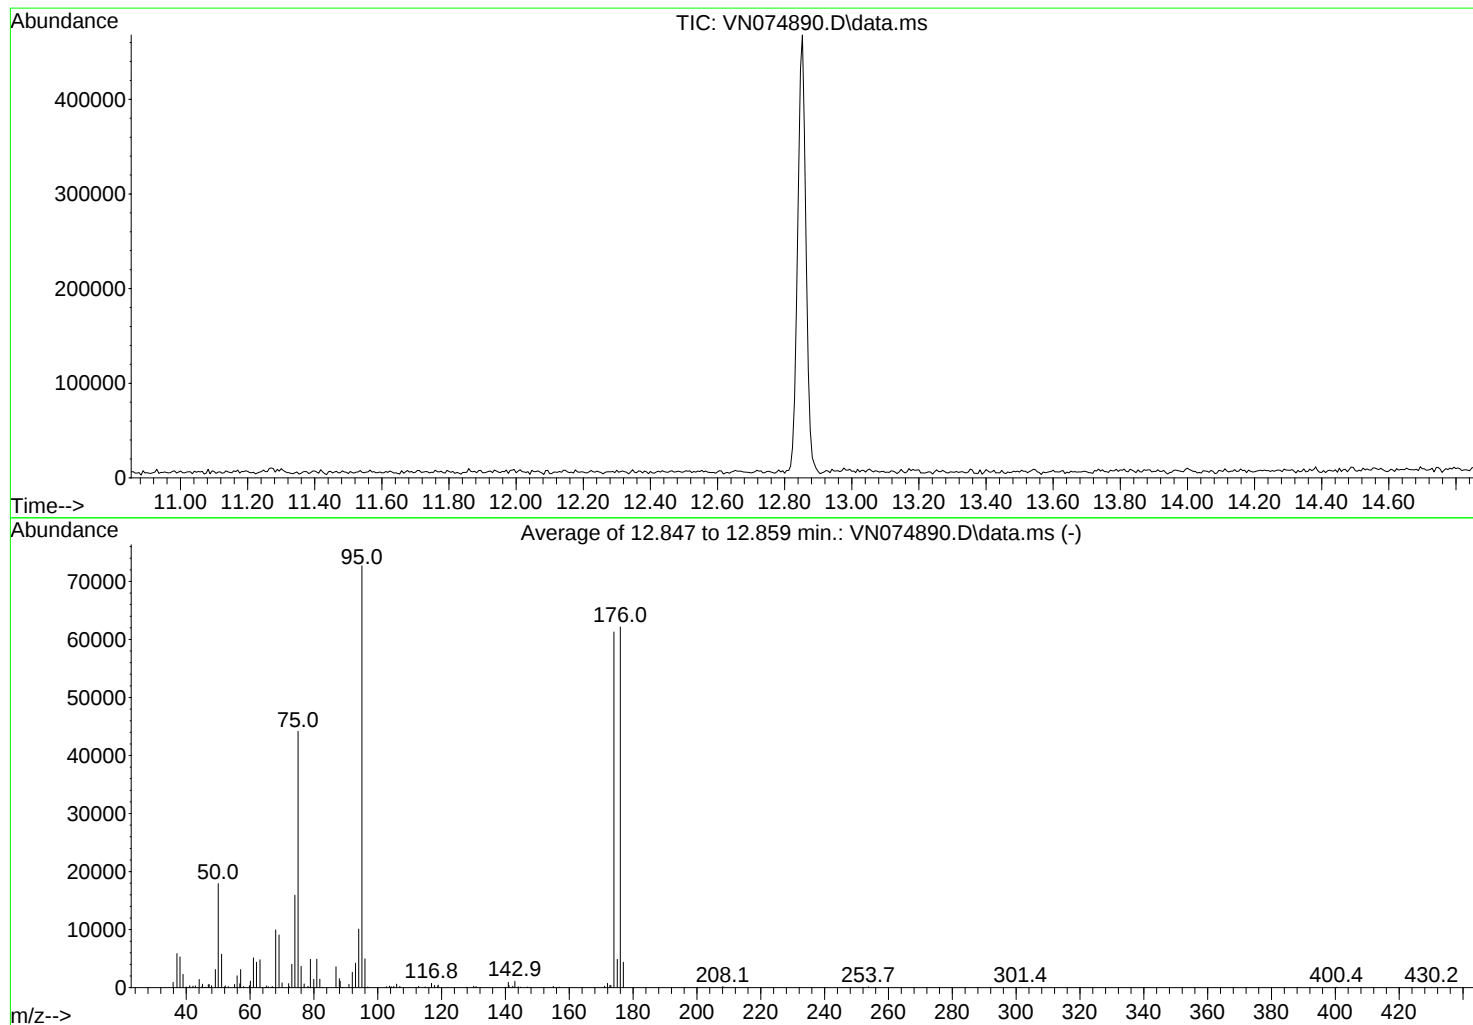

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.7	17928	PASS
75	95	30	60	60.8	44163	FAIL*
95	95	100	100	100.0	72685	PASS
96	95	5	9	6.8	4973	PASS
173	174	0.00	2	0.7	405	PASS
174	95	50	100	84.3	61301	PASS
175	174	5	9	8.0	4893	PASS
176	174	95	101	101.4	62136	FAIL*
177	176	5	9	7.1	4386	PASS