
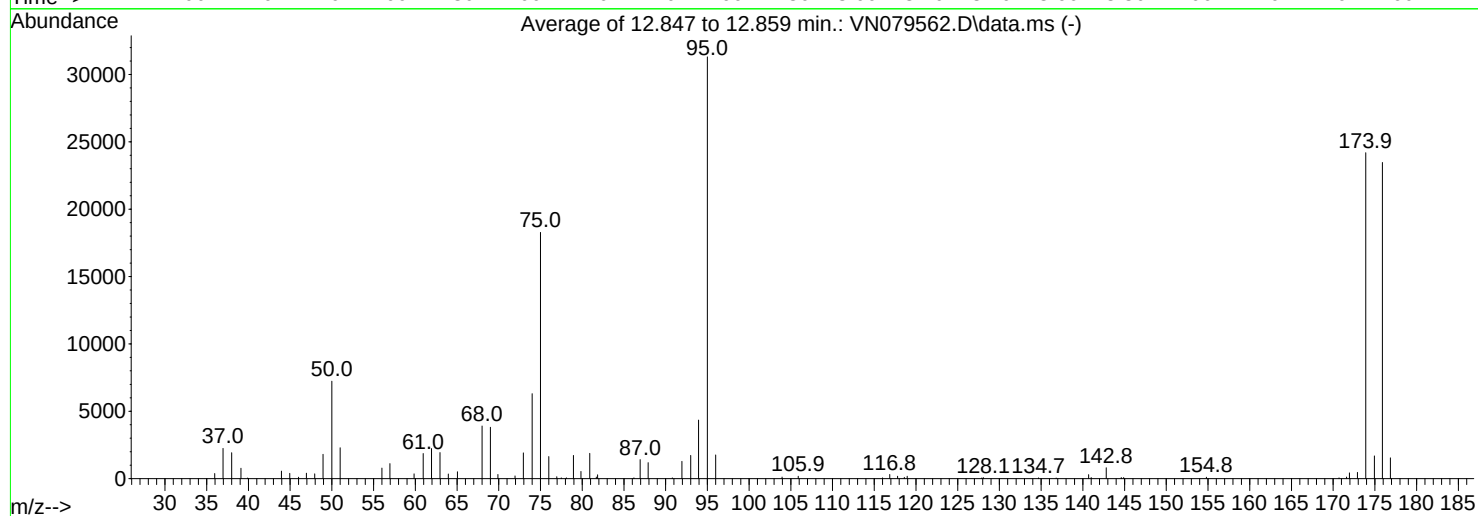


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101323\
Data File : VN079562.D
Acq On : 13 Oct 2023 09:52
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
Title : SW846 8260
Last Update : Fri Oct 06 03:34:49 2023

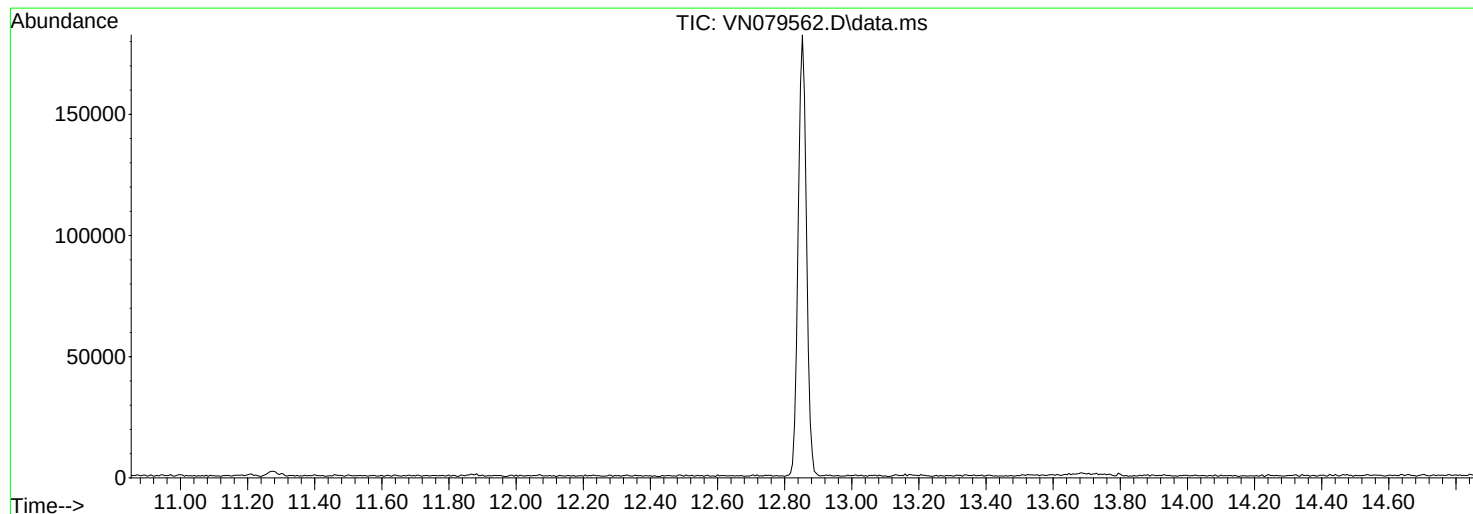

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	7234	PASS
75	95	30	60	58.4	18280	PASS
95	95	100	100	100.0	31309	PASS
96	95	5	9	5.6	1755	PASS
173	174	0.00	2	1.9	466	PASS
174	95	50	100	77.3	24189	PASS
175	174	5	9	7.0	1686	PASS
176	174	95	101	97.0	23469	PASS
177	176	5	9	6.6	1549	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	381	50.00	7234	69.00	3819	79.85	534
36.95	2248	51.00	2296	69.90	310	80.90	187
38.00	1920	56.00	783	71.95	207	81.70	12
39.10	769	56.95	1123	72.95	1917	81.85	28
39.90	52	59.85	357	74.00	6309	86.20	58
43.95	561	60.95	1869	75.00	18280	86.95	1409
44.95	393	61.95	2234	76.00	1641	87.90	1187
46.00	107	62.95	1935	76.95	142	90.80	64
46.95	405	63.95	342	77.50	58	91.95	1281
47.95	352	65.05	506	78.10	64	93.00	1723
48.95	1809	68.00	3913	78.95	1722	93.95	4347

Average of 12.847 to 12.859 min.: VN079562.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.00	31309	134.70	62	172.90	466		
96.00	1755	136.80	50	173.90	24189		
103.95	120	140.70	293	174.95	1686		
105.90	185	141.00	86	175.90	23469		
116.00	61	142.80	810	176.85	1549		
116.85	310	144.60	88				
117.80	180	144.90	83				
118.60	100	154.80	106				
118.95	184	170.70	60				
127.90	59	171.60	115				
128.10	71	171.95	423				

Instrument :

MSVOA_N

ClientSampleId :

BFB