


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN101419\
 Data File : VN058743.D
 Acq On : 14 Oct 2019 12:08
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101319W.M
 Title : SW846 8260
 Last Update : Sat Oct 12 00:00:30 2019

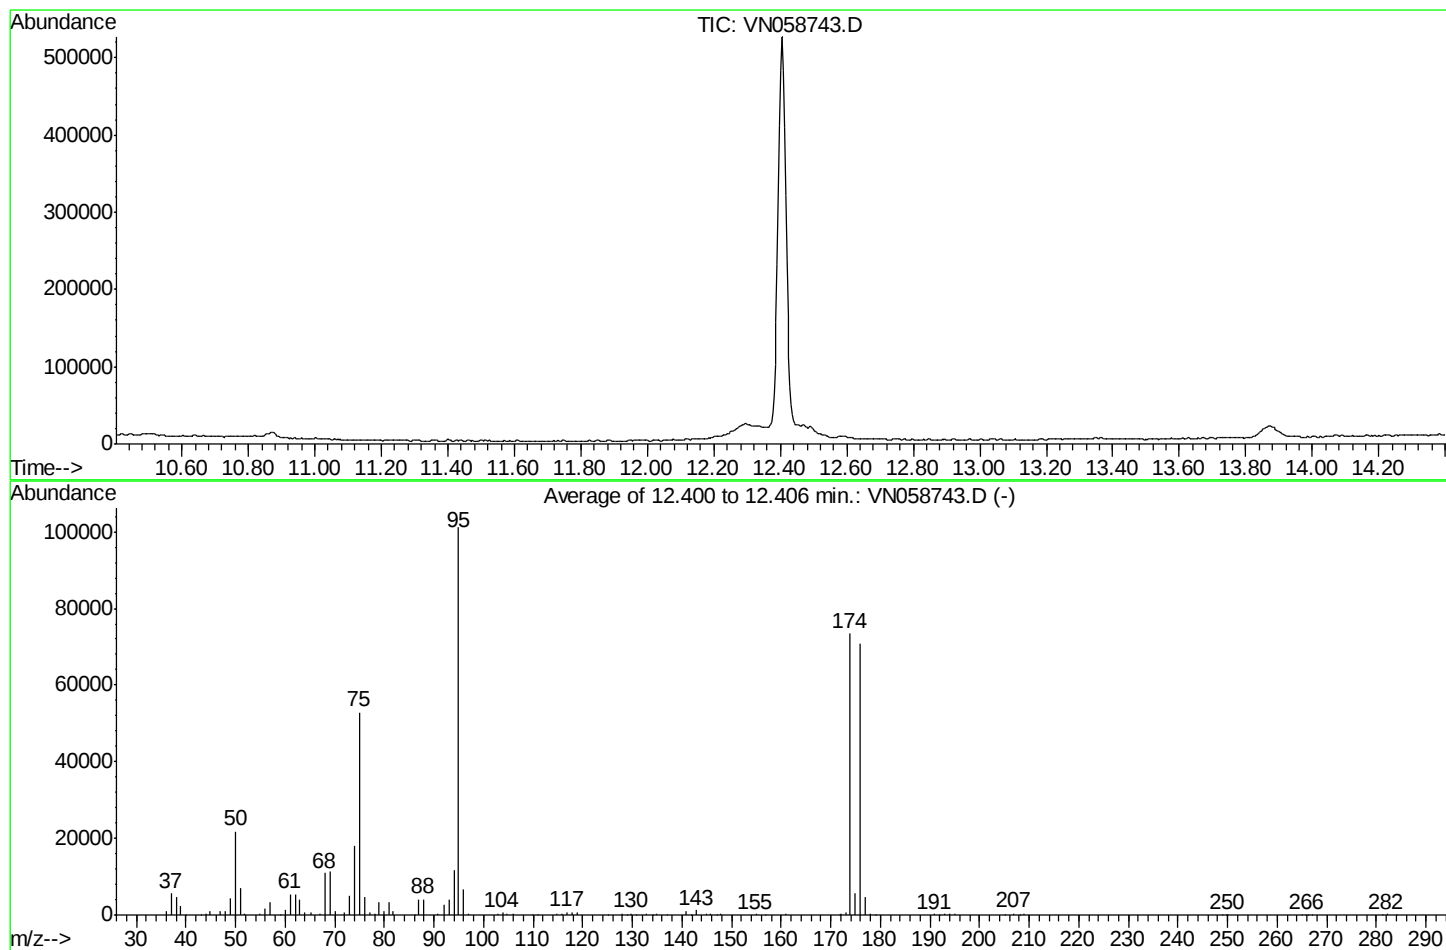

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	21861	PASS
75	95	30	60	52.3	52947	PASS
95	95	100	100	100.0	101168	PASS
96	95	5	9	6.5	6569	PASS
173	174	0.00	2	1.0	706	PASS
174	95	50	100	72.5	73338	PASS
175	174	5	9	7.8	5733	PASS
176	174	95	101	96.4	70722	PASS
177	176	5	9	6.7	4742	PASS