
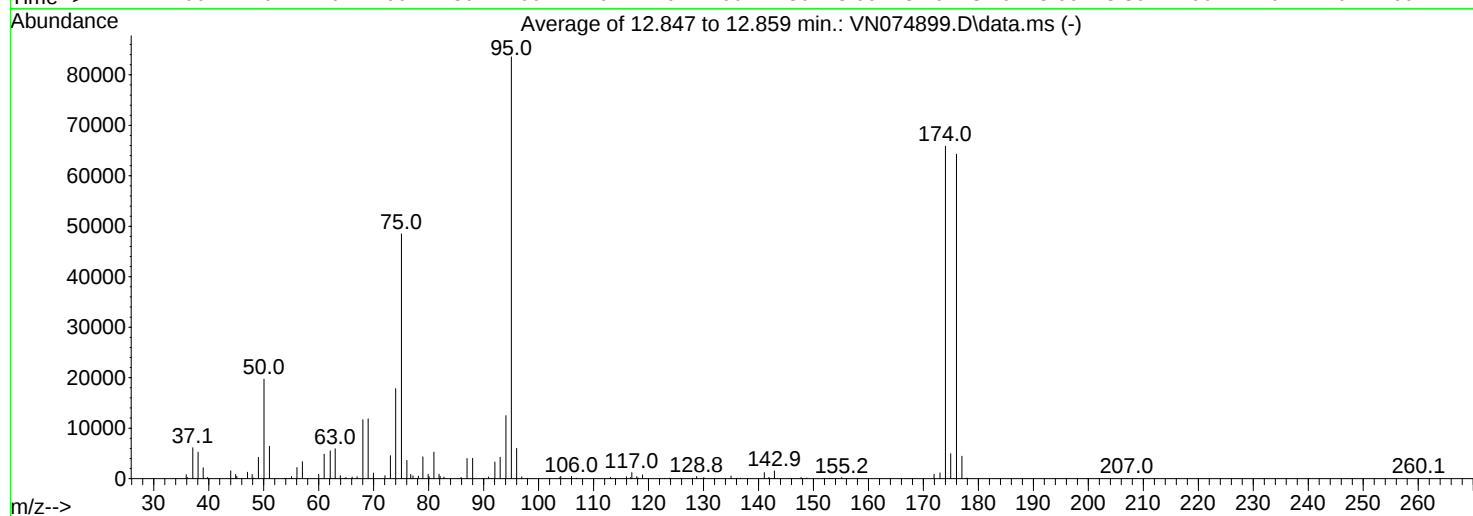


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101422\
 Data File : VN074899.D
 Acq On : 14 Oct 2022 09:13
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101422W.M
 Title : SW846 8260
 Last Update : Mon Oct 17 01:40:20 2022

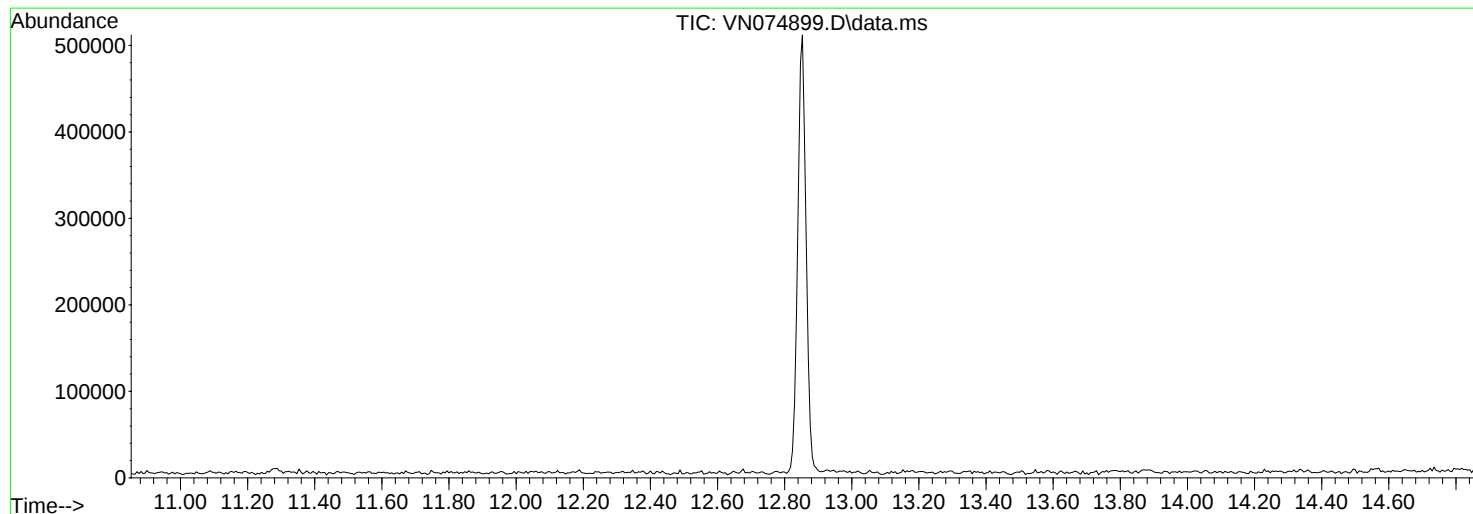

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	19732	PASS
75	95	30	60	58.1	48512	PASS
95	95	100	100	100.0	83568	PASS
96	95	5	9	7.2	5982	PASS
173	174	0.00	2	1.7	1144	PASS
174	95	50	100	78.8	65859	PASS
175	174	5	9	7.5	4951	PASS
176	174	95	101	97.6	64272	PASS
177	176	5	9	6.9	4436	PASS