
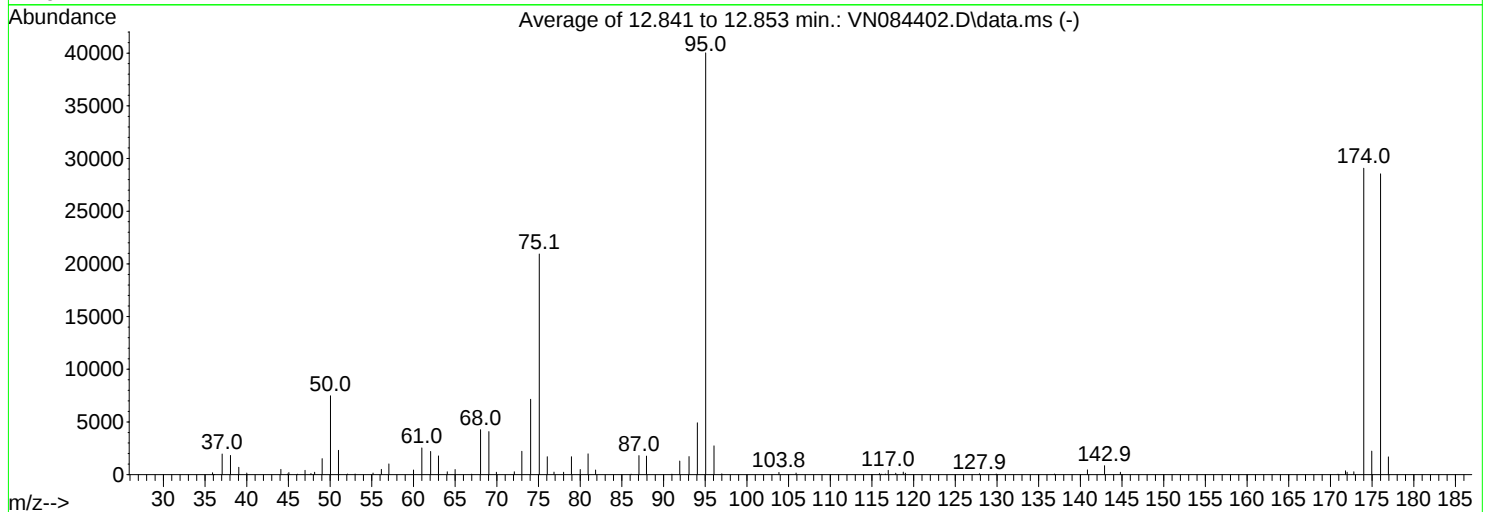


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101424\
Data File : VN084402.D
Acq On : 14 Oct 2024 08:11
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N100824W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Oct 09 02:22:28 2024

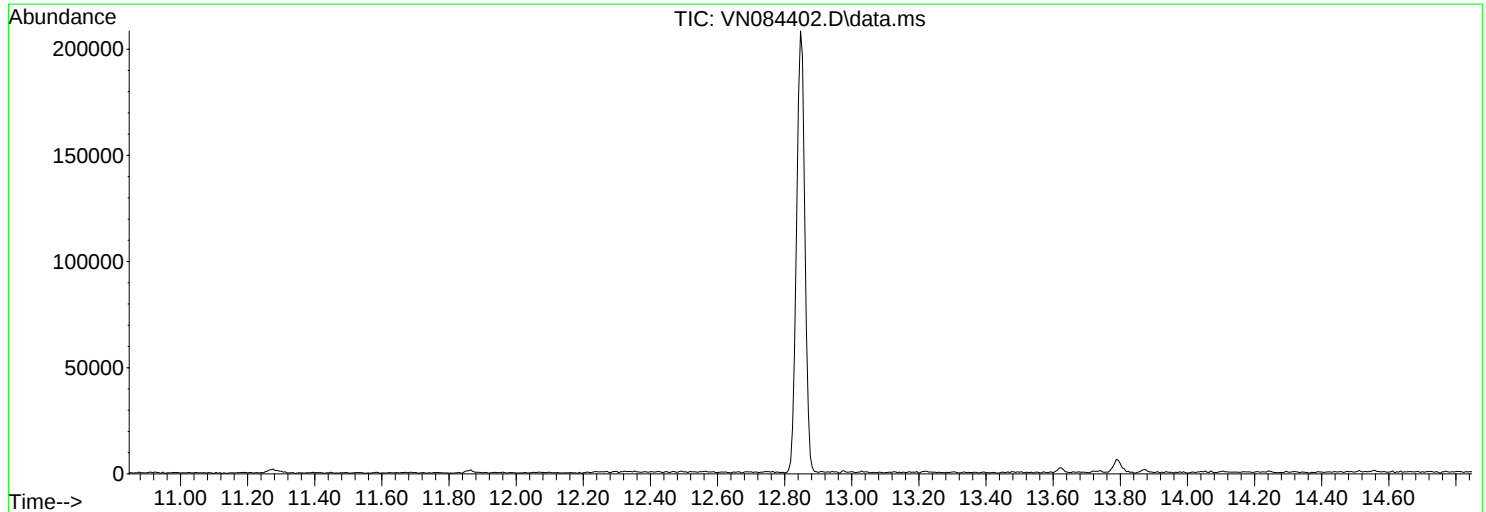

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.7	7481	PASS
75	95	30	60	52.3	20933	PASS
95	95	100	100	100.0	40027	PASS
96	95	5	9	6.8	2731	PASS
173	174	0.00	2	0.9	271	PASS
174	95	50	100	72.7	29085	PASS
175	174	5	9	7.7	2234	PASS
176	174	95	101	98.1	28544	PASS
177	176	5	9	5.9	1684	PASS