


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101518\
Data File : VN051861.D
Acq On : 15 Oct 2018 9:04
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N101218W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Oct 12 10:23:44 2018

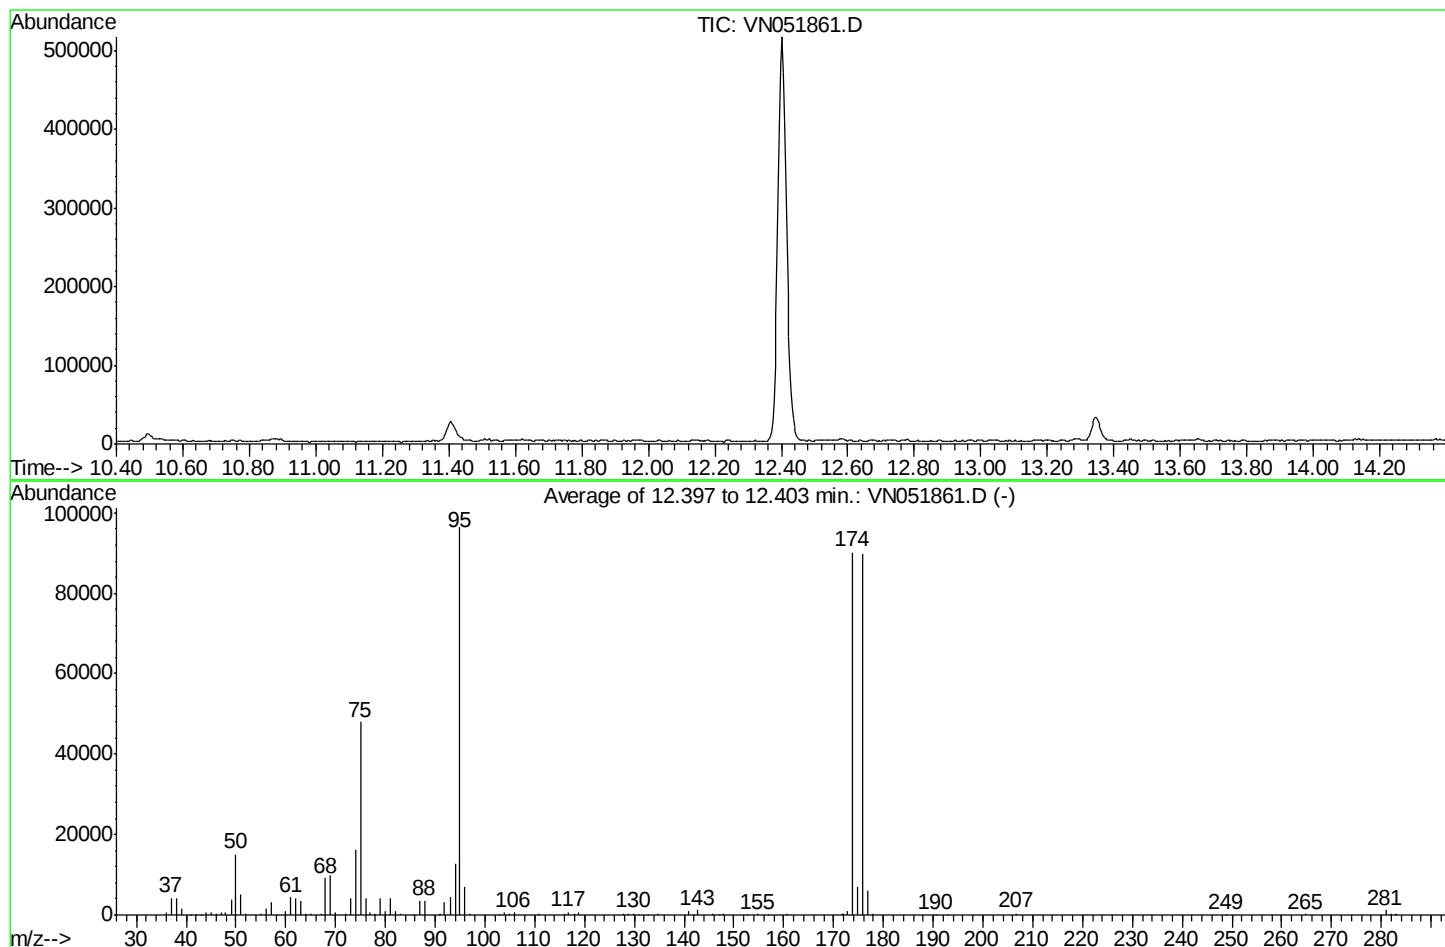

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	15091	PASS
75	95	30	60	49.8	48005	PASS
95	95	100	100	100.0	96384	PASS
96	95	5	9	7.2	6902	PASS
173	174	0.00	2	0.9	837	PASS
174	95	50	100	93.5	90090	PASS
175	174	5	9	7.9	7160	PASS
176	174	95	101	99.7	89856	PASS
177	176	5	9	6.9	6165	PASS