


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN101519\
Data File : VN058771.D
Acq On : 15 Oct 2019 8:23
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101319W.M
Title : SW846 8260
Last Update : Sat Oct 12 00:00:30 2019

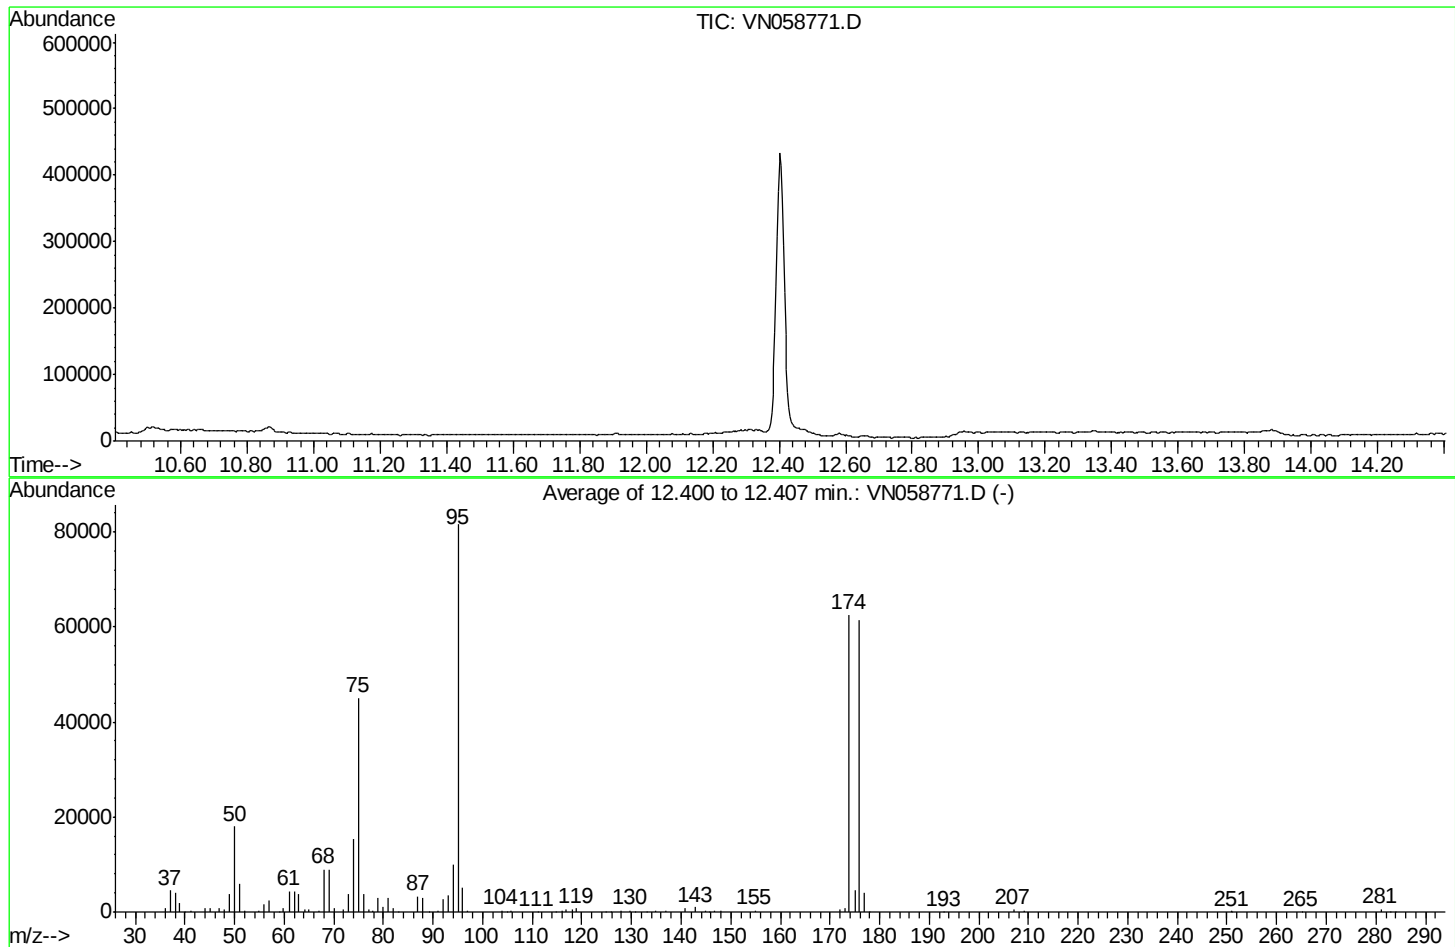

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	17960	PASS
75	95	30	60	55.3	45096	PASS
95	95	100	100	100.0	81613	PASS
96	95	5	9	6.4	5208	PASS
173	174	0.00	2	1.2	740	PASS
174	95	50	100	76.6	62554	PASS
175	174	5	9	7.5	4679	PASS
176	174	95	101	98.3	61490	PASS
177	176	5	9	6.6	4073	PASS