

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN101520\
 Data File : VN064150.D
 Acq On : 15 Oct 2020 17:55
 Operator : JC/MD
 Sample : L4221-05
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 OK-02-100120

Quant Time: Oct 16 15:19:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101420W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 15 01:16:44 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	280585	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	536439	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	560763	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	205439	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	224582	56.20	ug/l	0.00
Spiked Amount			Recovery	=	112.40%	
35) Dibromofluoromethane	7.55	113	187737	50.56	ug/l	0.00
Spiked Amount			Recovery	=	101.12%	
50) Toluene-d8	10.06	98	688527	49.15	ug/l	0.00
Spiked Amount			Recovery	=	98.30%	
62) 4-Bromofluorobenzene	12.38	95	239381	49.71	ug/l	0.00
Spiked Amount			Recovery	=	99.42%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN101520\
Data File : VN064150.D
Acq On : 15 Oct 2020 17:55
Operator : JC/MD
Sample : L4221-05
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
OK-02-100120

Quant Time: Oct 16 15:19:31 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N101420W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 15 01:16:44 2020
Response via : Initial Calibration

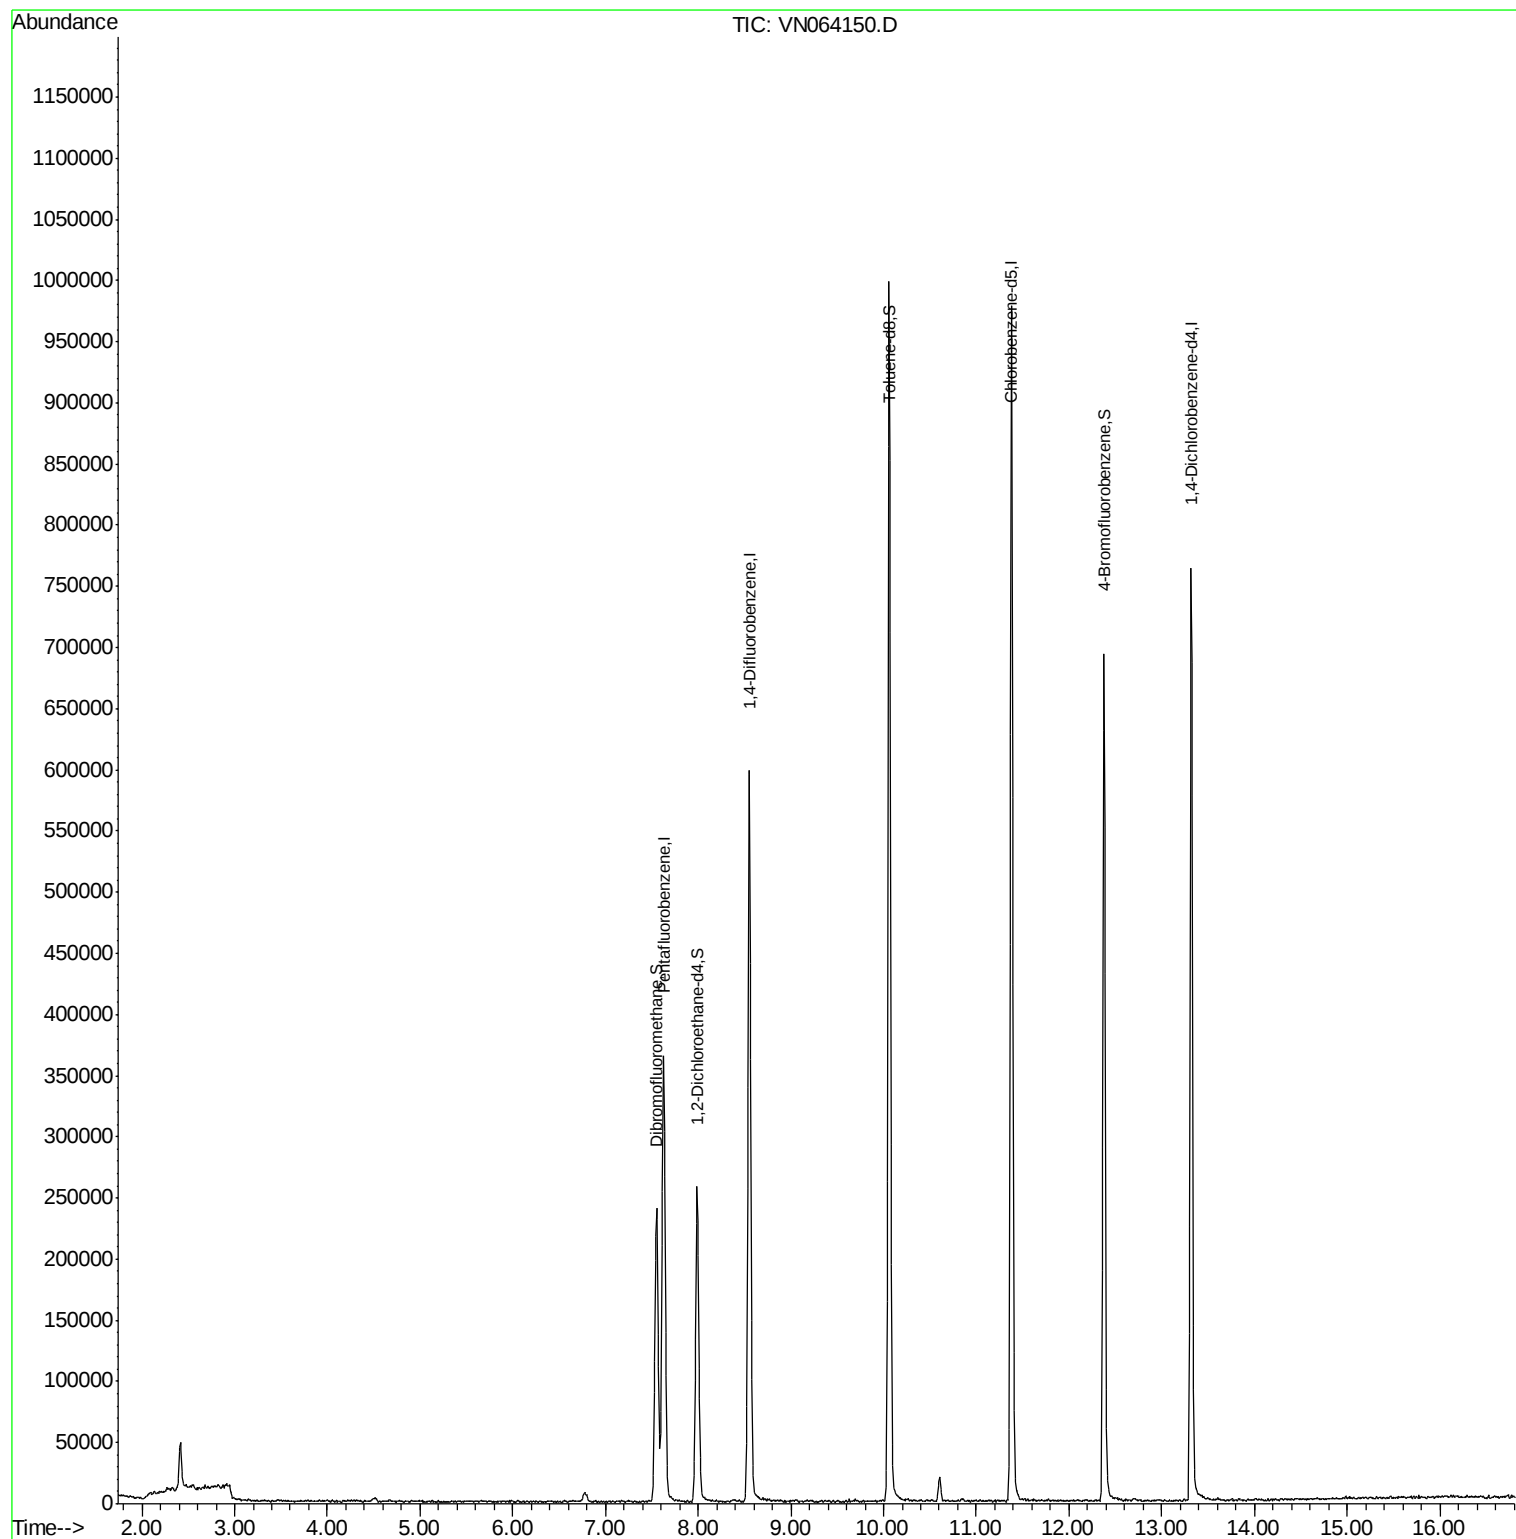

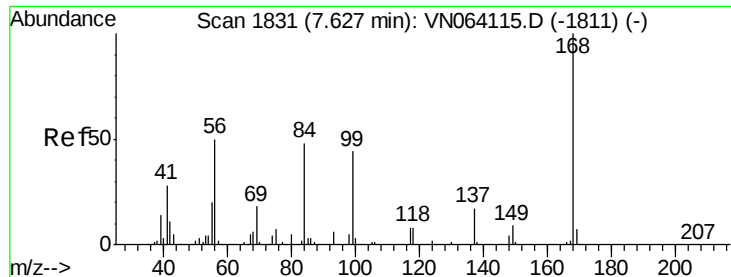

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN064150.D

Acq: 15 Oct 2020 17:55

Instrument :

MSVOA_N

ClientSampleId :


OK-02-100120

Tot Ion:168 Resp: 280585

Ion Ratio Lower Upper




168 100

99 59.1 43.6 65.4

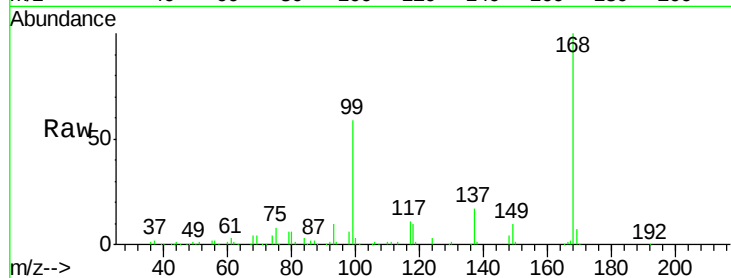

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

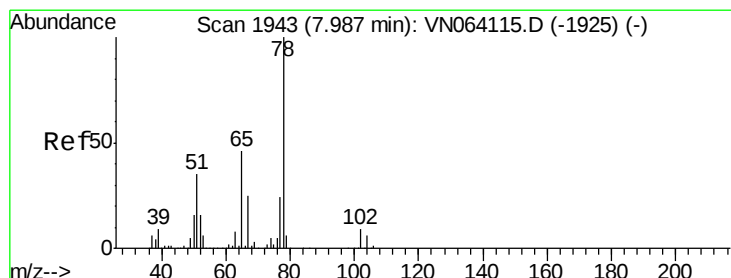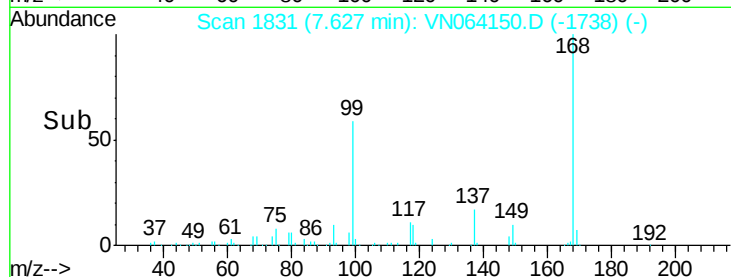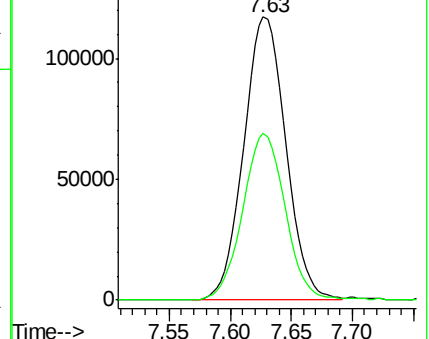

#33

1,2-Dichloroethane-d4

Concen: 56.200 ug/l

RT: 7.99 min Scan# 1943

Delta R.T. 0.00 min

Lab File: VN064150.D


Acq: 15 Oct 2020 17:55

Tgt Ion: 65 Resp: 224582

Ion Ratio Lower Upper



65 100


67 51.6 0.0 105.6

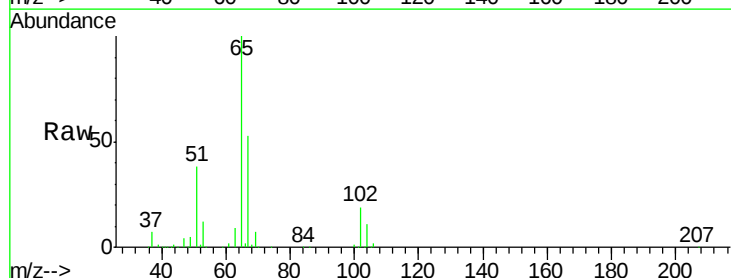

Abundance Ion 64.90 (64.60 to 65.60): VNO

Ion 66.90 (66.60 to 67.60): VNO

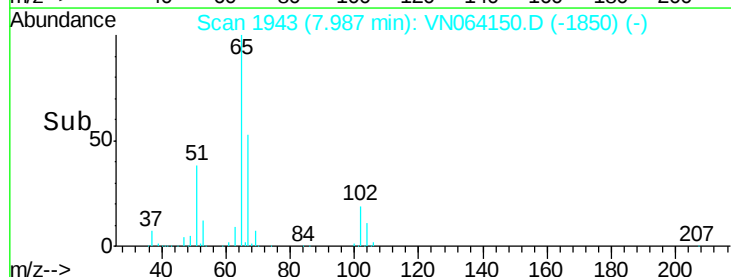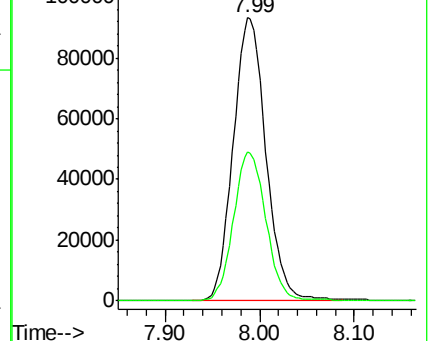

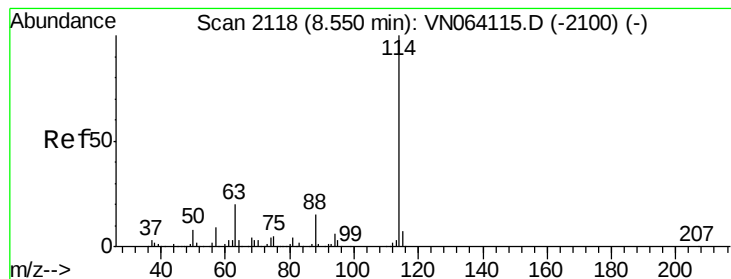

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.55 min Scan# 2119

Delta R.T. 0.00 min

Lab File: VN064150.D

Acq: 15 Oct 2020 17:55

Instrument :

MSVOA_N

ClientSampleId :

OK-02-100120


Tot Ion:114 Resp: 536439

Ion Ratio Lower Upper

114 100

63 19.6 0.0 41.0




88 14.6 0.0 29.2

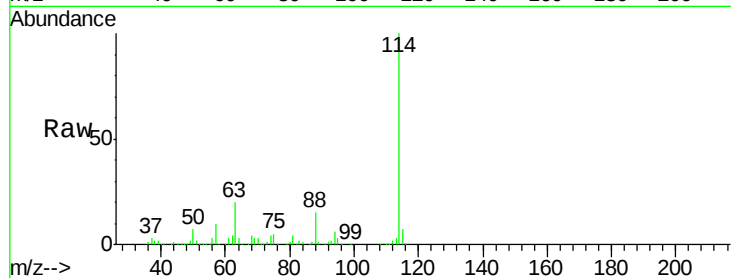

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

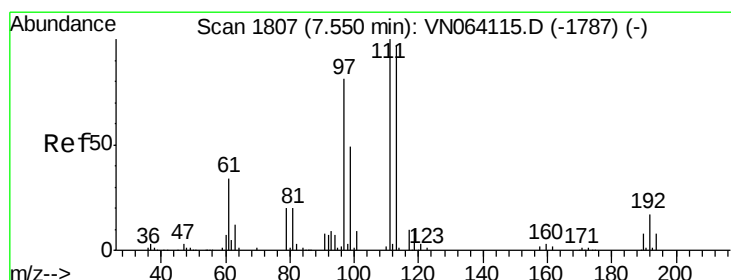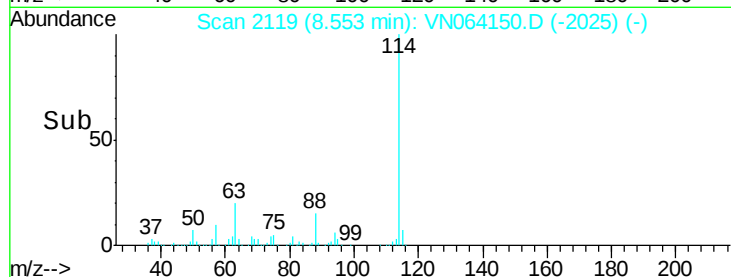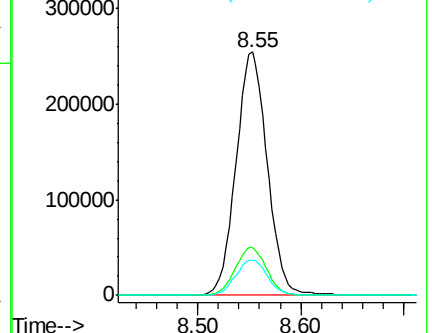

#35

Dibromofluoromethane

Concen: 50.563 ug/l

RT: 7.55 min Scan# 1808

Delta R.T. 0.00 min

Lab File: VN064150.D

Acq: 15 Oct 2020 17:55


Tgt Ion:113 Resp: 187737

Ion Ratio Lower Upper

113 100

111 101.8 81.9 122.9



192 17.8 14.3 21.5

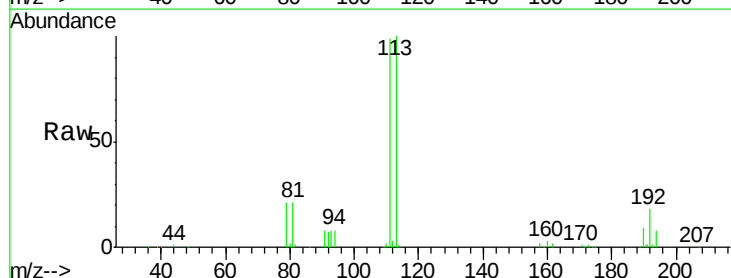


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

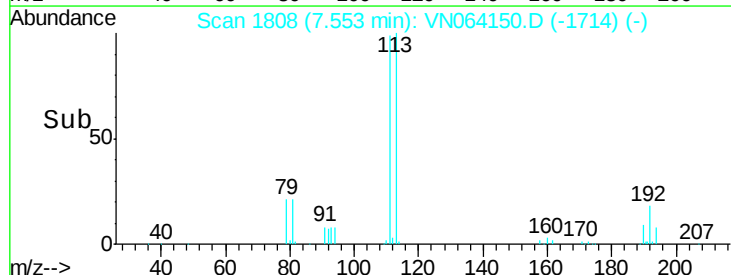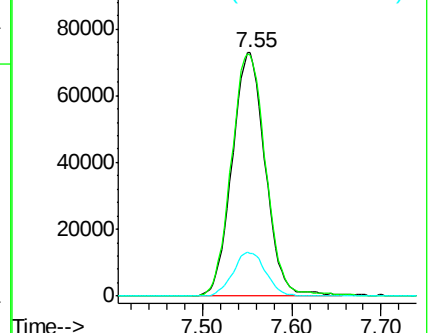

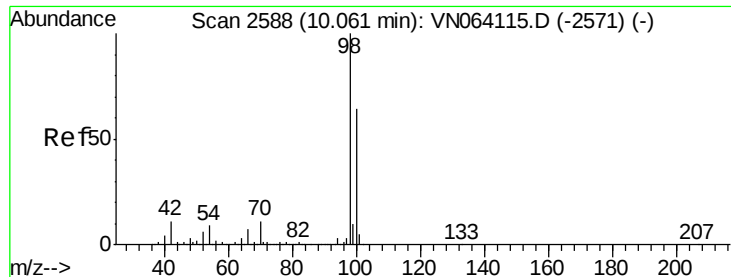

#50

Toluene-d8

Concen: 49.147 ug/l

RT: 10.06 min Scan# 2588

Delta R.T. 0.00 min

Lab File: VN064150.D

Acq: 15 Oct 2020 17:55

Instrument :

MSVOA_N

ClientSampled :





OK-02-100120

Tot Ion: 98 Resp: 688527

Ion Ratio Lower Upper

98 100

100 63.3 50.8 76.2

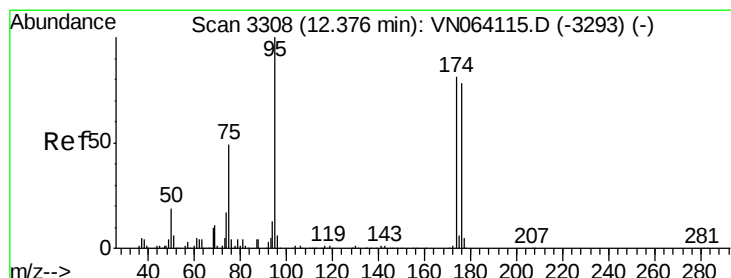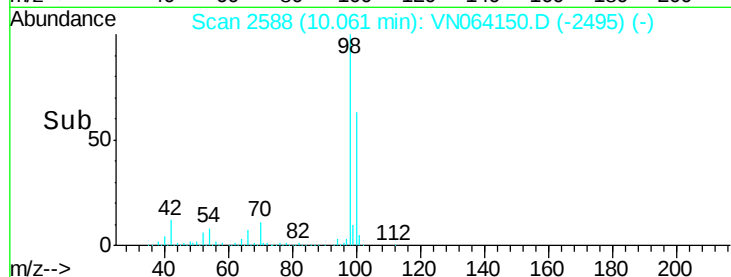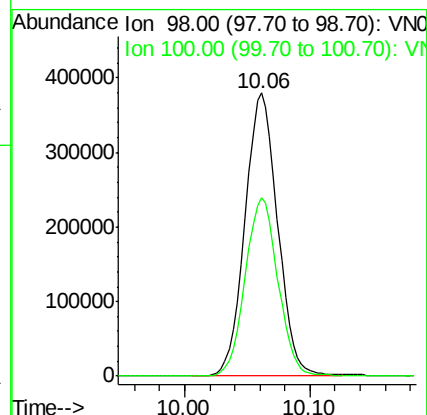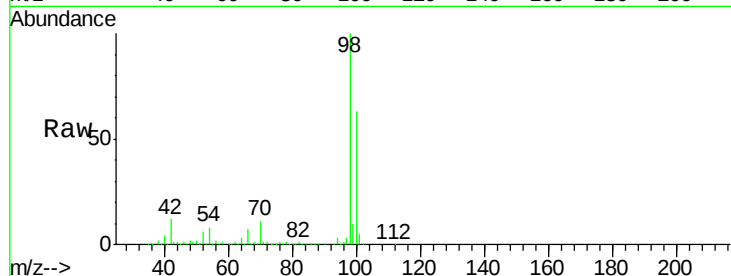

#62

4-Bromofluorobenzene

Concen: 49.711 ug/l

RT: 12.38 min Scan# 3309

Delta R.T. 0.00 min

Lab File: VN064150.D

Acq: 15 Oct 2020 17:55




Tgt Ion: 95 Resp: 239381


Ion Ratio Lower Upper

95 100

174 79.3 0.0 164.8

176 75.3 0.0 157.8

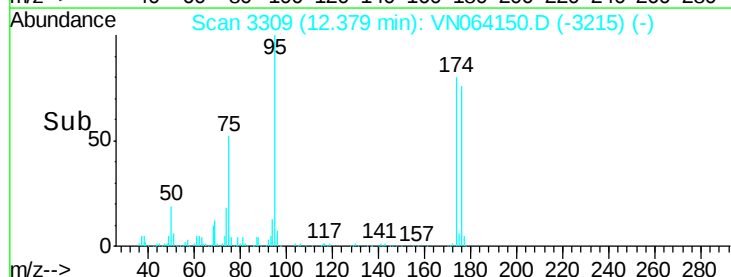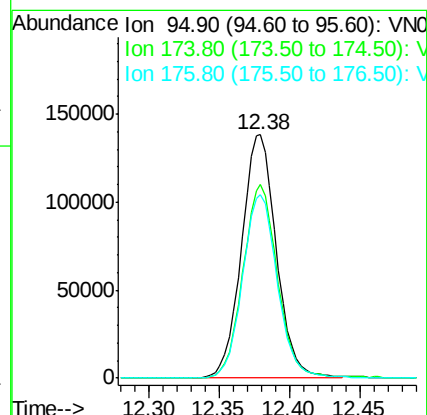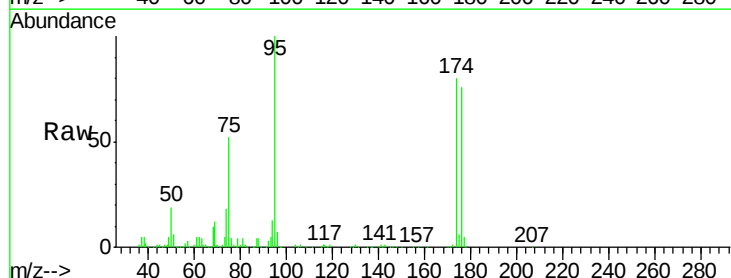


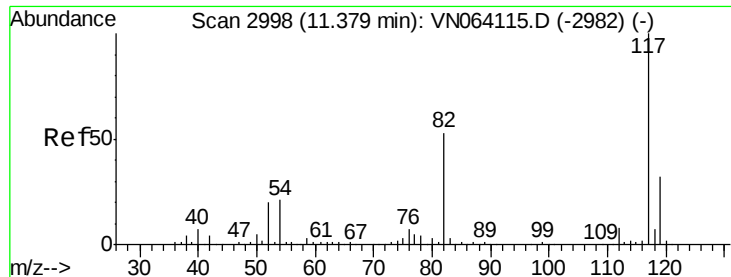




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN064150.D
Acq: 15 Oct 2020 17:55

Instrument :
MSVOA_N
ClientSampleId :
OK-02-100120

Tot Ion:117 Resp: 560763
Ion Ratio Lower Upper
117 100
82 53.5 42.6 63.8
119 32.3 25.5 38.3

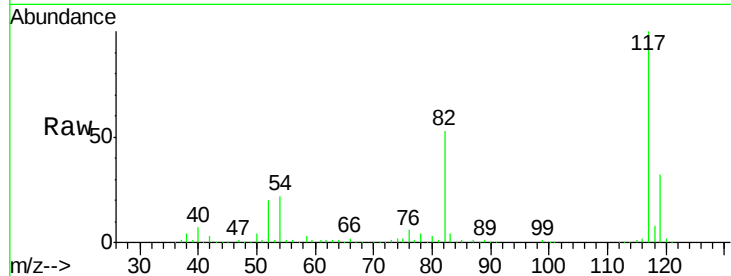


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

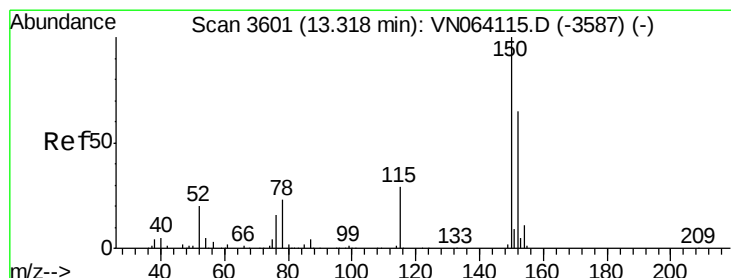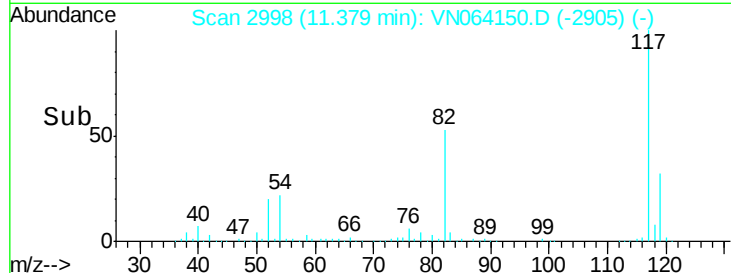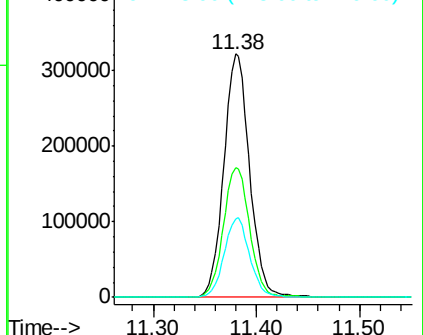

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3601
Delta R.T. 0.00 min
Lab File: VN064150.D
Acq: 15 Oct 2020 17:55

Tgt Ion:152 Resp: 205439
Ion Ratio Lower Upper
152 100
115 60.5 29.3 87.8
150 157.1 0.0 346.0

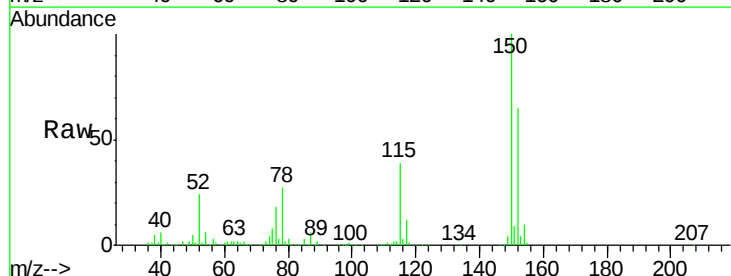

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

