


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN101520\
Data File : VN064134.D
Acq On : 15 Oct 2020 10:39
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101420W.M
Title : SW846 8260
Last Update : Thu Oct 15 01:16:44 2020

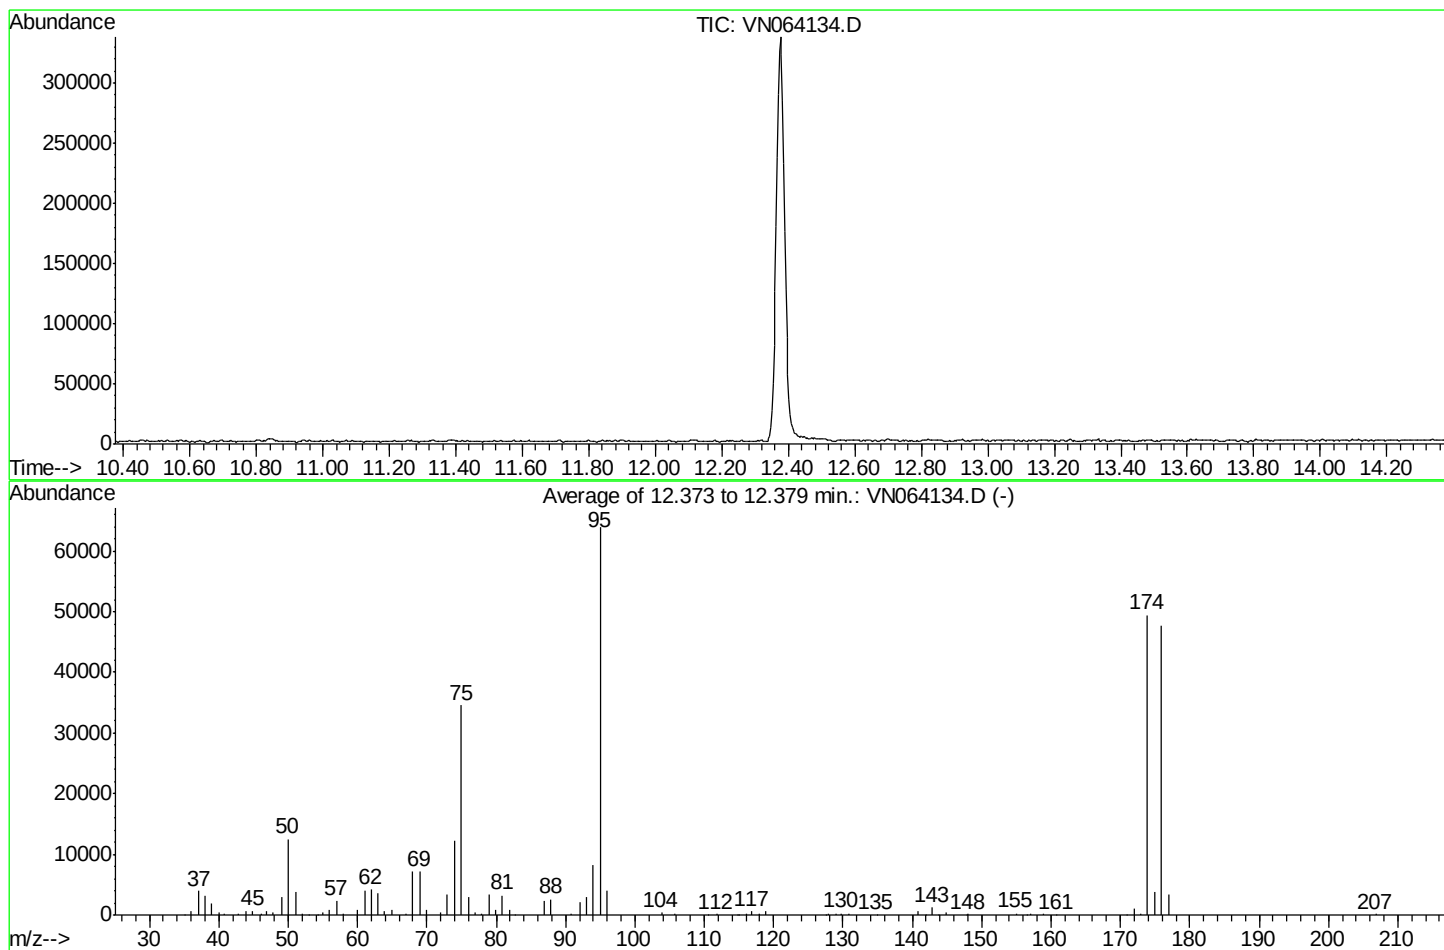

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	12514	PASS
75	95	30	60	54.1	34578	PASS
95	95	100	100	100.0	63914	PASS
96	95	5	9	6.4	4118	PASS
173	174	0.00	2	0.6	299	PASS
174	95	50	100	77.3	49410	PASS
175	174	5	9	7.9	3896	PASS
176	174	95	101	96.3	47602	PASS
177	176	5	9	7.0	3344	PASS