
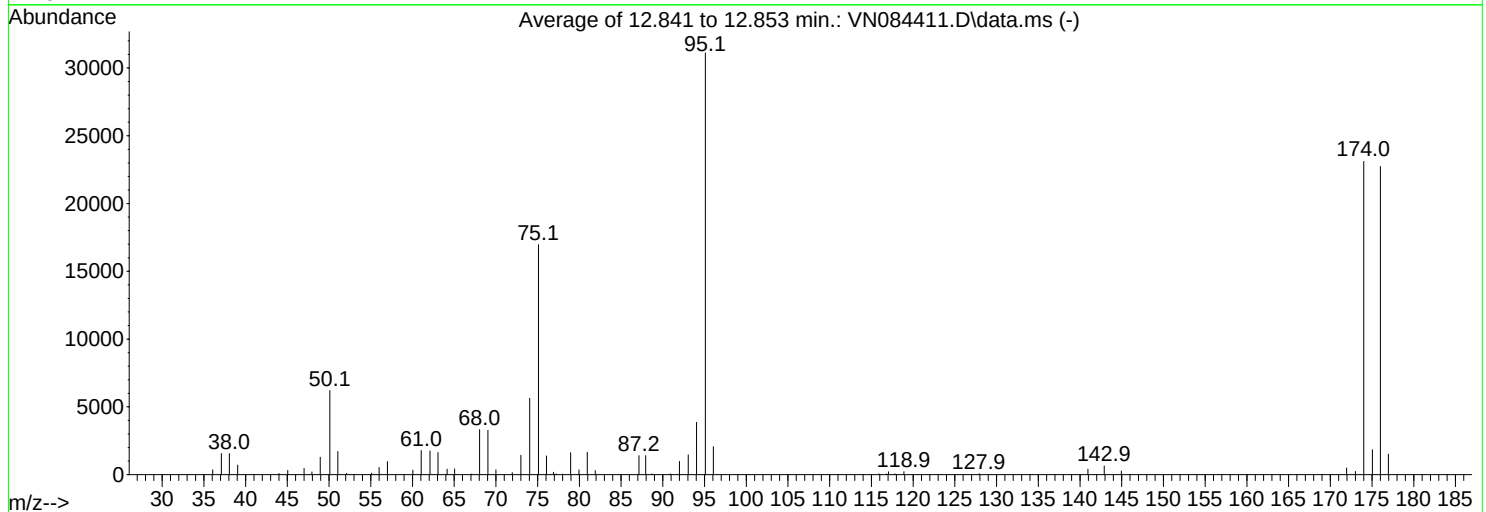


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101524\
Data File : VN084411.D
Acq On : 15 Oct 2024 12:15
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N100824W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Oct 09 02:22:28 2024

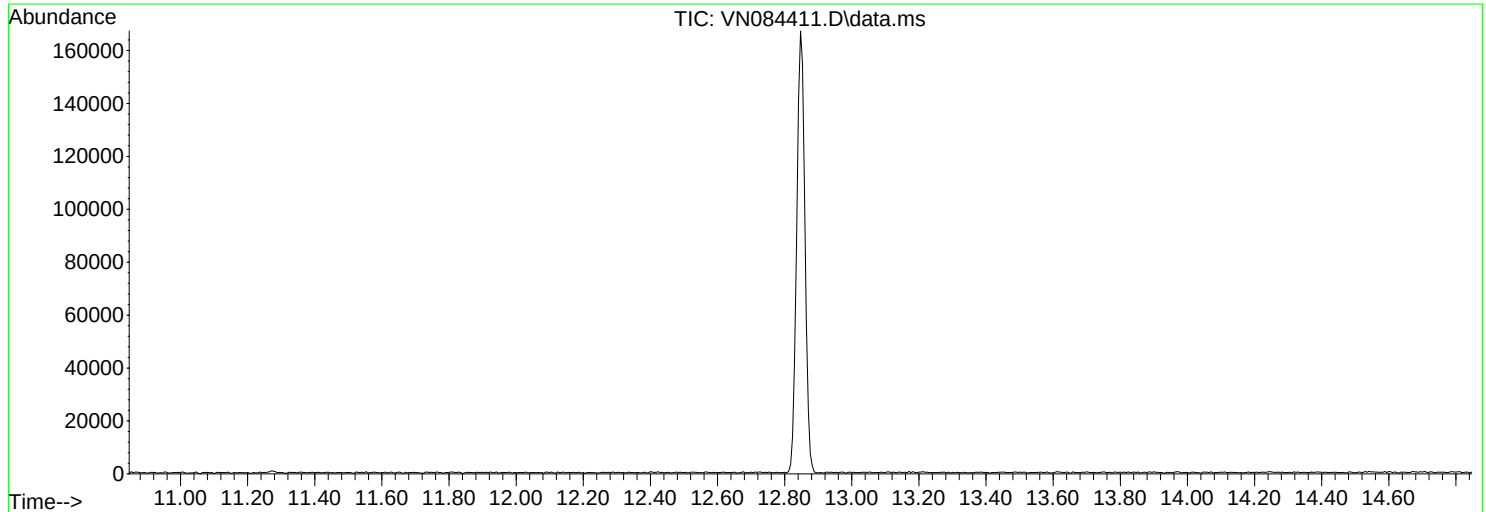

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.0	6208	PASS
75	95	30	60	54.5	16966	PASS
95	95	100	100	100.0	31117	PASS
96	95	5	9	6.6	2065	PASS
173	174	0.00	2	1.0	237	PASS
174	95	50	100	74.3	23117	PASS
175	174	5	9	8.0	1841	PASS
176	174	95	101	98.4	22739	PASS
177	176	5	9	6.6	1510	PASS