

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN101618\
 Data File : VN051882.D
 Acq On : 16 Oct 2018 9:33
 Operator : MD\SY
 Sample : VN1016MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 4 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1016MBL01

Quant Time: Oct 17 03:05:57 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101118W.M
 Quant Title : SW846 8260
 QLast Update : Fri Oct 12 09:51:20 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	867838	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1237807	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1051462	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	345201	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	467152	56.32	ug/l	0.00
Spiked Amount	50.000		Recovery	=	112.64%	
35) Dibromofluoromethane	7.59	113	463549	60.23	ug/l	0.00
Spiked Amount	50.000		Recovery	=	120.46%	
50) Toluene-d8	10.09	98	1680951	58.61	ug/l	0.00
Spiked Amount	50.000		Recovery	=	117.22%	
62) 4-Bromofluorobenzene	12.40	95	462099	46.67	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.34%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN101618\
Data File : VN051882.D
Acq On : 16 Oct 2018 9:33
Operator : MD\SY
Sample : VN1016MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 4 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
VN1016MBL01

Quant Time: Oct 17 03:05:57 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N101118W.M
Quant Title : SW846 8260
QLast Update : Fri Oct 12 09:51:20 2018
Response via : Initial Calibration

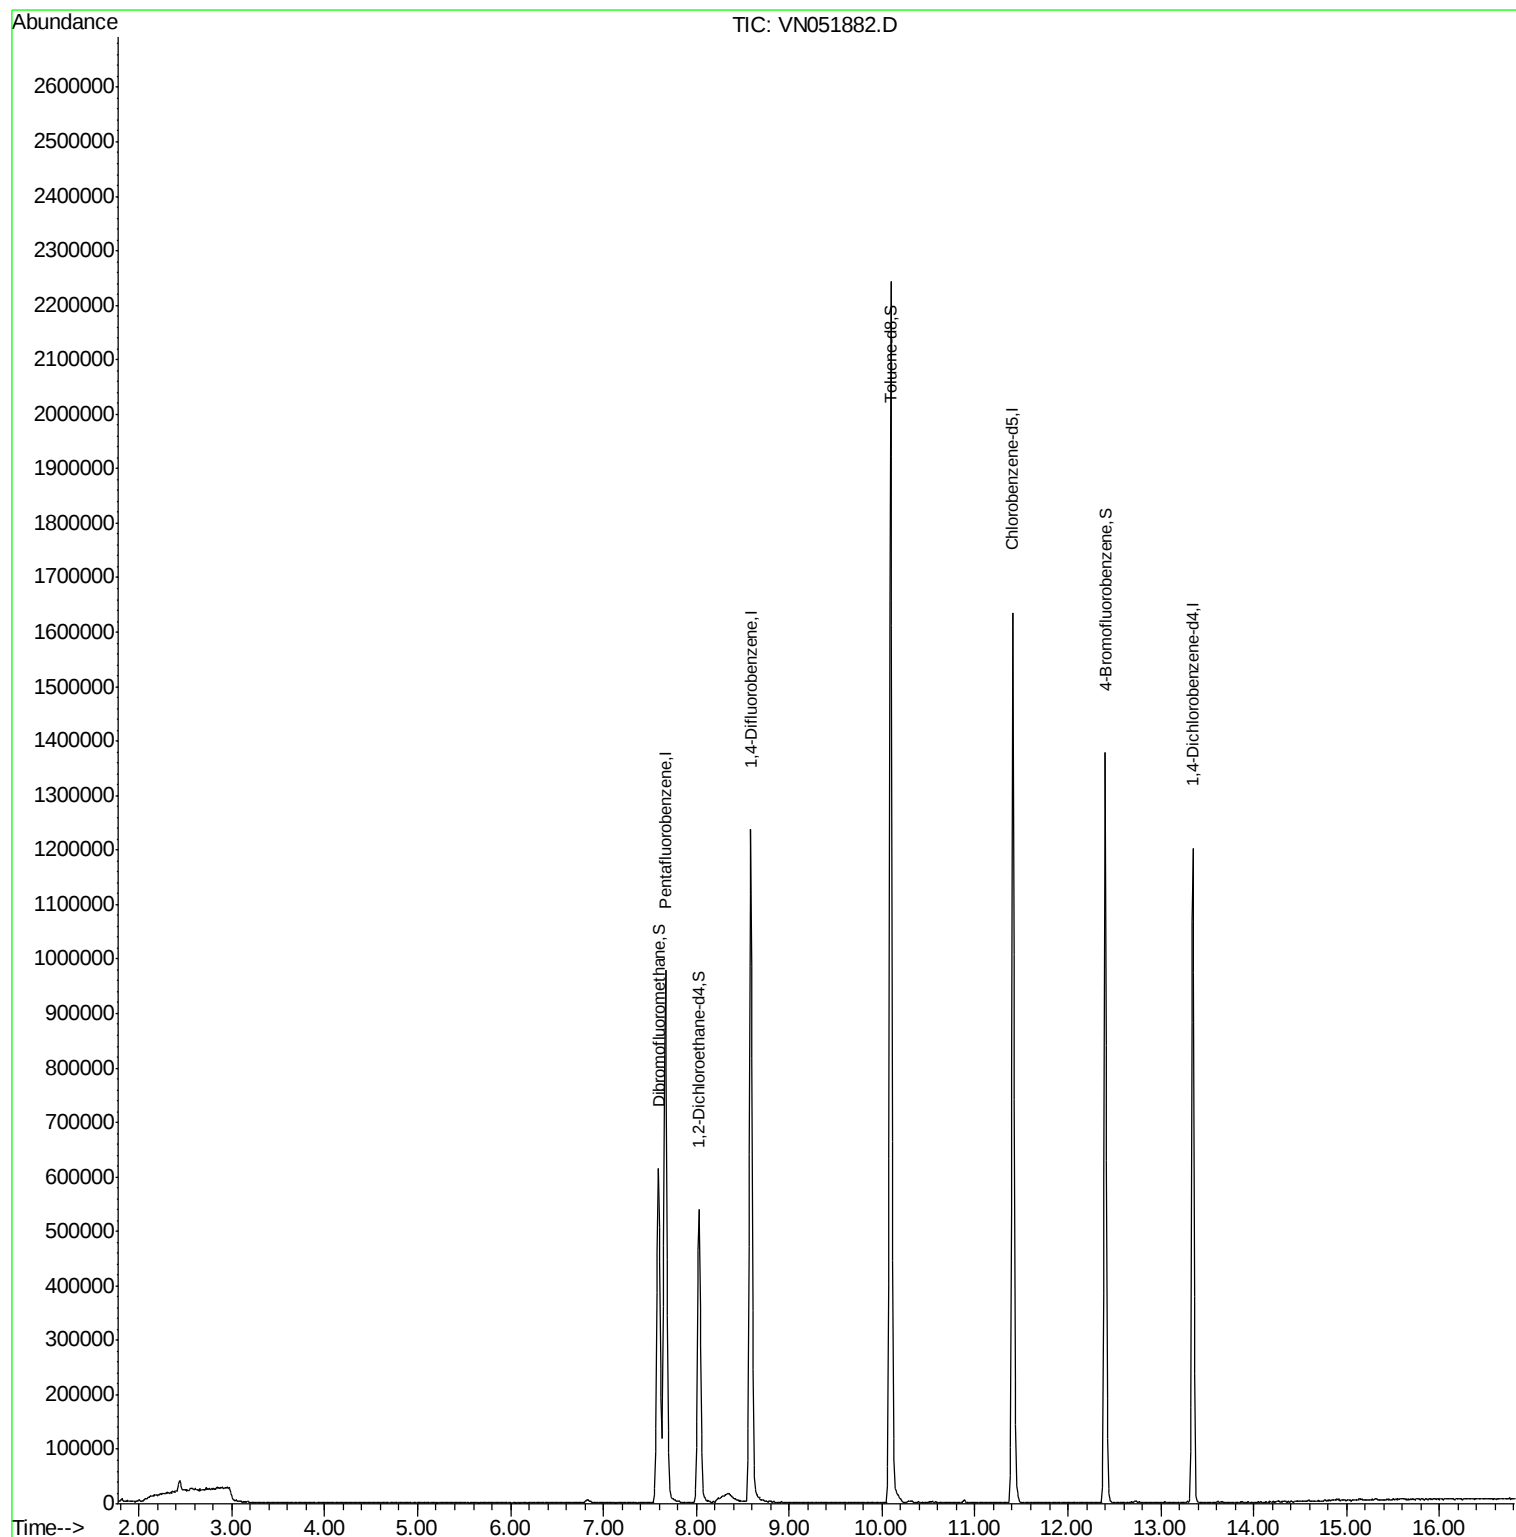

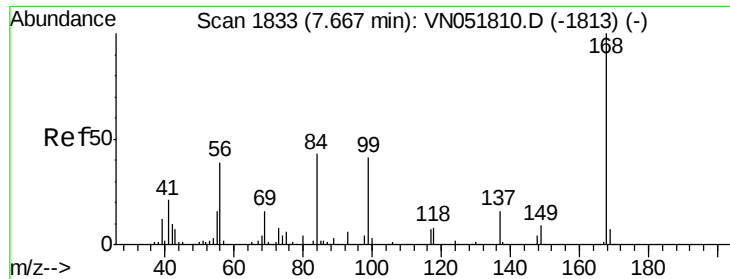

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. 0.00 min

Lab File: VN051882.D

Acq: 16 Oct 2018 9:33

Instrument :

MSVOA_N

ClientSampleId :


VN1016MBL01

Tgt Ion: 168 Resp: 867838

Ion Ratio Lower Upper

168 100

99 48.0 39.6 59.4

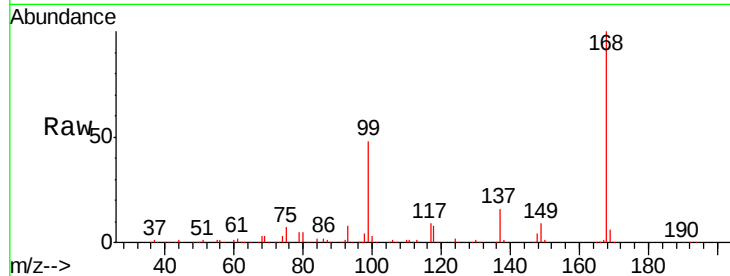

Abundance Ion 167.90 (167.60 to 168.60): VN051810.D (-1813) (-)

Ion 98.90 (98.60 to 99.60): VN051810.D (-1813) (-)

7.67

400000

300000



200000

100000

0

7.60 7.70 7.80

Time-->

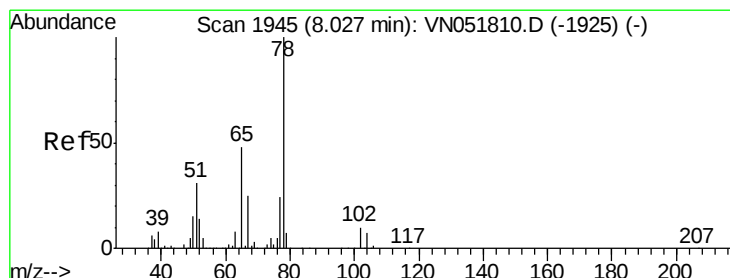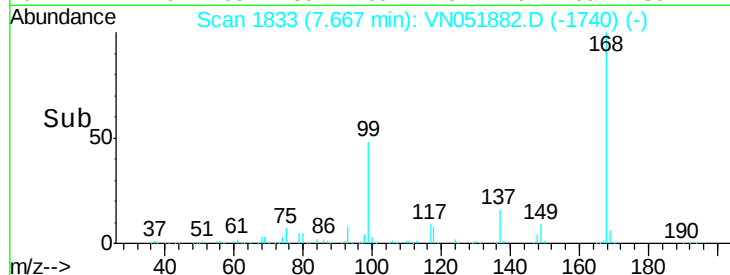

#33

1,2-Dichloroethane-d4

Concen: Below ug/l

RT: 8.03 min Scan# 1946

Delta R.T. 0.00 min

Lab File: VN051882.D


Acq: 16 Oct 2018 9:33

Tgt Ion: 65 Resp: 467152

Ion Ratio Lower Upper

65 100

67 51.3 0.0 110.4

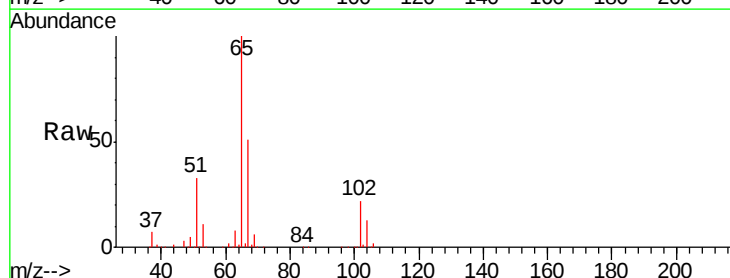

Abundance Ion 64.90 (64.60 to 65.60): VN051810.D (-1925) (-)

Ion 66.90 (66.60 to 67.60): VN051810.D (-1925) (-)

8.03

200000

150000


100000


50000

0

7.90 8.00 8.10

Time-->

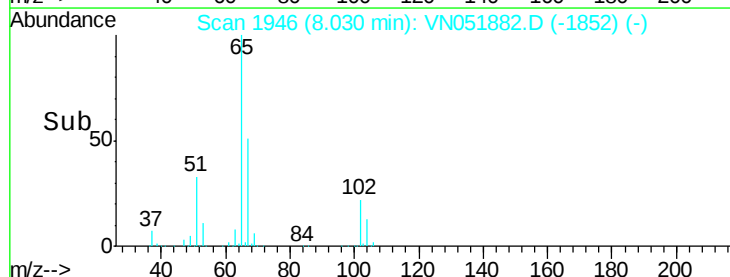

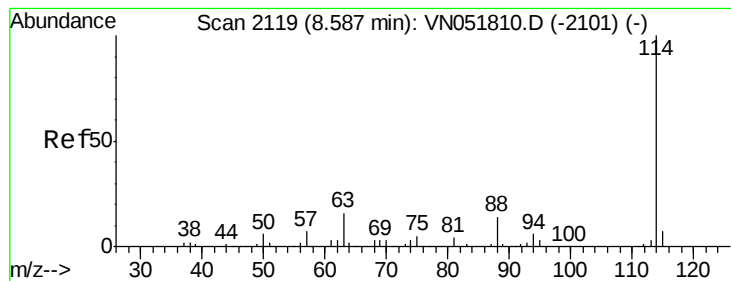

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 8.59 min Scan# 2119

Delta R.T. 0.00 min

Lab File: VN051882.D

Acq: 16 Oct 2018 9:33

Instrument :

MSVOA_N

ClientSampleId :

VN1016MBL01


Tgt Ion:114 Resp: 1237807

Ion Ratio Lower Upper

114 100

63 16.8 0.0 38.6




88 14.0 0.0 30.6

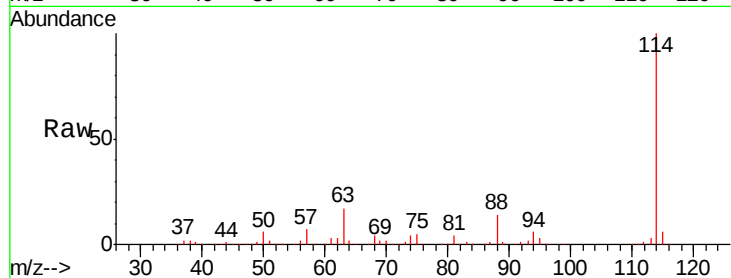

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN0

Ion 87.90 (87.60 to 88.60): VN0

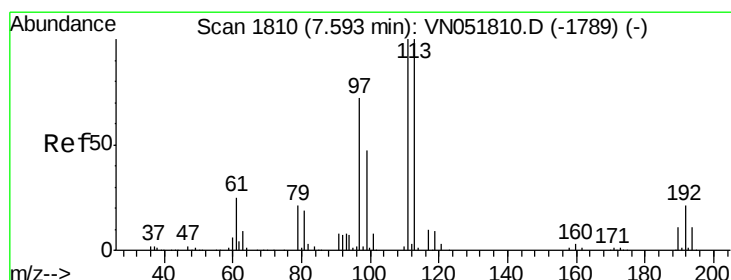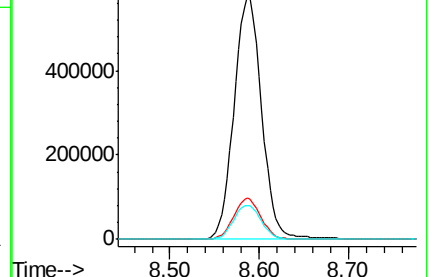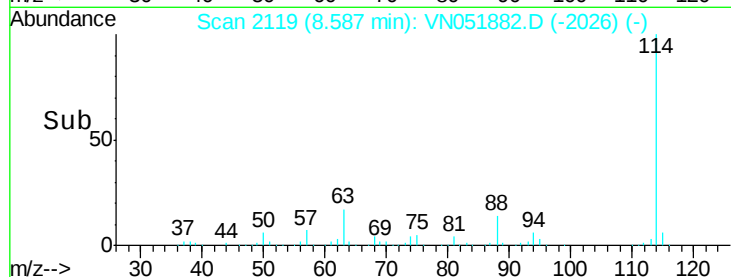

#35

Dibromofluoromethane

Concen: 50.00 ug/l

RT: 7.59 min Scan# 1810

Delta R.T. 0.00 min

Lab File: VN051882.D

Acq: 16 Oct 2018 9:33


Tgt Ion:113 Resp: 463549

Ion Ratio Lower Upper

113 100

111 102.9 82.6 123.8



192 21.3 18.0 27.0

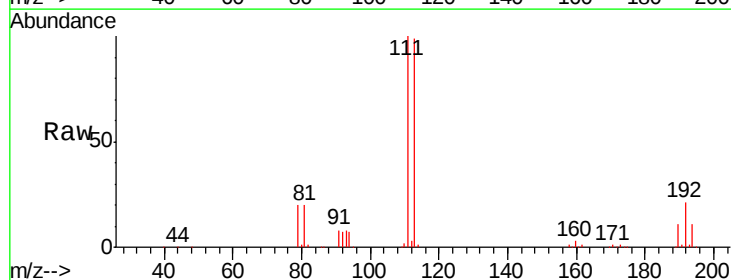


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

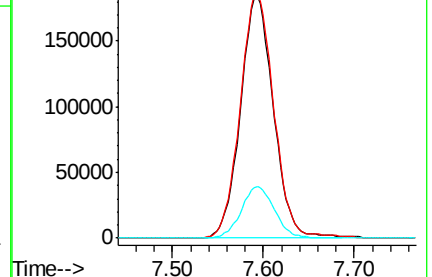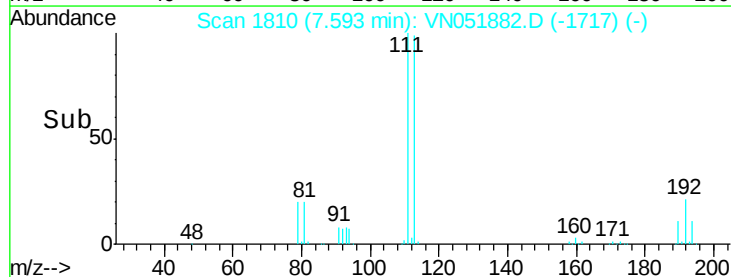

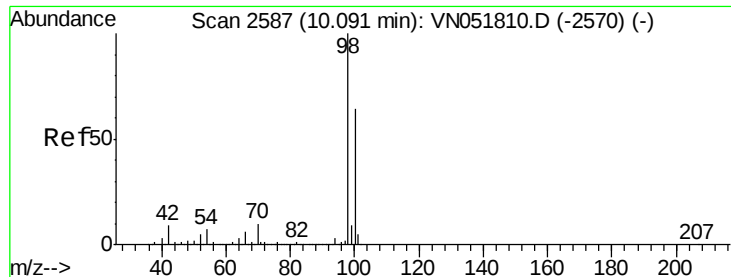

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.09 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN051882.D

Acq: 16 Oct 2018 9:33

Instrument :

MSVOA_N

ClientSampled :


VN1016MBL01

Tgt Ion: 98 Resp: 1680951

Ion Ratio Lower Upper




98 100

100 63.5 51.5 77.3

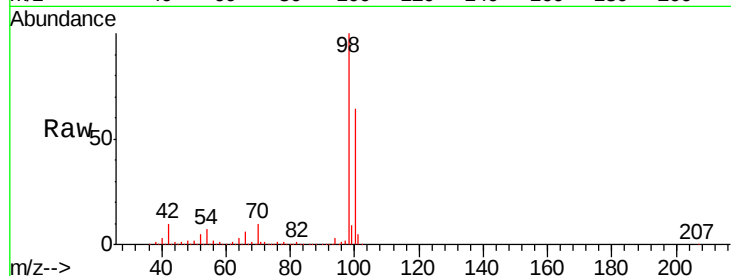

Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN

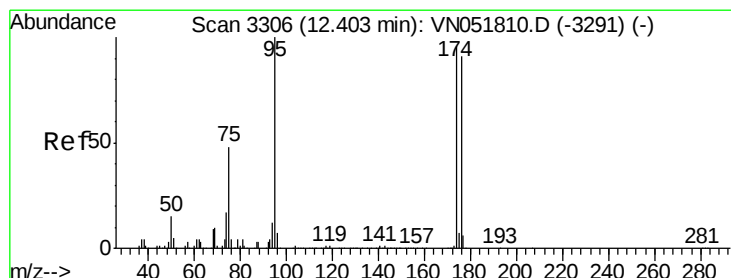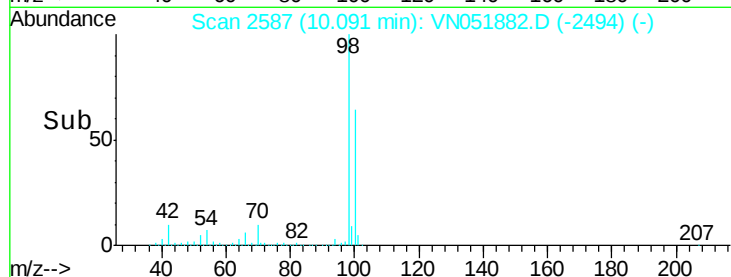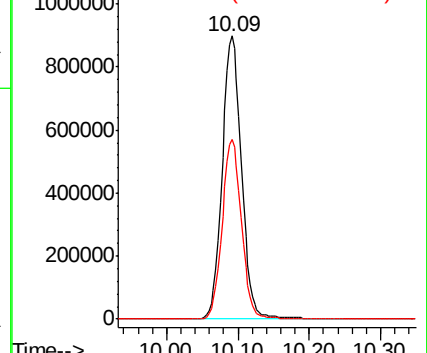

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.00 min

Lab File: VN051882.D

Acq: 16 Oct 2018 9:33


Tgt Ion: 95 Resp: 462099

Ion Ratio Lower Upper

95 100

174 96.1 0.0 183.0



176 92.0 0.0 178.8

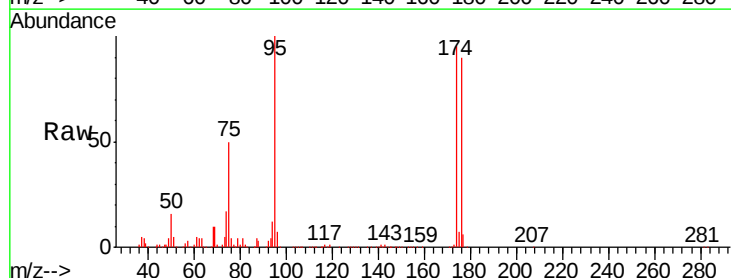


Abundance Ion 94.90 (94.60 to 95.60): VN0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

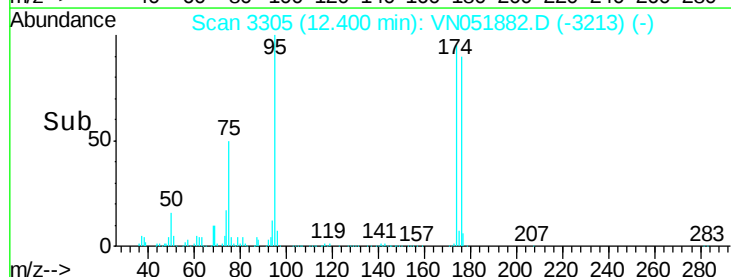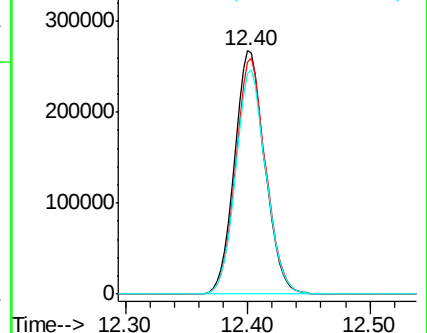


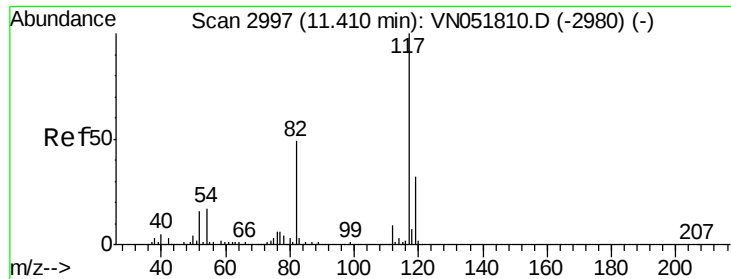




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. -0.00 min
Lab File: VN051882.D
Acq: 16 Oct 2018 9:33

Instrument :
MSVOA_N
ClientSampleId :
VN1016MBL01

Tgt Ion:117 Resp: 1051462
Ion Ratio Lower Upper
117 100
82 50.0 42.6 64.0
119 32.7 25.8 38.6

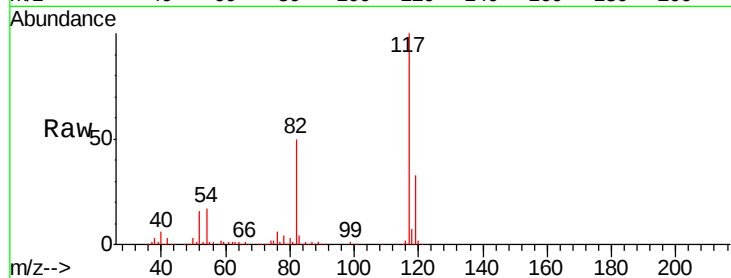


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VN0
Ion 118.90 (118.60 to 119.60): V

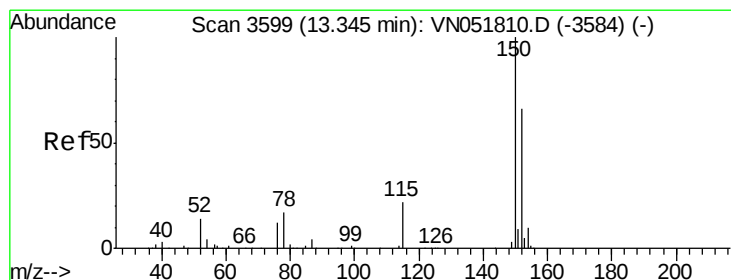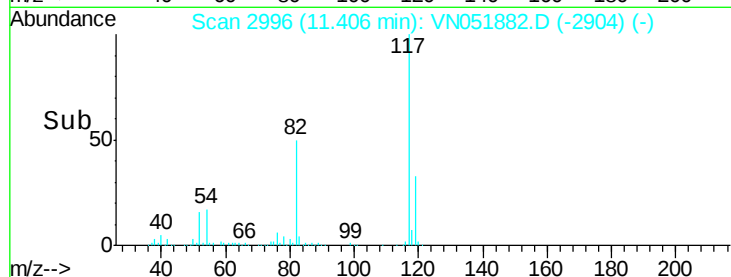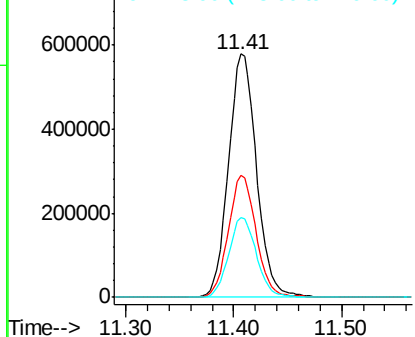

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.35 min Scan# 3599
Delta R.T. 0.00 min
Lab File: VN051882.D
Acq: 16 Oct 2018 9:33

Tgt Ion:152 Resp: 345201
Ion Ratio Lower Upper
152 100
115 56.0 27.8 83.4
150 158.5 0.0 351.4

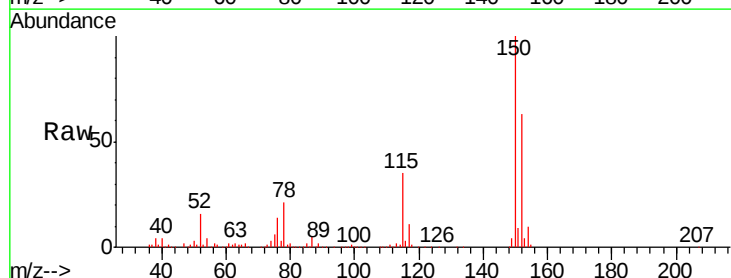

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

