

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN101618\
 Data File : VN051888.D
 Acq On : 16 Oct 2018 12:00
 Operator : MD\SY
 Sample : PB113865ZHE#03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 PB113865ZHE#03

Quant Time: Oct 17 04:00:55 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101118W.M
 Quant Title : SW846 8260
 QLast Update : Fri Oct 12 09:51:20 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	816634	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1176948	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1031645	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	344836	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	444216	56.91	ug/l	0.00
Spiked Amount 50.000			Recovery	=	113.82%	
35) Dibromofluoromethane	7.59	113	439653	60.08	ug/l	0.00
Spiked Amount 50.000			Recovery	=	120.16%	
50) Toluene-d8	10.09	98	1607460	58.94	ug/l	0.00
Spiked Amount 50.000			Recovery	=	117.88%	
62) 4-Bromofluorobenzene	12.40	95	445618	47.34	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.68%	
Target Compounds						
16) Acetone	3.82	43	10749	6.39	ug/l	91
20) Methylene Chloride	4.55	84	8750	1.26	ug/l #	79
43) Isopropyl Acetate	8.17	43	252915	25.64	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN101618\
Data File : VN051888.D
Acq On : 16 Oct 2018 12:00
Operator : MD\SY
Sample : PB113865ZHE#03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
PB113865ZHE#03

Quant Time: Oct 17 04:00:55 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N101118W.M
Quant Title : SW846 8260
QLast Update : Fri Oct 12 09:51:20 2018
Response via : Initial Calibration

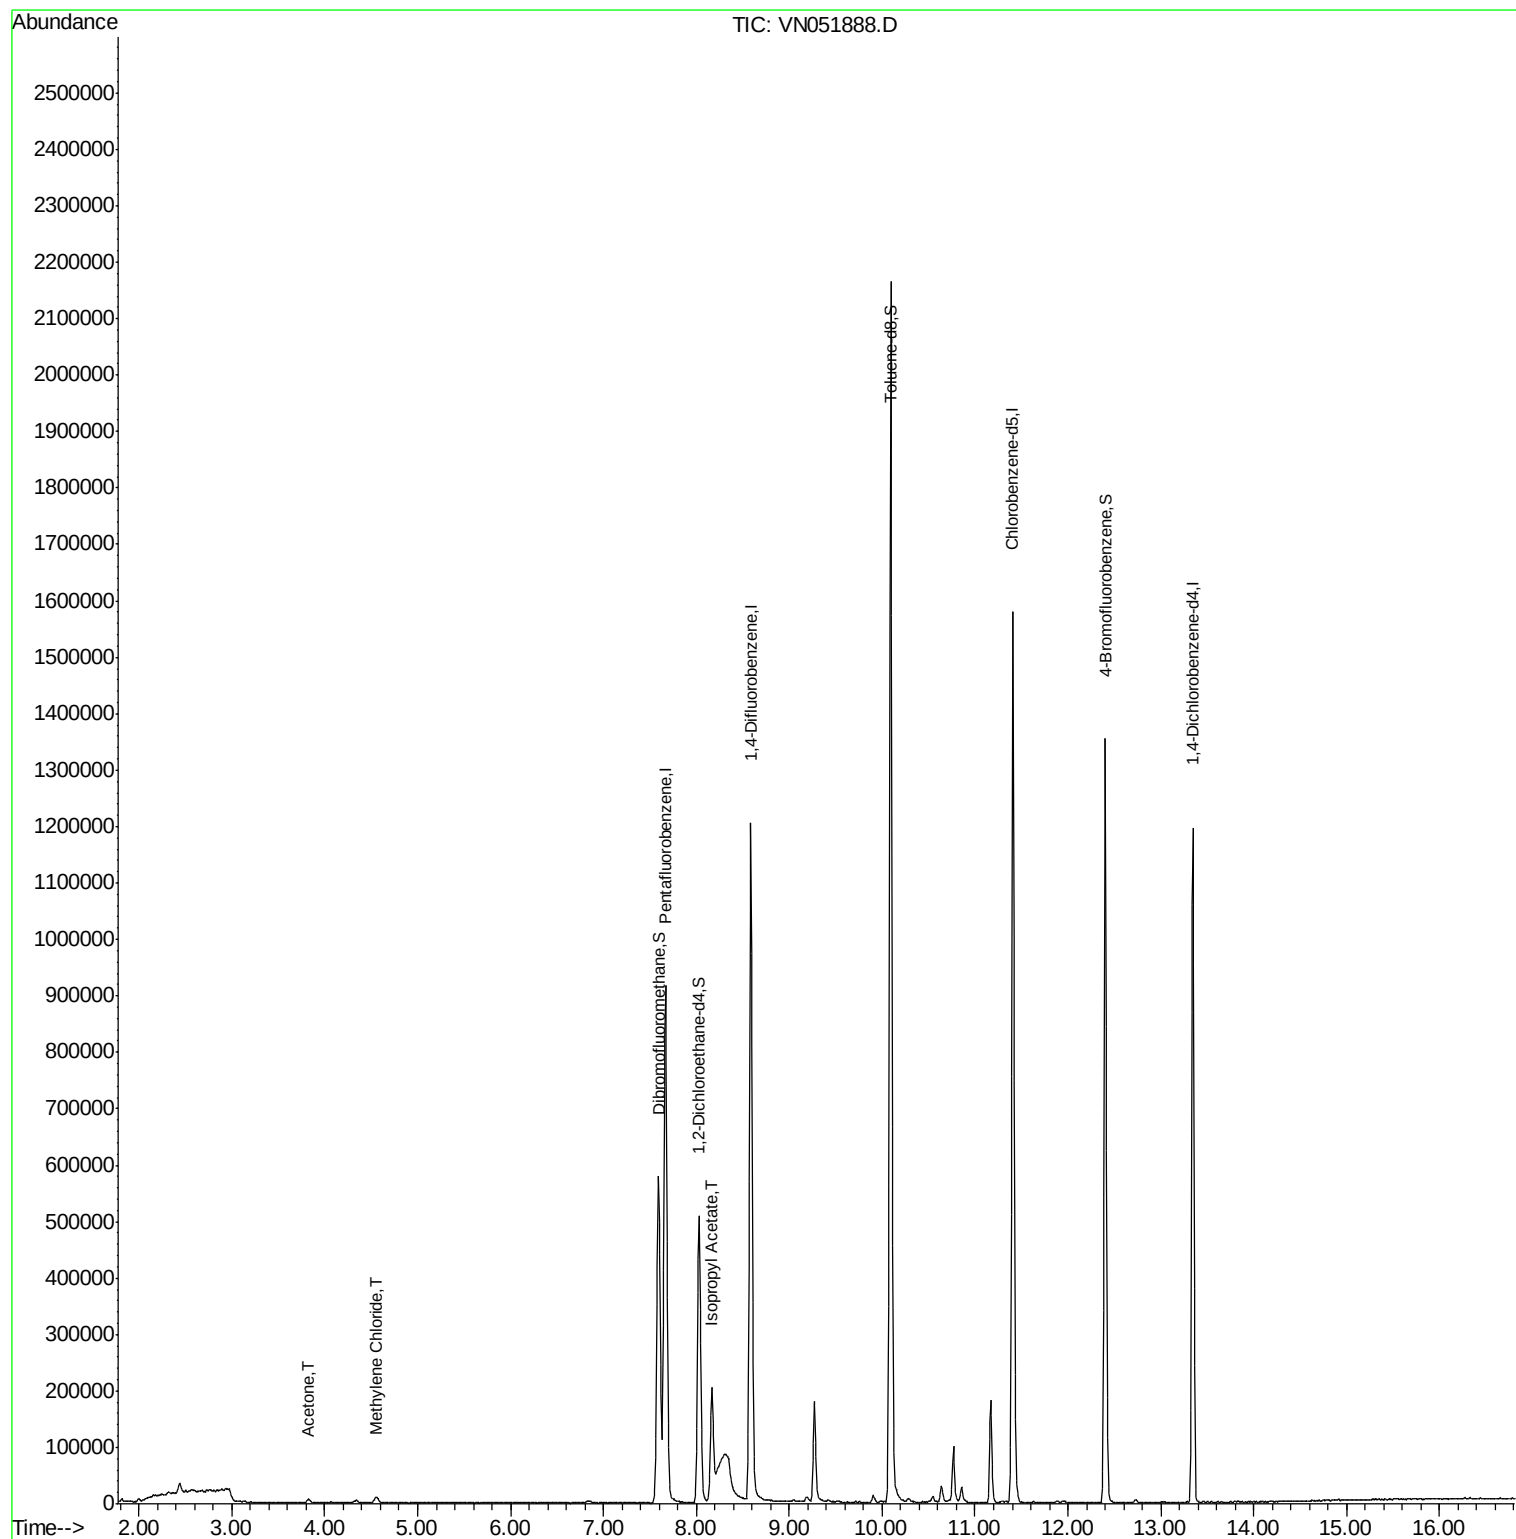

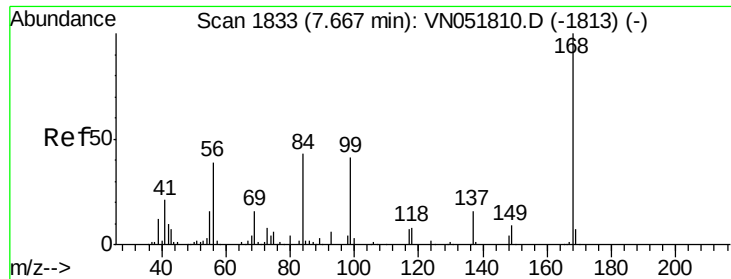

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.67 min Scan# 1834

Delta R.T. 0.00 min

Lab File: VN051888.D

Acq: 16 Oct 2018 12:00

Instrument :

MSVOA_N

ClientSampleId :


PB113865ZHE#03

Tgt Ion:168 Resp: 816634

Ion Ratio Lower Upper

168 100

99 48.8 39.6 59.4

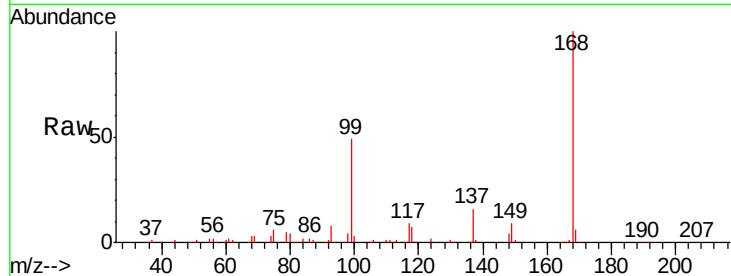

Abundance Ion 167.90 (167.60 to 168.60): VN051810.D (-1813) (-)

Ion 98.90 (98.60 to 99.60): VN051810.D (-1813) (-)

7.67



300000

200000

100000

0

Time-->

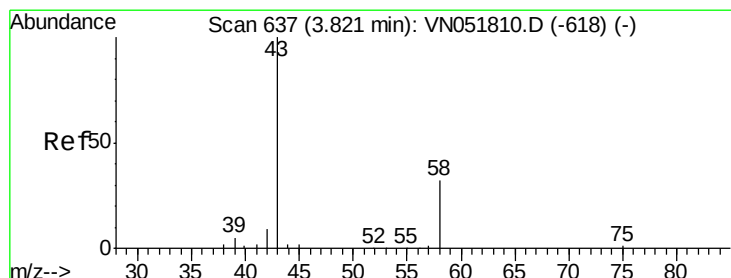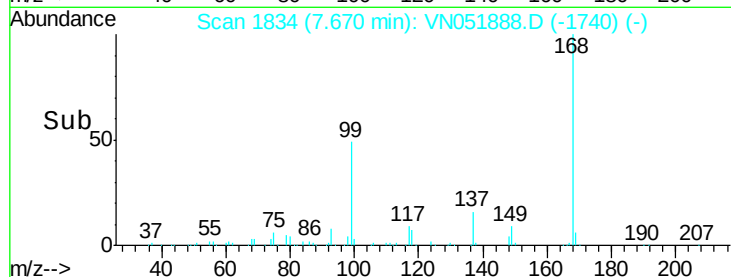

#16

Acetone

Concen: 6.39 ug/l

RT: 3.82 min Scan# 637

Delta R.T. -0.00 min

Lab File: VN051888.D


Acq: 16 Oct 2018 12:00

Tgt Ion: 43 Resp: 10749

Ion Ratio Lower Upper

43 100

58 39.1 27.2 40.8

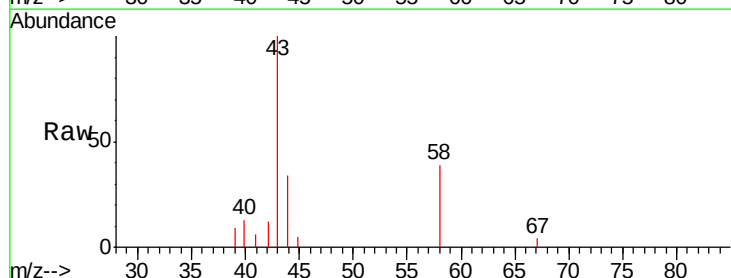

Abundance Ion 43.00 (42.70 to 43.70): VN051810.D (-618) (-)

Ion 58.00 (57.70 to 58.70): VN051810.D (-618) (-)

3.82

4000


3000


2000

1000

0

Time-->

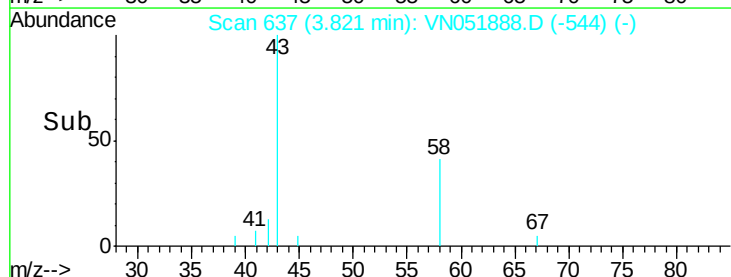


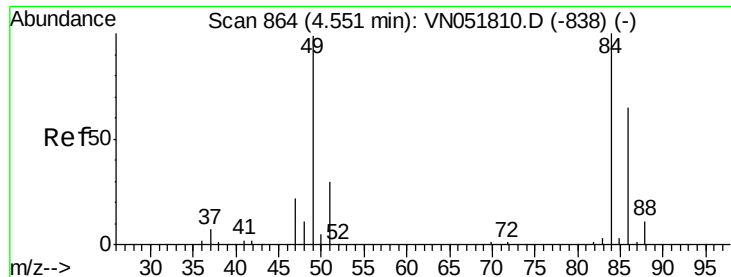




#20
Methylene Chloride
Concen: 1.26 ug/l
RT: 4.55 min Scan# 864
Delta R.T. -0.00 min
Lab File: VN051888.D
Acq: 16 Oct 2018 12:00

Instrument :
MSVOA_N
ClientSampleId :
PB113865ZHE#03

Tgt Ion: 84 Resp: 8750
Ion Ratio Lower Upper
84 100
49 88.3 93.2 139.8#
51 26.3 29.0 43.6#
86 50.8 49.8 74.8

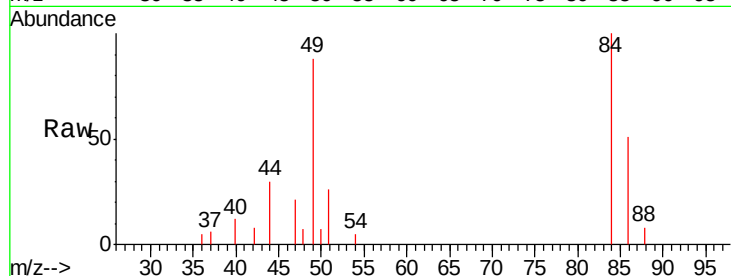


Abundance Ion 83.90 (83.60 to 84.60): VN051810.D (-838) (-)
Ion 48.90 (48.60 to 49.60): VN051810.D (-838) (-)
Ion 50.90 (50.60 to 51.60): VN051810.D (-838) (-)
Ion 85.90 (85.60 to 86.60): VN051810.D (-838) (-)

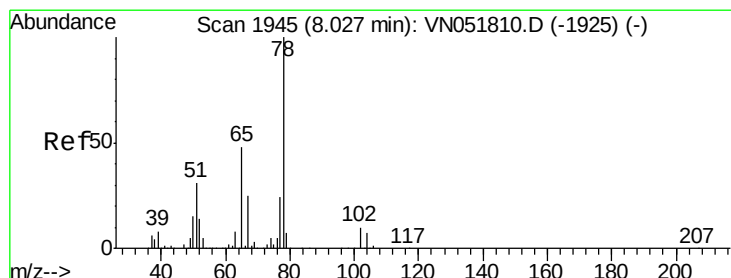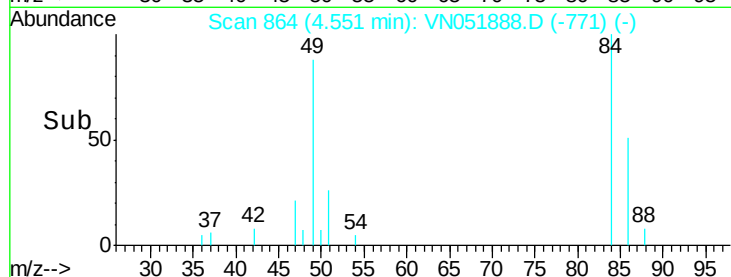
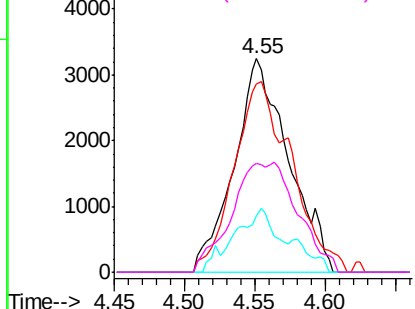



#33
1,2-Dichloroethane-d4
Concen: Below ug/l
RT: 8.03 min Scan# 1946
Delta R.T. 0.00 min
Lab File: VN051888.D
Acq: 16 Oct 2018 12:00

Tgt Ion: 65 Resp: 444216
Ion Ratio Lower Upper
65 100
67 51.4 0.0 110.4

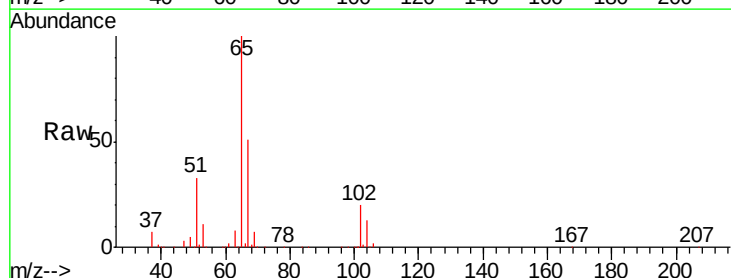

Abundance Ion 64.90 (64.60 to 65.60): VN051810.D (-1925) (-)
Ion 66.90 (66.60 to 67.60): VN051810.D (-1925) (-)

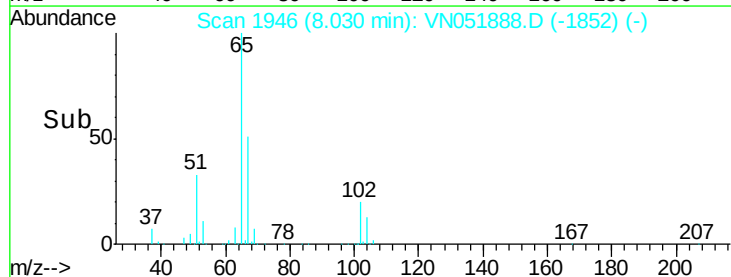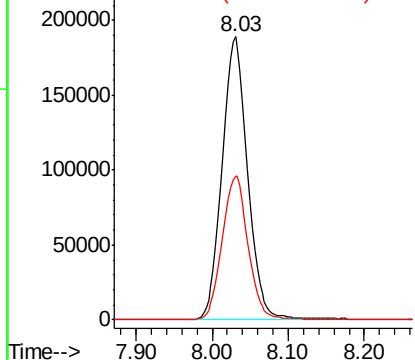


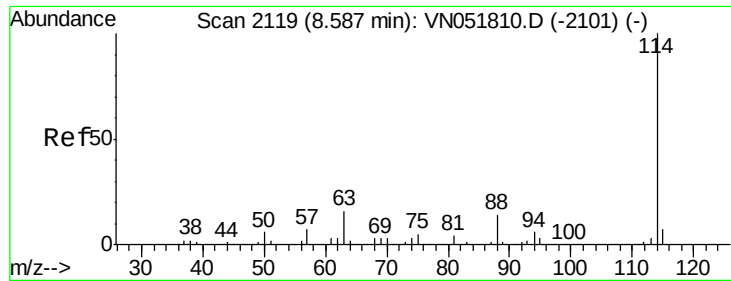




#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. -0.00 min
 Lab File: VN051888.D
 Acq: 16 Oct 2018 12:00

Instrument :
 MSVOA_N
 ClientSampleId :
 PB113865ZHE#03

Tgt Ion:114 Resp: 1176948
 Ion Ratio Lower Upper
 114 100
 63 16.3 0.0 38.6
 88 14.6 0.0 30.6

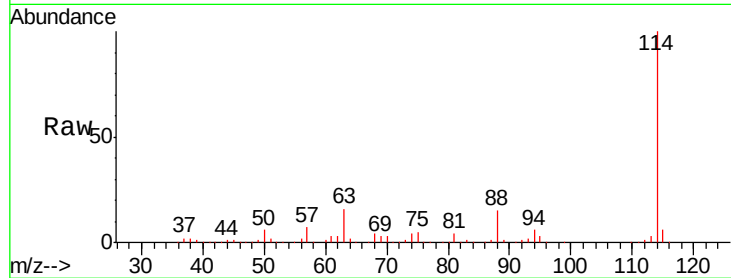


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

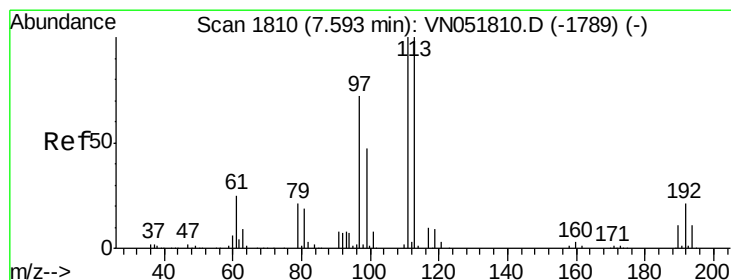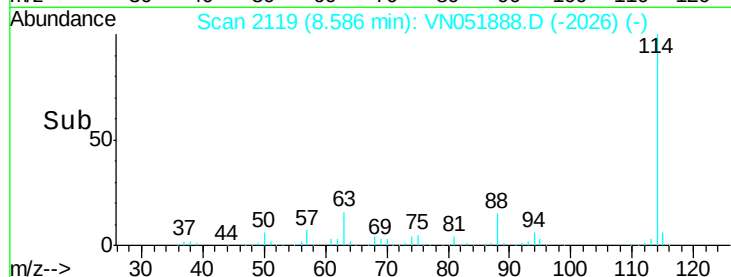
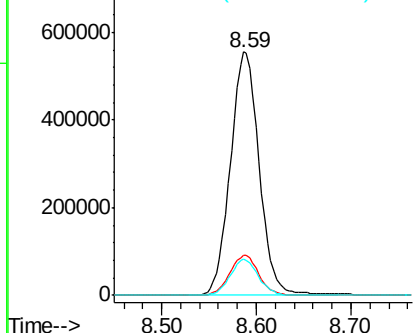



#35
 Dibromofluoromethane
 Concen: 50.00 ug/l
 RT: 7.59 min Scan# 1810
 Delta R.T. -0.00 min
 Lab File: VN051888.D
 Acq: 16 Oct 2018 12:00

Tgt Ion:113 Resp: 439653
 Ion Ratio Lower Upper
 113 100
 111 101.5 82.6 123.8
 192 21.1 18.0 27.0

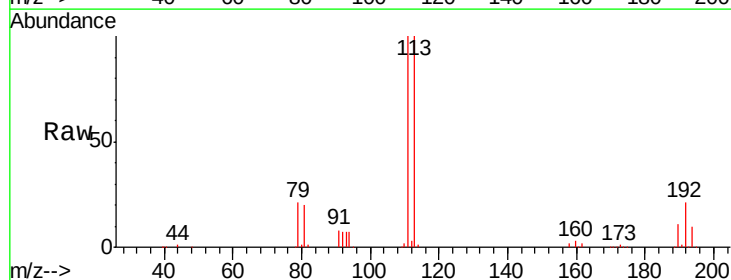

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

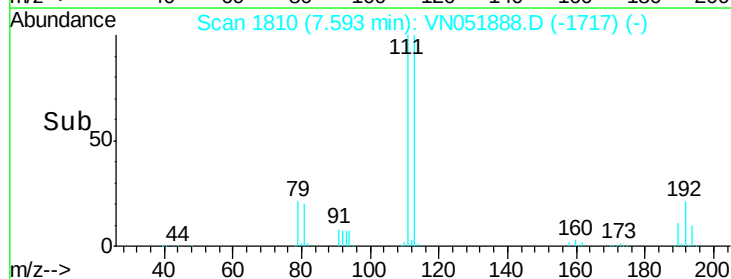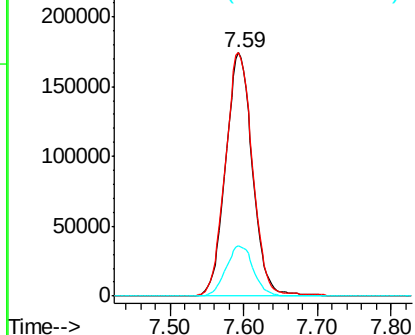

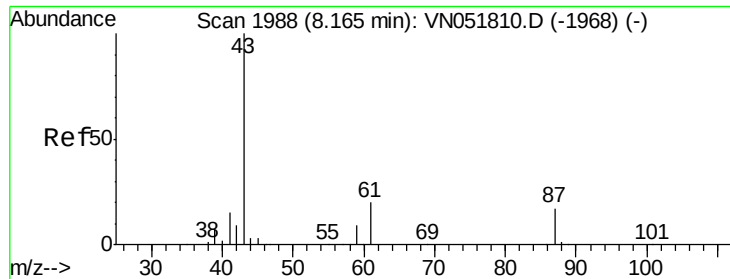

#43

Isopropyl Acetate

Concen: 25.64 ug/l

RT: 8.17 min Scan# 1989

Delta R.T. 0.00 min

Lab File: VN051888.D

Acq: 16 Oct 2018 12:00

Instrument :

MSVOA_N

ClientSampleId :

PB113865ZHE#03


Tgt Ion: 43 Resp: 252915

Ion Ratio Lower Upper

43 100

61 19.4 17.5 26.3




87 16.2 11.3 16.9

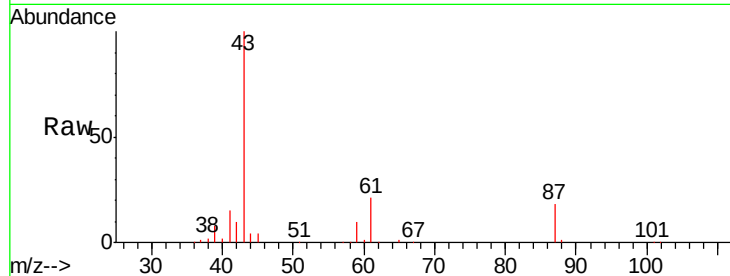

Abundance Ion 43.00 (42.70 to 43.70): VN051810.D (-1968) (-)

Ion 61.00 (60.70 to 61.70): VN051810.D (-1968) (-)

Ion 87.00 (86.70 to 87.70): VN051810.D (-1968) (-)

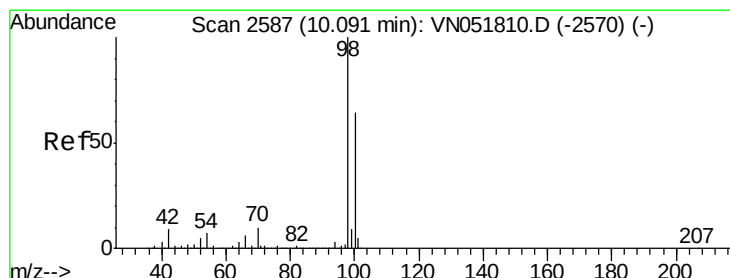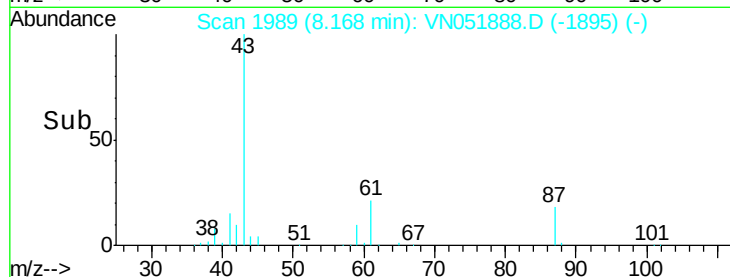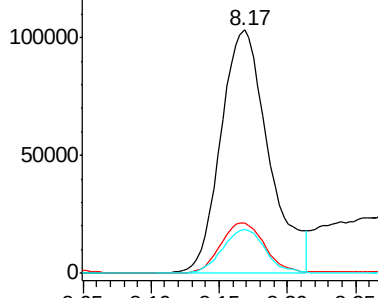

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.09 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN051888.D


Acq: 16 Oct 2018 12:00

Tgt Ion: 98 Resp: 1607460

Ion Ratio Lower Upper



98 100


100 64.1 51.5 77.3

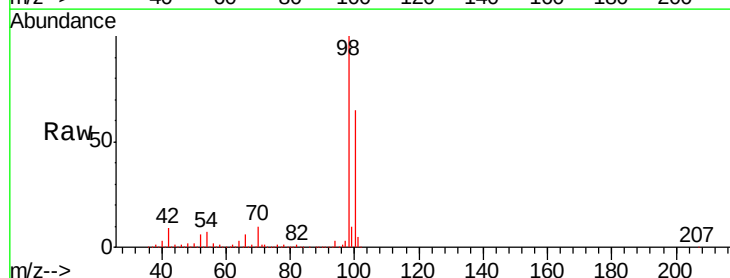

Abundance Ion 98.00 (97.70 to 98.70): VN051810.D (-2570) (-)

Ion 100.00 (99.70 to 100.70): VN051810.D (-2570) (-)

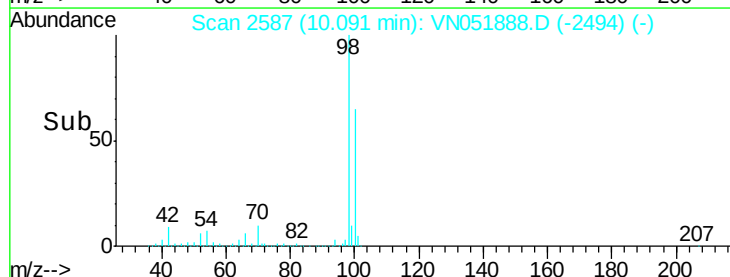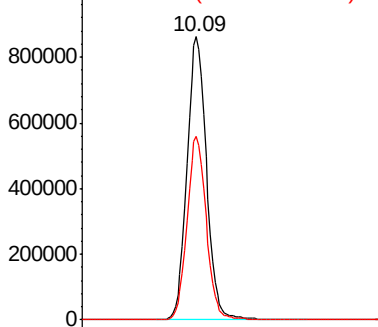

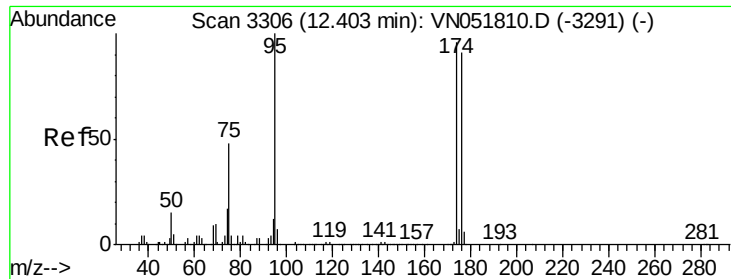

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 12.40 min Scan# 3306

Delta R.T. -0.00 min

Lab File: VN051888.D

Acq: 16 Oct 2018 12:00

Instrument :

MSVOA_N

ClientSampleId :

PB113865ZHE#03


Tgt Ion: 95 Resp: 445618

Ion Ratio Lower Upper

95 100

174 96.5 0.0 183.0




176 93.2 0.0 178.8

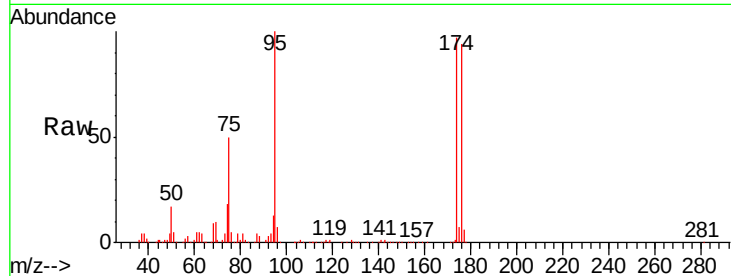

Abundance Ion 94.90 (94.60 to 95.60): VN051810.D (-3291) (-)

Ion 173.80 (173.50 to 174.50): VN051810.D (-3291) (-)

Ion 175.80 (175.50 to 176.50): VN051810.D (-3291) (-)

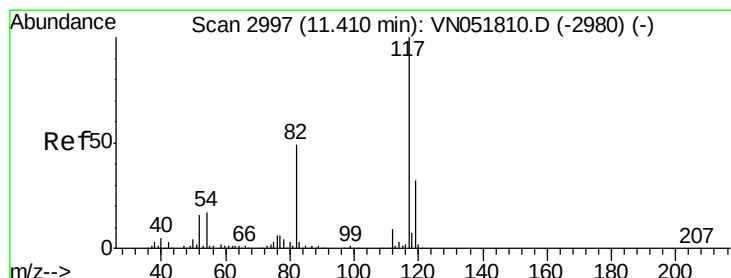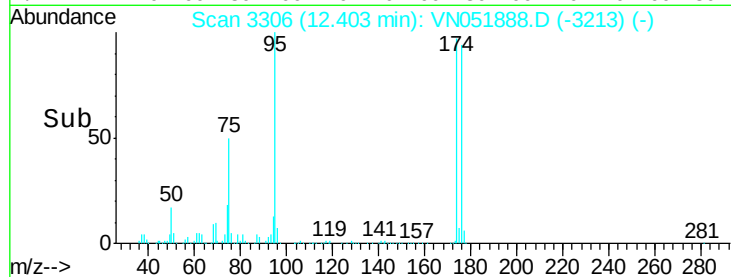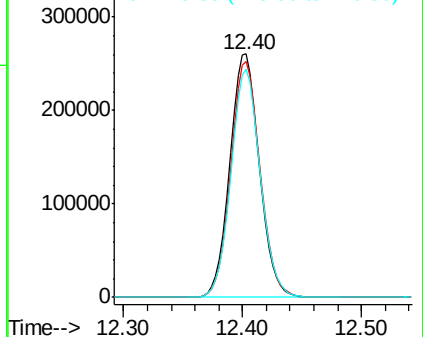

#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 11.41 min Scan# 2997

Delta R.T. -0.00 min

Lab File: VN051888.D

Acq: 16 Oct 2018 12:00


Tgt Ion: 117 Resp: 1031645

Ion Ratio Lower Upper

117 100

82 48.7 42.6 64.0



119 32.5 25.8 38.6

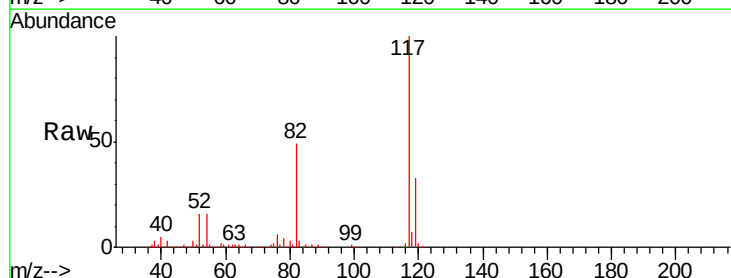


Abundance Ion 116.90 (116.60 to 117.60): VN051810.D (-2980) (-)

Ion 82.00 (81.70 to 82.70): VN051810.D (-2980) (-)

Ion 118.90 (118.60 to 119.60): VN051810.D (-2980) (-)

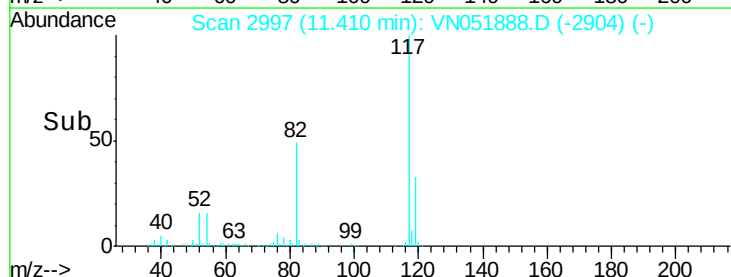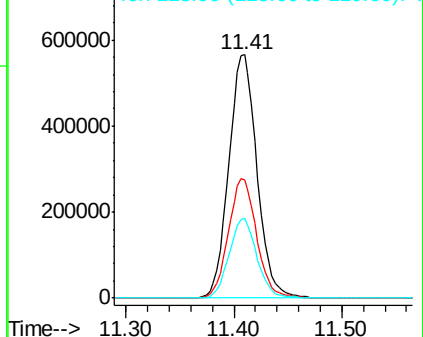

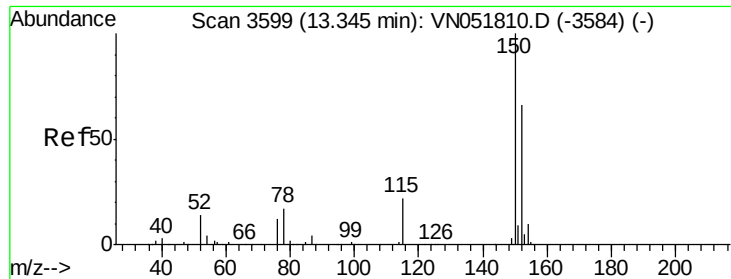

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.35 min Scan# 3599

Delta R.T. -0.00 min

Lab File: VN051888.D


Acq: 16 Oct 2018 12:00

Instrument :

MSVOA_N

ClientSampleId :

PB113865ZHE#03

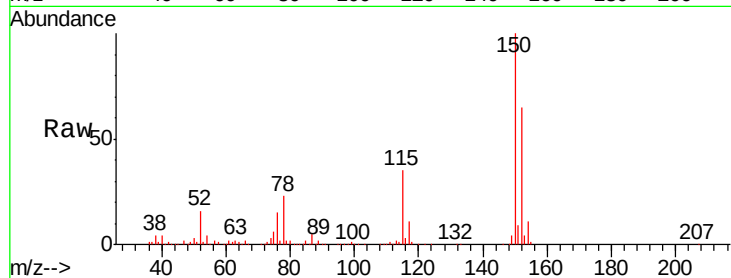


Tgt Ion:152 Resp: 344836

Ion Ratio Lower Upper

152 100

115 54.3 27.8 83.4

150 157.0 0.0 351.4

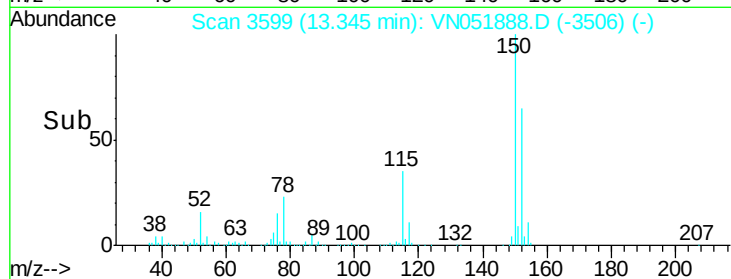

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

