


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN101618\  
Data File : VN051879.D  
Acq On : 16 Oct 2018 8:04  
Operator : MD\SY  
Sample : BFB  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 28

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N101118W.M  
Title : SW846 8260  
Last Update : Fri Oct 12 09:51:20 2018

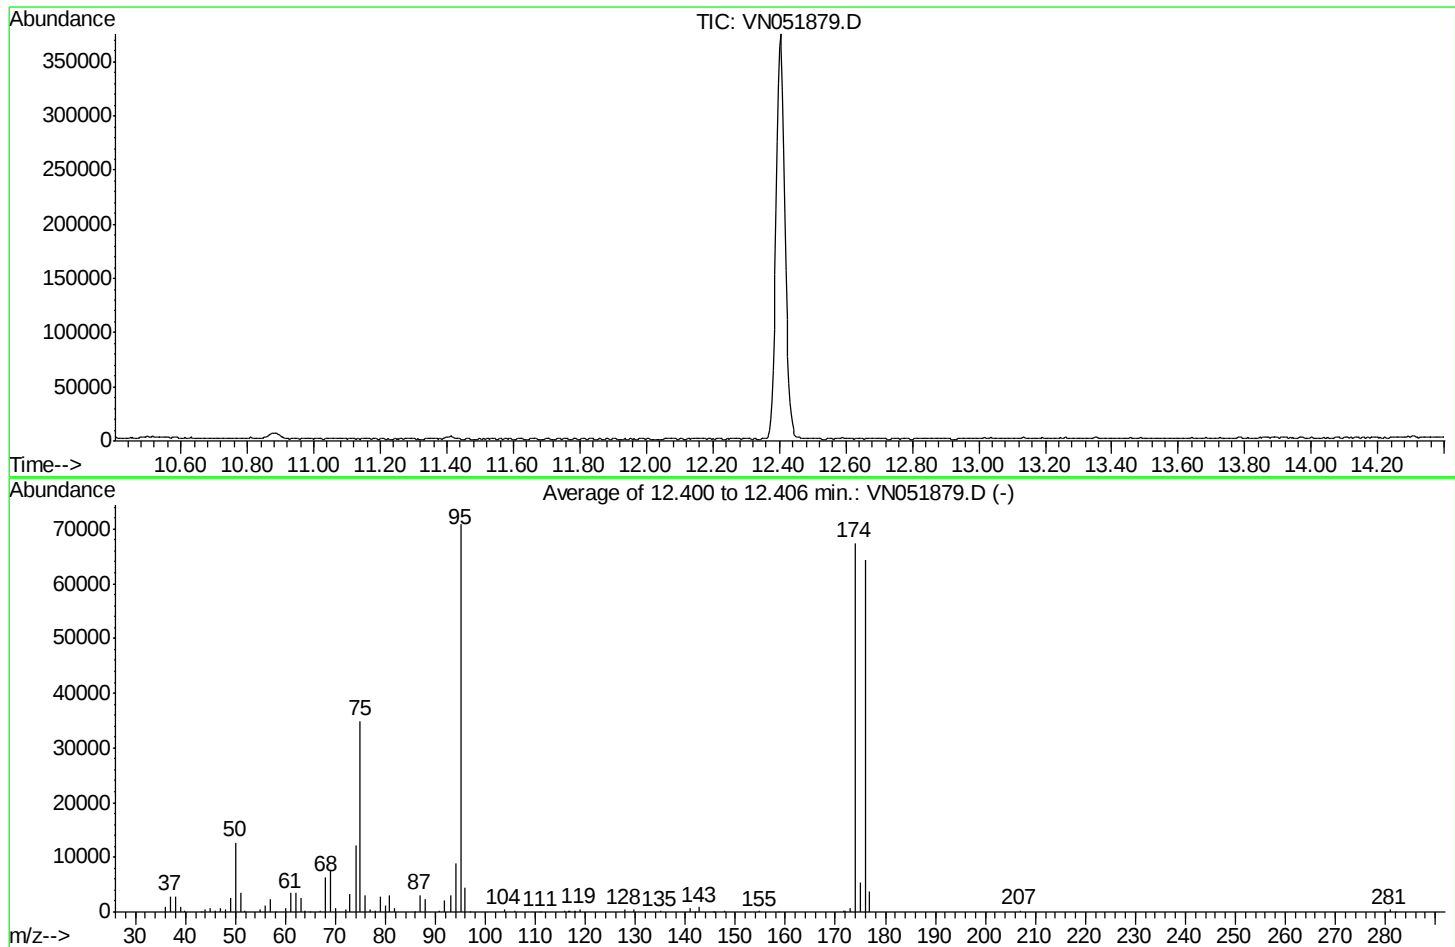

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 17.8      | 12637   | PASS             |
| 75          | 95           | 30           | 60           | 49.3      | 34925   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 70858   | PASS             |
| 96          | 95           | 5            | 9            | 6.3       | 4476    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.1       | 734     | PASS             |
| 174         | 95           | 50           | 100          | 95.1      | 67413   | PASS             |
| 175         | 174          | 5            | 9            | 8.0       | 5416    | PASS             |
| 176         | 174          | 95           | 101          | 95.4      | 64314   | PASS             |
| 177         | 176          | 5            | 9            | 5.9       | 3776    | PASS             |