

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN101620\
 Data File : VN064180.D
 Acq On : 16 Oct 2020 21:29
 Operator : JC/MD
 Sample : L4406-08
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 JC-02-101420-A

Quant Time: Oct 17 01:33:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101420W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 15 01:16:44 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	314832	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	668526	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	690033	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	242204	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	281956	62.88	ug/l	0.00
Spiked Amount			Recovery	=	125.76%	
35) Dibromofluoromethane	7.55	113	223459	48.29	ug/l	0.00
Spiked Amount			Recovery	=	96.58%	
50) Toluene-d8	10.06	98	876756	50.22	ug/l	0.00
Spiked Amount			Recovery	=	100.44%	
62) 4-Bromofluorobenzene	12.38	95	290275	48.37	ug/l	0.00
Spiked Amount			Recovery	=	96.74%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	4.73	59	206	0.415	ug/l #	71
13) Acrolein	3.66	56	91	0.223	ug/l	94
16) Acetone	3.78	43	20759	15.608	ug/l	96
18) Methyl Acetate	4.28	43	2904	0.870	ug/l	97
20) Methylene Chloride	4.50	84	5275	1.282	ug/l	89
29) Tetrahydrofuran	7.16	42	659	0.551	ug/l #	44
31) Cyclohexane	7.62	56	8278	1.670	ug/l #	23
36) 1,1-Dichloropropene	7.63	75	28516	4.425	ug/l #	49
38) Carbon Tetrachloride	7.63	117	33281	4.803	ug/l #	17
43) Isopropyl Acetate	8.13	43	101605	10.707	ug/l #	88
48) Methyl methacrylate	9.15	41	5349	1.220	ug/l #	10
49) 1,4-Dioxane	9.24	88	145	2.178	ug/l #	1
51) 4-Methyl-2-Pentanone	9.96	43	10673	1.901	ug/l	97
54) cis-1,3-Dichloropropene	9.87	75	45663	5.707	ug/l #	77
56) Ethyl methacrylate	10.33	69	170	2.321	ug/l #	26
57) 1,3-Dichloropropane	10.74	76	7544	0.922	ug/l #	43
58) 2-Chloroethyl Vinyl ether	9.90	63	32	12.227	ug/l #	48
59) 2-Hexanone	10.74	43	115233	32.661	ug/l #	53
68) m/p-Xylenes	11.60	106	72	2.199	ug/l #	52
70) Styrene	11.94	104	150	2.045	ug/l #	24
71) Bromoform	12.36	173	116	2.255	ug/l #	30
74) N-amyl acetate	12.01	43	4067	0.619	ug/l #	49
76) 1,2,3-Trichloropropane	12.38	75	153580	27.028	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.38	75	153580	82.575	ug/l #	12
86) p-Isopropyltoluene	13.32	119	93	0.668	ug/l #	1
95) Naphthalene	15.12	128	448	3.832	ug/l #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN101620\
Data File : VN064180.D
Acq On : 16 Oct 2020 21:29
Operator : JC/MD
Sample : L4406-08
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
JC-02-101420-A

Quant Time: Oct 17 01:33:13 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N101420W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 15 01:16:44 2020
Response via : Initial Calibration

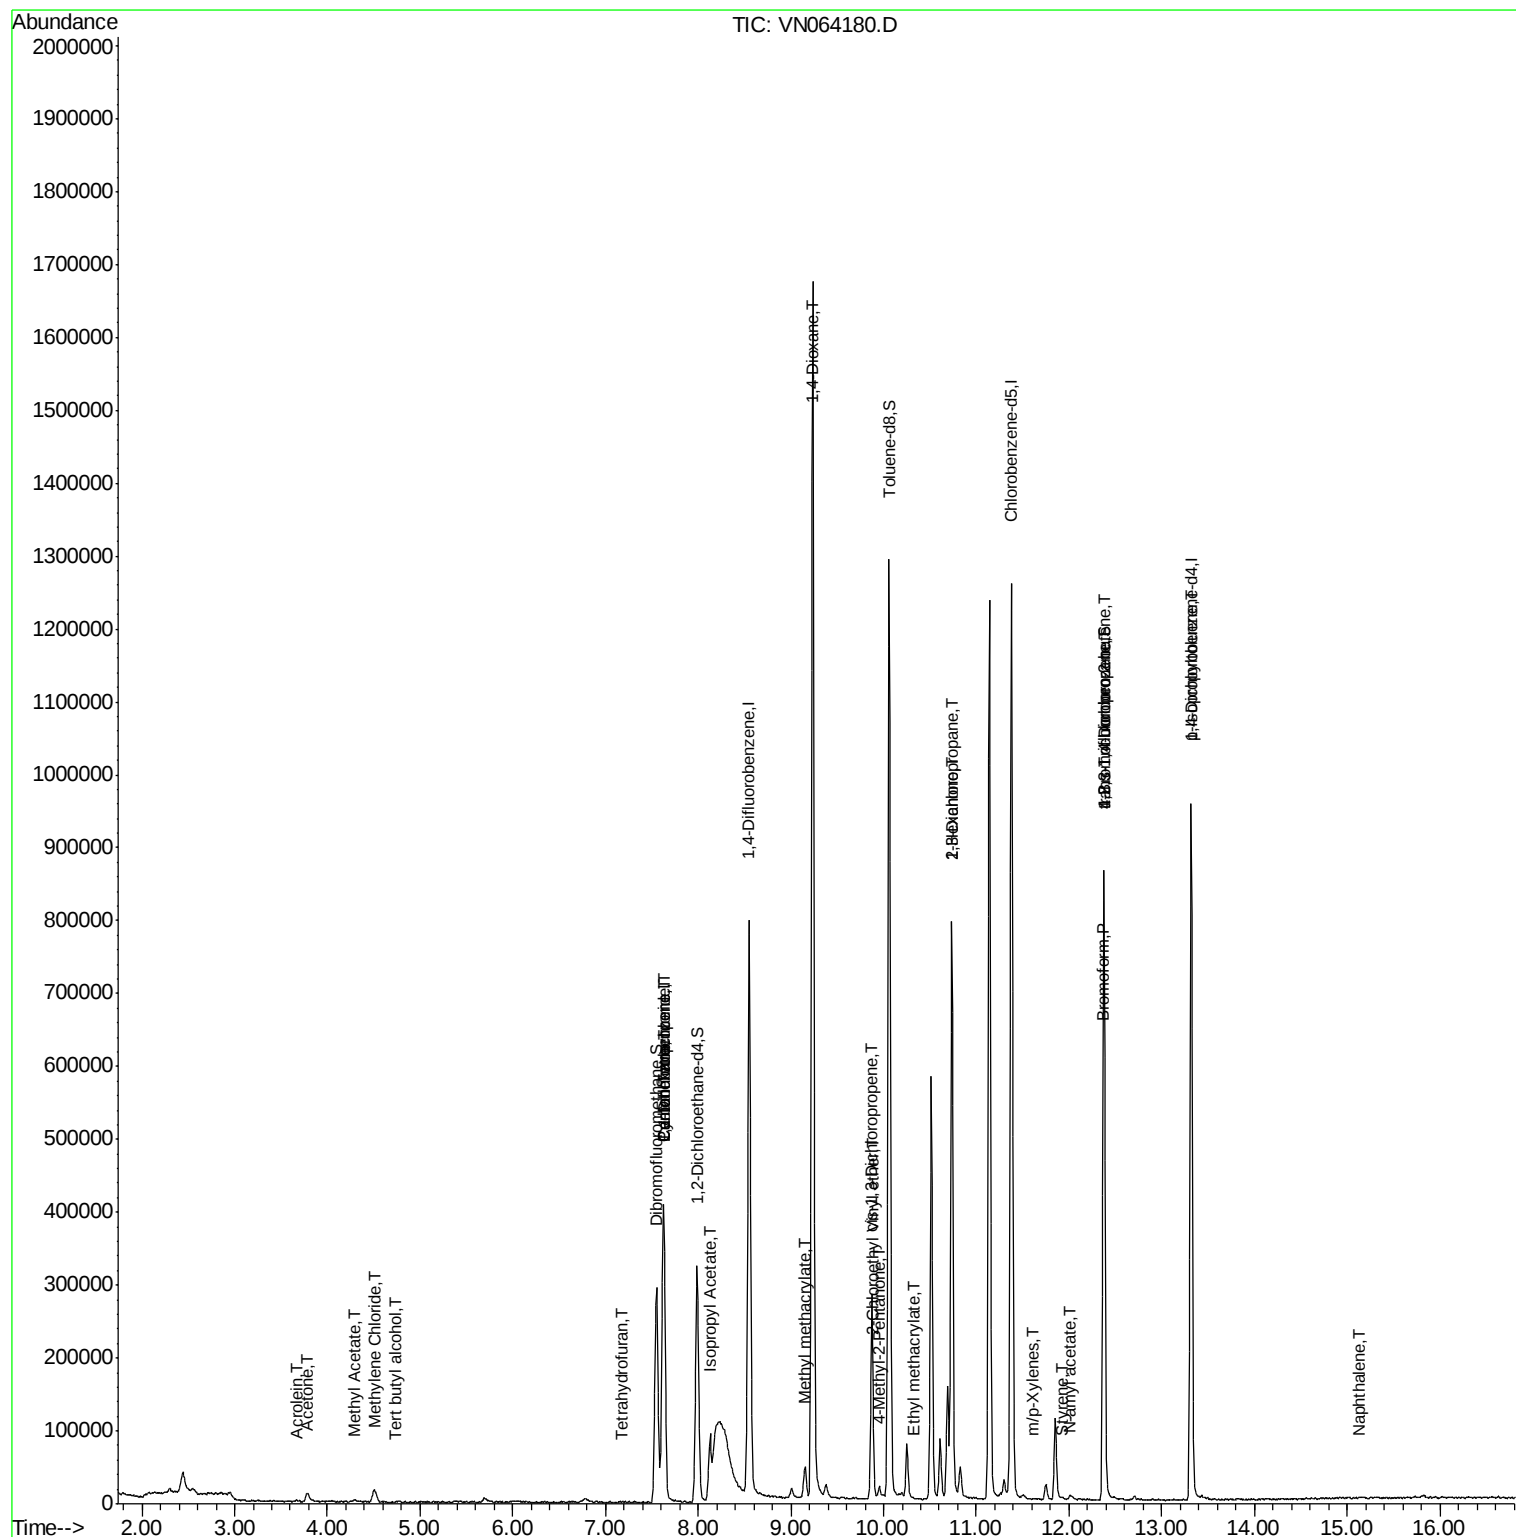



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN064180.D

Acq: 16 Oct 2020 21:29

Instrument :

MSVOA_N

ClientSampleId :


JC-02-101420-A

Tot Ion:168 Resp: 314832

Ion Ratio Lower Upper

168 100

99 62.1 43.6 65.4



Abundance Ion 167.90 (167.60 to 168.60): VN064180.D (-1738) (-)

Ion 98.90 (98.60 to 99.60): VN064180.D (-1738) (-)

7.63



150000

100000

50000

0

Time--> 7.50 7.60 7.70



#11

Tert butyl alcohol

Concen: 0.415 ug/l

RT: 4.73 min Scan# 929

Delta R.T. -0.00 min

Lab File: VN064180.D


Acq: 16 Oct 2020 21:29

Tgt Ion: 59 Resp: 206

Ion Ratio Lower Upper

59 100

57 0.0 8.9 13.3#



Abundance Ion 59.00 (58.70 to 59.70): VN064180.D (-837) (-)

Ion 57.00 (56.70 to 57.70): VN064180.D (-837) (-)

4.73

250

200


150


100

50

0

Time--> 4.71 4.72 4.73 4.74





#13

Acrolein

Concen: 0.223 ug/l

RT: 3.66 min Scan# 598

Delta R.T. 0.10 min

Lab File: VN064180.D

Acq: 16 Oct 2020 21:29

Instrument :

MSVOA_N

ClientSampleId :





JC-02-101420-A

Tot Ion: 56 Resp: 91

Ion Ratio Lower Upper

56 100

55 74.7 55.8 83.6

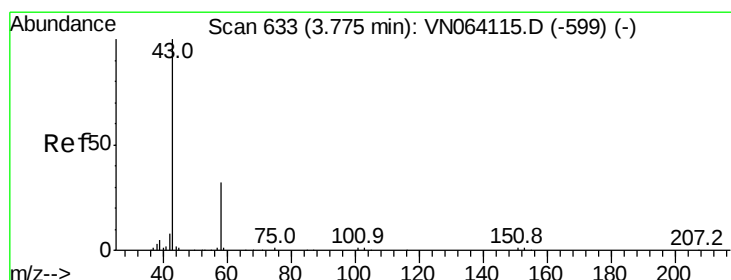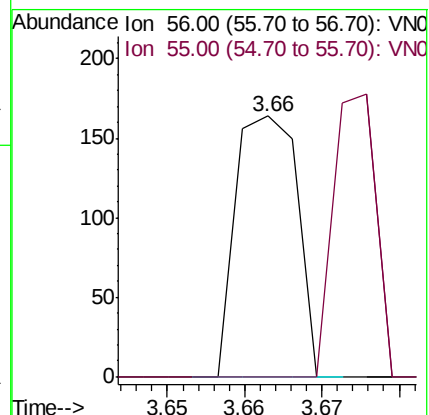

#16

Acetone

Concen: 15.608 ug/l

RT: 3.78 min Scan# 635

Delta R.T. 0.01 min

Lab File: VN064180.D




Acq: 16 Oct 2020 21:29


Tgt Ion: 43 Resp: 20759

Ion Ratio Lower Upper

43 100

58 29.5 25.2 37.8



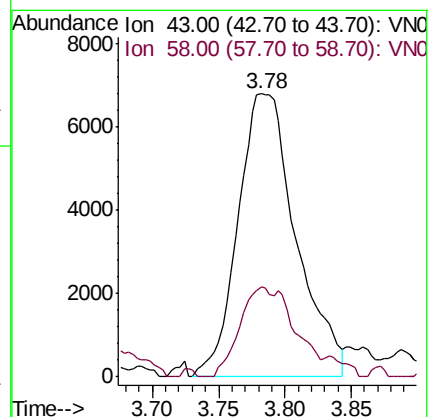





#18
Methyl Acetate
Concen: 0.870 ug/l
RT: 4.28 min Scan# 791
Delta R.T. 0.01 min
Lab File: VN064180.D
Acq: 16 Oct 2020 21:29




Instrument :
MSVOA_N
ClientSampleId :
JC-02-101420-A


Tot Ion: 43 Resp: 2904
Ion Ratio Lower Upper
43 100
74 22.9 19.7 29.5

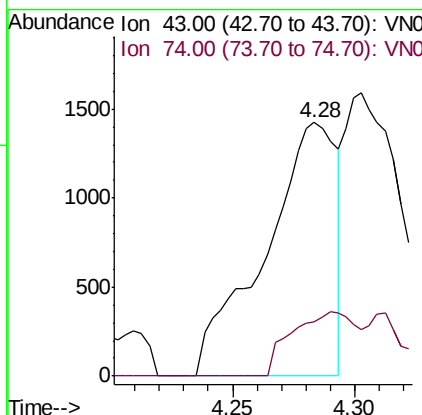

#20
Methylene Chloride
Concen: 1.282 ug/l
RT: 4.50 min Scan# 858
Delta R.T. -0.00 min
Lab File: VN064180.D
Acq: 16 Oct 2020 21:29

Tgt Ion: 84 Resp: 5275
Ion Ratio Lower Upper
84 100
49 140.8 97.4 146.0
51 43.1 29.7 44.5
86 64.9 52.5 78.7



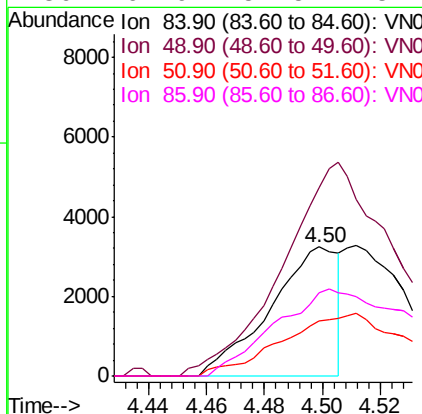





#29
Tetrahydrofuran
Concen: 0.551 ug/l
RT: 7.16 min Scan# 1687
Delta R.T. 0.00 min
Lab File: VN064180.D
Acq: 16 Oct 2020 21:29




Instrument :
MSVOA_N
ClientSampleId :
JC-02-101420-A


Tot Ion: 42 Resp: 659
Ion Ratio Lower Upper
42 100
72 16.7 37.8 56.6#
71 0.0 35.3 52.9#

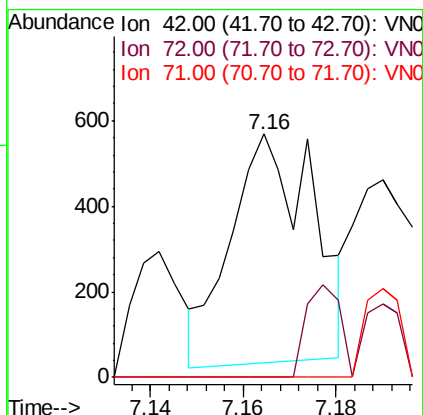

#31
Cyclohexane
Concen: 1.670 ug/l
RT: 7.62 min Scan# 1829
Delta R.T. 0.01 min
Lab File: VN064180.D
Acq: 16 Oct 2020 21:29

Tgt Ion: 56 Resp: 8278
Ion Ratio Lower Upper
56 100
69 171.7 27.8 41.6#
84 107.1 73.2 109.8



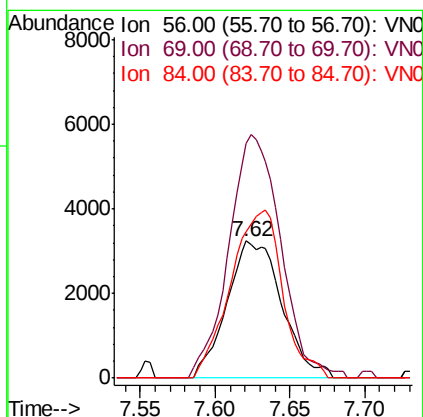



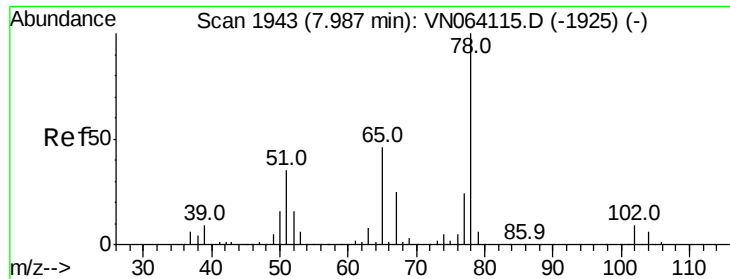

#33
 1,2-Dichloroethane-d4
 Concen: 62.882 ug/l
 RT: 7.99 min Scan# 1943
 Delta R.T. 0.00 min
 Lab File: VN064180.D
 Acq: 16 Oct 2020 21:29




Instrument :
 MSVOA_N
 ClientSampleId :
 JC-02-101420-A


Tot Ion: 65 Resp: 281956
 Ion Ratio Lower Upper
 65 100
 67 51.9 0.0 105.6

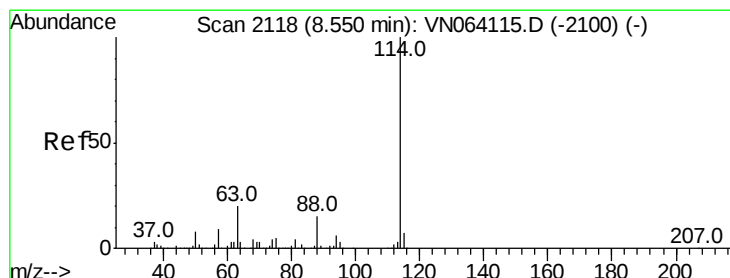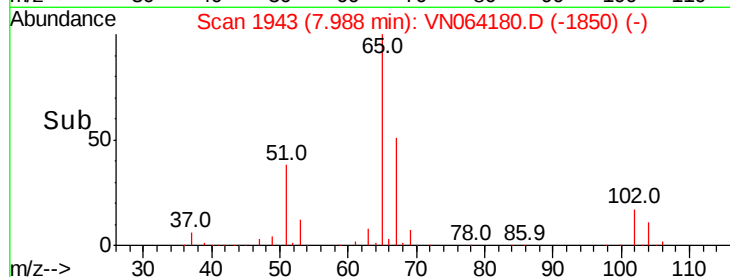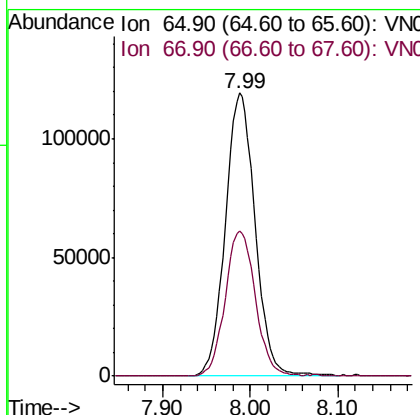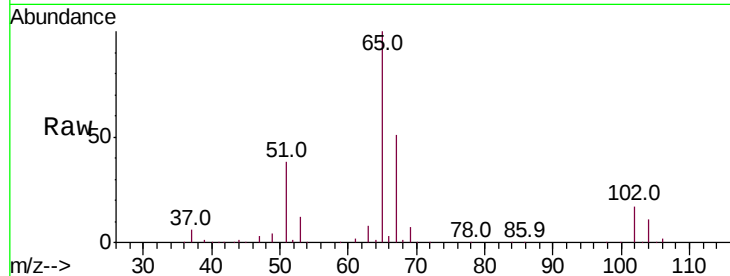

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2118
 Delta R.T. 0.00 min
 Lab File: VN064180.D
 Acq: 16 Oct 2020 21:29

Tgt Ion: 114 Resp: 668526
 Ion Ratio Lower Upper
 114 100
 63 22.0 0.0 41.0
 88 15.8 0.0 29.2


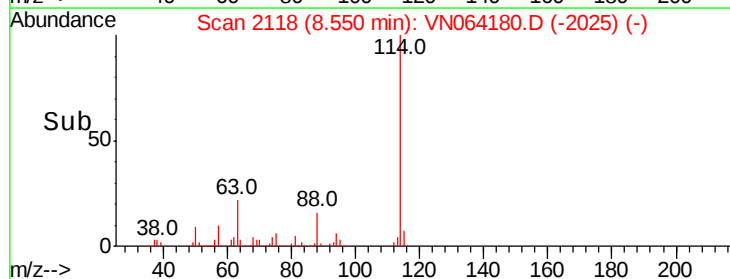
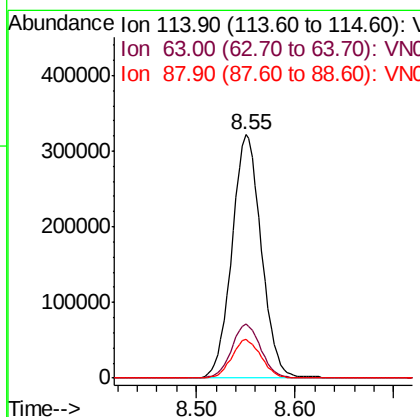
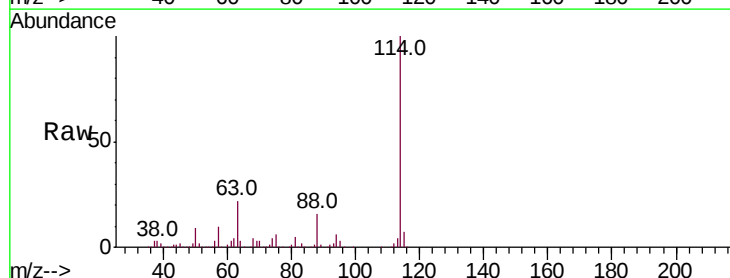




#35
 Dibromofluoromethane
 Concen: 48.292 ug/l
 RT: 7.55 min Scan# 1807
 Delta R.T. 0.00 min
 Lab File: VN064180.D
 Acq: 16 Oct 2020 21:29




Instrument :
 MSVOA_N
 ClientSampleId :
 JC-02-101420-A


Tot Ion	Ratio	Lower	Upper
113	100		
111	101.7	81.9	122.9
192	17.7	14.3	21.5

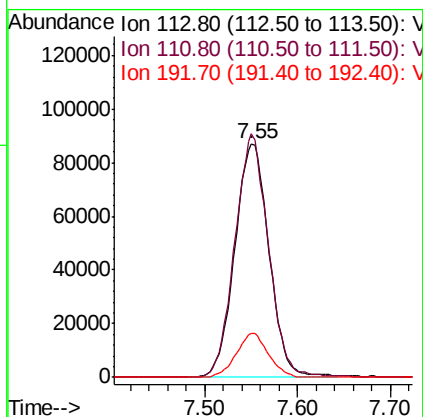

#36
 1,1-Dichloropropene
 Concen: 4.425 ug/l
 RT: 7.63 min Scan# 1831
 Delta R.T. -0.13 min
 Lab File: VN064180.D
 Acq: 16 Oct 2020 21:29

Tgt Ion	Ratio	Lower	Upper
75	100		
110	8.2	17.8	53.3#
77	0.1	24.9	37.3#

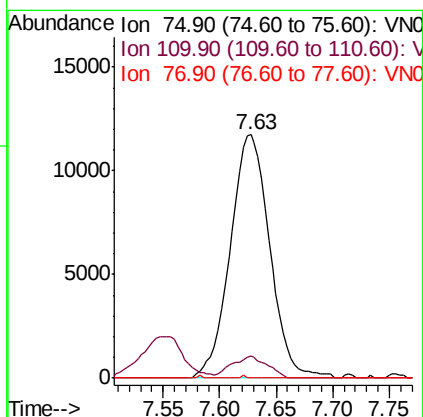


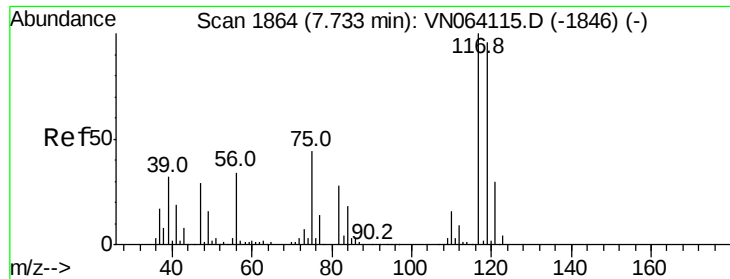




#38
Carbon Tetrachloride
Concen: 4.803 ug/l
RT: 7.63 min Scan# 1831
Delta R.T. -0.11 min
Lab File: VN064180.D
Acq: 16 Oct 2020 21:29

Instrument :
MSVOA_N
ClientSampleId :
JC-02-101420-A

Tot Ion:117 Resp: 33281
Ion Ratio Lower Upper
117 100
119 6.4 77.0 115.4#
121 0.0 24.2 36.4#

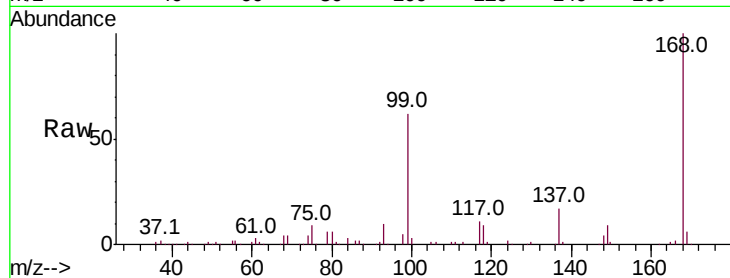


Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V

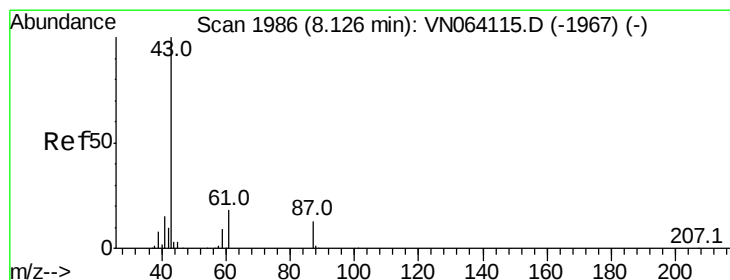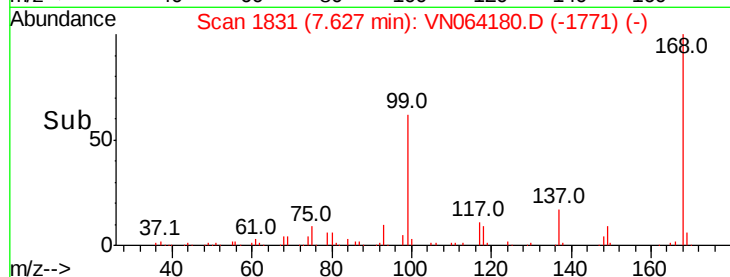
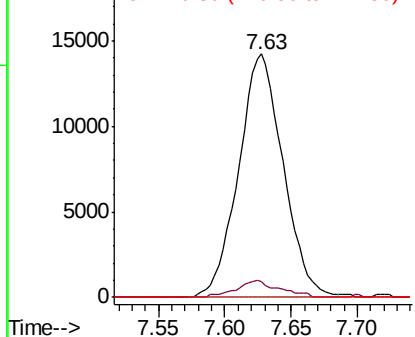



#43
Isopropyl Acetate
Concen: 10.707 ug/l
RT: 8.13 min Scan# 1987
Delta R.T. 0.00 min
Lab File: VN064180.D
Acq: 16 Oct 2020 21:29

Tgt Ion: 43 Resp: 101605
Ion Ratio Lower Upper
43 100
61 18.6 21.9 32.9#
87 12.5 11.0 16.4

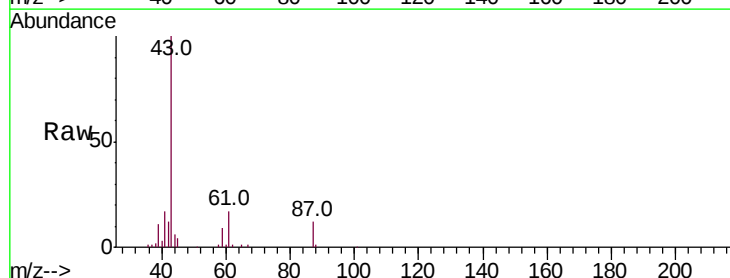

Abundance Ion 43.00 (42.70 to 43.70): V
Ion 61.00 (60.70 to 61.70): V
Ion 87.00 (86.70 to 87.70): V

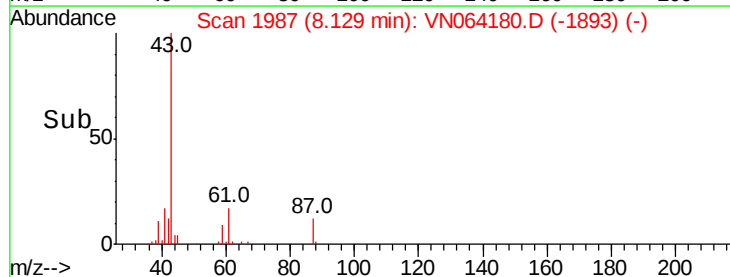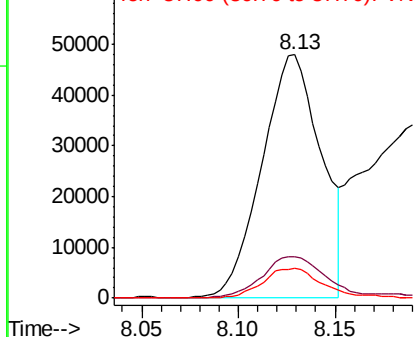







#48
Methvl methacrylate
Concen: 1.220 ug/l
RT: 9.15 min Scan# 2305
Delta R.T. -0.02 min
Lab File: VN064180.D
Acq: 16 Oct 2020 21:29

Instrument :
MSVOA_N
ClientSampleId :
JC-02-101420-A

Tot Ion: 41 Resp: 5349
Ion Ratio Lower Upper
41 100
69 0.0 71.4 107.2#
39 0.0 52.5 78.7#




Abundance Ion 41.00 (40.70 to 41.70): VNC
Ion 69.00 (68.70 to 69.70): VNC
Ion 39.00 (38.70 to 39.70): VNC


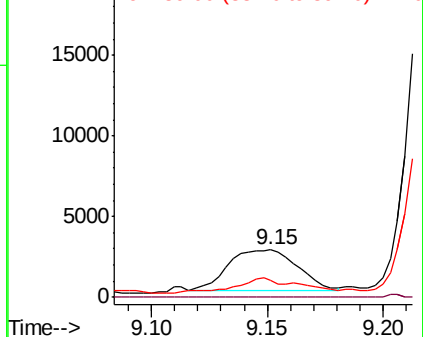



#49
1,4-Dioxane
Concen: 2.178 ug/l
RT: 9.24 min Scan# 2331
Delta R.T. 0.07 min
Lab File: VN064180.D
Acq: 16 Oct 2020 21:29

Tgt Ion: 88 Resp: 145
Ion Ratio Lower Upper
88 100
43 1137133.1 27.2 40.8#
58 7415.9 52.6 78.8#



Abundance Ion 88.00 (87.70 to 88.70): VNC
Ion 43.00 (42.70 to 43.70): VNC
Ion 58.00 (57.70 to 58.70): VNC




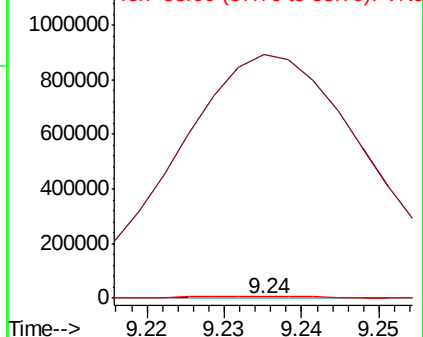




#50
Toluene-d8
Concen: 50.218 ug/l
RT: 10.06 min Scan# 2588
Delta R.T. 0.00 min
Lab File: VN064180.D
Acq: 16 Oct 2020 21:29




Instrument :
MSVOA_N
ClientSampleId :
JC-02-101420-A


Tot Ion: 98 Resp: 876756
Ion Ratio Lower Upper
98 100
100 62.1 50.8 76.2

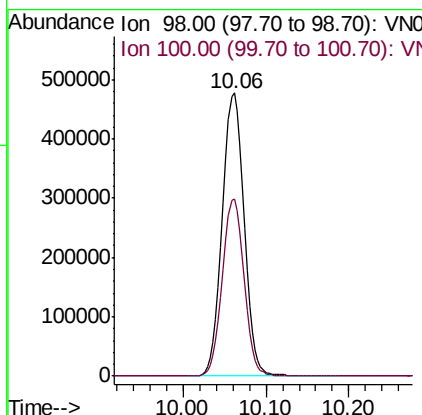

#51
4-Methyl-2-Pentanone
Concen: 1.901 ug/l
RT: 9.96 min Scan# 2555
Delta R.T. 0.00 min
Lab File: VN064180.D
Acq: 16 Oct 2020 21:29

Tgt Ion: 43 Resp: 10673
Ion Ratio Lower Upper
43 100
58 37.3 31.2 46.8


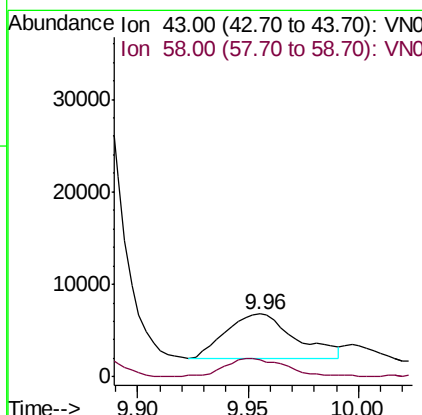






#54
 cis-1,3-Dichloropropene
 Concen: 5.707 ug/l
 RT: 9.87 min Scan# 2530
 Delta R.T. 0.07 min
 Lab File: VN064180.D
 Acq: 16 Oct 2020 21:29




Instrument :
 MSVOA_N
 ClientSampleId :
 JC-02-101420-A


Tot Ion: 75 Resp: 45663
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.2 37.8#
 39 48.6 39.8 59.8

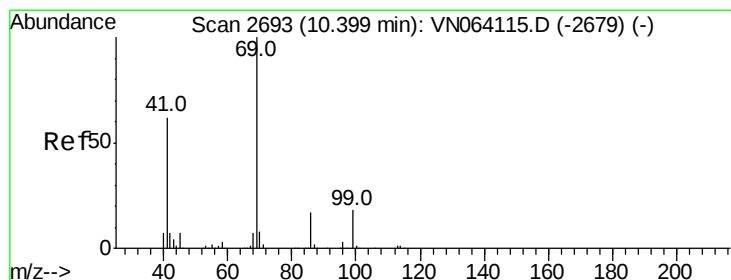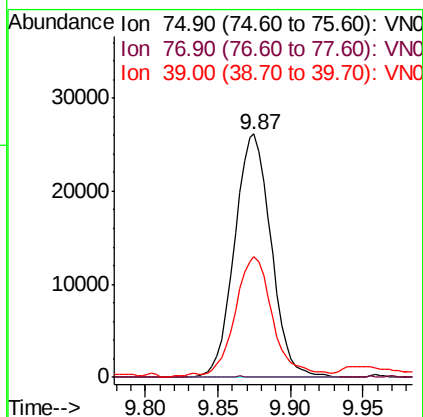

#56
 Ethyl methacrylate
 Concen: 2.321 ug/l
 RT: 10.33 min Scan# 2672
 Delta R.T. -0.07 min
 Lab File: VN064180.D
 Acq: 16 Oct 2020 21:29

Tgt Ion: 69 Resp: 170
 Ion Ratio Lower Upper
 69 100
 41 0.0 49.3 73.9#
 39 0.0 32.7 49.1#

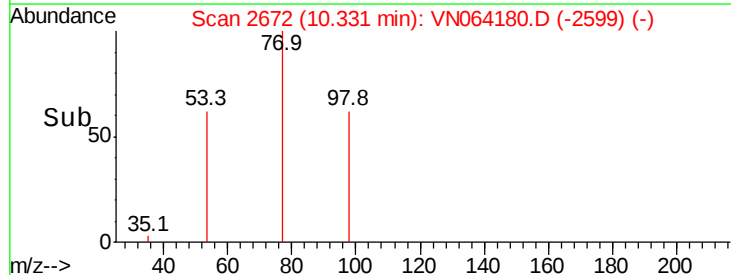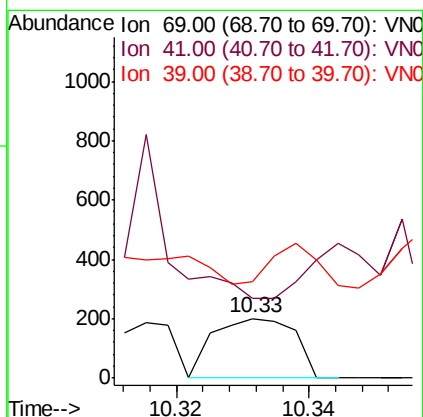



#57

1,3-Dichloropropane

Concen: 0.922 ug/l

RT: 10.74 min Scan# 2798

Delta R.T. 0.06 min





Lab File: VN064180.D

Acq: 16 Oct 2020 21:29

Instrument :
MSVOA_N
ClientSampleId :
JC-02-101420-A

Tot Ion: 76 Resp: 7544

Ion	Ratio	Lower	Upper
76	100		
78	0.8	26.1	39.1#

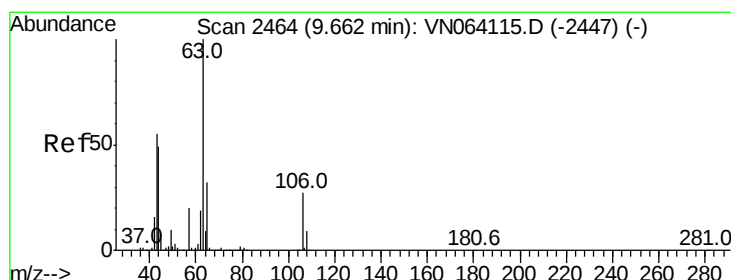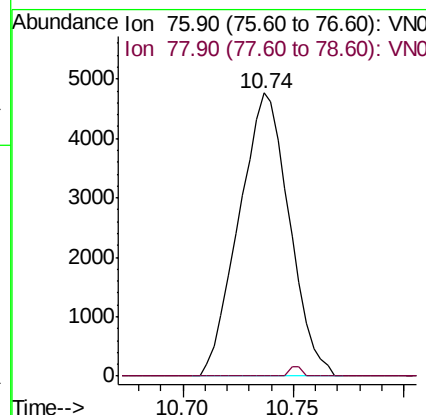

#58

2-Chloroethyl Vinyl ether

Concen: 12.227 ug/l

RT: 9.90 min Scan# 2537




Delta R.T. 0.24 min


Lab File: VN064180.D

Acq: 16 Oct 2020 21:29

Tgt Ion: 63 Resp: 32

Ion	Ratio	Lower	Upper
63	100		
106	0.0	21.8	32.6#



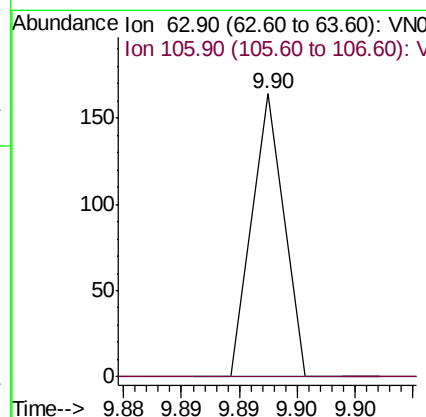





#59
2-Hexanone
Concen: 32.661 ug/l
RT: 10.74 min Scan# 2798
Delta R.T. 0.01 min
Lab File: VN064180.D
Acq: 16 Oct 2020 21:29




Instrument :
MSVOA_N
ClientSampleId :
JC-02-101420-A


Tot Ion: 43 Resp: 115233
Ion Ratio Lower Upper
43 100
58 20.7 27.2 81.6#

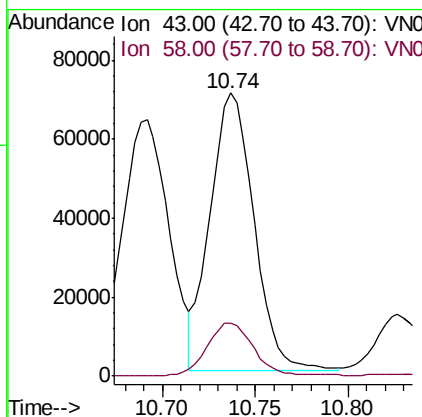

#62
4-Bromofluorobenzene
Concen: 48.370 ug/l
RT: 12.38 min Scan# 3308
Delta R.T. 0.00 min
Lab File: VN064180.D
Acq: 16 Oct 2020 21:29

Tgt Ion: 95 Resp: 290275
Ion Ratio Lower Upper
95 100
174 76.8 0.0 164.8
176 72.4 0.0 157.8

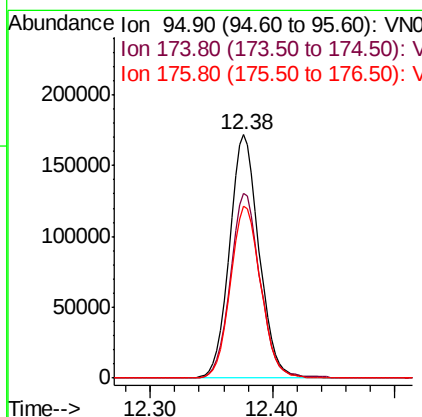







#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN064180.D
Acq: 16 Oct 2020 21:29

Instrument :
MSVOA_N
ClientSampled :
JC-02-101420-A

Tot Ion:117 Resp: 690033
Ion Ratio Lower Upper
117 100
82 57.0 42.6 63.8
119 32.3 25.5 38.3




Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VN
Ion 118.90 (118.60 to 119.60): V

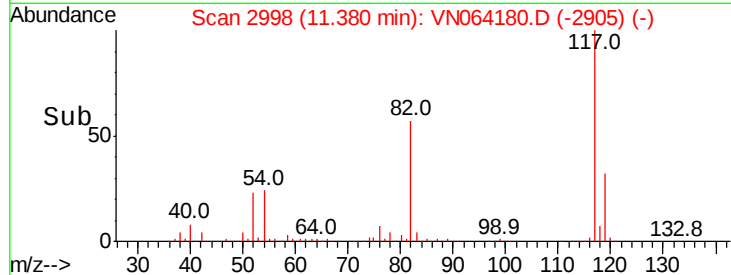
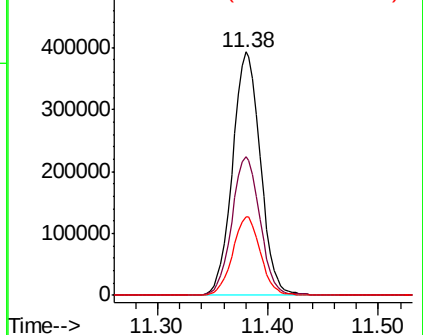



#68
m/p-Xylenes
Concen: 2.199 ug/l
RT: 11.60 min Scan# 3068
Delta R.T. 0.01 min
Lab File: VN064180.D
Acq: 16 Oct 2020 21:29

Tgt Ion:106 Resp: 72
Ion Ratio Lower Upper
106 100
91 276.4 162.1 243.1#



Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VN

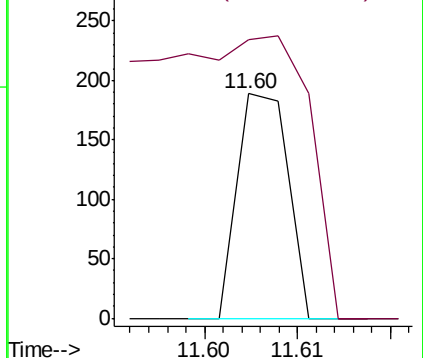



#70

Stvrene

Concen: 2.045 ug/l

RT: 11.94 min Scan# 3171

Delta R.T. -0.00 min

Lab File: VN064180.D

Acq: 16 Oct 2020 21:29

Instrument :

MSVOA_N

ClientSampleId :

JC-02-101420-A


Tot Ion:104 Resp: 150

Ion Ratio Lower Upper

104 100

78 0.0 39.7 59.5#




103 112.7 44.2 66.2#



Abundance Ion 104.00 (103.70 to 104.70): V

Ion 78.00 (77.70 to 78.70): VN0

Ion 103.00 (102.70 to 103.70): V

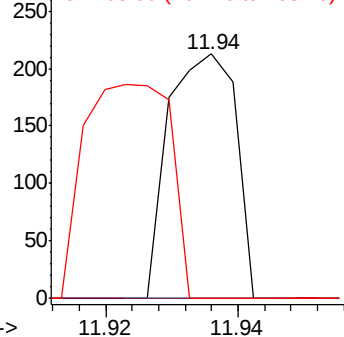

#71

Bromoform

Concen: 2.255 ug/l

RT: 12.36 min Scan# 3302

Delta R.T. 0.26 min

Lab File: VN064180.D

Acq: 16 Oct 2020 21:29


Tgt Ion:173 Resp: 116

Ion Ratio Lower Upper

173 100

175 0.0 23.4 70.2#



254 0.0 0.1 0.1#




Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

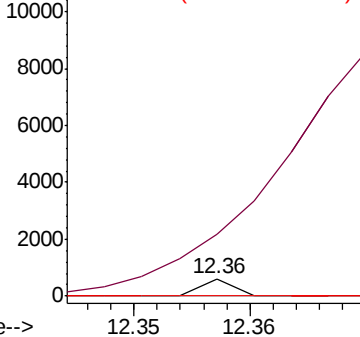



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3601

Delta R.T. 0.00 min

Lab File: VN064180.D

Acq: 16 Oct 2020 21:29

Instrument :

MSVOA_N

ClientSampleId :

JC-02-101420-A


Tot Ion:152 Resp: 242204

Ion Ratio Lower Upper

152 100

115 61.3 29.3 87.8




150 161.4 0.0 346.0



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

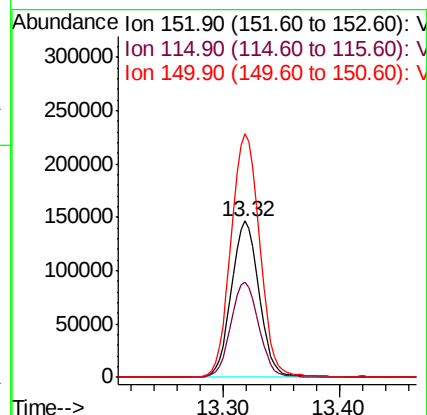

#74

N-ethyl acetate

Concen: 0.619 ug/l

RT: 12.01 min Scan# 3193

Delta R.T. -0.04 min

Lab File: VN064180.D

Acq: 16 Oct 2020 21:29

Tgt Ion: 43 Resp: 4067


Ion Ratio Lower Upper

43 100

70 2.7 33.2 49.8#

55 6.6 19.9 29.9#

61 0.0 18.8 28.2#






Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 70.00 (69.70 to 70.70): VNO

Ion 55.00 (54.70 to 55.70): VNO

Ion 61.00 (60.70 to 61.70): VNO



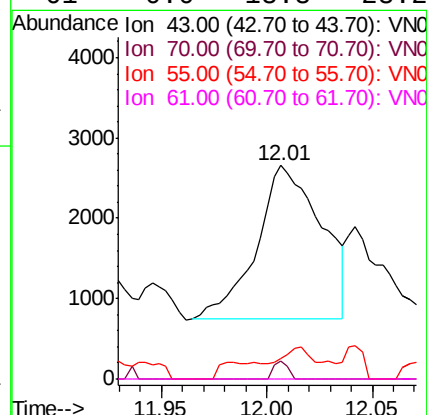





#76
 1,2,3-Trichloropropane
 Concen: 27.028 ug/l
 RT: 12.38 min Scan# 3308
 Delta R.T. -0.15 min
 Lab File: VN064180.D
 Acq: 16 Oct 2020 21:29




Instrument :
 MSVOA_N
 ClientSampleId :
 JC-02-101420-A


Tot Ion: 75 Resp: 153580
 Ion Ratio Lower Upper
 75 100
 77 1.4 0.0 0.0#

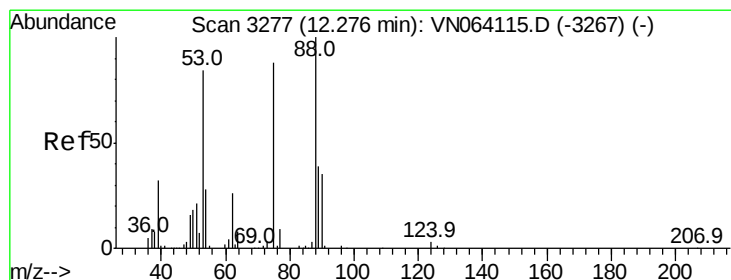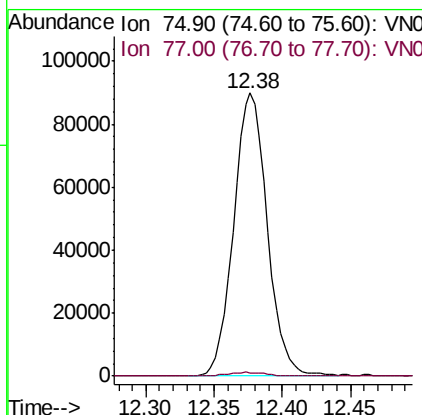

#81
 trans-1,4-Dichloro-2-butene
 Concen: 82.575 ug/l
 RT: 12.38 min Scan# 3308
 Delta R.T. 0.10 min
 Lab File: VN064180.D
 Acq: 16 Oct 2020 21:29

Tgt Ion: 75 Resp: 153580
 Ion Ratio Lower Upper
 75 100
 53 0.3 75.7 113.5#
 89 0.1 36.6 55.0#

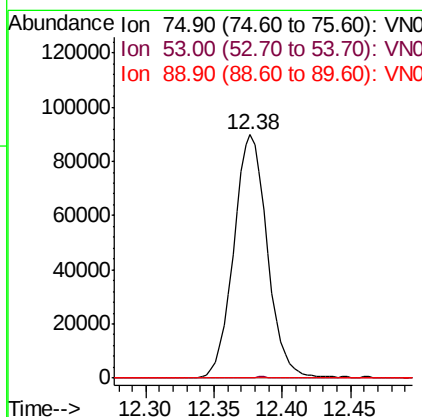







#86
 p-Isopropyltoluene
 Concen: 0.668 ug/l
 RT: 13.32 min Scan# 3600
 Delta R.T. 0.05 min
 Lab File: VN064180.D
 Acq: 16 Oct 2020 21:29

Instrument :
 MSVOA_N
 ClientSampleId :
 JC-02-101420-A

Tot Ion:119 Resp: 93
 Ion Ratio Lower Upper
 119 100
 134 348.4 13.2 39.5#
 91 1026.9 12.0 36.1#




Abundance Ion 119.00 (118.70 to 119.70): V
 Ion 134.00 (133.70 to 134.70): V
 Ion 91.00 (90.70 to 91.70): V

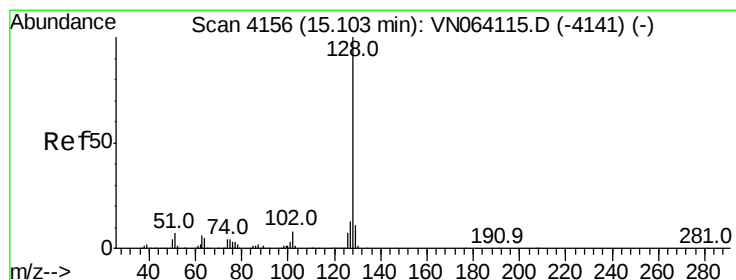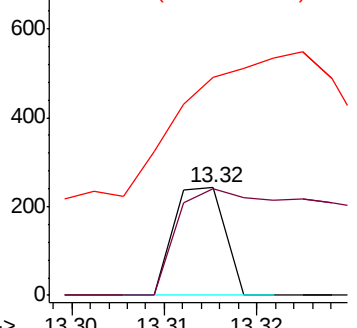

#95
 Naphthalene
 Concen: 3.832 ug/l
 RT: 15.12 min Scan# 4162
 Delta R.T. 0.02 min
 Lab File: VN064180.D
 Acq: 16 Oct 2020 21:29

Tgt Ion:128 Resp: 448
 Ion Ratio Lower Upper
 128 100
 127 0.0 10.2 15.4#
 129 22.5 8.5 12.7#



Abundance Ion 128.00 (127.70 to 128.70): V
 Ion 127.00 (126.70 to 127.70): V
 Ion 129.00 (128.70 to 129.70): V

