

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN101620\
 Data File : VN064171.D
 Acq On : 16 Oct 2020 17:56
 Operator : JC/MD
 Sample : PB132400ZHE#02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132400ZHE#02

Manual Integrations
 APPROVED

MMDadoda
 10/19/2020 4:22:30 PM

Quant Time: Oct 17 02:07:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101420W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 15 01:16:44 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	343228	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	688958	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	730663	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	265431	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.99	65	293829	60.11	ug/l	0.00
Spiked Amount 50.000			Recovery	=	120.22%	
35) Dibromofluoromethane	7.55	113	232274	48.71	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.42%	
50) Toluene-d8	10.06	98	917082	50.97	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.94%	
62) 4-Bromofluorobenzene	12.38	95	311789	50.41	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.82%	
Target Compounds						
16) Acetone	3.78	43	24463m	16.872	ug/l	Qvalue
18) Methyl Acetate	4.31	43	4323	1.189	ug/l #	55
20) Methylene Chloride	4.51	84	21506	4.793	ug/l	95
43) Isopropyl Acetate	8.13	43	115688	11.829	ug/l #	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN101620\
Data File : VN064171.D
Acq On : 16 Oct 2020 17:56
Operator : JC/MD
Sample : PB132400ZHE#02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 10 Sample Multiplier: 1


Instrument :
MSVOA_N
ClientSampleId :
PB132400ZHE#02

Manual Integrations
APPROVED

MMDadoda
10/19/2020 4:22:30 PM

Quant Time: Oct 17 02:07:53 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N101420W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 15 01:16:44 2020
Response via : Initial Calibration

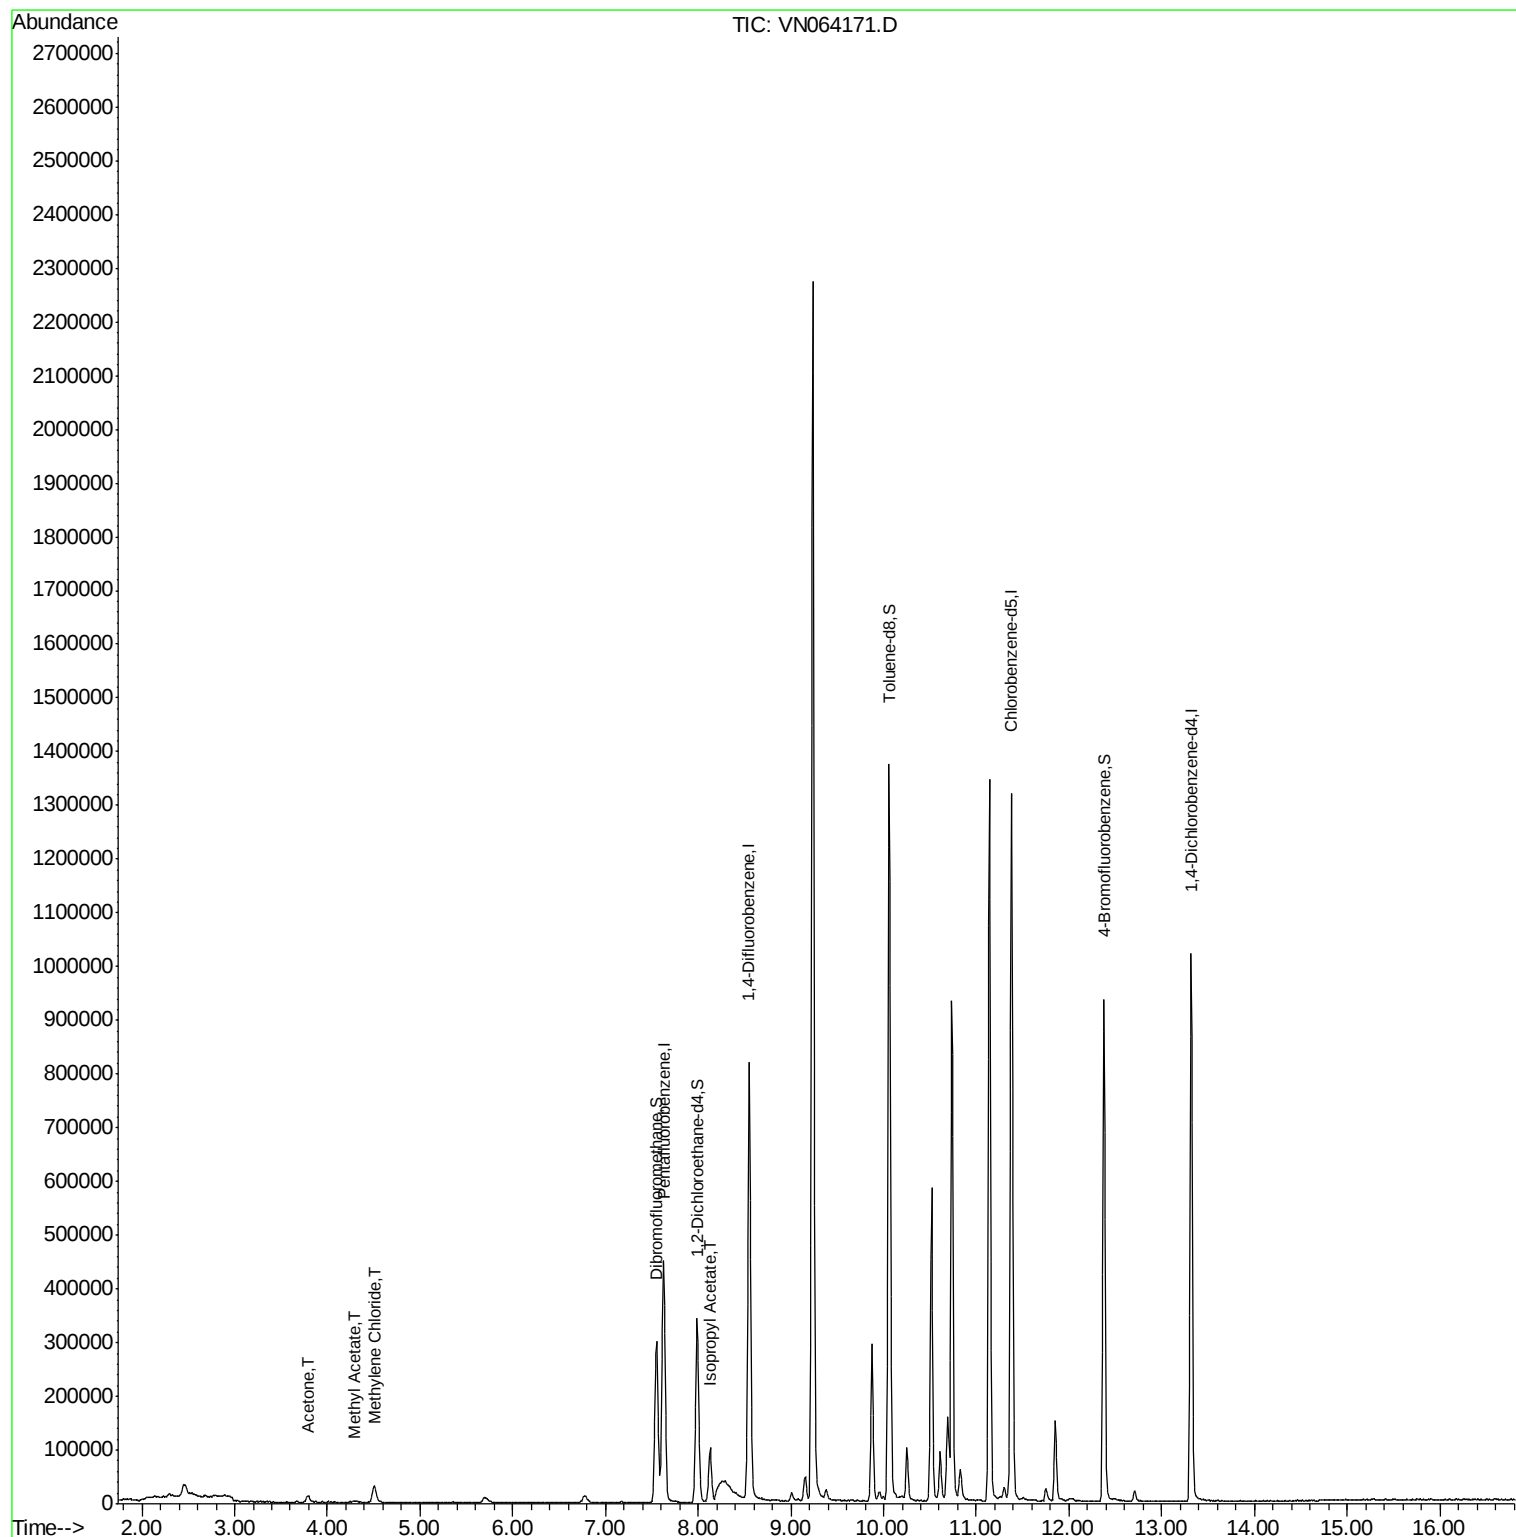

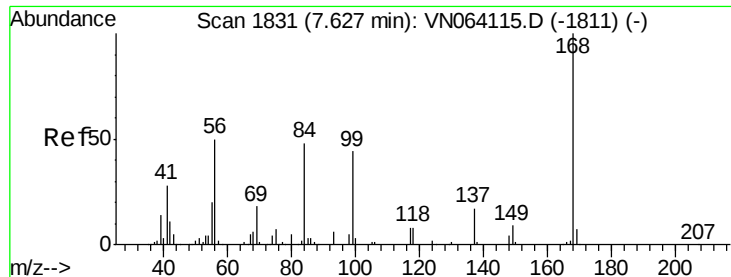

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN064171.D

Acq: 16 Oct 2020 17:56

Instrument :

MSVOA_N

ClientSampleId :

PB132400ZHE#02

Tot Ion:168 Resp: 343228

Ion Ratio Lower Upper

168 100


99 57.6 43.6 65.4

Manual Integrations

APPROVED

MMDadoda

10/19/2020 4:22:30 PM

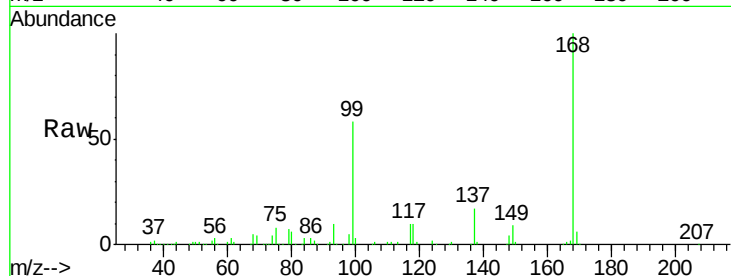

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.63



150000

100000

50000

0

Time--> 7.50 7.60 7.70

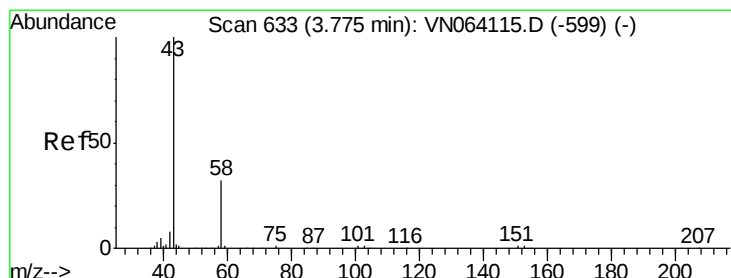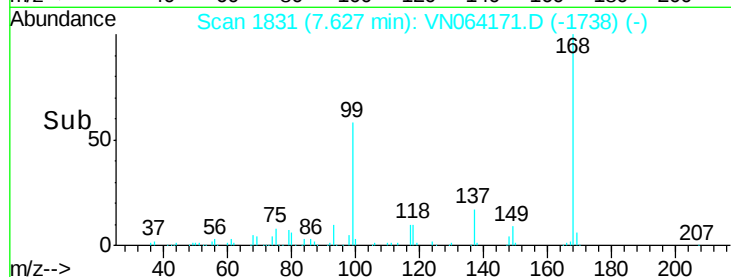

#16

Acetone

Concen: 16.872 ug/l m

RT: 3.78 min Scan# 636

Delta R.T. 0.01 min

Lab File: VN064171.D


Acq: 16 Oct 2020 17:56

Tgt Ion: 43 Resp: 24463

Ion Ratio Lower Upper

43 100

58 28.3 25.2 37.8

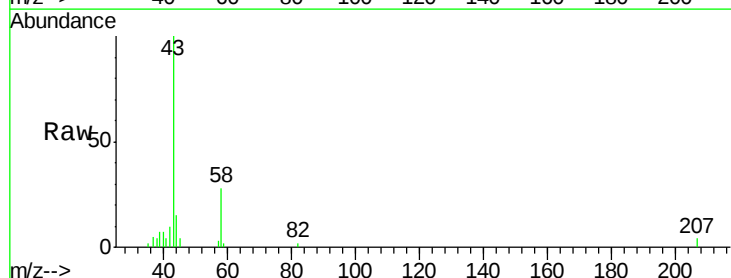

Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 58.00 (57.70 to 58.70): VNO

3.78

8000


6000


4000

2000

0

Time--> 3.70 3.80 3.90

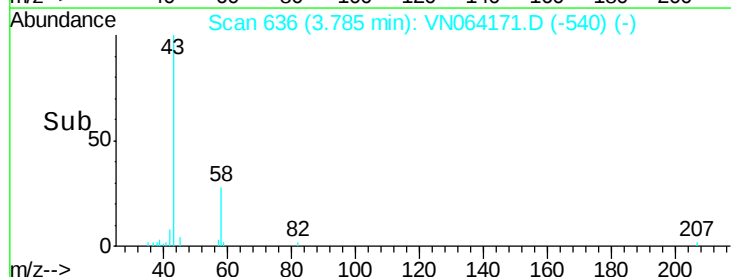

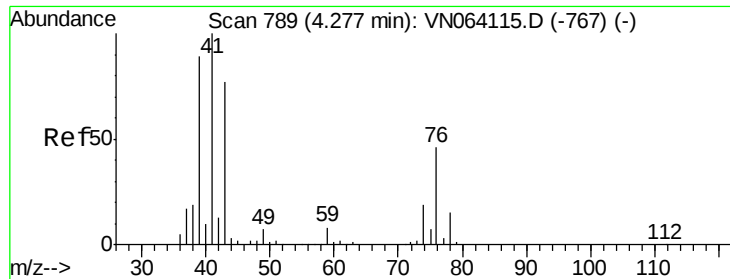





#18
Methyl Acetate
Concen: 1.189 ug/l
RT: 4.31 min Scan# 798
Delta R.T. 0.03 min
Lab File: VN064171.D
Acq: 16 Oct 2020 17:56

Instrument :
MSVOA_N
ClientSampleId :
PB132400ZHE#02

Tot Ion: 43 Resp: 4323
Ion Ratio Lower Upper
43 100
74 2.2 19.7 29.5#




Manual Integrations
APPROVED


MMDadoda
10/19/2020 4:22:30 PM

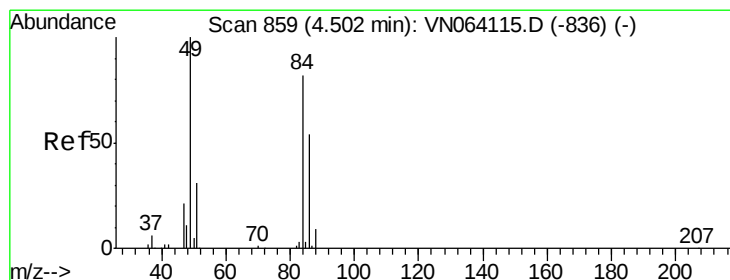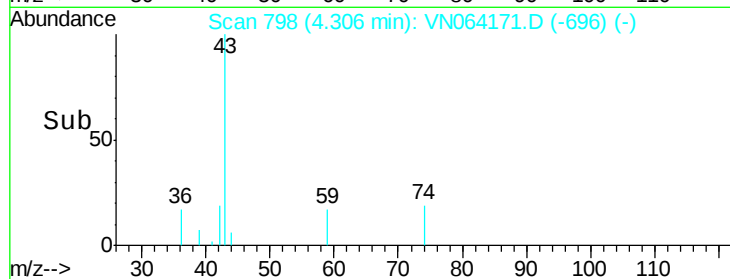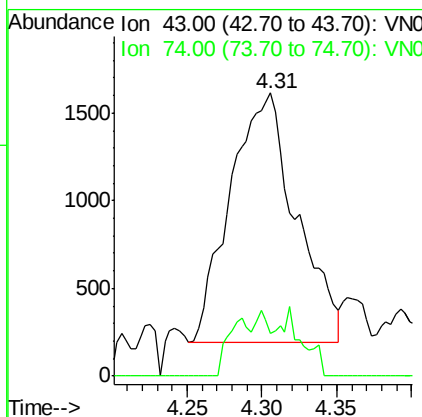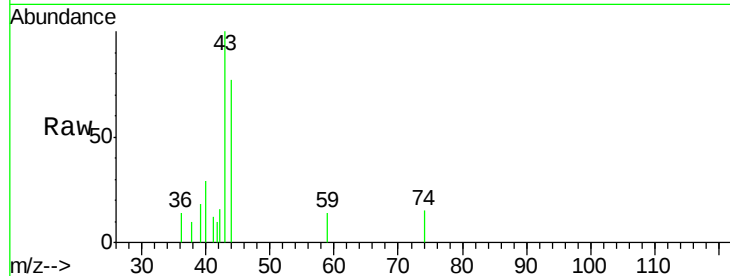

#20
Methylene Chloride
Concen: 4.793 ug/l
RT: 4.51 min Scan# 861
Delta R.T. 0.01 min
Lab File: VN064171.D
Acq: 16 Oct 2020 17:56

Tgt Ion: 84 Resp: 21506
Ion Ratio Lower Upper
84 100
49 126.2 97.4 146.0
51 39.5 29.7 44.5
86 71.1 52.5 78.7

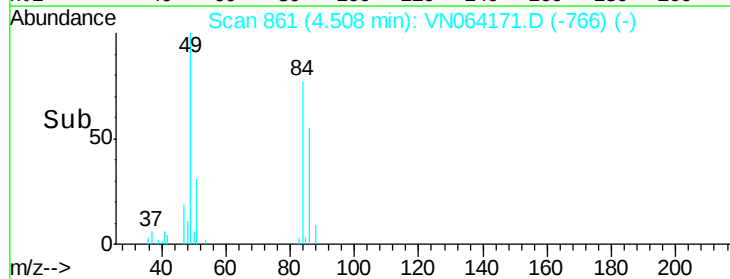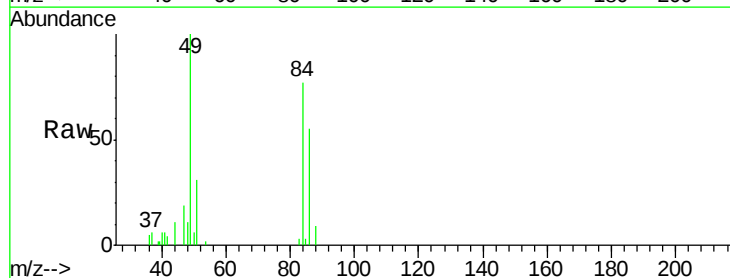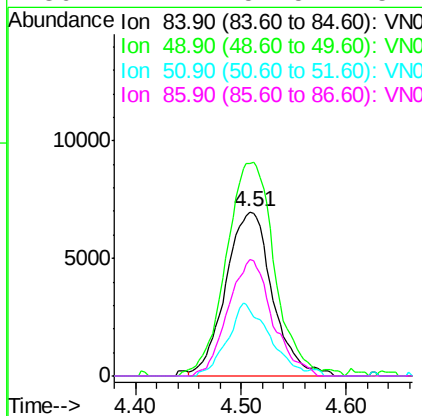

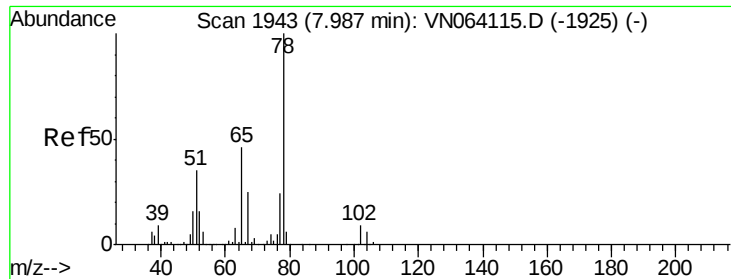





#33
 1,2-Dichloroethane-d4
 Concen: 60.109 ug/l
 RT: 7.99 min Scan# 1943
 Delta R.T. 0.00 min
 Lab File: VN064171.D
 Acq: 16 Oct 2020 17:56

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132400ZHE#02

Tot Ion	Ratio	Resp	Lower	Upper
65	100	293829		
67	51.1	0.0	105.6	




Manual Integrations
 APPROVED


MMDadoda
 10/19/2020 4:22:30 PM

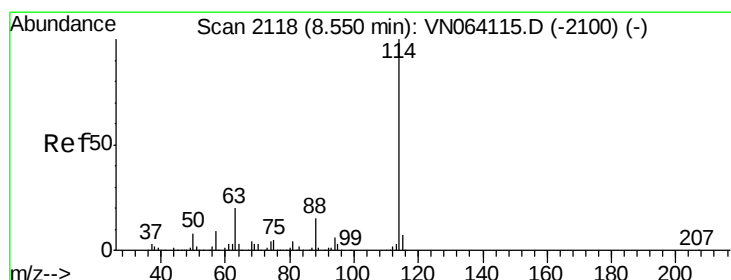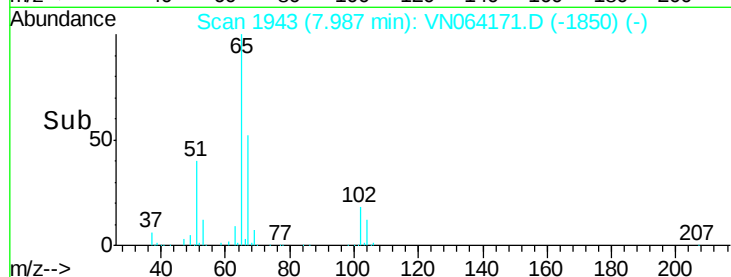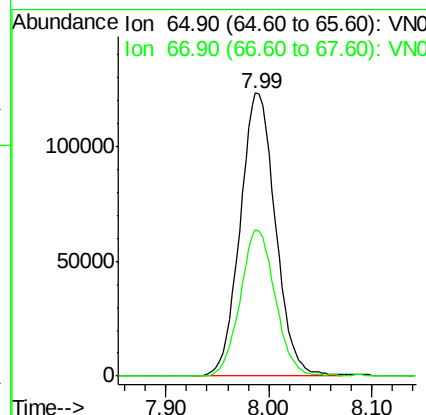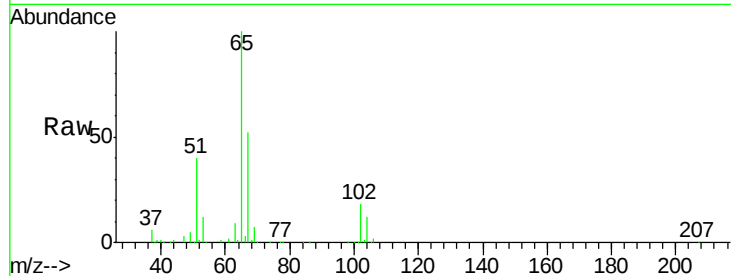

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2118
 Delta R.T. 0.00 min
 Lab File: VN064171.D
 Acq: 16 Oct 2020 17:56

Tgt Ion	Ratio	Resp	Lower	Upper
114	100	688958		
63	22.0	0.0	41.0	
88	15.6	0.0	29.2	

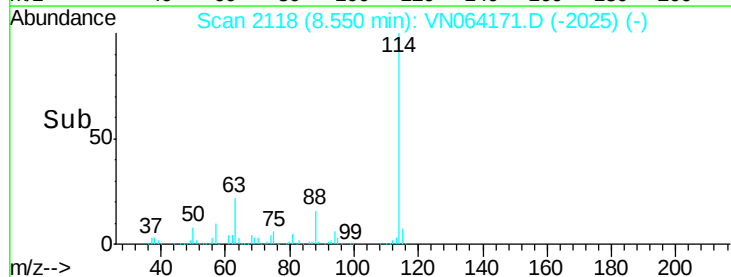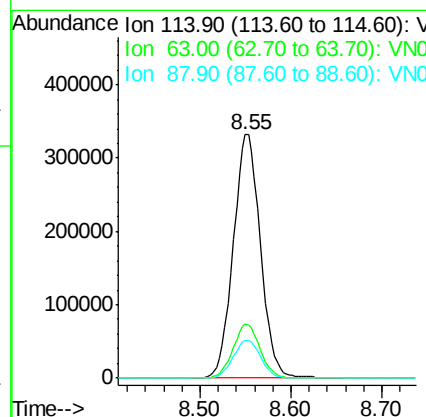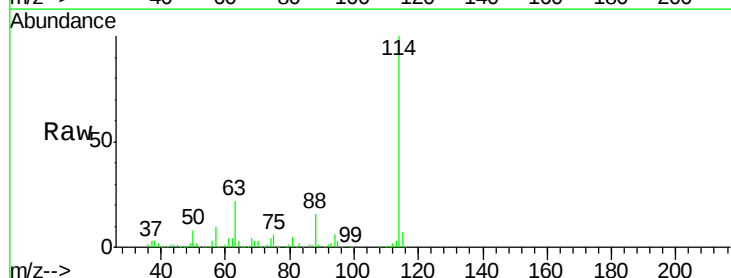

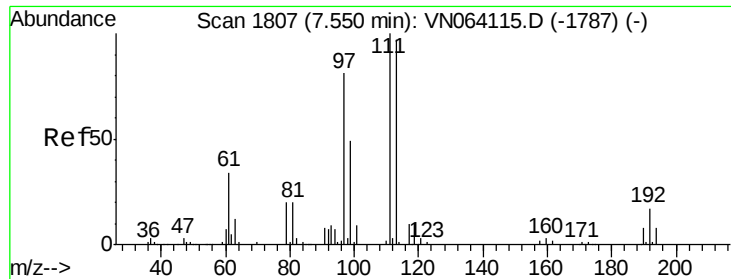





#35
 Dibromofluoromethane
 Concen: 48.709 ug/l
 RT: 7.55 min Scan# 1807
 Delta R.T. 0.00 min
 Lab File: VN064171.D
 Acq: 16 Oct 2020 17:56

Instrument :
 MSVOA_N
 ClientSampleId :
 PB132400ZHE#02

Tot Ion	Ratio	Resp	Lower	Upper
113	100	232274		
111	100.9	81.9	122.9	
192	17.8	14.3	21.5	




Manual Integrations
 APPROVED


MMDadoda
 10/19/2020 4:22:30 PM

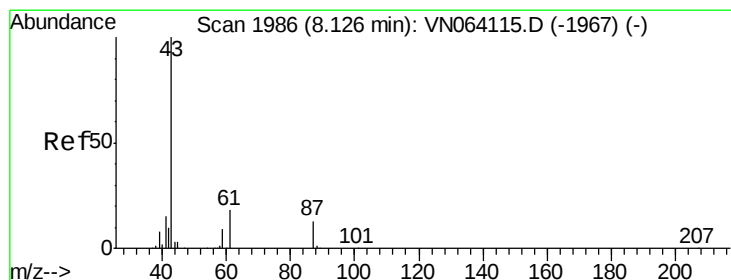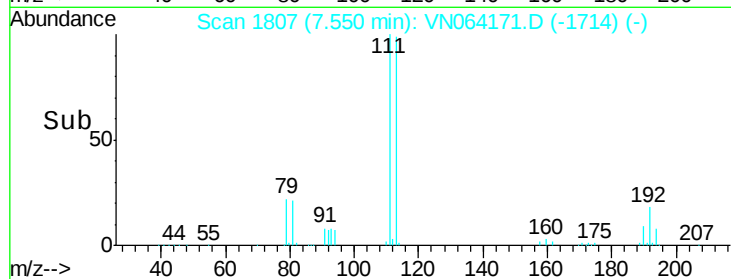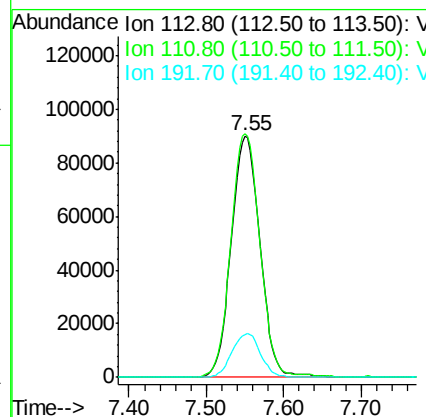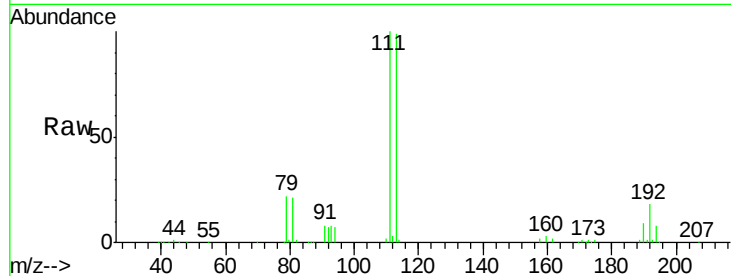

#43
 Isopropyl Acetate
 Concen: 11.829 ug/l
 RT: 8.13 min Scan# 1987
 Delta R.T. 0.00 min
 Lab File: VN064171.D
 Acq: 16 Oct 2020 17:56

Tgt Ion	Ratio	Resp	Lower	Upper
43	100	115688		
61	18.9	21.9	32.9#	
87	12.0	11.0	16.4	

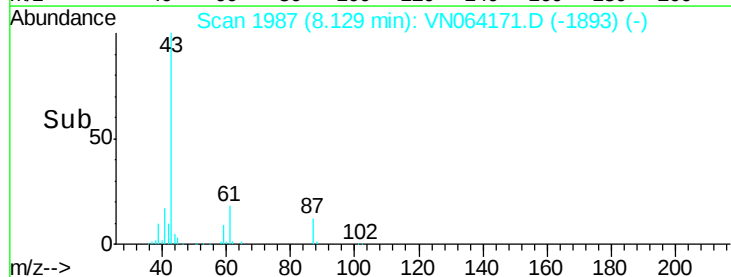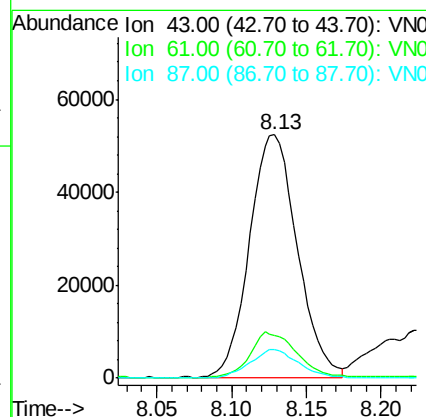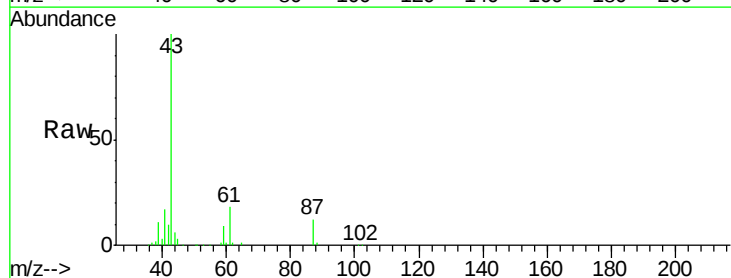

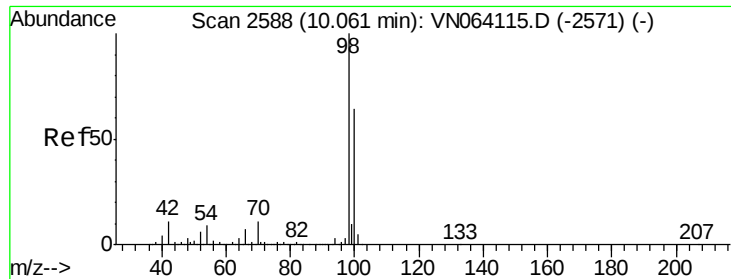

#50

Toluene-d8

Concen: 50.970 ug/l

RT: 10.06 min Scan# 2588

Delta R.T. 0.00 min

Lab File: VN064171.D

Acq: 16 Oct 2020 17:56

Instrument :

MSVOA_N

ClientSampleId :

PB132400ZHE#02

Tot Ion: 98 Resp: 917082

Ion Ratio Lower Upper

98 100





100 63.6 50.8 76.2

Manual Integrations

APPROVED

MMDadoda

10/19/2020 4:22:30 PM

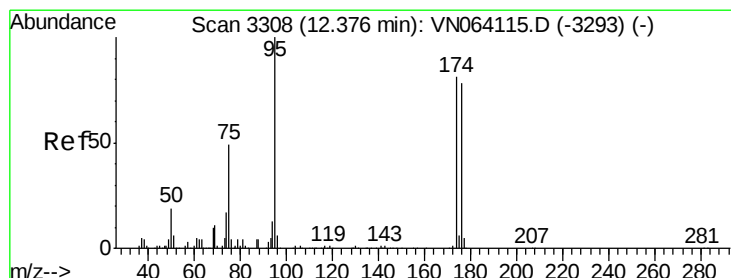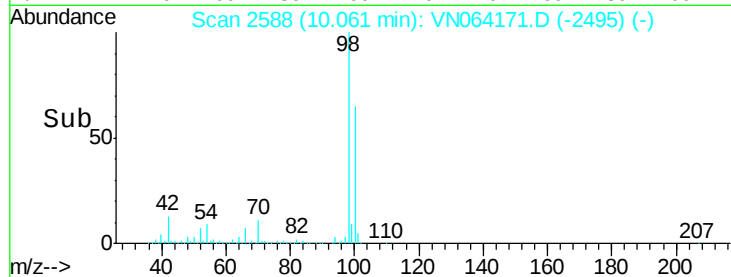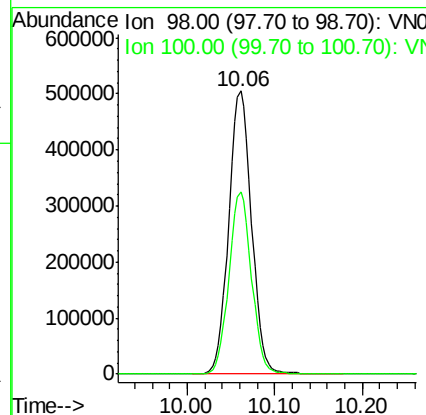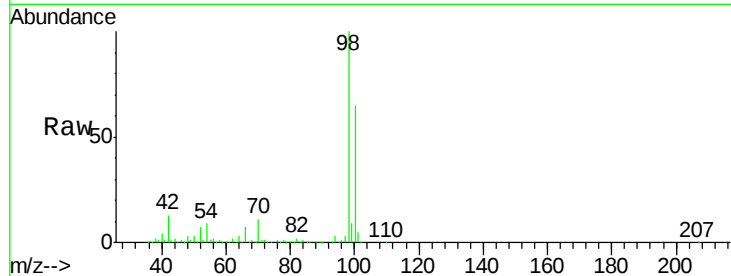

#62

4-Bromofluorobenzene

Concen: 50.414 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.00 min

Lab File: VN064171.D

Acq: 16 Oct 2020 17:56




Tgt Ion: 95 Resp: 311789


Ion Ratio Lower Upper

95 100

174 77.9 0.0 164.8

176 73.4 0.0 157.8

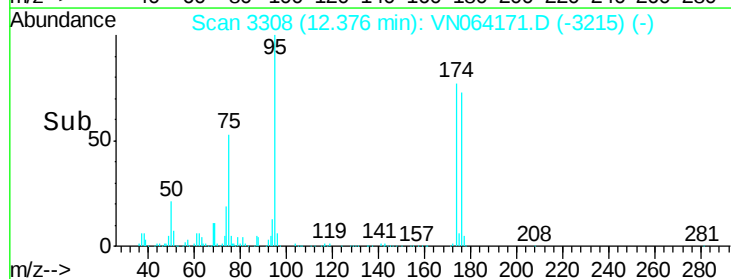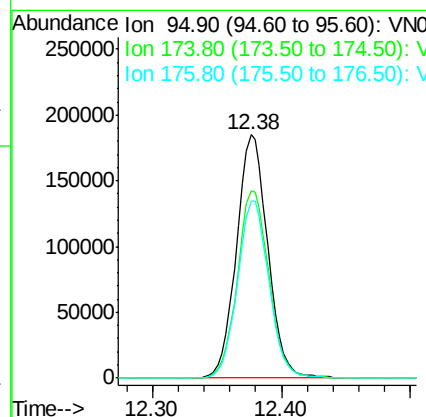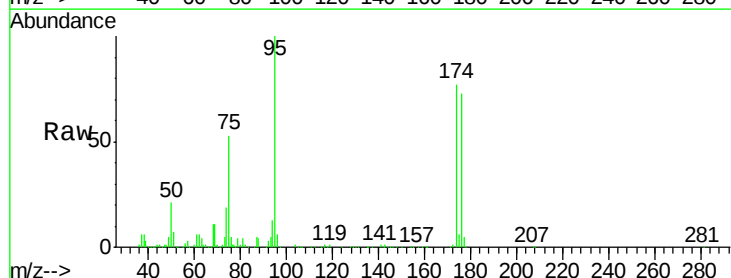

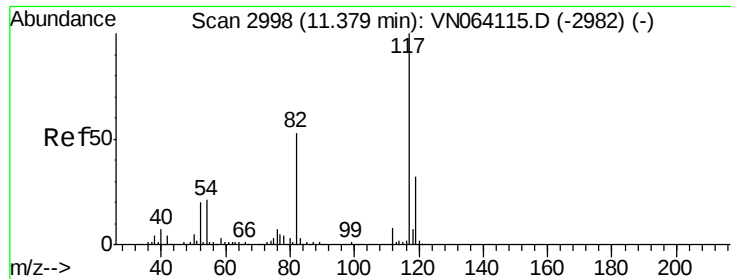





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. 0.00 min
Lab File: VN064171.D
Acq: 16 Oct 2020 17:56

Instrument :
MSVOA_N
ClientSampleId :
PB132400ZHE#02

Tot Ion	Ratio	Resp	Lower	Upper
117	100	730663		
82	56.8	42.6	63.8	
119	31.8	25.5	38.3	

Manual Integrations
APPROVED

MMDadoda
10/19/2020 4:22:30 PM

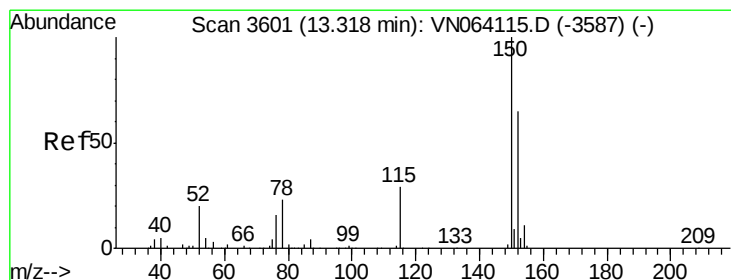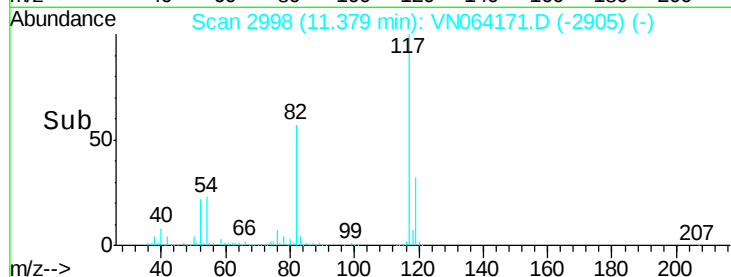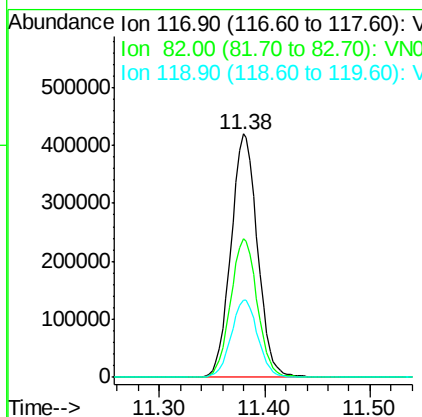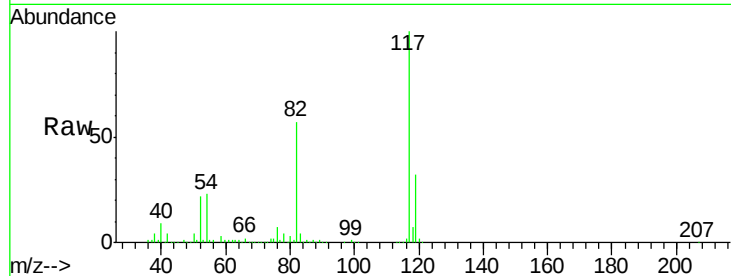

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.32 min Scan# 3601
Delta R.T. 0.00 min
Lab File: VN064171.D
Acq: 16 Oct 2020 17:56

Tgt Ion	Ratio	Resp	Lower	Upper
152	100	265431		
115	61.3	29.3	87.8	
150	154.4	0.0	346.0	

