



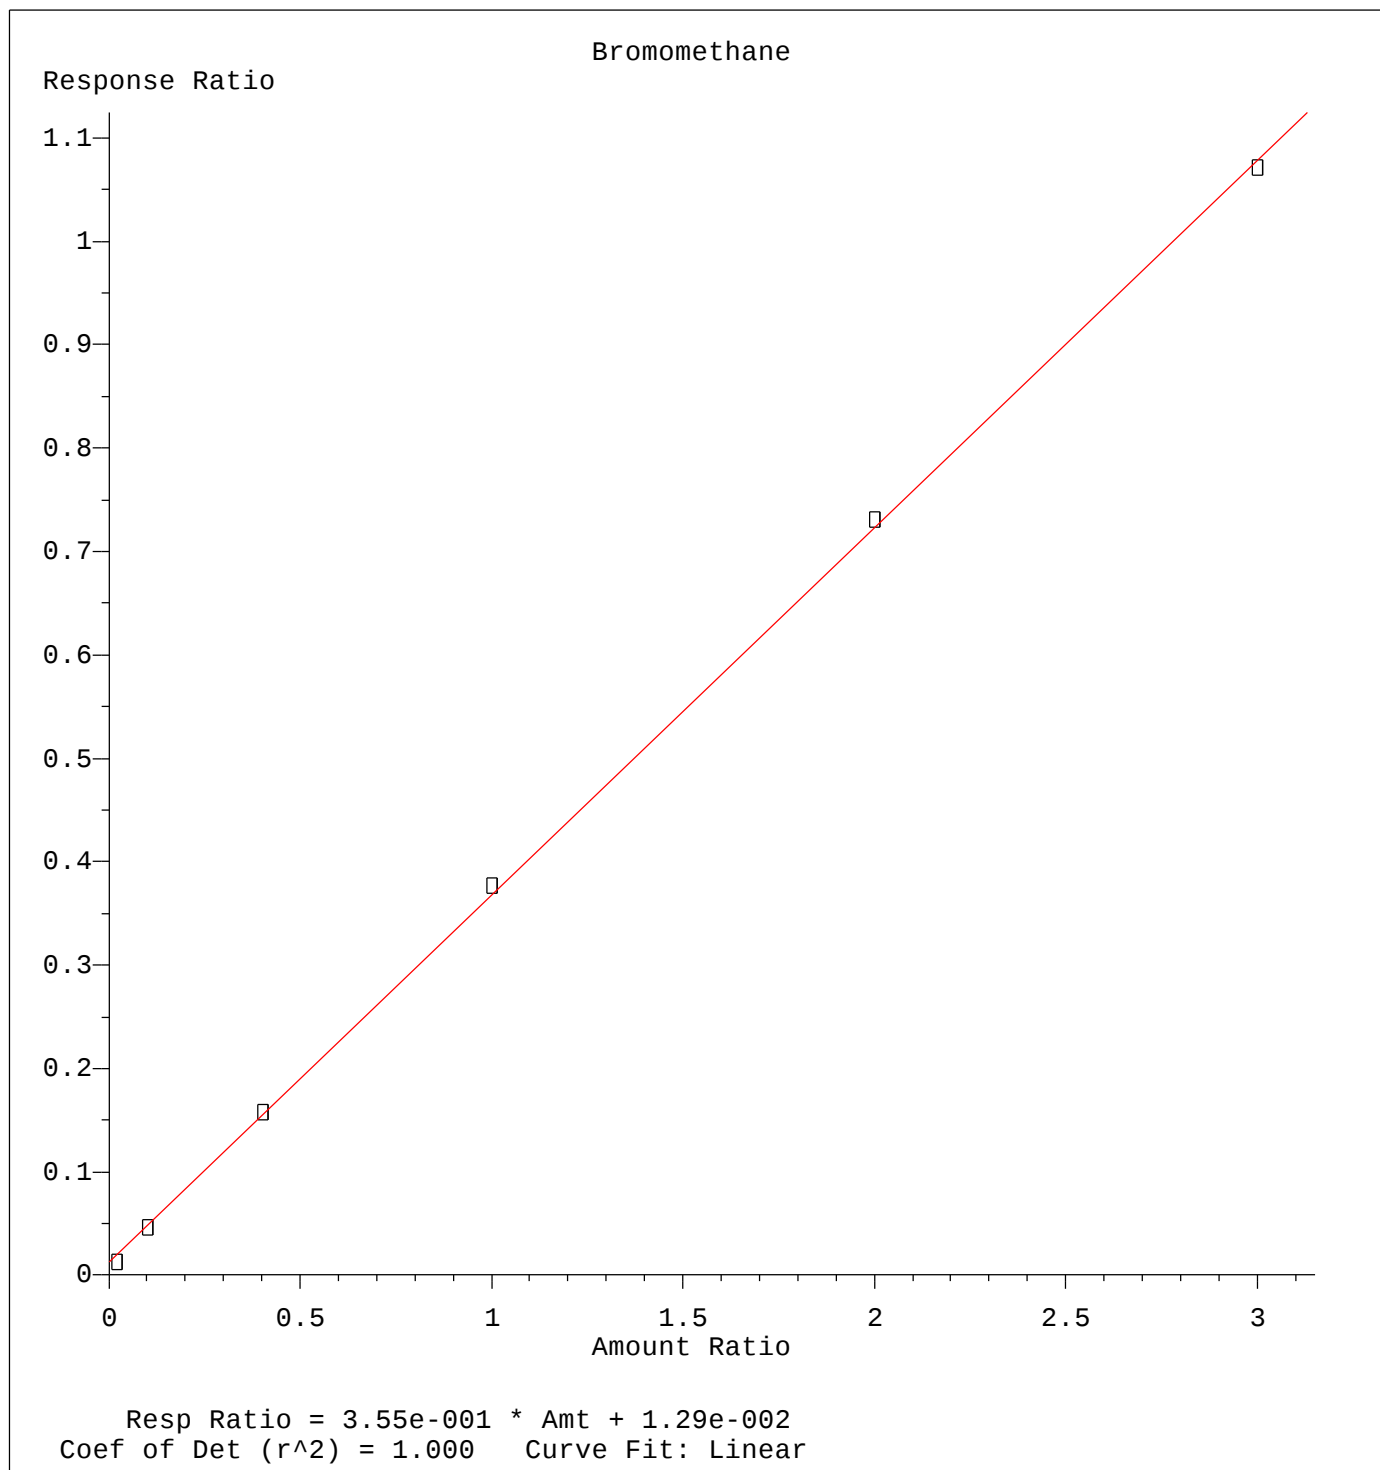

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101718W.M
Calibration Table Last Updated: Fri Oct 19 05:11:28 2018

2-Chloroethyl Vinyl ether

Response Ratio

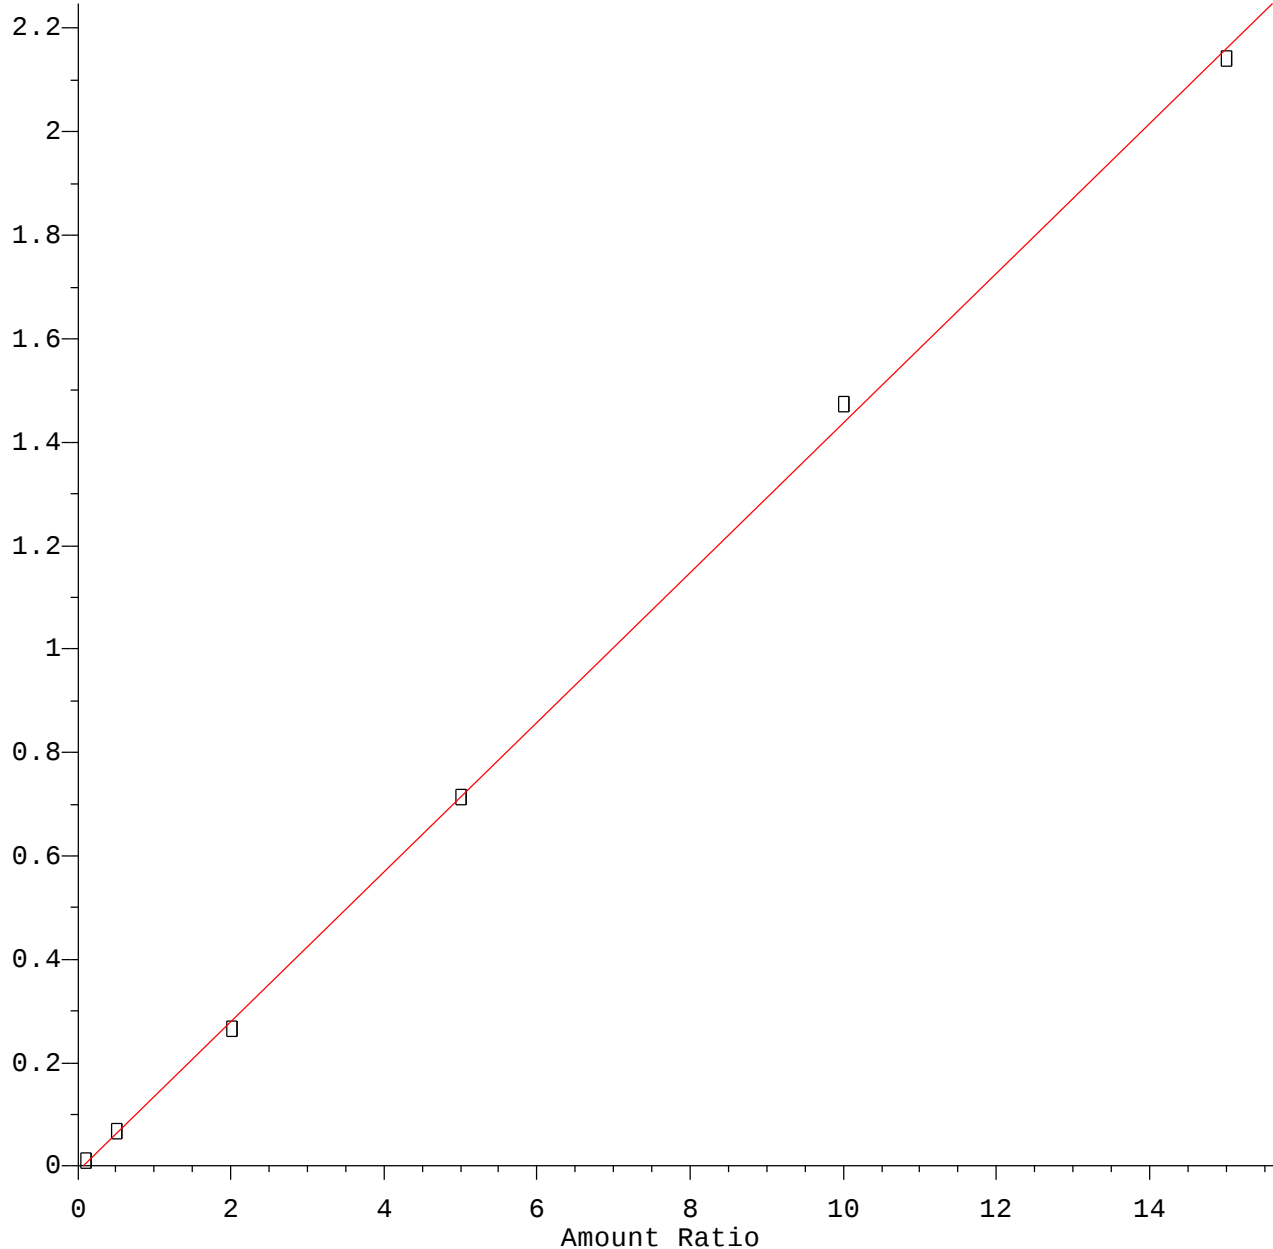


Resp Ratio = 1.45×10^{-1} * Amt - 7.96×10^{-3}
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101718W.M
Calibration Table Last Updated: Fri Oct 19 05:11:28 2018


Isopropyl Acetate

Response Ratio

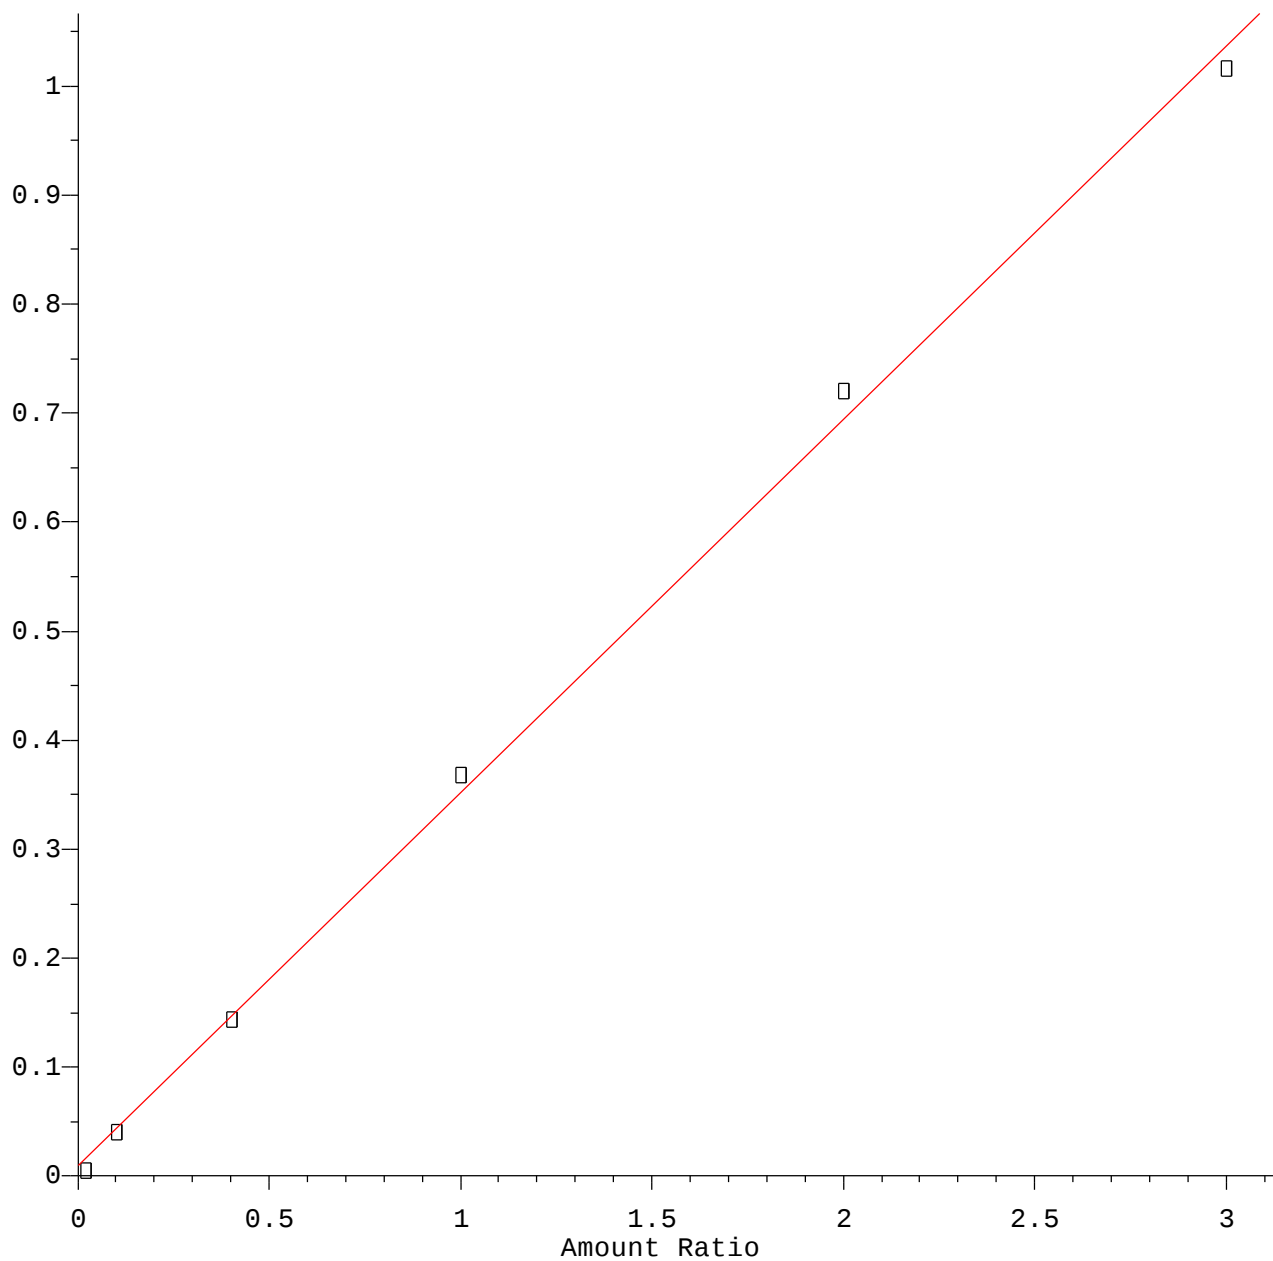


Resp Ratio = $3.43 \times 10^{-1} \times \text{Amt} + 9.76 \times 10^{-3}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101718W.M
Calibration Table Last Updated: Fri Oct 19 05:11:28 2018

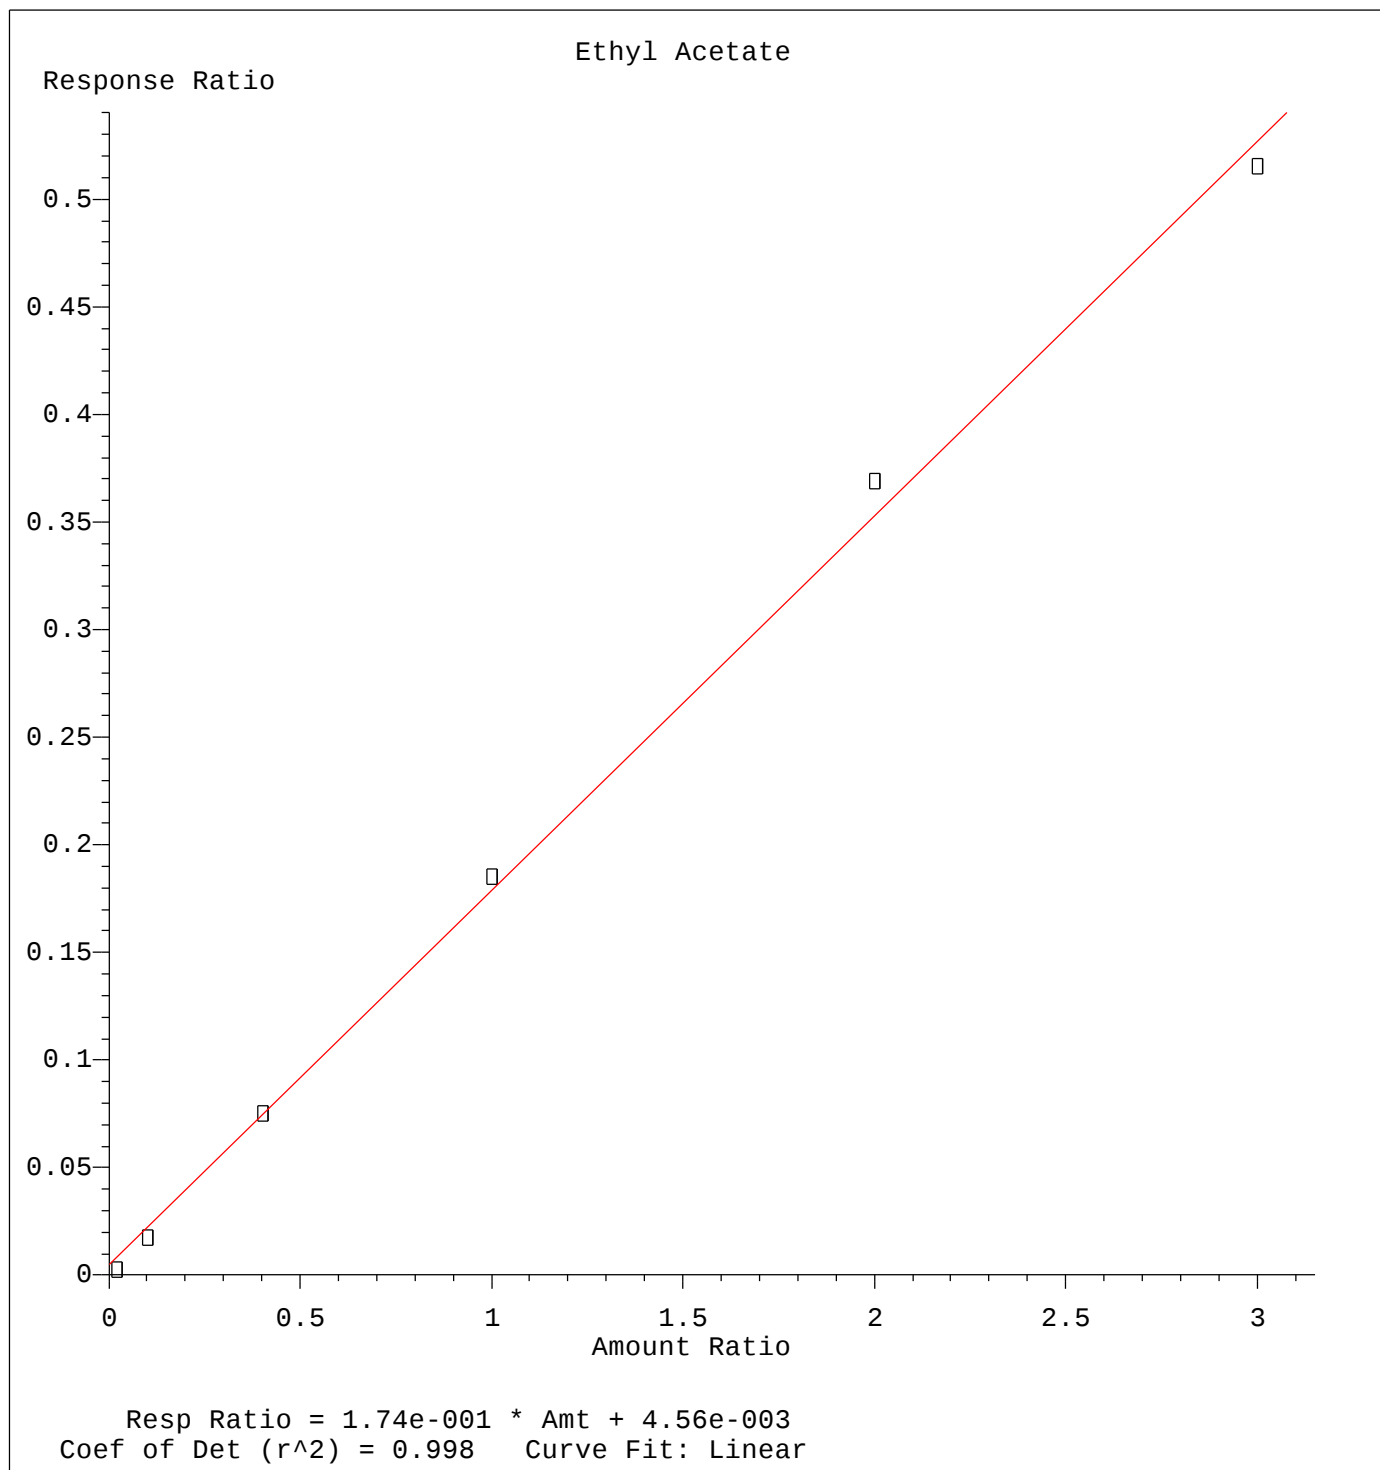


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101718W.M
Calibration Table Last Updated: Fri Oct 19 05:11:28 2018

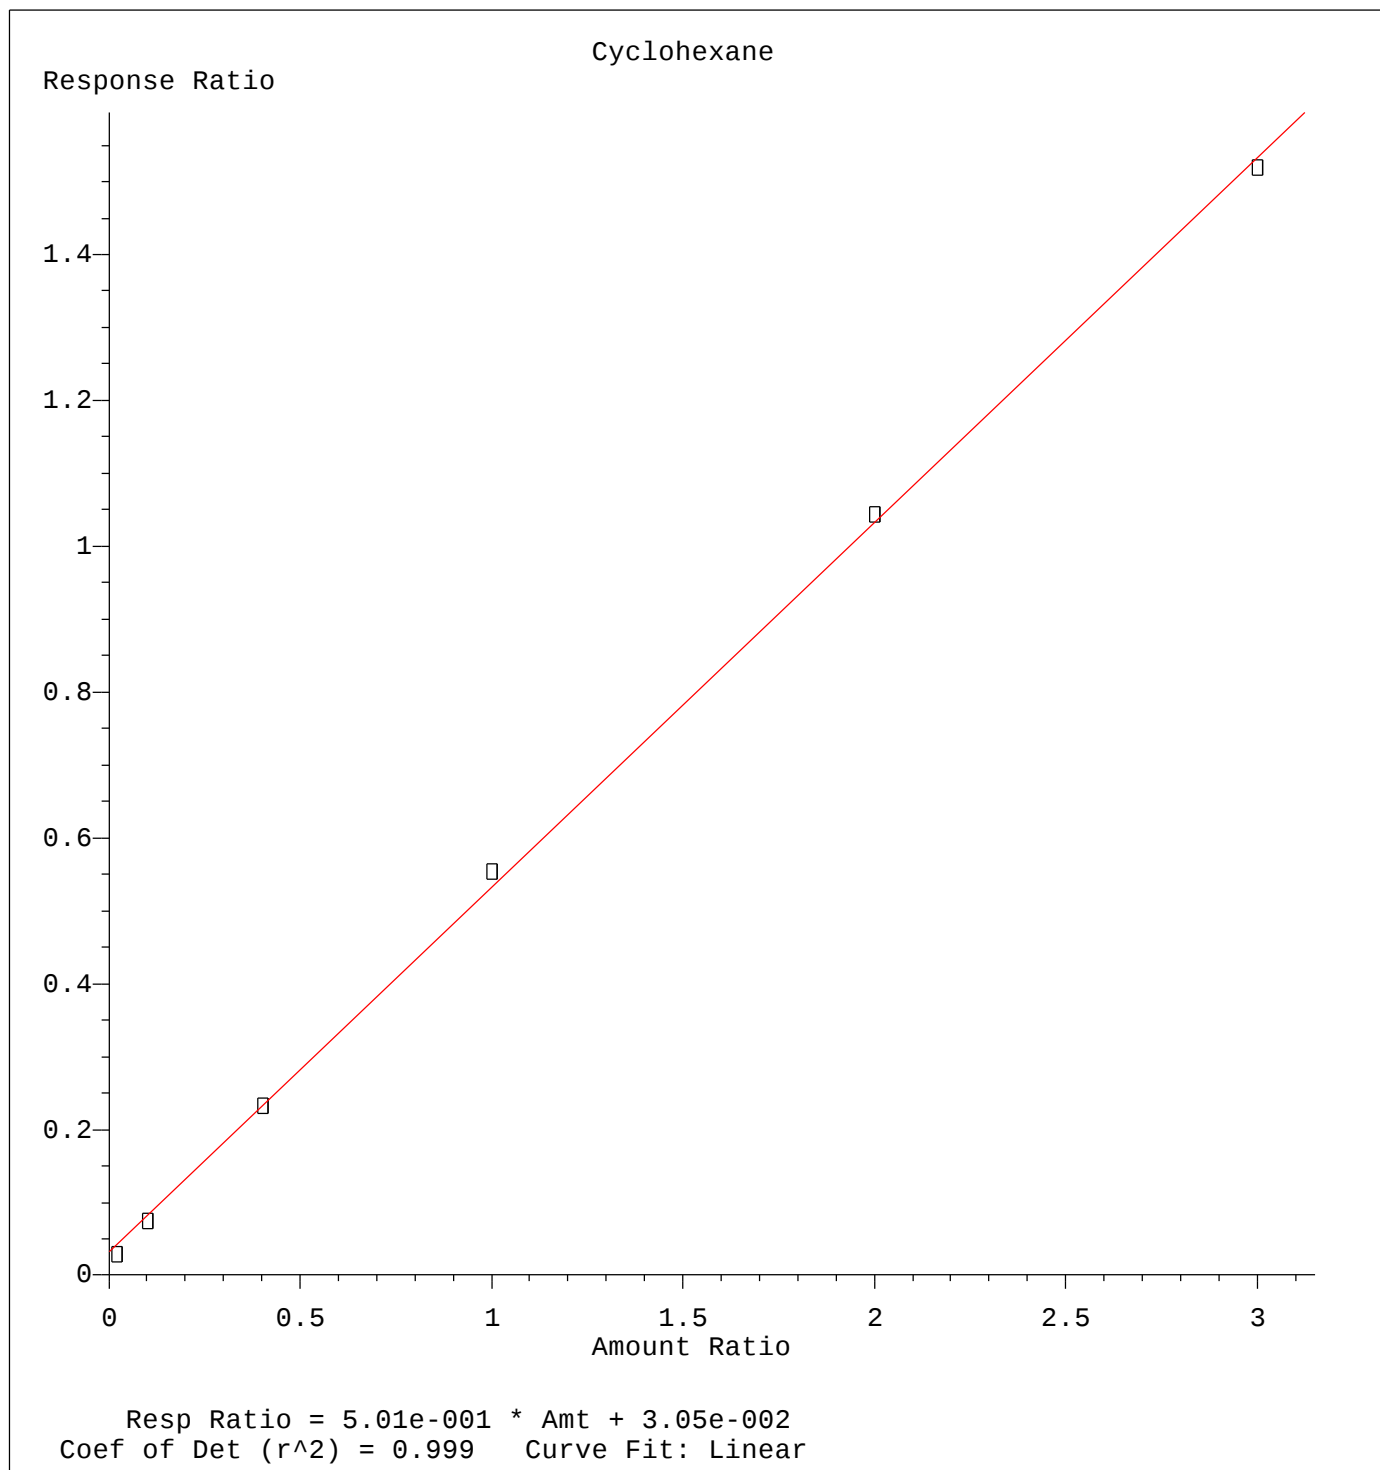


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101718W.M
Calibration Table Last Updated: Fri Oct 19 05:11:28 2018

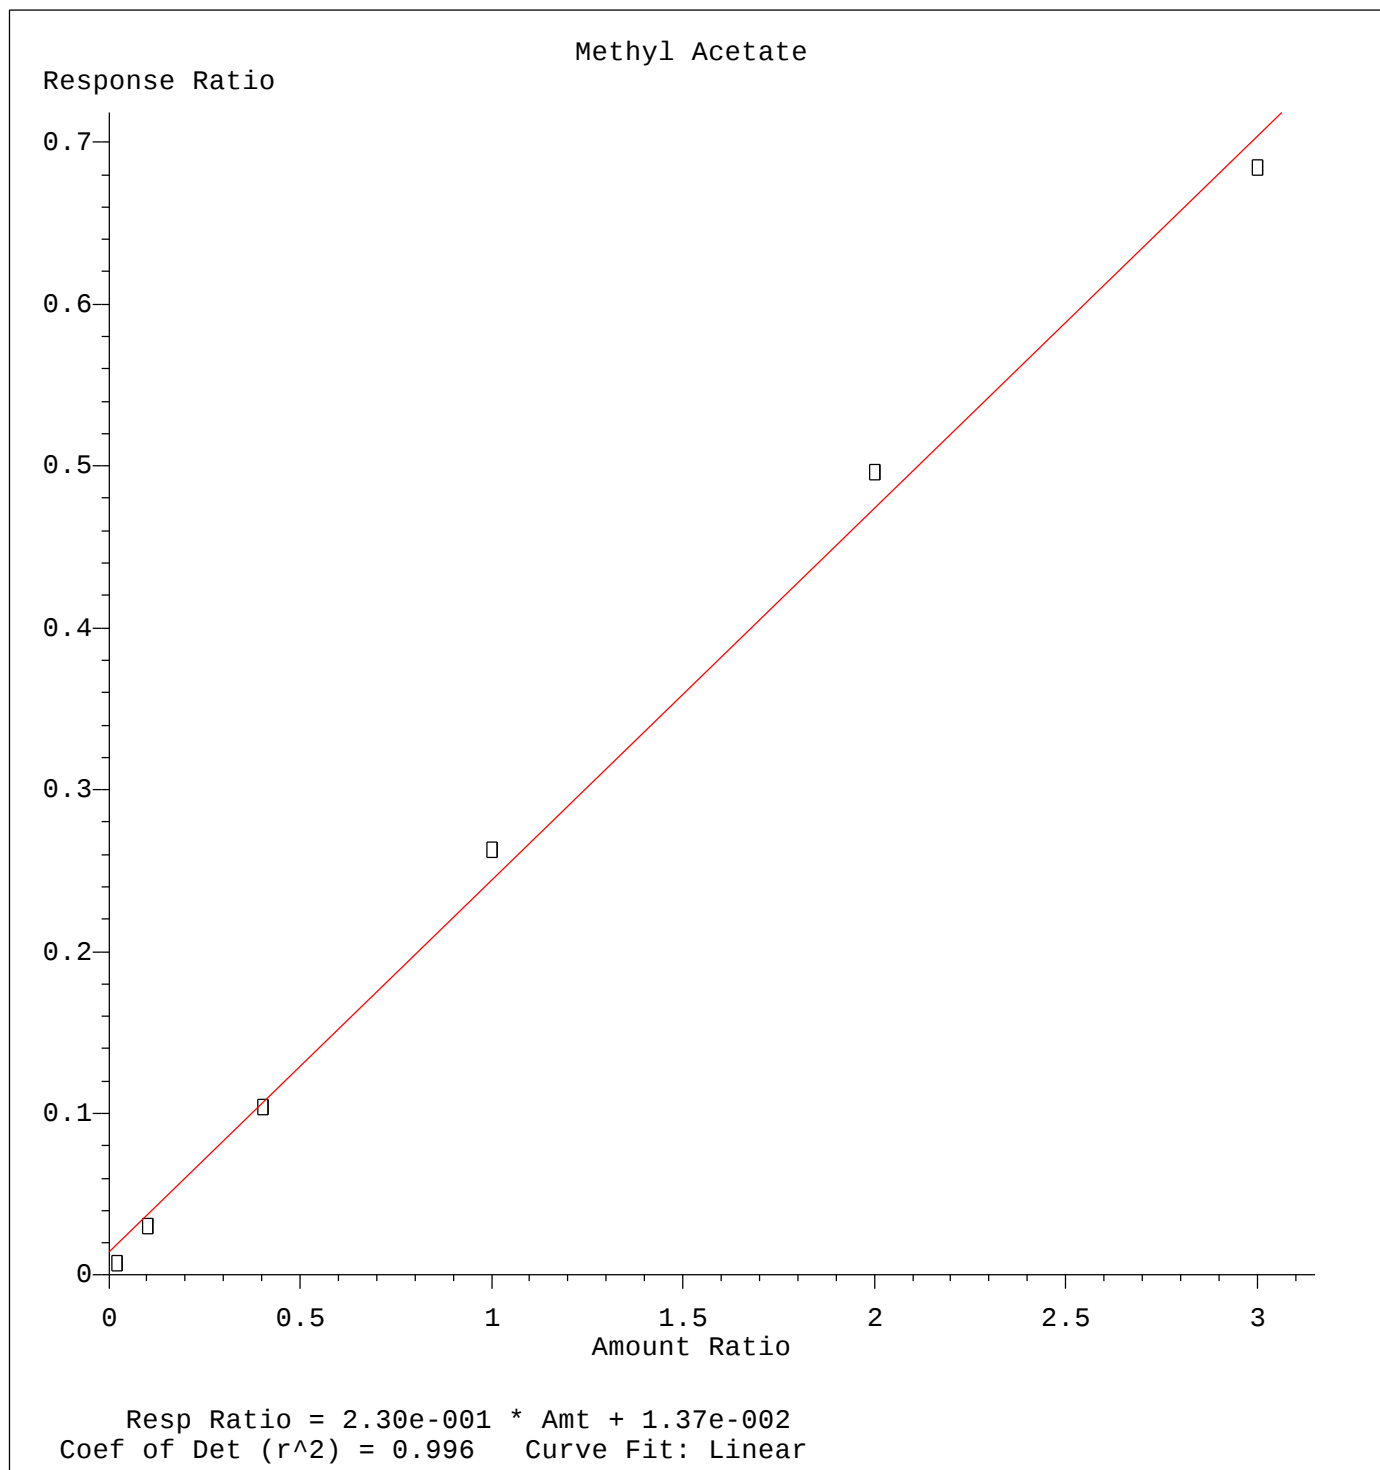

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101718W.M
Calibration Table Last Updated: Fri Oct 19 05:11:28 2018

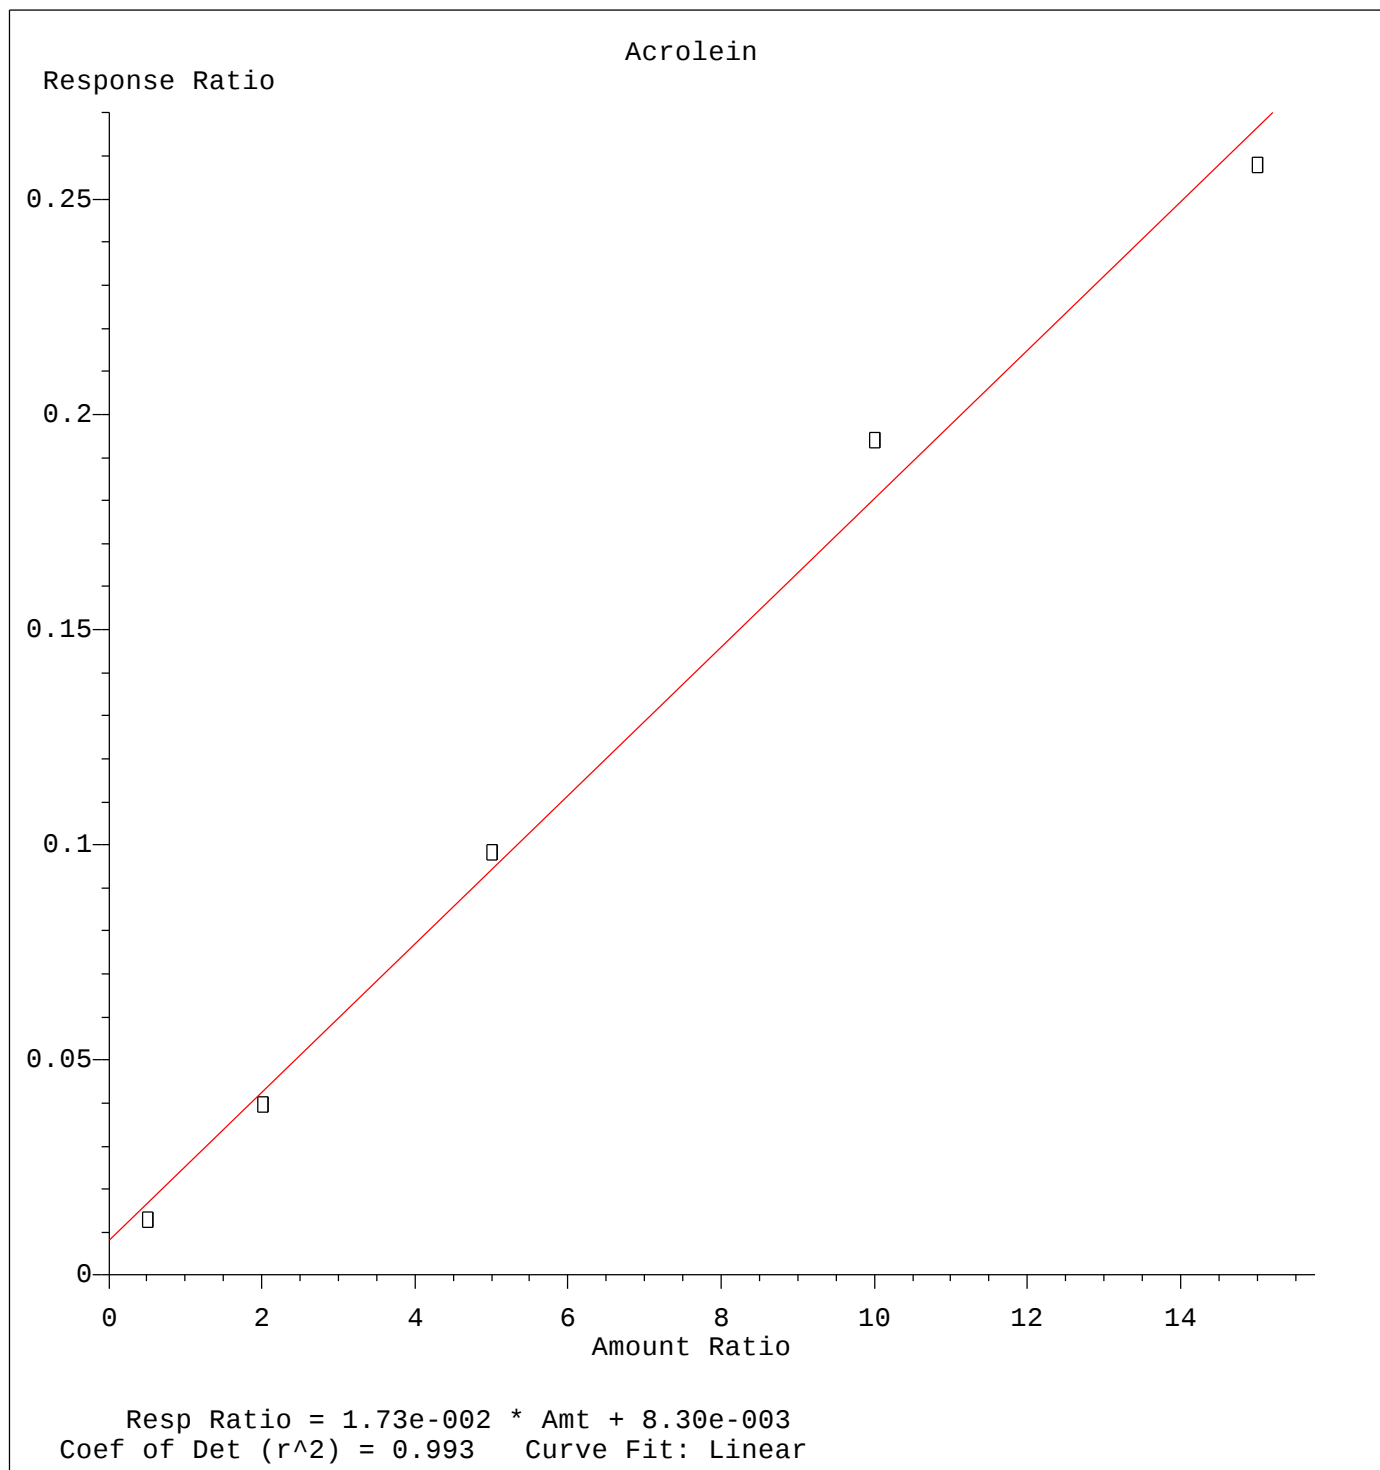


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101718W.M
Calibration Table Last Updated: Fri Oct 19 05:11:28 2018

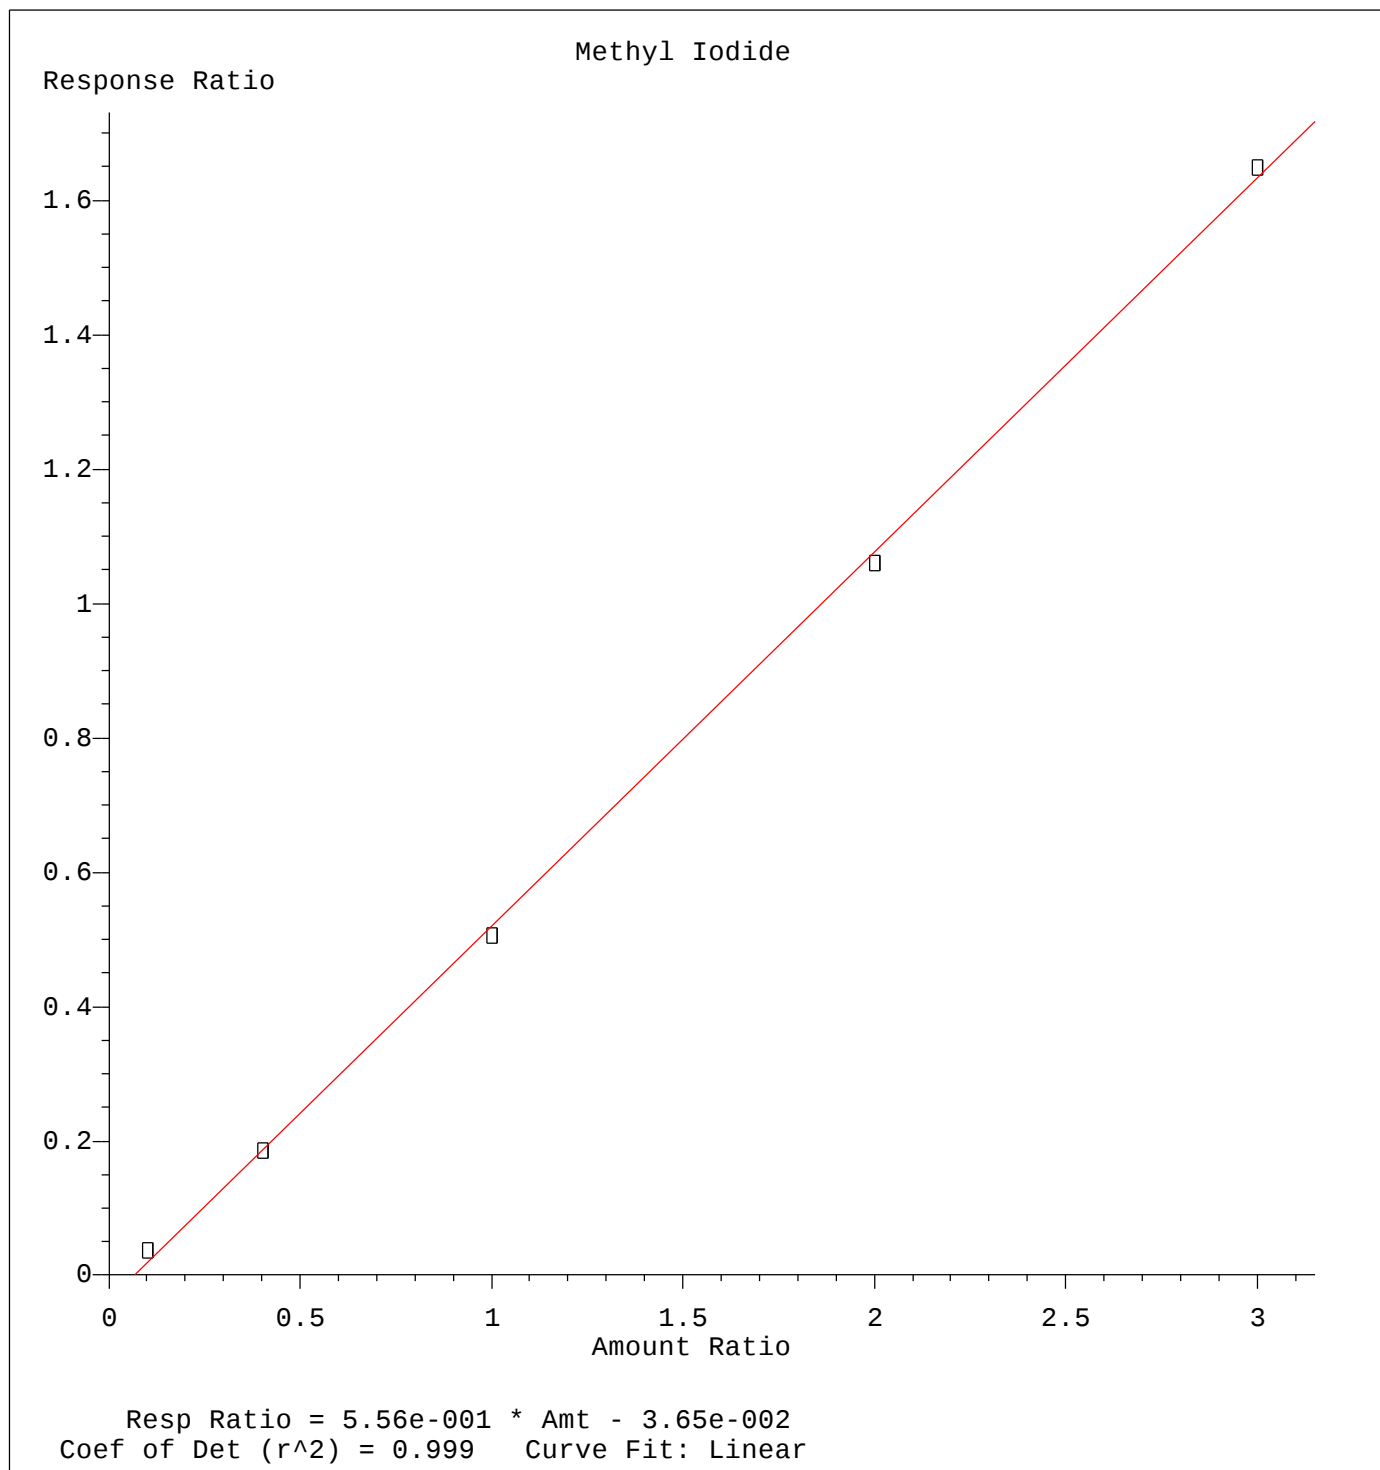

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101718W.M
Calibration Table Last Updated: Fri Oct 19 05:11:28 2018

1,2,3-Trichlorobenzene

Response Ratio

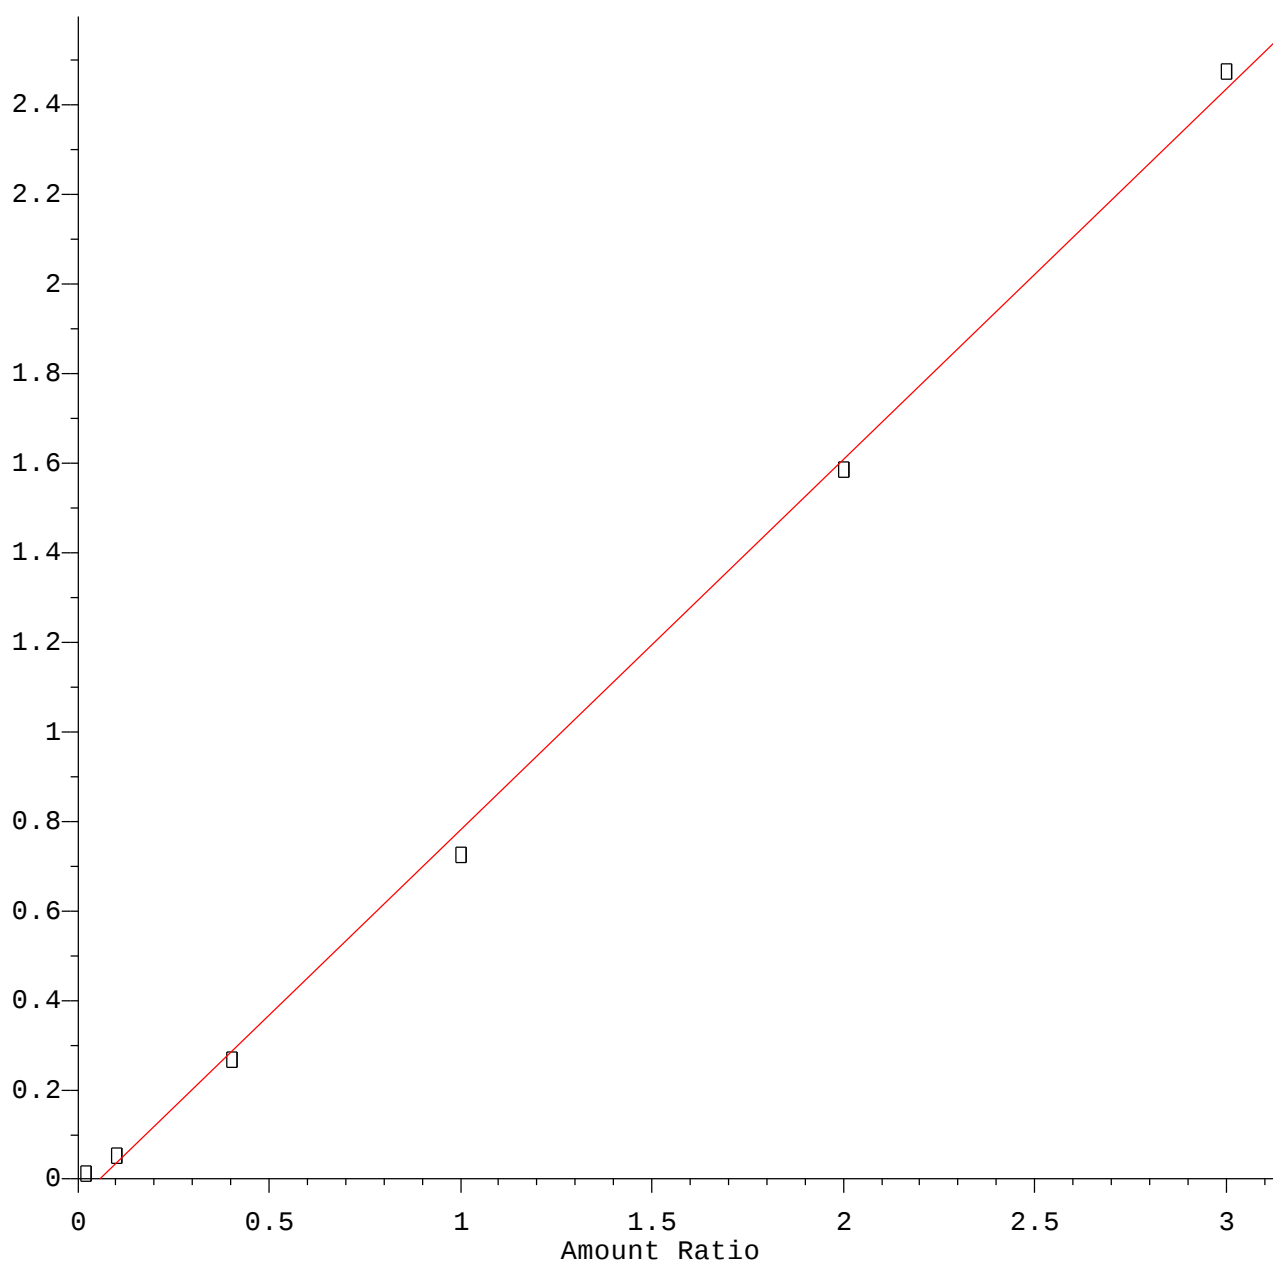


Resp Ratio = $8.28 \times 10^{-1} \times \text{Amt} - 4.82 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101718W.M
Calibration Table Last Updated: Fri Oct 19 05:11:28 2018

Naphthalene

Response Ratio

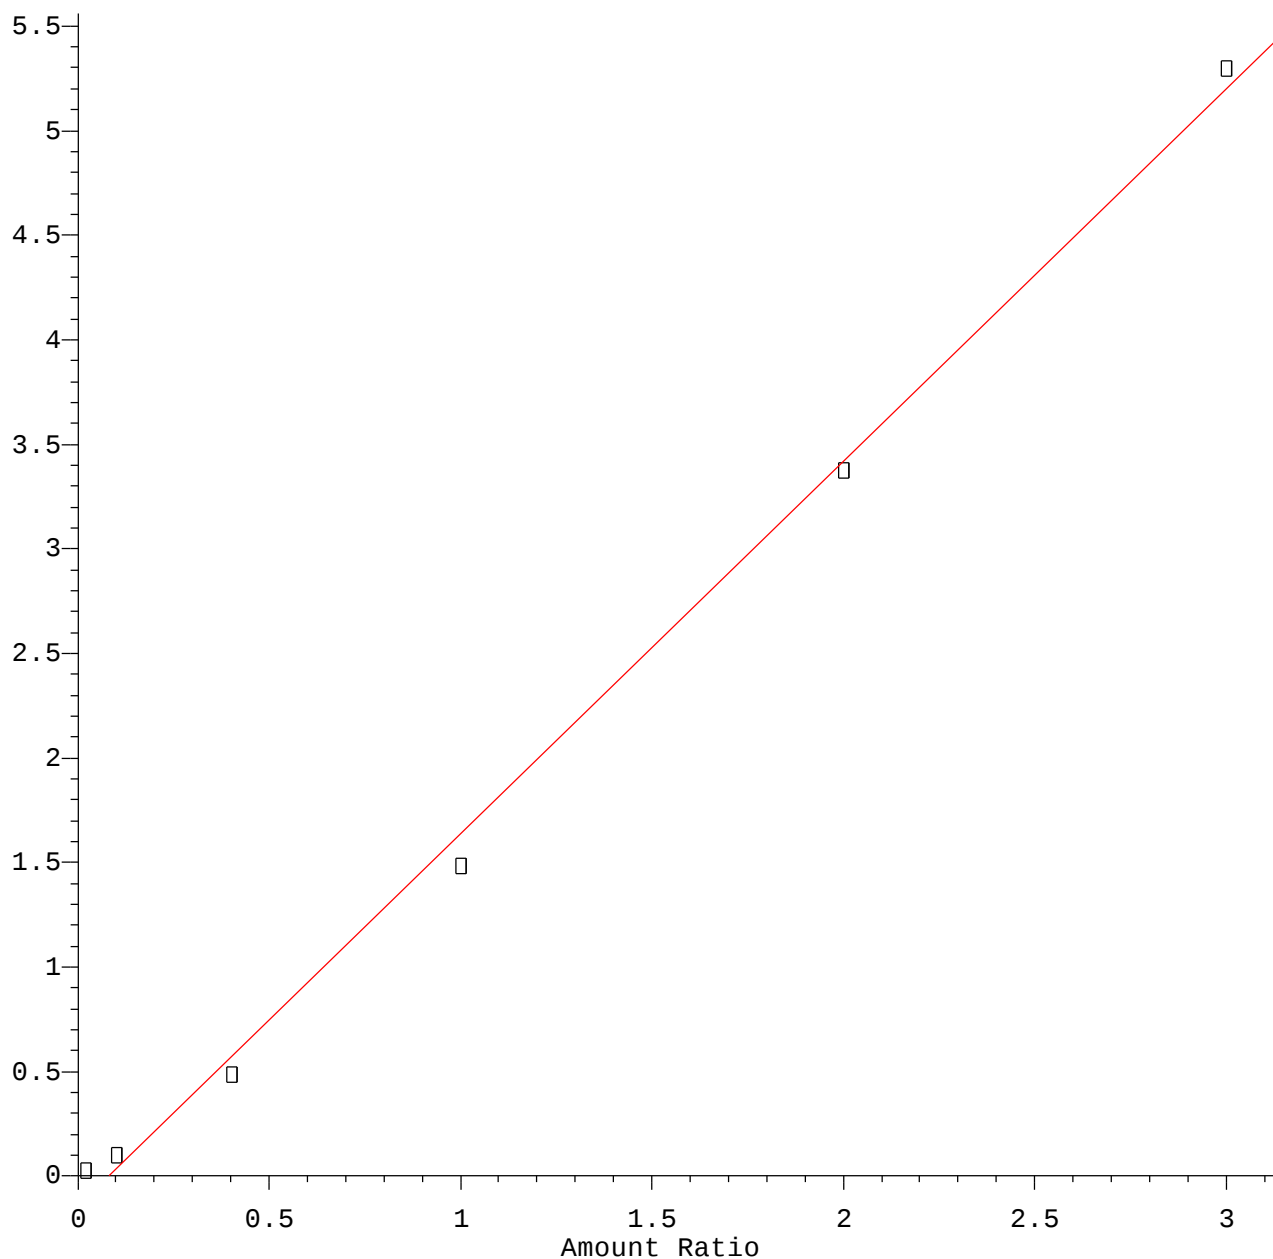


Resp Ratio = 1.78e+000 * Amt - 1.45e-001
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101718W.M
Calibration Table Last Updated: Fri Oct 19 05:11:28 2018

1,2,4-Trichlorobenzene


Response Ratio

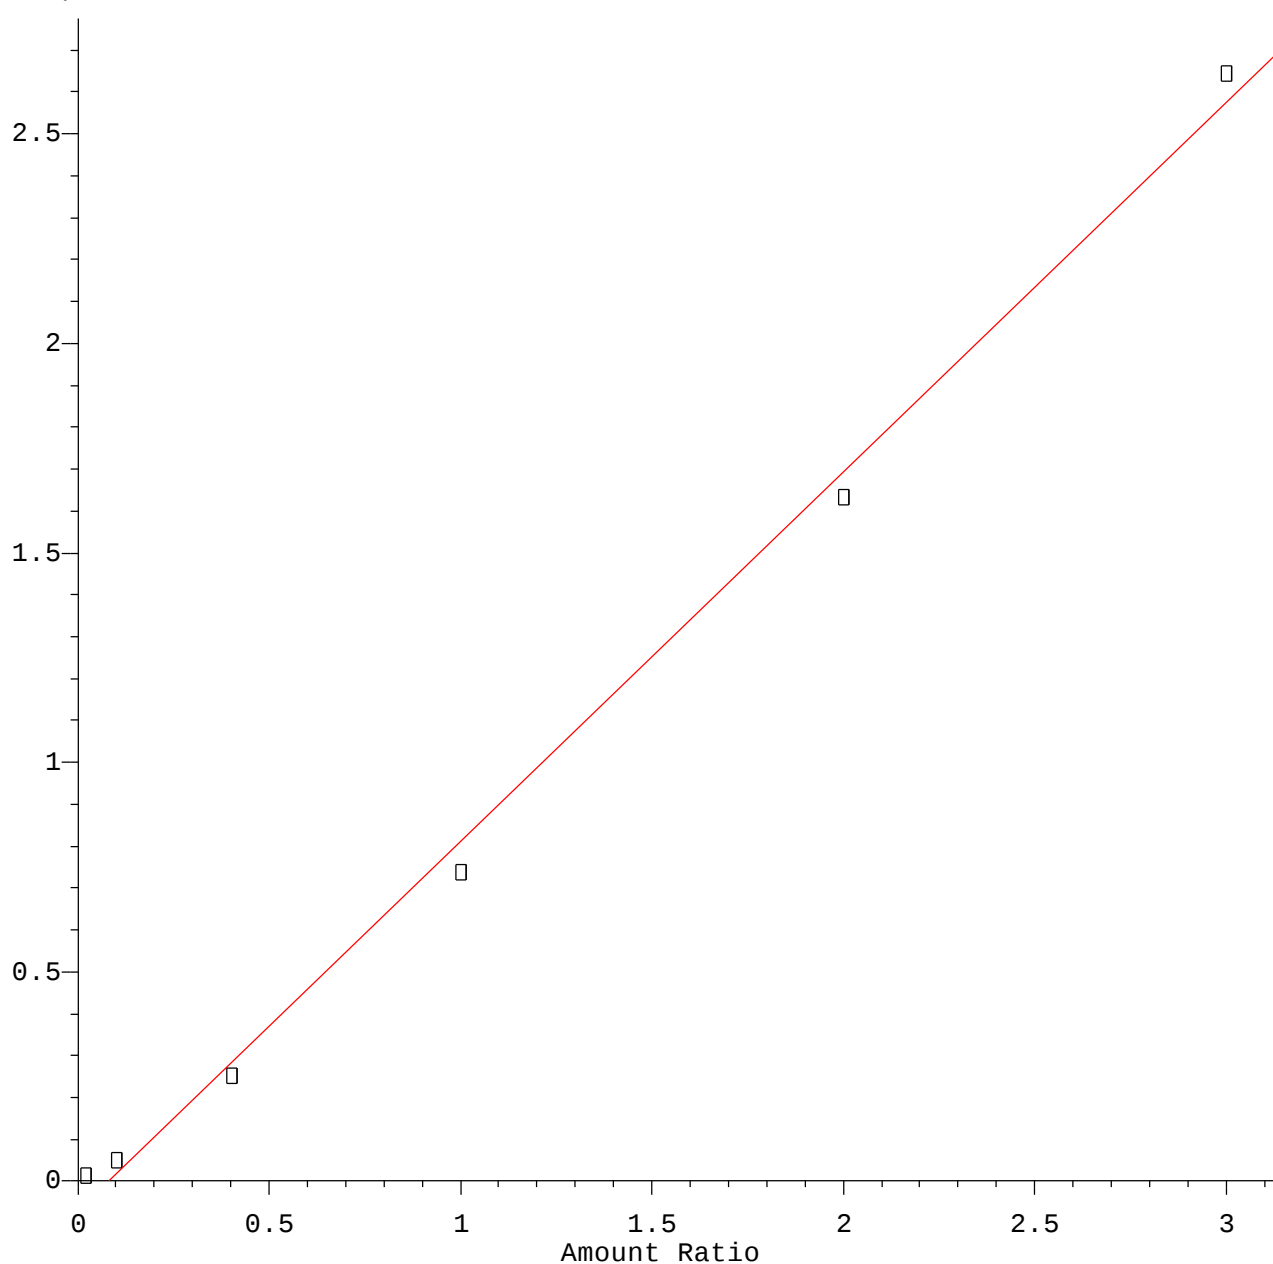

Resp Ratio = $8.82 \times 10^{-1} \times \text{Amt} - 7.16 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101718W.M
Calibration Table Last Updated: Fri Oct 19 05:11:28 2018

trans-1,4-Dichloro-2-butene

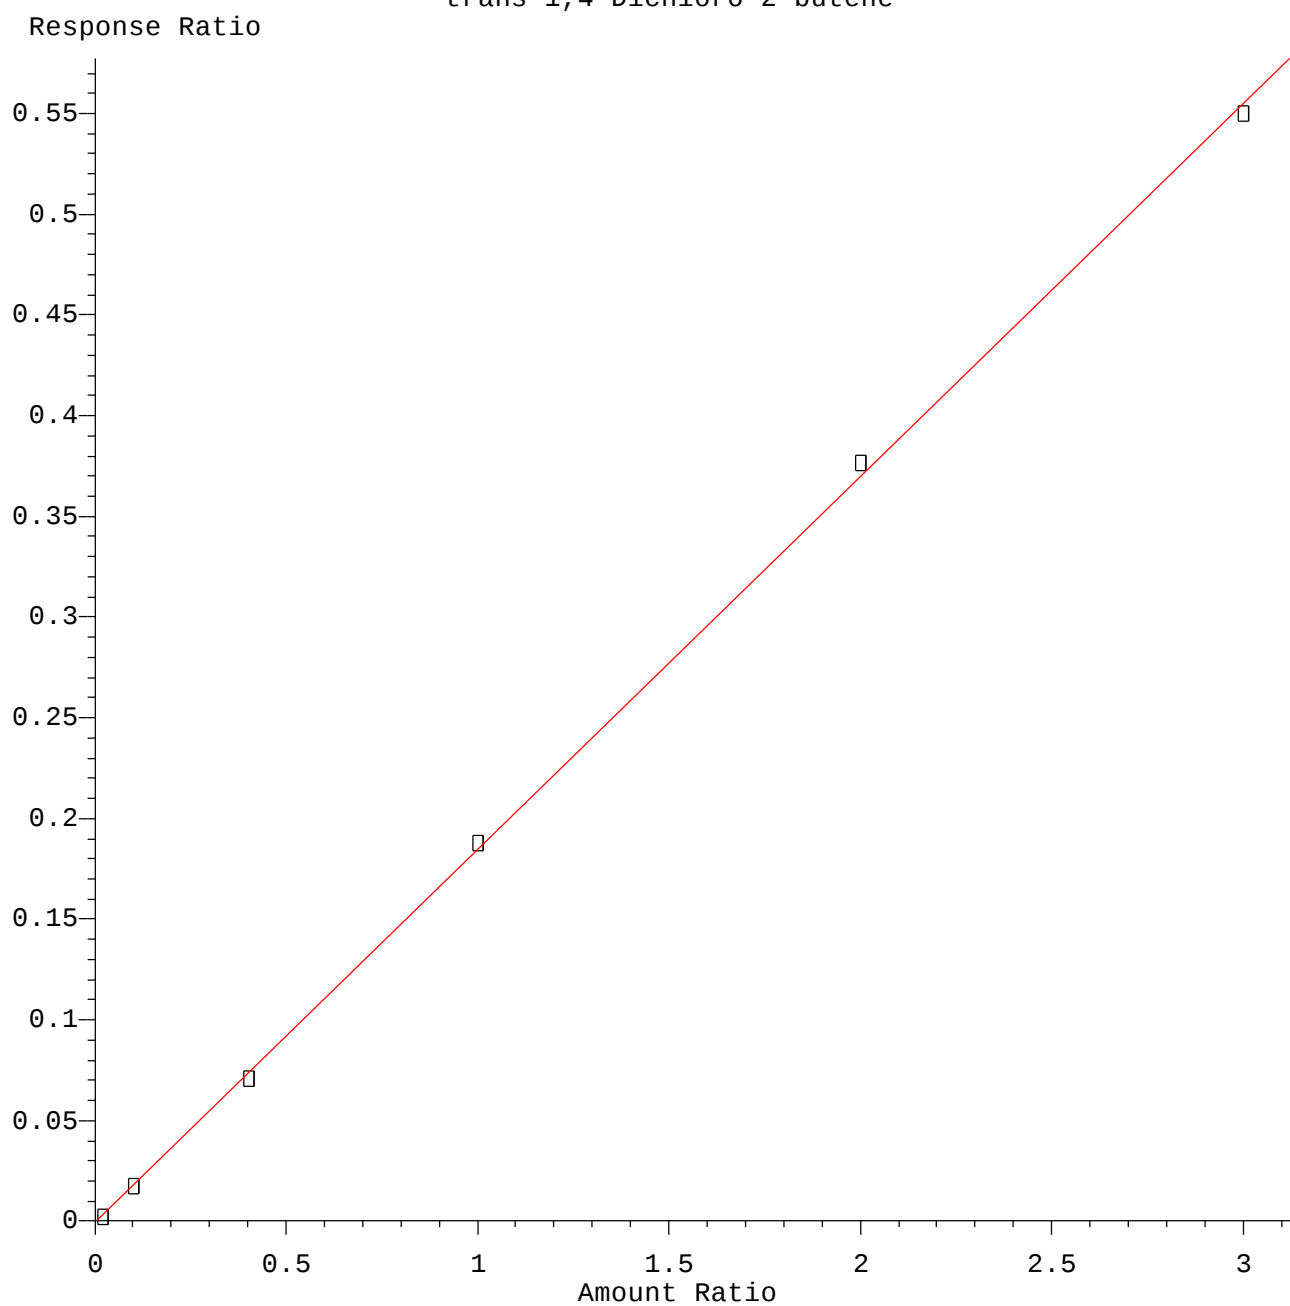


Resp Ratio = $1.85 \times 10^{-1} \times \text{Amt} - 6.48 \times 10^{-4}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101718W.M
Calibration Table Last Updated: Fri Oct 19 05:11:28 2018


2-Chlorotoluene

Response Ratio

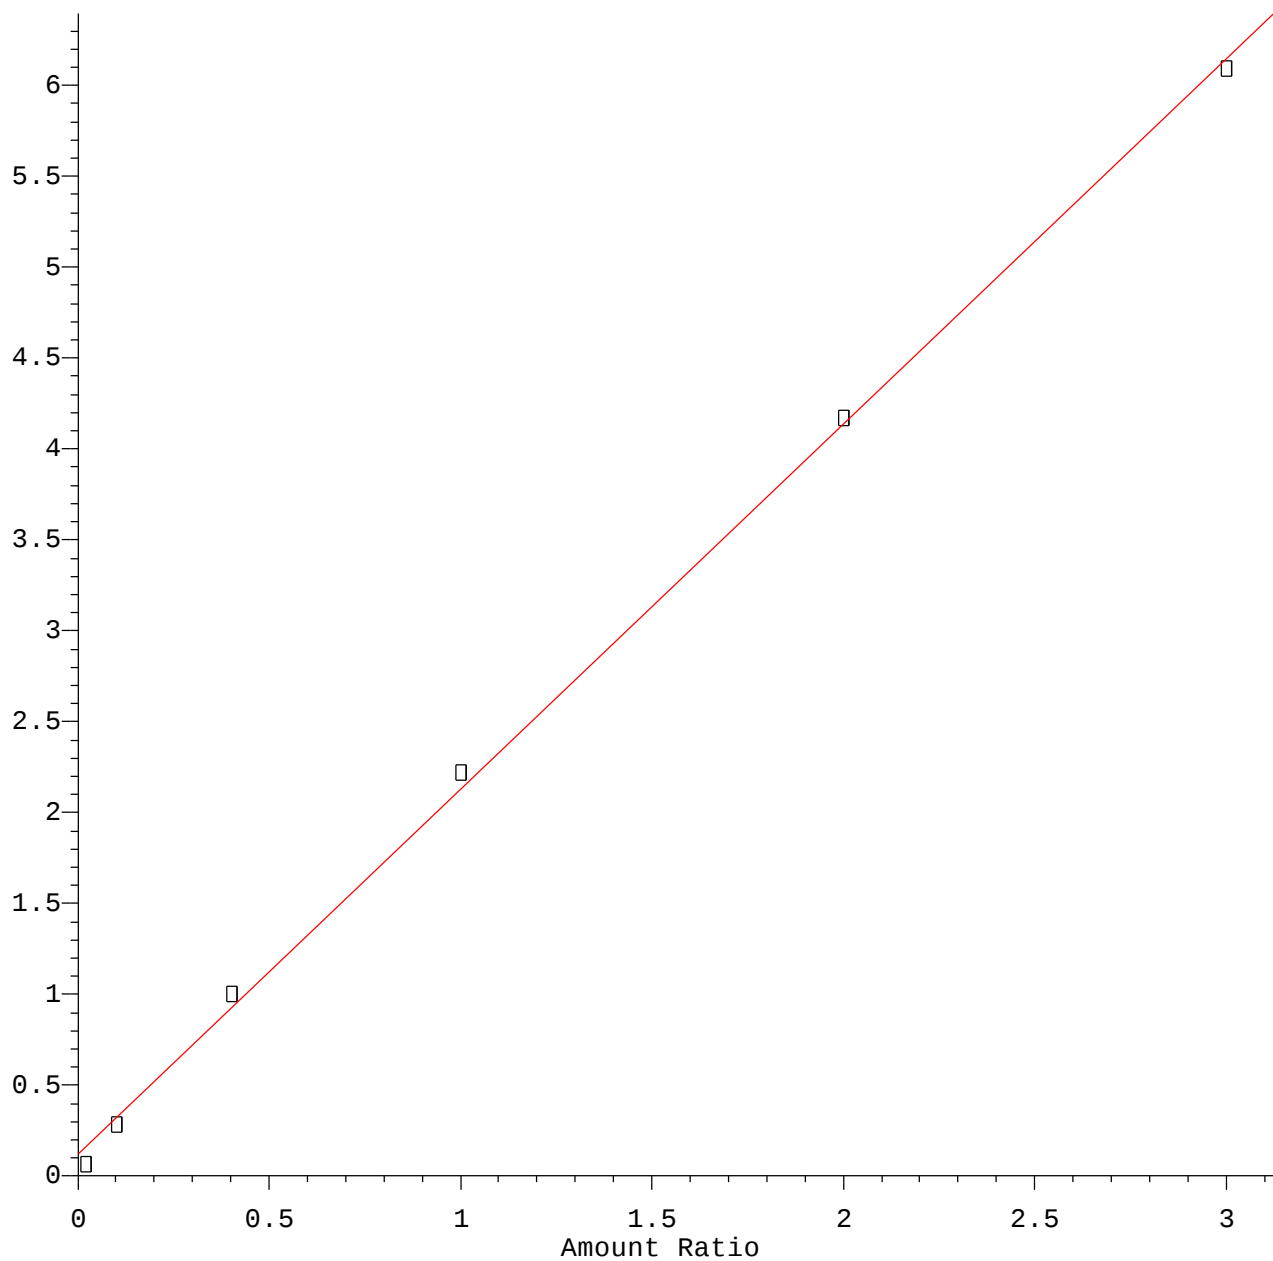


Resp Ratio = 2.01e+000 * Amt + 1.20e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101718W.M
Calibration Table Last Updated: Fri Oct 19 05:11:28 2018

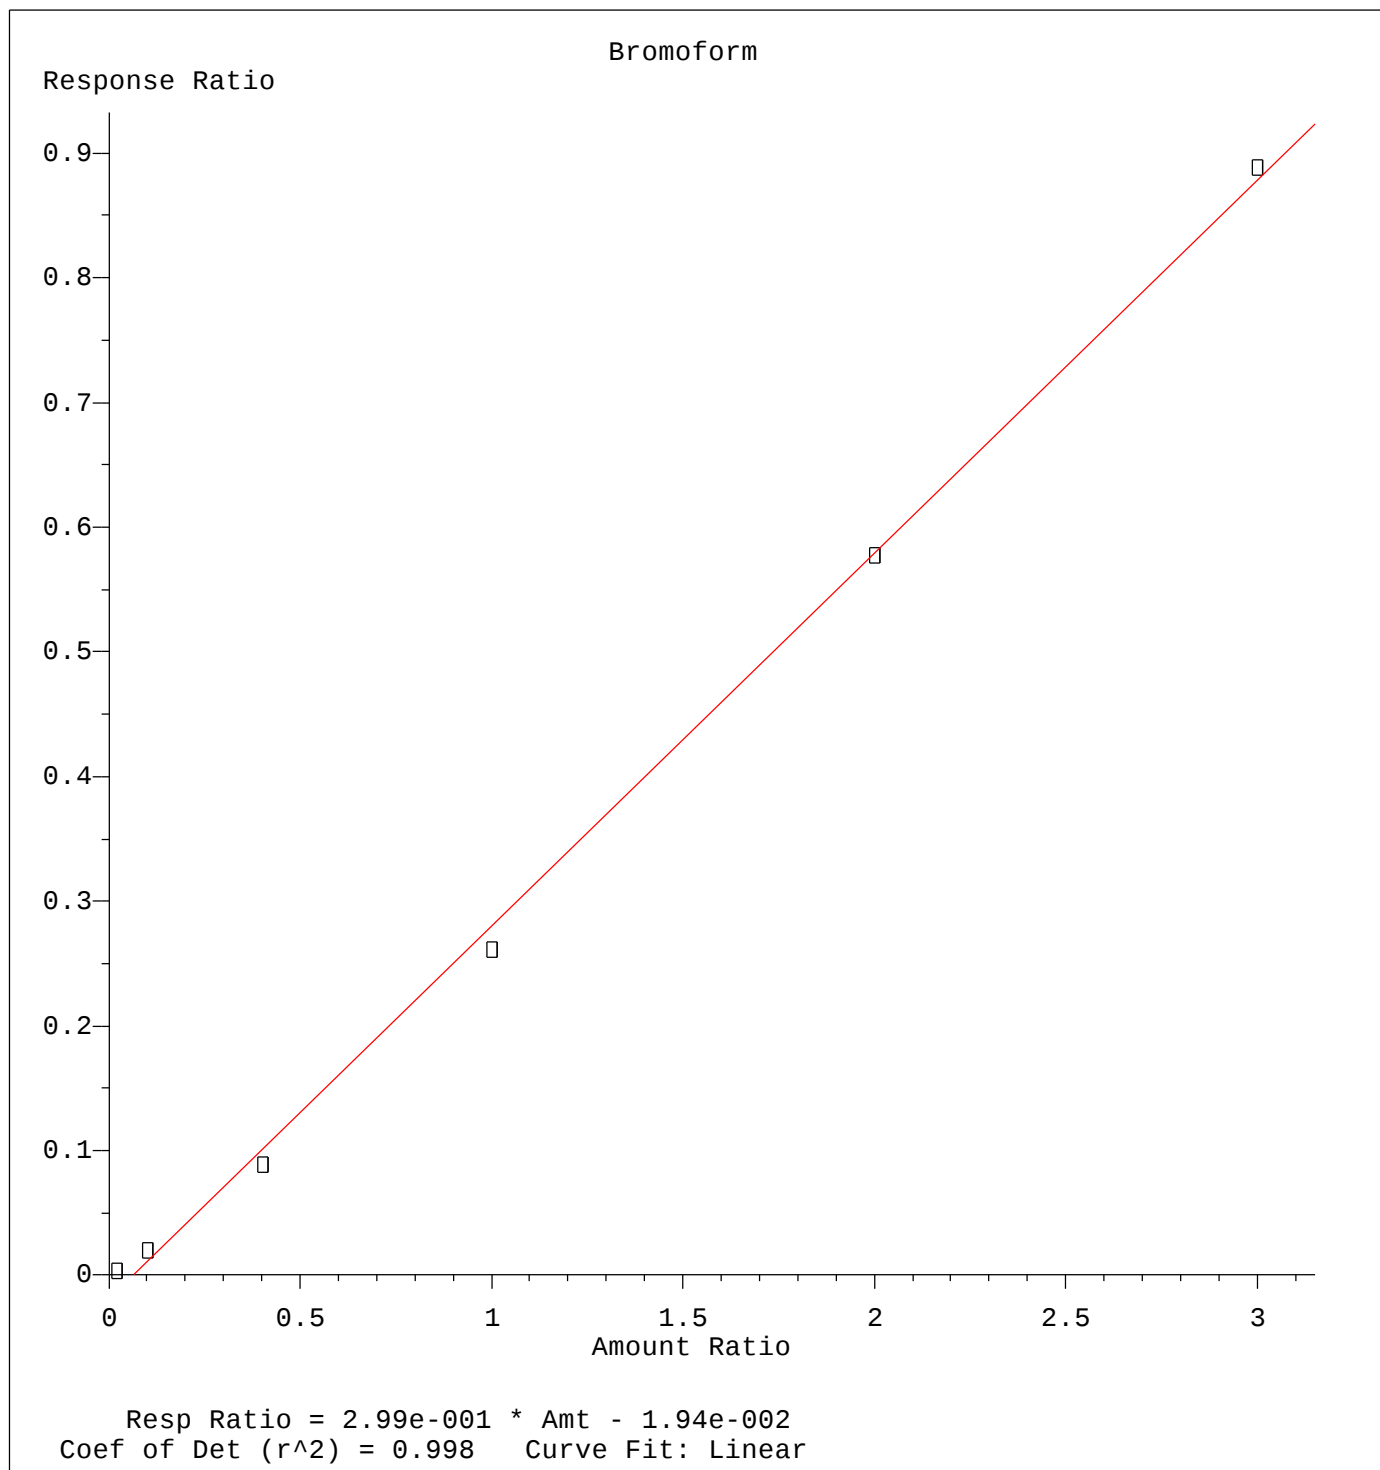

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101718W.M
Calibration Table Last Updated: Fri Oct 19 05:11:28 2018

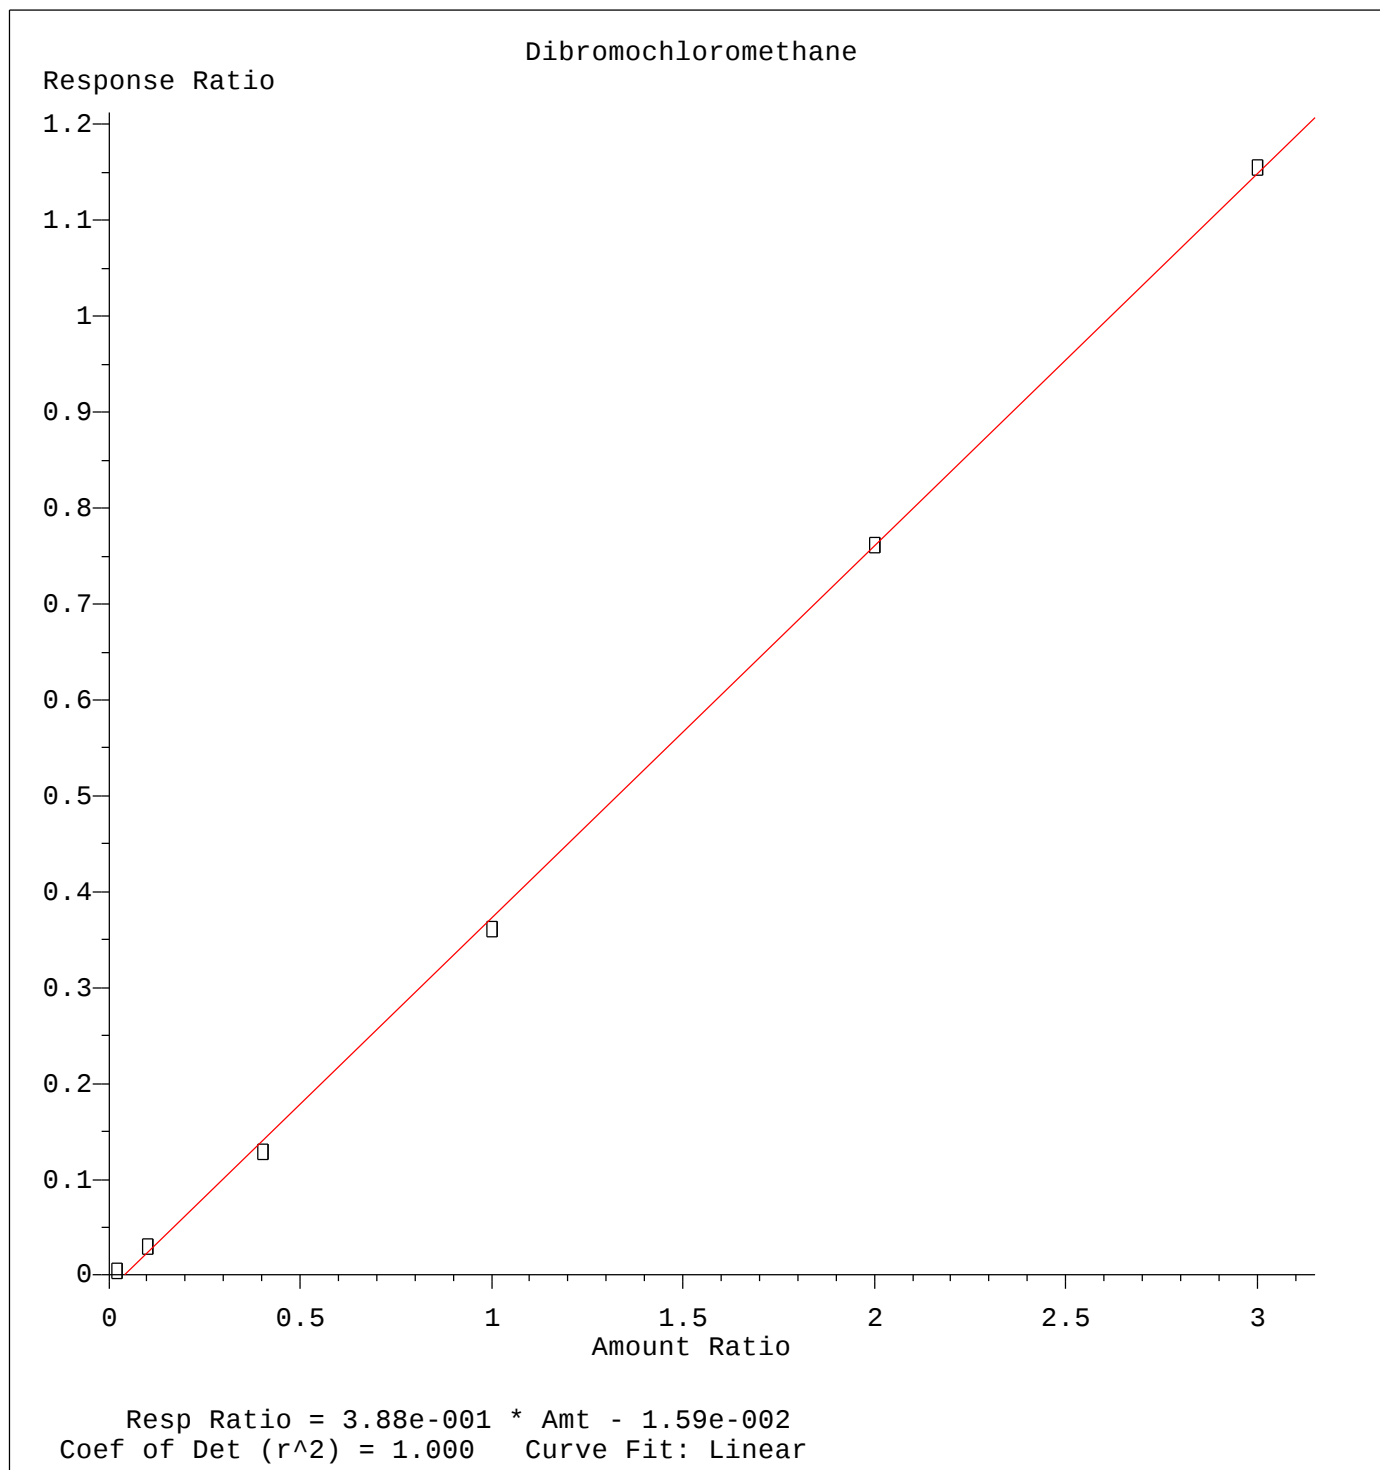

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101718W.M
Calibration Table Last Updated: Fri Oct 19 05:11:28 2018