


Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_N\DATA\VN101718\  
Data File : VN051896.D  
Acq On : 17 Oct 2018 7:32  
Operator : MD\SY  
Sample : BFB  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 28

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N101718W.M  
Title : SW846 8260  
Last Update : Fri Oct 19 05:11:28 2018

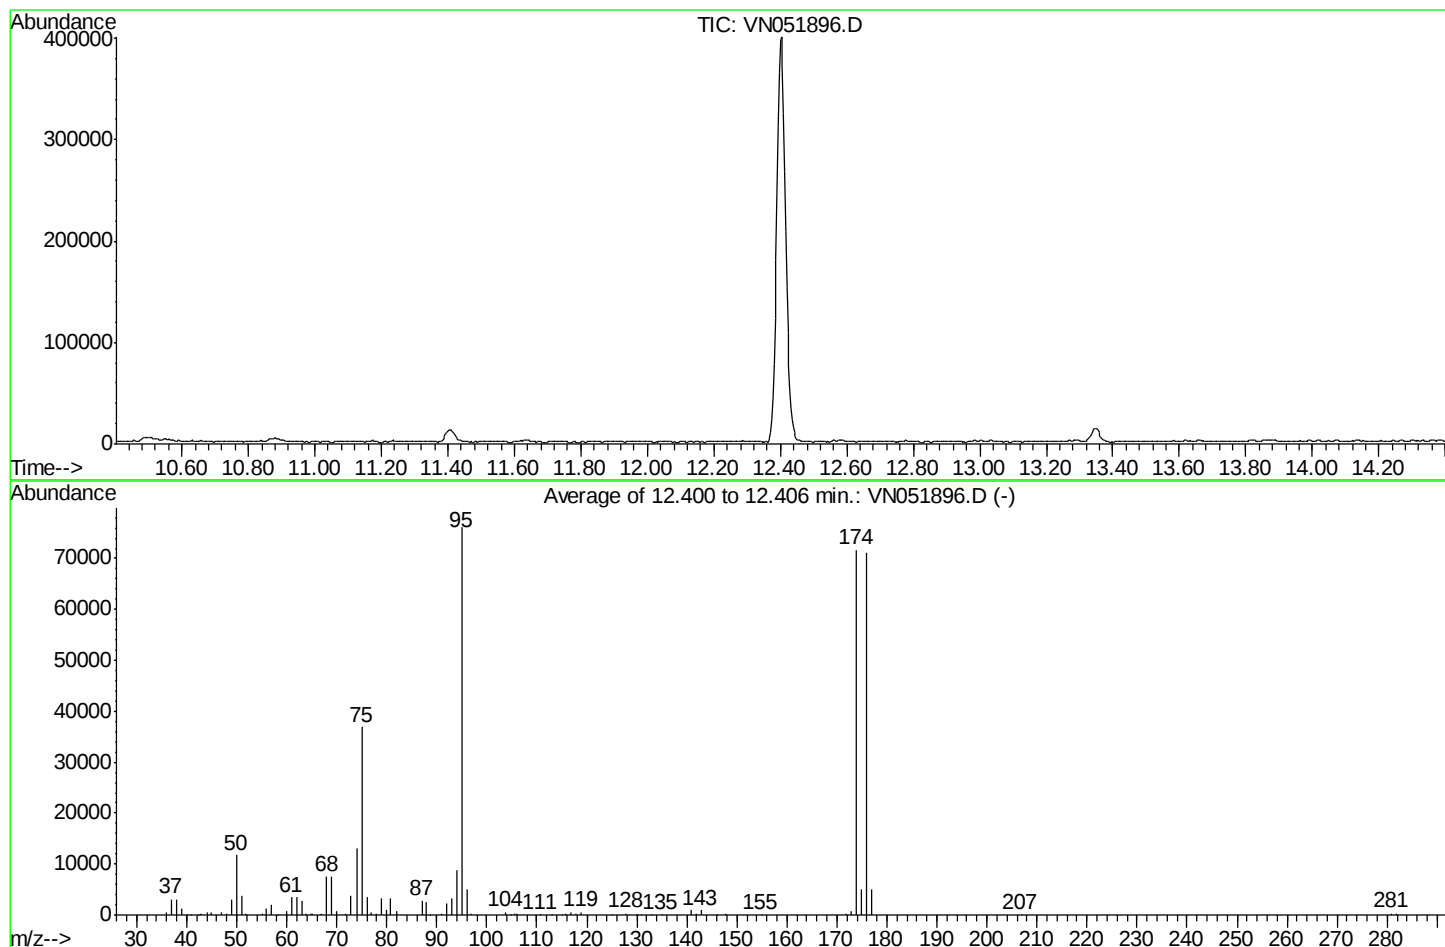

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 15.5      | 11776   | PASS             |
| 75          | 95           | 30           | 60           | 48.4      | 36842   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 76112   | PASS             |
| 96          | 95           | 5            | 9            | 6.6       | 5019    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.9       | 663     | PASS             |
| 174         | 95           | 50           | 100          | 94.2      | 71674   | PASS             |
| 175         | 174          | 5            | 9            | 7.2       | 5145    | PASS             |
| 176         | 174          | 95           | 101          | 99.2      | 71093   | PASS             |
| 177         | 176          | 5            | 9            | 7.2       | 5091    | PASS             |