

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101722\
 Data File : VN074923.D
 Acq On : 17 Oct 2022 18:08
 Operator : JC\MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Quant Time: Oct 18 03:05:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101722W.M
 Quant Title : SW846 8260
 QLast Update : Mon Oct 17 16:03:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.235	168	265028	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	506857	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	522297	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	215443	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	389581	55.726	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 111.460%			
35) Dibromofluoromethane	8.177	113	309604	54.329	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 108.660%			
50) Toluene-d8	10.571	98	1146466	48.515	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 97.020%			
62) 4-Bromofluorobenzene	12.847	95	272437	39.682	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 79.360%#			
Target Compounds						
					Qvalue	
3) Chloromethane	2.395	50	3519	Below Cal	#	14
4) Vinyl Chloride	2.530	62	2585	0.235	ug/l #	51
5) Bromomethane	2.959	94	5636	Below Cal		91
11) Tert butyl alcohol	5.583	59	599	0.394	ug/l #	73
13) Acrolein	4.206	56	1229	0.820	ug/l	87
16) Acetone	4.459	43	3363	1.023	ug/l #	66
18) Methyl Acetate	5.077	43	9237	0.906	ug/l #	85
20) Methylene Chloride	5.306	84	1407	0.231	ug/l #	45
27) cis-1,2-Dichloroethene	7.500	96	1606	0.258	ug/l	90
31) Cyclohexane	8.230	56	8213	0.908	ug/l #	42
36) 1,1-Dichloropropene	8.235	75	24338	3.252	ug/l #	53
38) Carbon Tetrachloride	8.230	117	28790	3.801	ug/l #	20
42) 1,2-Dichloroethane	8.694	62	3970	0.464	ug/l	100
44) Trichloroethene	9.359	130	1776	0.336	ug/l	84
51) 4-Methyl-2-Pentanone	10.441	43	3354	0.289	ug/l #	37
52) Toluene	10.635	92	3176	0.210	ug/l #	74
53) t-1,3-Dichloropropene	10.835	75	2161	0.233	ug/l #	82
58) 2-Chloroethyl Vinyl ether	10.159	63	1599	9.664	ug/l #	85
59) 2-Hexanone	11.206	43	5680	0.654	ug/l	97
65) Chlorobenzene	11.906	112	7156	0.477	ug/l	93
68) m/p-Xylenes	12.076	106	2451	0.241	ug/l #	40
69) o-Xylene	12.400	106	2700	0.261	ug/l	85
70) Styrene	12.412	104	3521	0.216	ug/l	92
75) 1,1,2,2-Tetrachloroethane	12.935	83	2608	0.333	ug/l	88
76) 1,2,3-Trichloropropane	12.853	75	155832	25.591	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	155832	61.513	ug/l #	9
91) 1,2-Dichlorobenzene	14.106	146	1871	0.253	ug/l #	79
92) 1,2-Dibromo-3-Chloropr...	14.735	75	887	0.696	ug/l	72
94) Hexachlorobutadiene	15.506	225	1937	1.172	ug/l	80
95) Naphthalene	15.635	128	3076	0.206	ug/l #	74
96) 1,2,3-Trichlorobenzene	15.829	180	902	0.250	ug/l #	40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101722\
Data File : VN074923.D
Acq On : 17 Oct 2022 18:08
Operator : JC\MD
Sample : IBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Time: Oct 18 03:05:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101722W.M
Quant Title : SW846 8260
QLast Update : Mon Oct 17 16:03:54 2022
Response via : Initial Calibration




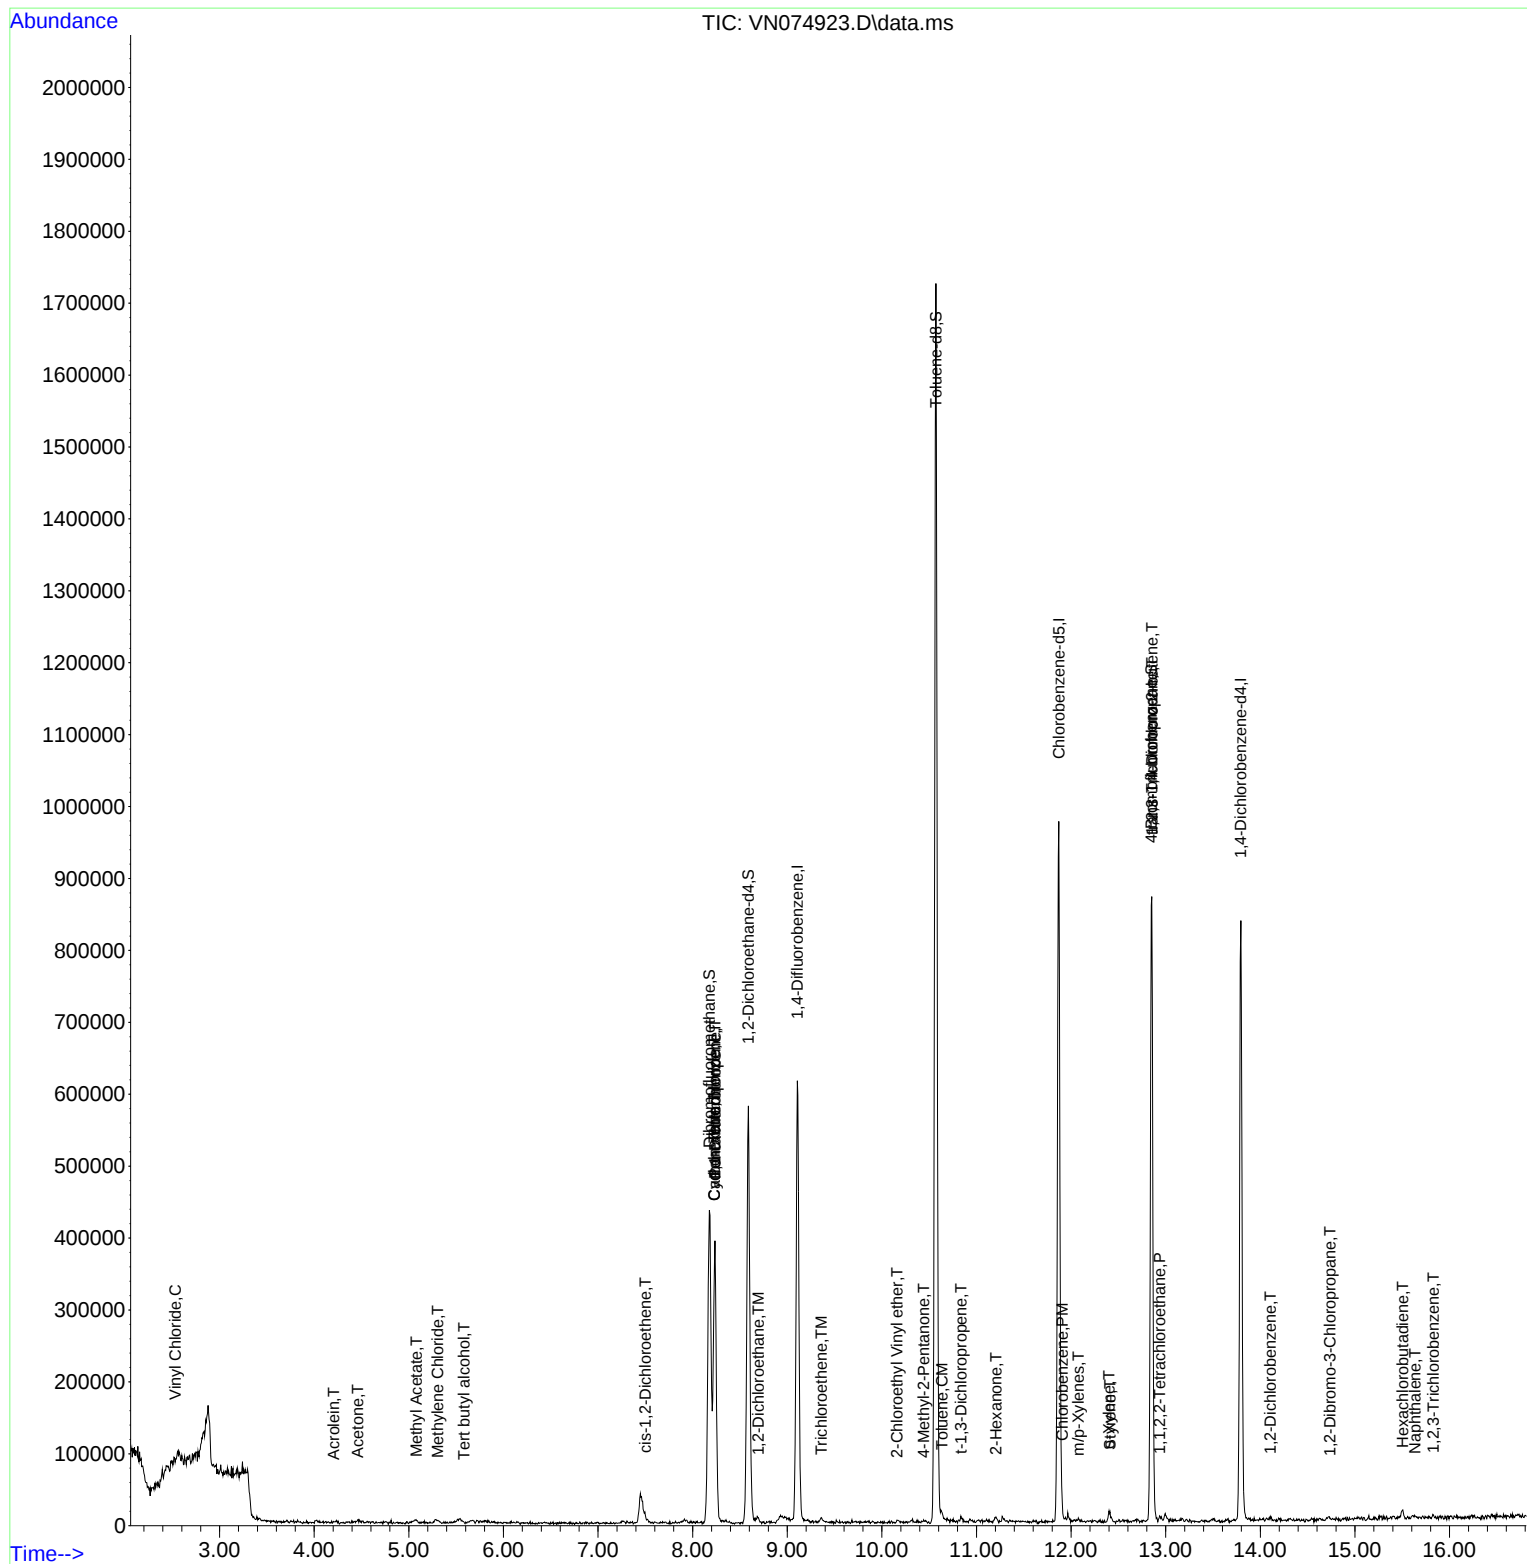




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.235 min Scan# 1051
Delta R.T. -0.001 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 265028
Ion Ratio Lower Upper
168 100
99 57.2 47.6 71.4

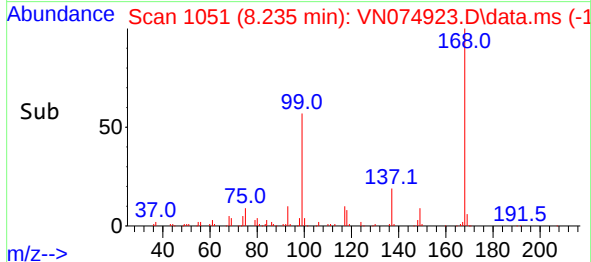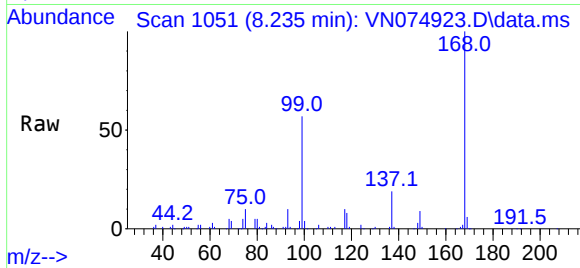

#3
Chloromethane
Concen: Below Cal
RT: 2.395 min Scan# 58
Delta R.T. 0.006 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08

Tgt Ion: 50 Resp: 3519
Ion Ratio Lower Upper
50 100
52 80.9 26.1 39.1#


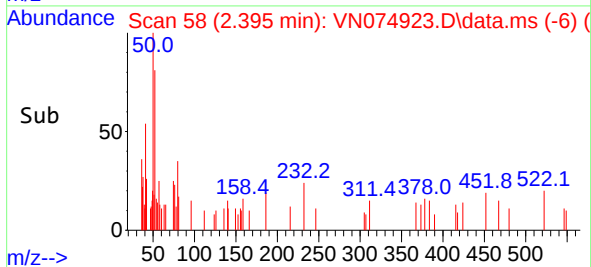

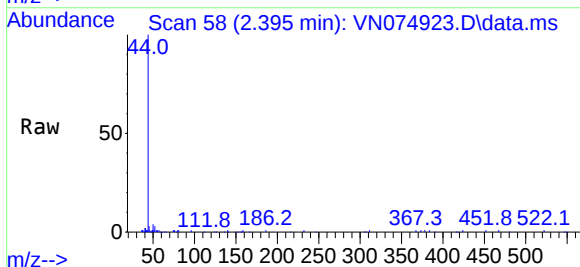


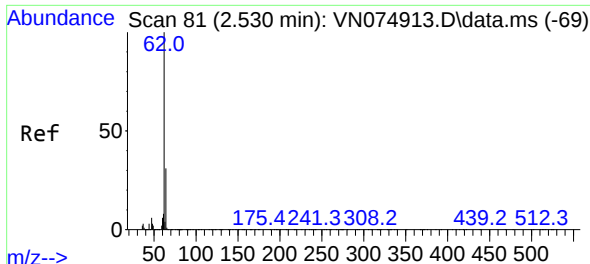

#4
 Vinyl Chloride
 Concen: 0.235 ug/l
 RT: 2.530 min Scan# 81
 Delta R.T. -0.000 min
 Lab File: VN074923.D
 Acq: 17 Oct 2022 18:08




Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK


Tgt Ion: 62 Resp: 2585
 Ion Ratio Lower Upper
 62 100
 64 57.7 24.8 37.2#

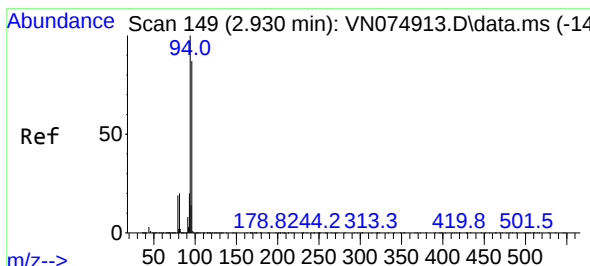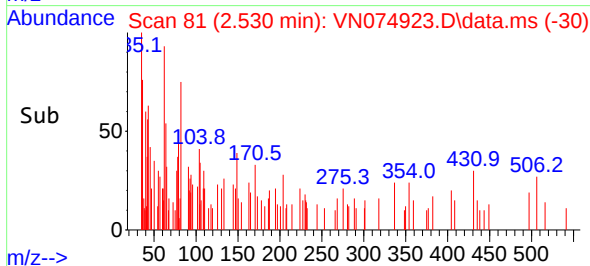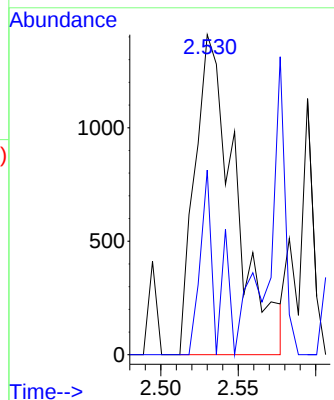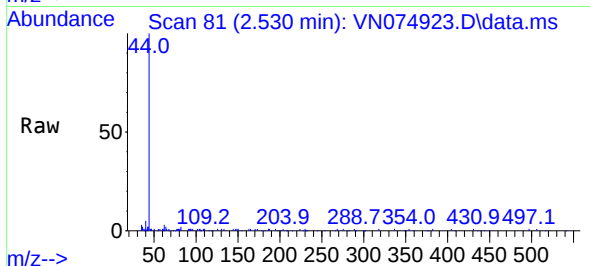

#5
 Bromomethane
 Concen: Below Cal
 RT: 2.959 min Scan# 154
 Delta R.T. 0.029 min
 Lab File: VN074923.D
 Acq: 17 Oct 2022 18:08

Tgt Ion: 94 Resp: 5636
 Ion Ratio Lower Upper
 94 100
 96 78.9 70.0 105.0


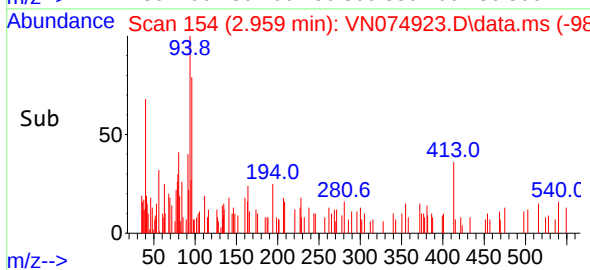
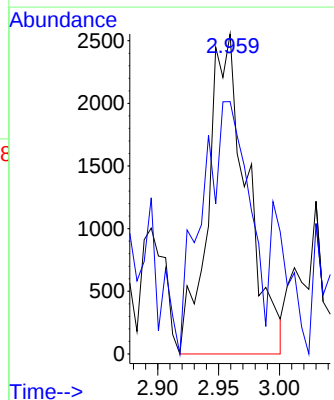
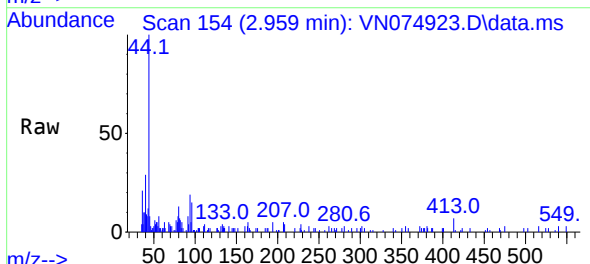




#11
Tert butyl alcohol
Concen: 0.394 ug/l
RT: 5.583 min Scan# 60
Delta R.T. 0.018 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 59 Resp: 599
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#

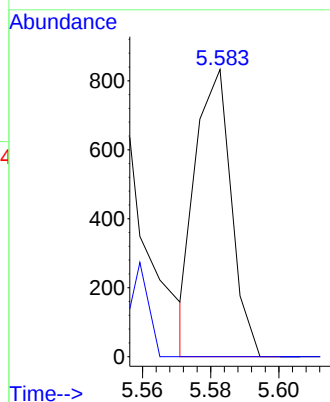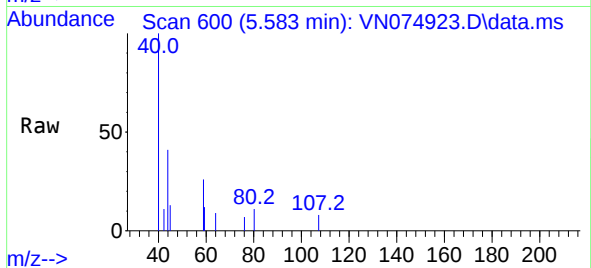

#13
Acrolein
Concen: 0.820 ug/l
RT: 4.206 min Scan# 366
Delta R.T. -0.000 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08

Tgt Ion: 56 Resp: 1229
Ion Ratio Lower Upper
56 100
55 76.7 53.4 80.0


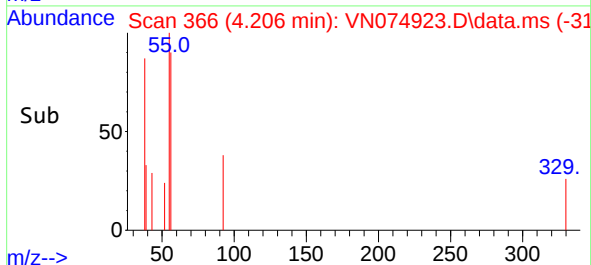

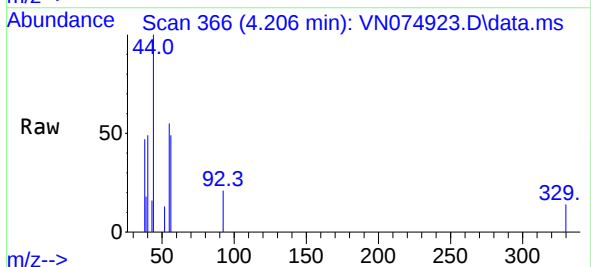




#16
Acetone
Concen: 1.023 ug/l
RT: 4.459 min Scan# 409
Delta R.T. -0.000 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 43 Resp: 3363
Ion Ratio Lower Upper
43 100
58 13.5 25.8 38.8#

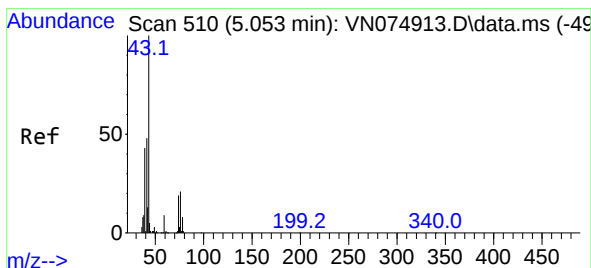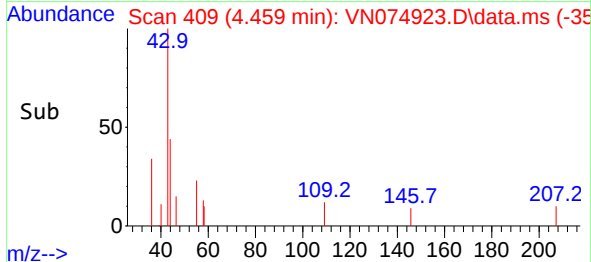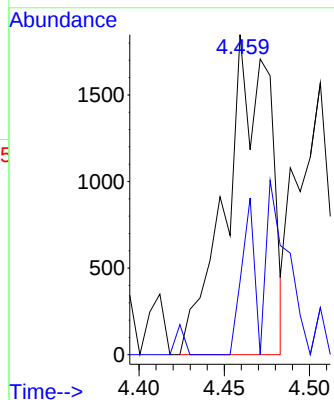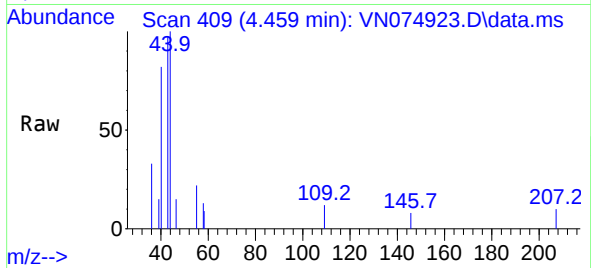

#18
Methyl Acetate
Concen: 0.906 ug/l
RT: 5.077 min Scan# 514
Delta R.T. 0.024 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08

Tgt Ion: 43 Resp: 9237
Ion Ratio Lower Upper
43 100
74 14.4 17.0 25.6#

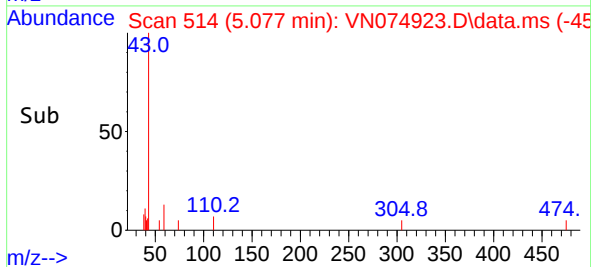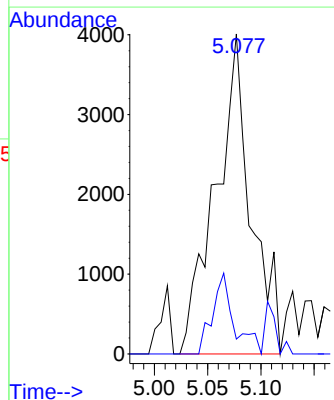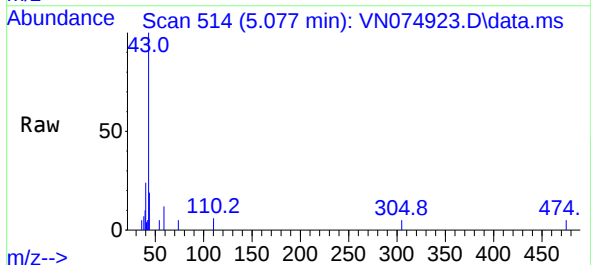



#20

Methylene Chloride

Concen: 0.231 ug/l

RT: 5.306 min Scan# 5

Delta R.T. 0.011 min

Lab File: VN074923.D

Acq: 17 Oct 2022 18:08

Instrument :

MSVOA_N

ClientSampleId :

IBLK

Tgt Ion: 84 Resp: 1407





Ion Ratio Lower Upper

84 100

49 45.0 104.6 156.8#

51 27.9 31.8 47.8#

86 29.9 48.5 72.7#

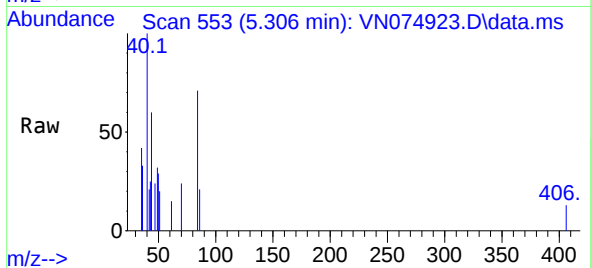

#27

cis-1,2-Dichloroethene

Concen: 0.258 ug/l

RT: 7.500 min Scan# 926

Delta R.T. -0.000 min

Lab File: VN074923.D

Acq: 17 Oct 2022 18:08




Tgt Ion: 96 Resp: 1606


Ion Ratio Lower Upper

96 100

61 133.9 0.0 288.6

98 74.5 0.0 128.0


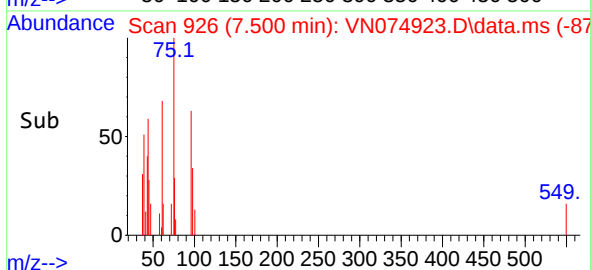






#31
Cyclohexane
Concen: 0.908 ug/l
RT: 8.230 min Scan# 1056
Delta R.T. -0.035 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 56 Resp: 8213
Ion Ratio Lower Upper
56 100
69 80.9 23.4 35.0#
84 129.5 69.9 104.9#

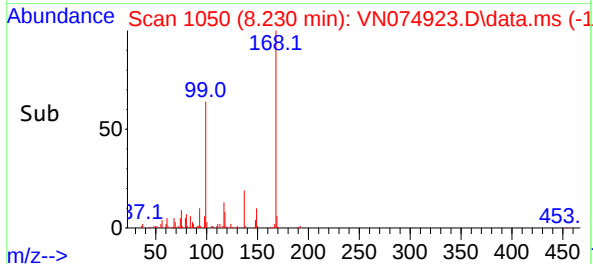

#33
1,2-Dichloroethane-d4
Concen: 55.726 ug/l
RT: 8.588 min Scan# 1111
Delta R.T. -0.000 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08

Tgt Ion: 65 Resp: 389581
Ion Ratio Lower Upper
65 100
67 55.7 0.0 108.2


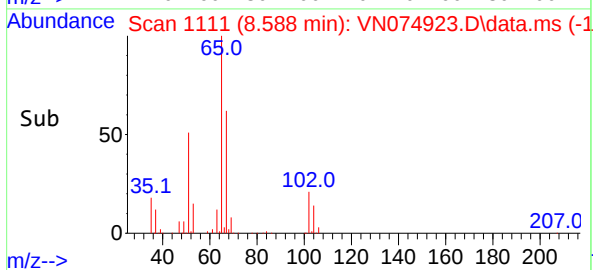

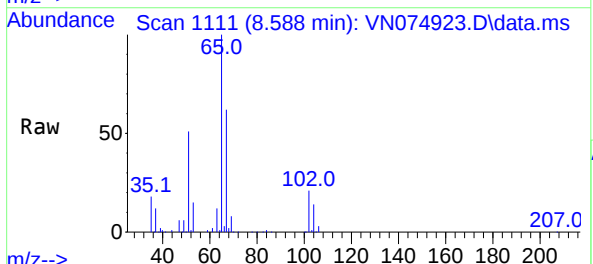




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 1199
Delta R.T. -0.000 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:114 Resp: 506857
Ion Ratio Lower Upper
114 100
63 20.4 0.0 41.2
88 13.3 0.0 30.2

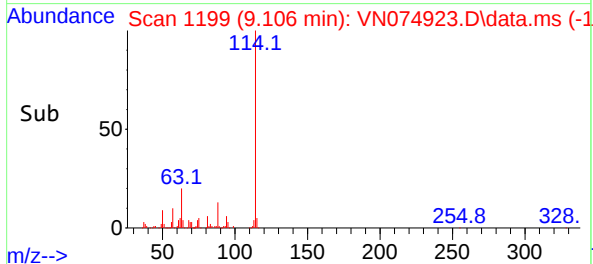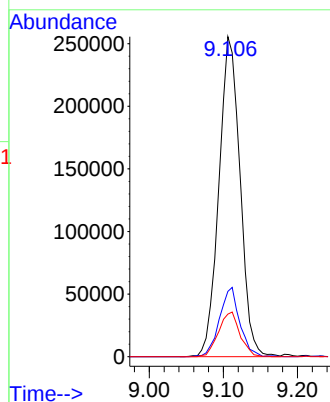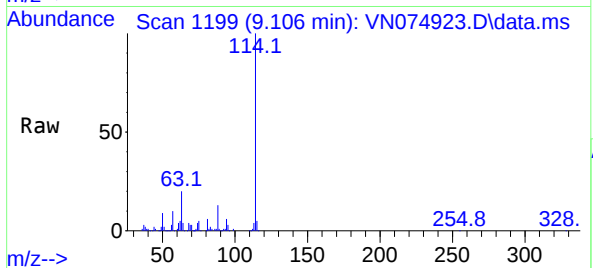

#35
Dibromofluoromethane
Concen: 54.329 ug/l
RT: 8.177 min Scan# 1041
Delta R.T. -0.006 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08

Tgt Ion:113 Resp: 309604
Ion Ratio Lower Upper
113 100
111 101.0 82.9 124.3
192 15.4 14.2 21.2

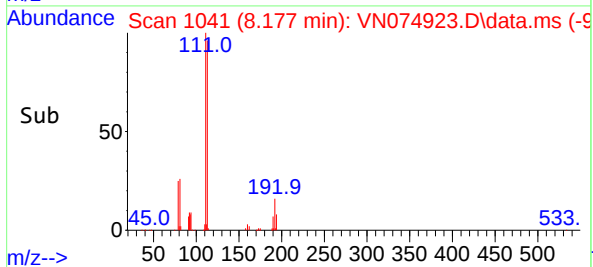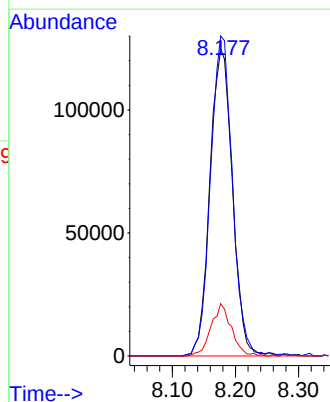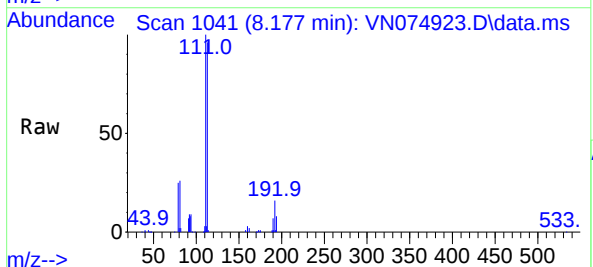



#36

1,1-Dichloropropene

Concen: 3.252 ug/l

RT: 8.235 min Scan# 1051

Delta R.T. -0.141 min

Lab File: VN074923.D

Acq: 17 Oct 2022 18:08

Instrument :

MSVOA_N

ClientSampleId :

IBLK





Tgt Ion: 75 Resp: 24338

Ion Ratio Lower Upper

75 100

110 9.4 16.1 48.3#

77 0.2 23.3 34.9#

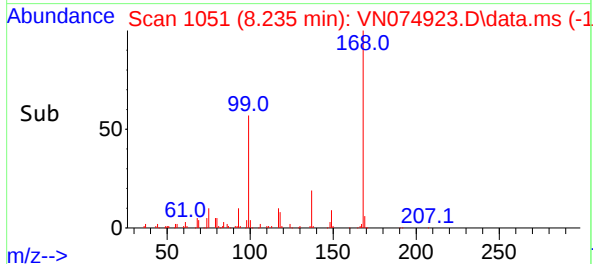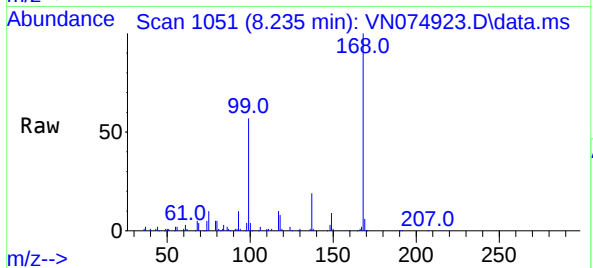

#38

Carbon Tetrachloride

Concen: 3.801 ug/l

RT: 8.230 min Scan# 1050

Delta R.T. -0.141 min

Lab File: VN074923.D

Acq: 17 Oct 2022 18:08




Tgt Ion: 117 Resp: 28790


Ion Ratio Lower Upper

117 100

119 6.2 71.0 106.6#

121 0.0 22.2 33.4#


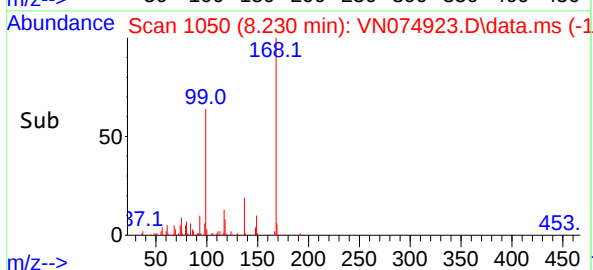






#42
1,2-Dichloroethane
Concen: 0.464 ug/l
RT: 8.694 min Scan# 1129
Delta R.T. 0.012 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 62 Resp: 3970
Ion Ratio Lower Upper
62 100
98 9.7 0.0 19.0

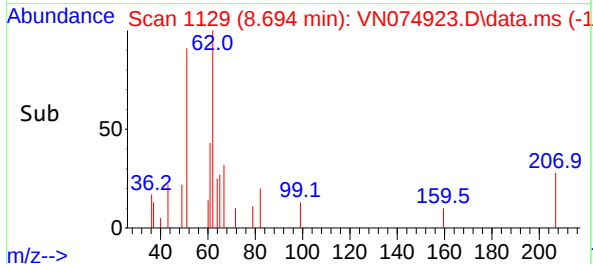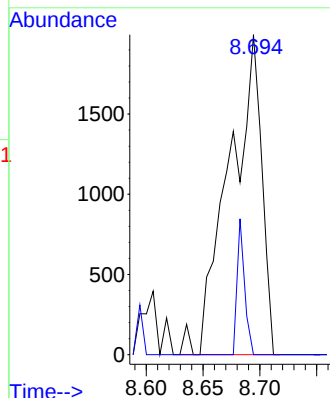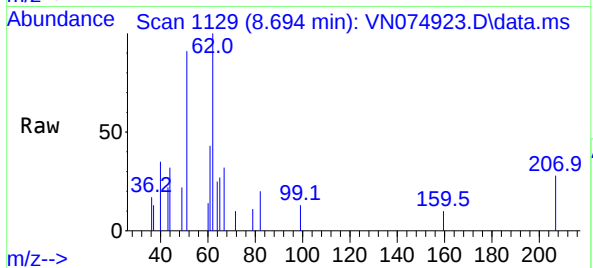

#44
Trichloroethene
Concen: 0.336 ug/l
RT: 9.359 min Scan# 1242
Delta R.T. -0.000 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08

Tgt Ion: 130 Resp: 1776
Ion Ratio Lower Upper
130 100
95 121.5 0.0 210.4


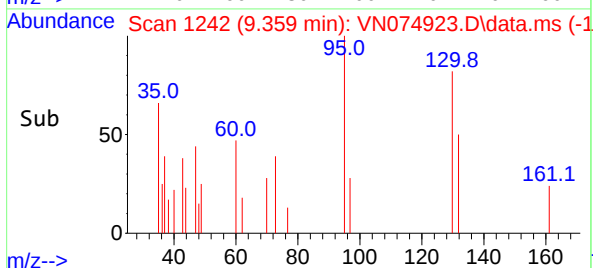

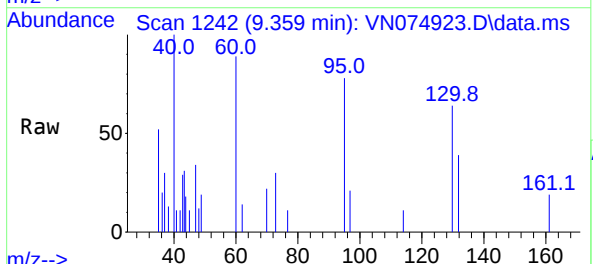




#50
Toluene-d8
Concen: 48.515 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 1146466
Ion Ratio Lower Upper
98 100
100 63.5 50.7 76.1



#51
4-Methyl-2-Pentanone
Concen: 0.289 ug/l
RT: 10.441 min Scan# 1426
Delta R.T. -0.012 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08

Tgt Ion: 43 Resp: 3354
Ion Ratio Lower Upper
43 100
58 0.0 30.0 45.0#


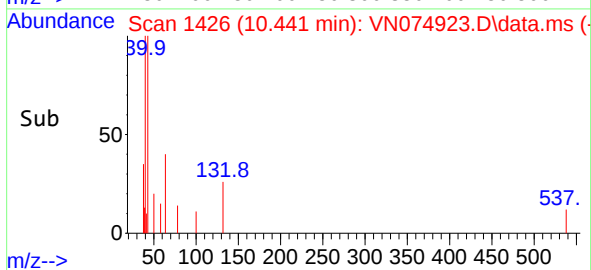






#52
Toluene
Concen: 0.210 ug/l
RT: 10.635 min Scan# 1459
Delta R.T. -0.000 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 92 Resp: 3176
Ion Ratio Lower Upper
92 100
91 139.3 141.0 211.6#

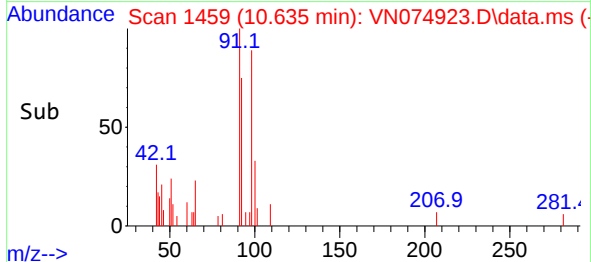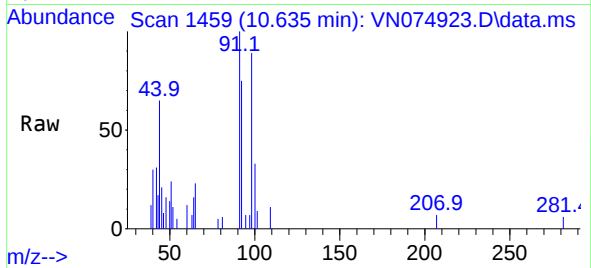

#53
t-1,3-Dichloropropene
Concen: 0.233 ug/l
RT: 10.835 min Scan# 1493
Delta R.T. -0.000 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08

Tgt Ion: 75 Resp: 2161
Ion Ratio Lower Upper
75 100
77 19.8 23.4 35.0#


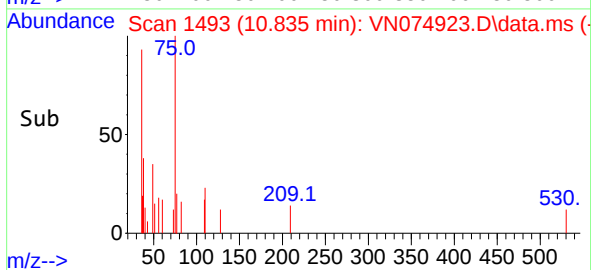






#58
2-Chloroethyl Vinyl ether
Concen: 9.664 ug/l
RT: 10.159 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 63 Resp: 1599
Ion Ratio Lower Upper
63 100
106 18.1 20.8 31.2#



#59
2-Hexanone
Concen: 0.654 ug/l
RT: 11.206 min Scan# 1556
Delta R.T. 0.006 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08

Tgt Ion: 43 Resp: 5680
Ion Ratio Lower Upper
43 100
58 50.4 26.3 78.9


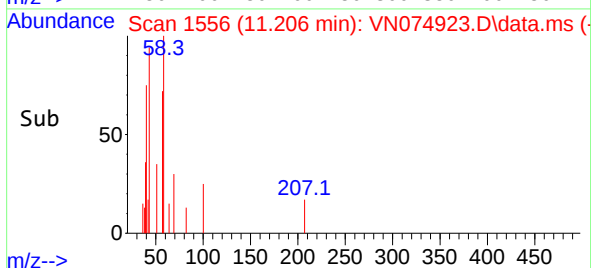
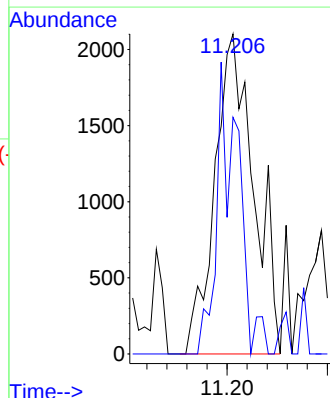





#62
4-Bromofluorobenzene
Concen: 39.682 ug/l
RT: 12.847 min Scan# 1836
Delta R.T. -0.006 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 95 Resp: 272437
Ion Ratio Lower Upper
95 100
174 82.4 0.0 157.8
176 79.7 0.0 148.0

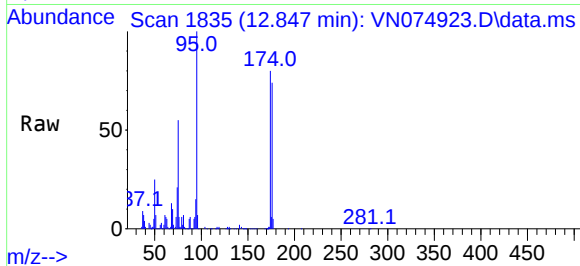

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1669
Delta R.T. 0.006 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08

Tgt Ion: 117 Resp: 522297
Ion Ratio Lower Upper
117 100
82 57.7 48.0 72.0
119 32.7 26.1 39.1


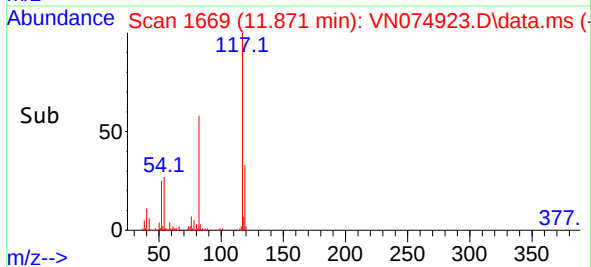

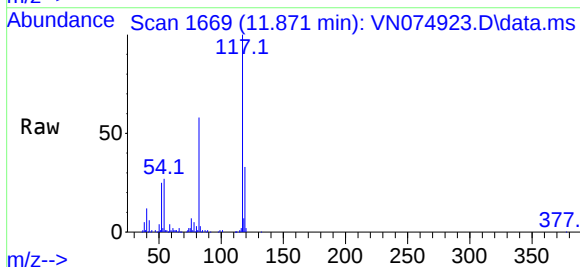




#65
Chlorobenzene
Concen: 0.477 ug/l
RT: 11.906 min Scan# 11
Delta R.T. 0.012 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:112 Resp: 7156
Ion Ratio Lower Upper
112 100
114 35.4 25.2 37.8

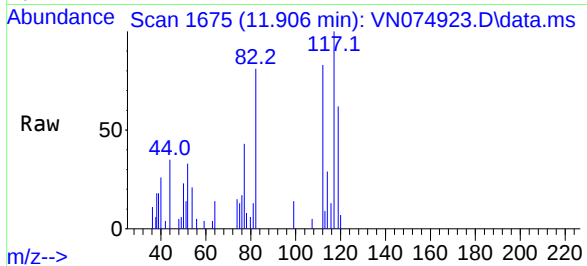

#68
m/p-Xylenes
Concen: 0.241 ug/l
RT: 12.076 min Scan# 1704
Delta R.T. -0.000 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08

Tgt Ion:106 Resp: 2451
Ion Ratio Lower Upper
106 100
91 109.7 160.6 240.8#


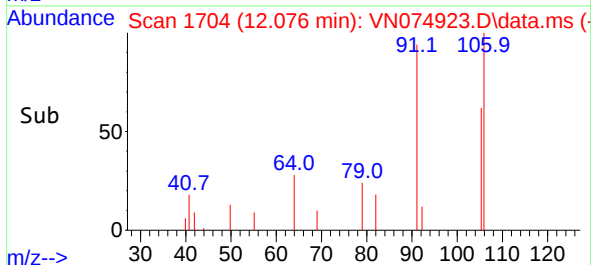
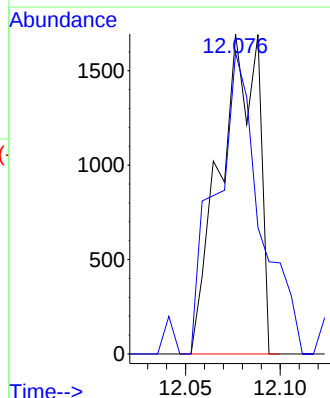
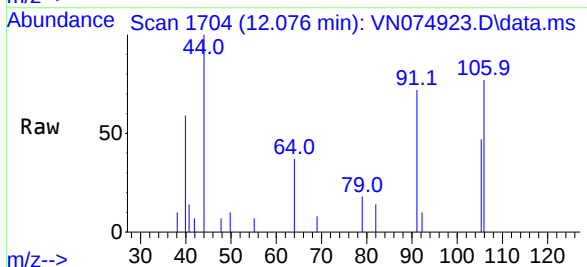




#69
o-Xylene
Concen: 0.261 ug/l
RT: 12.400 min Scan# 1759
Delta R.T. -0.000 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:106 Resp: 2700
Ion Ratio Lower Upper
106 100
91 187.6 105.9 317.7



#70
Styrene
Concen: 0.216 ug/l
RT: 12.412 min Scan# 1761
Delta R.T. -0.000 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08

Tgt Ion:104 Resp: 3521
Ion Ratio Lower Upper
104 100
78 44.3 38.8 58.2
103 49.6 45.0 67.4


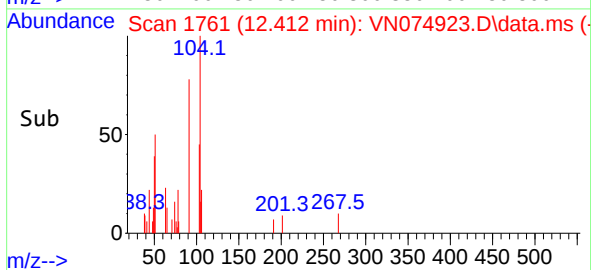






#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.794 min Scan# 1996
 Delta R.T. -0.000 min
 Lab File: VN074923.D
 Acq: 17 Oct 2022 18:08




Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK


Tgt Ion:152 Resp: 215443
 Ion Ratio Lower Upper
 152 100
 115 58.8 29.7 89.1
 150 154.9 0.0 341.6



#75
 1,1,2,2-Tetrachloroethane
 Concen: 0.333 ug/l
 RT: 12.935 min Scan# 1850
 Delta R.T. -0.006 min
 Lab File: VN074923.D
 Acq: 17 Oct 2022 18:08

Tgt Ion: 83 Resp: 2608
 Ion Ratio Lower Upper
 83 100
 131 8.6 4.3 12.8
 85 76.0 32.6 97.8


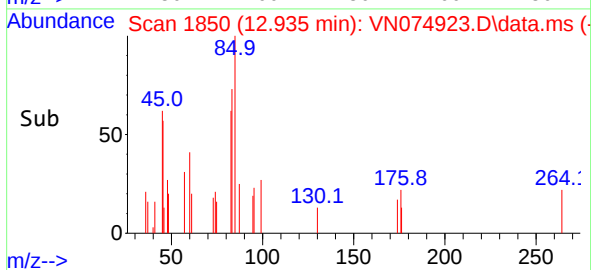




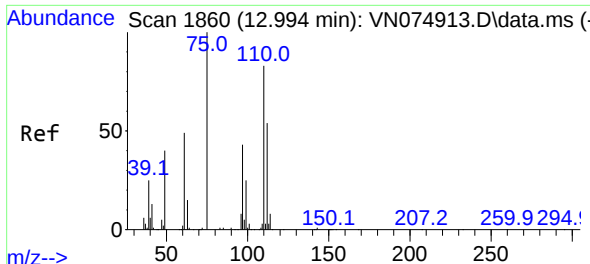

#76
1,2,3-Trichloropropane
Concen: 25.591 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.141 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 75 Resp: 155832
Ion Ratio Lower Upper
75 100
77 1.9 77.8 233.5#

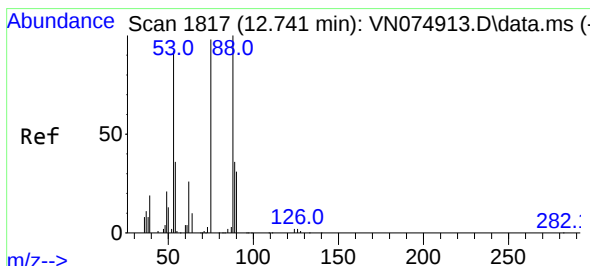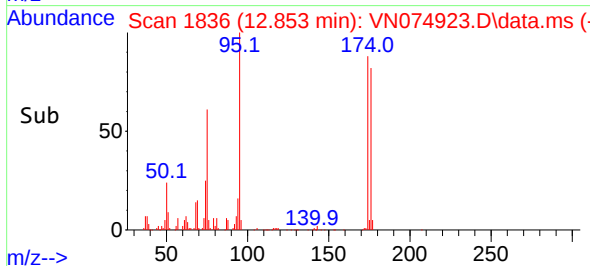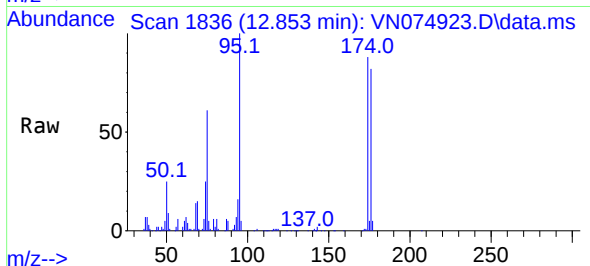

#81
trans-1,4-Dichloro-2-butene
Concen: 61.513 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.112 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08

Tgt Ion: 75 Resp: 155832
Ion Ratio Lower Upper
75 100
53 0.0 82.4 123.6#
89 0.1 34.7 52.1#

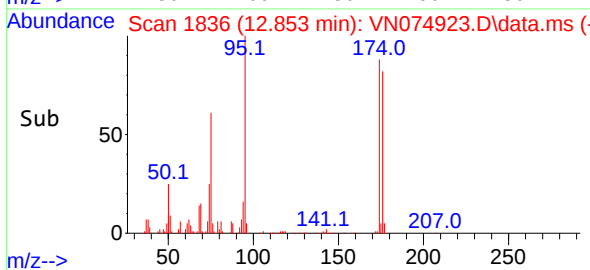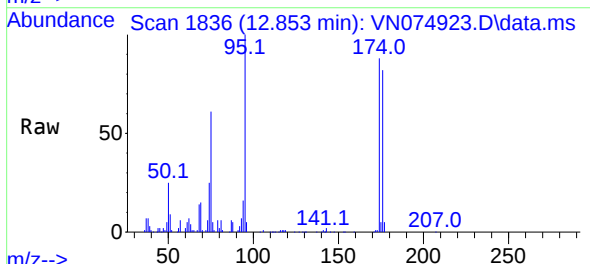



#91

1,2-Dichlorobenzene

Concen: 0.253 ug/l

RT: 14.106 min Scan# 2049

Delta R.T. -0.000 min

Lab File: VN074923.D

Acq: 17 Oct 2022 18:08

Instrument :

MSVOA_N

ClientSampleId :

IBLK





Tgt Ion:146 Resp: 1871

Ion Ratio Lower Upper

146 100

111 64.7 20.4 61.3#

148 56.4 32.1 96.3

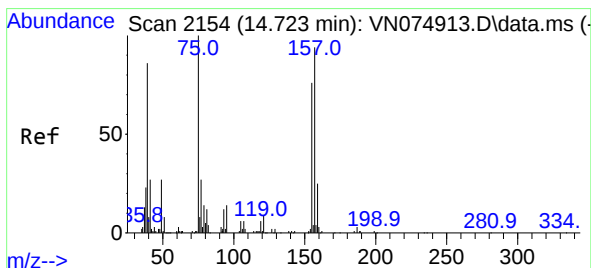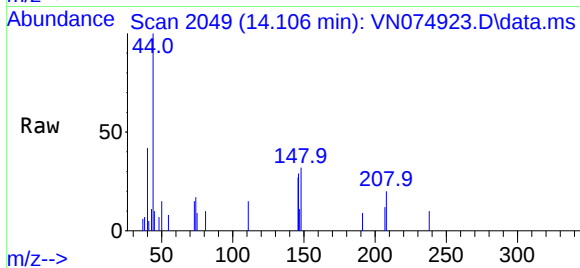

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.696 ug/l

RT: 14.735 min Scan# 2156

Delta R.T. 0.012 min

Lab File: VN074923.D

Acq: 17 Oct 2022 18:08




Tgt Ion: 75 Resp: 887


Ion Ratio Lower Upper

75 100

155 52.4 39.9 119.6

157 74.6 50.6 151.8


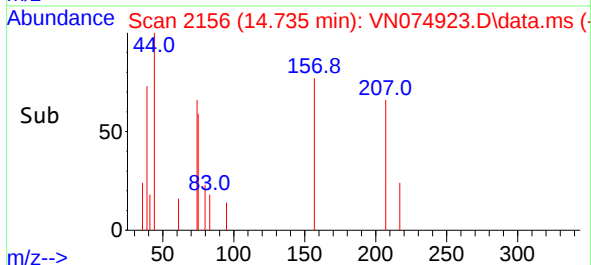
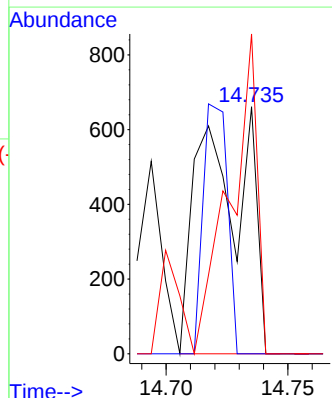
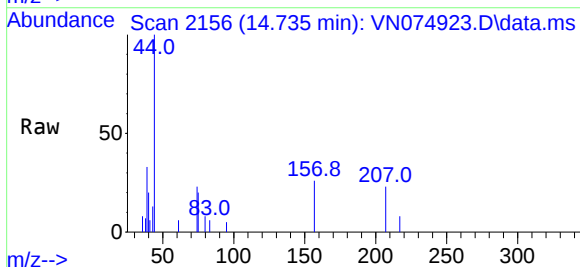




#94
Hexachlorobutadiene
Concen: 1.172 ug/l
RT: 15.506 min Scan# 21
Delta R.T. 0.006 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:	225	Resp:	1937
Ion	Ratio	Lower	Upper
225	100		
223	67.1	29.8	89.5
227	37.9	30.1	90.5



#95
Naphthalene
Concen: 0.206 ug/l
RT: 15.635 min Scan# 2309
Delta R.T. -0.006 min
Lab File: VN074923.D
Acq: 17 Oct 2022 18:08

Tgt Ion:	128	Resp:	3076
Ion	Ratio	Lower	Upper
128	100		
127	0.0	10.8	16.2#
129	4.2	8.7	13.1#

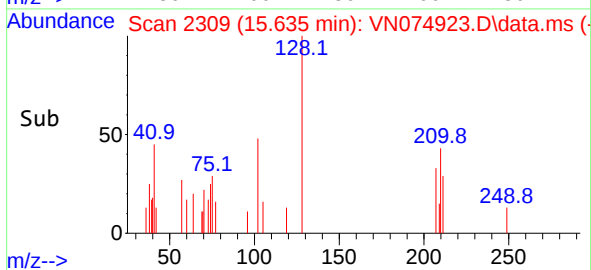



#96
 1,2,3-Trichlorobenzene
 Concen: 0.250 ug/l
 RT: 15.829 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: VN074923.D
 Acq: 17 Oct 2022 18:08

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Tgt Ion:180 Resp: 902
 Ion Ratio Lower Upper
 180 100
 182 34.8 46.9 140.6#
 145 0.0 15.8 47.4#

