
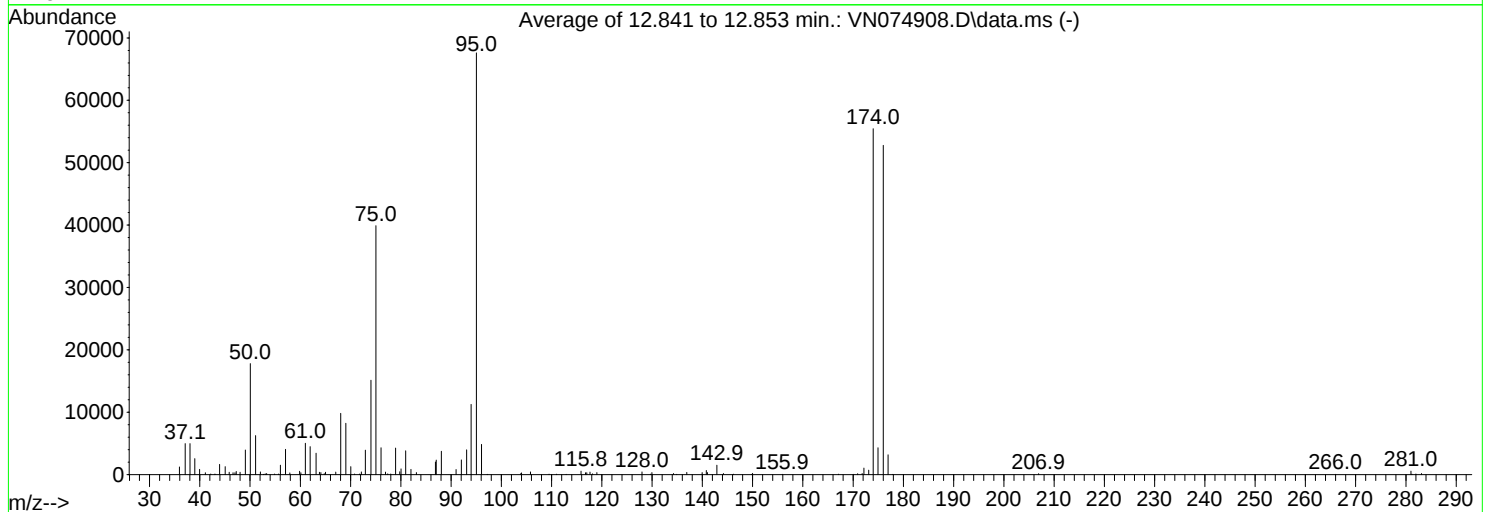


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101722\
Data File : VN074908.D
Acq On : 17 Oct 2022 09:47
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101722W.M
Title : SW846 8260
Last Update : Mon Oct 17 16:03:54 2022

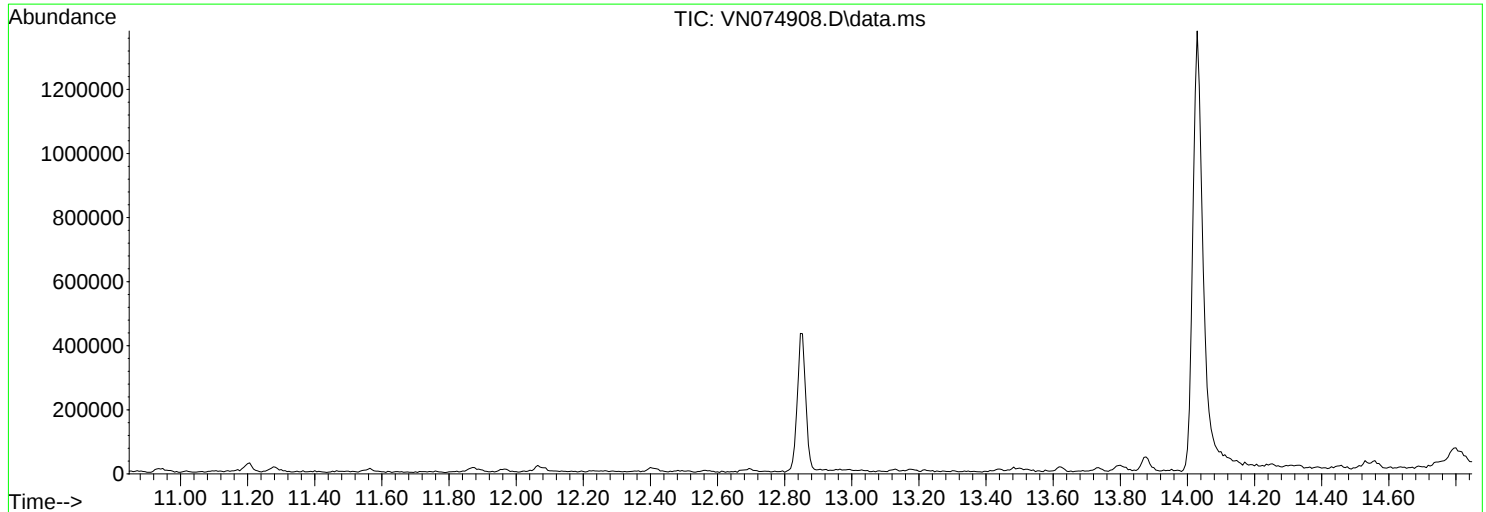

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.3	17808	PASS
75	95	30	60	59.0	39909	PASS
95	95	100	100	100.0	67608	PASS
96	95	5	9	7.2	4847	PASS
173	174	0.00	2	1.3	728	PASS
174	95	50	100	82.0	55453	PASS
175	174	5	9	7.8	4308	PASS
176	174	95	101	95.2	52787	PASS
177	176	5	9	6.0	3175	PASS