


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101818\
Data File : VN051907.D
Acq On : 18 Oct 2018 10:47
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N101218W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Oct 12 10:23:44 2018

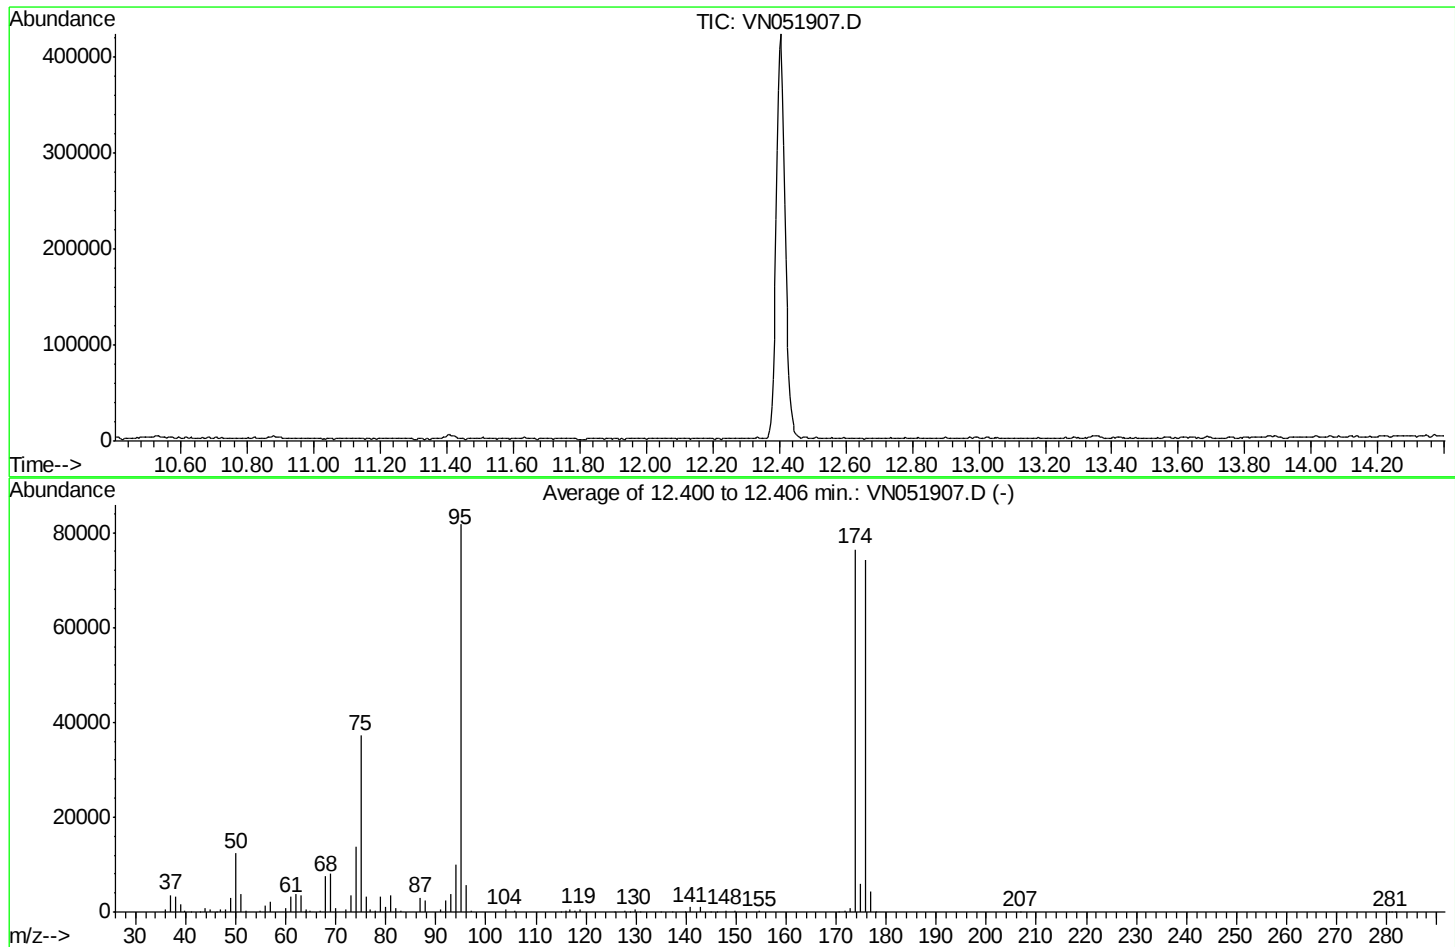

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	12335	PASS
75	95	30	60	45.5	37192	PASS
95	95	100	100	100.0	81749	PASS
96	95	5	9	6.9	5604	PASS
173	174	0.00	2	1.1	862	PASS
174	95	50	100	93.6	76488	PASS
175	174	5	9	7.7	5897	PASS
176	174	95	101	97.2	74314	PASS
177	176	5	9	5.9	4348	PASS