



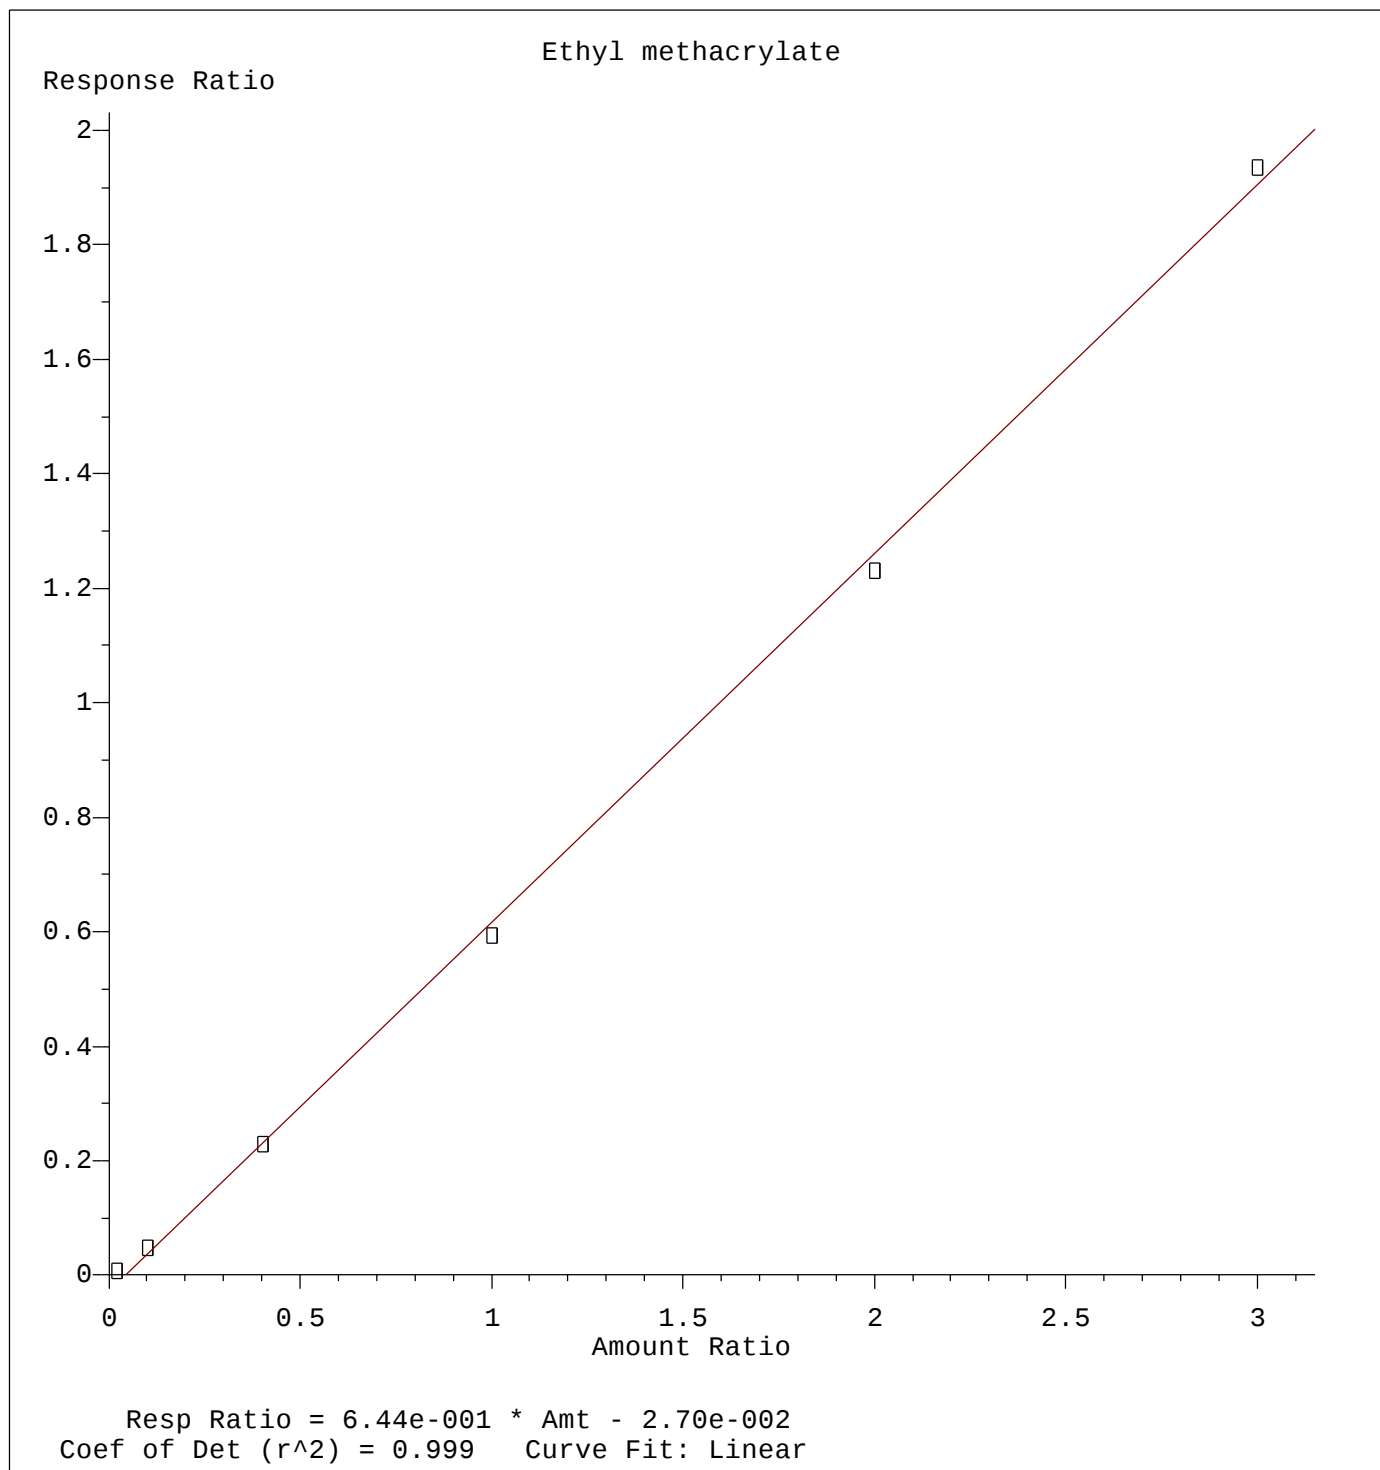

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
Calibration Table Last Updated: Sat Oct 19 00:16:20 2019


2-Chloroethyl Vinyl ether

Response Ratio

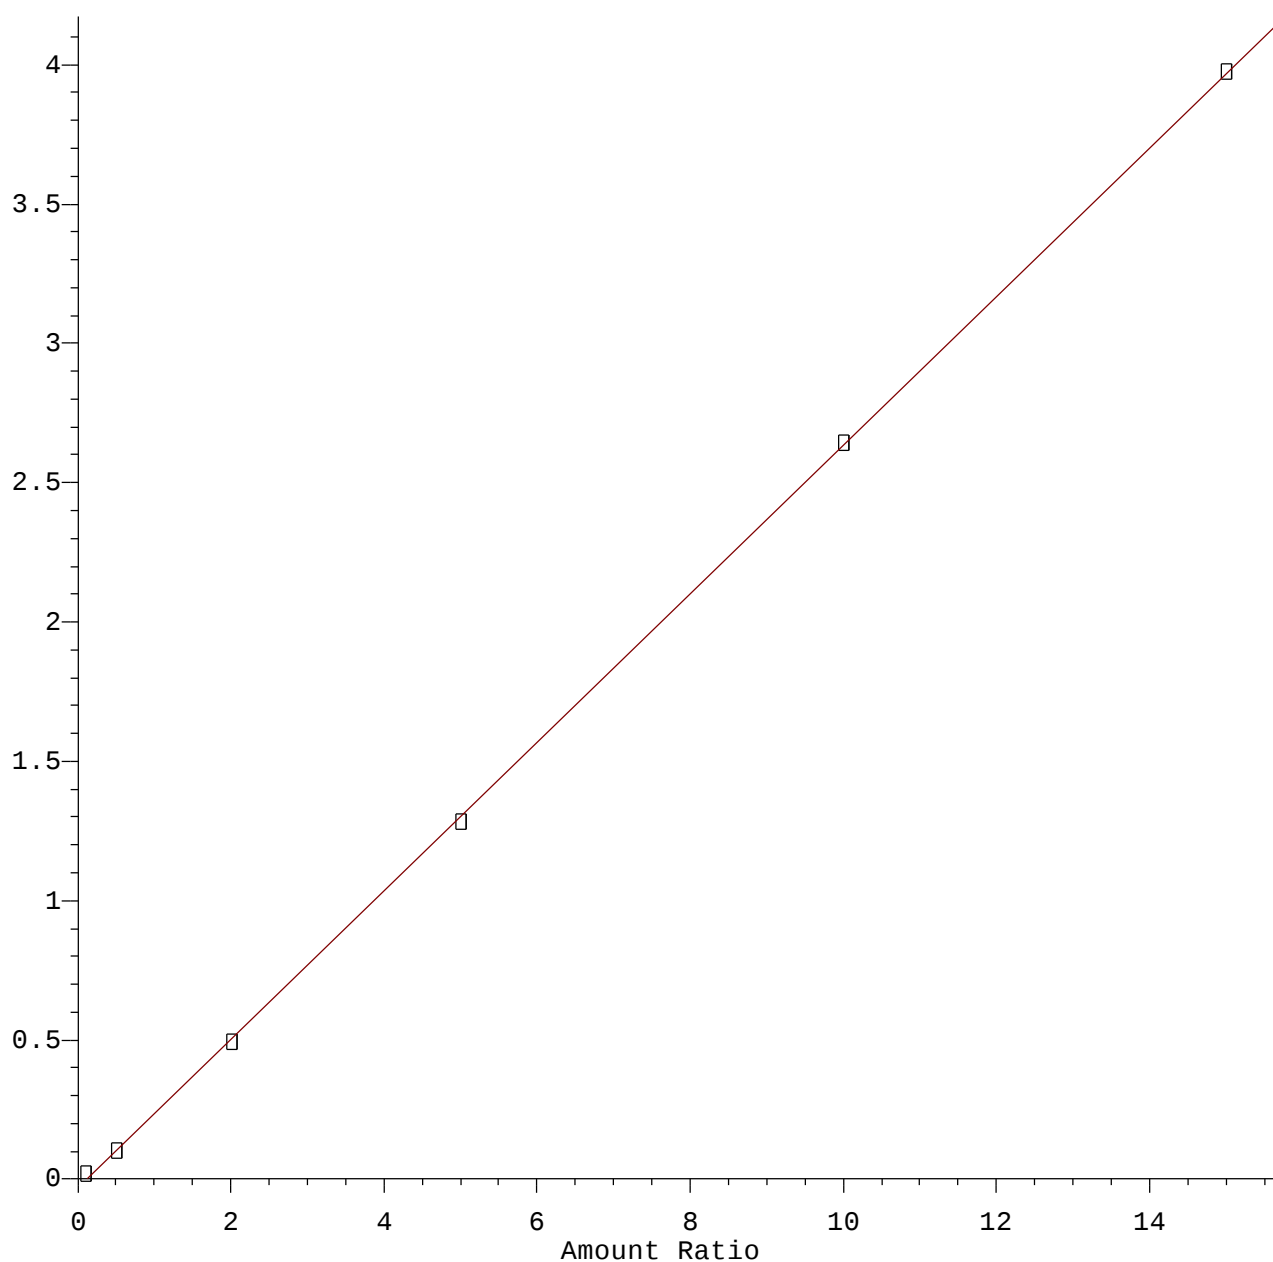

Resp Ratio = $2.67 \times 10^{-1} \times \text{Amt} - 3.02 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
Calibration Table Last Updated: Sat Oct 19 00:16:20 2019

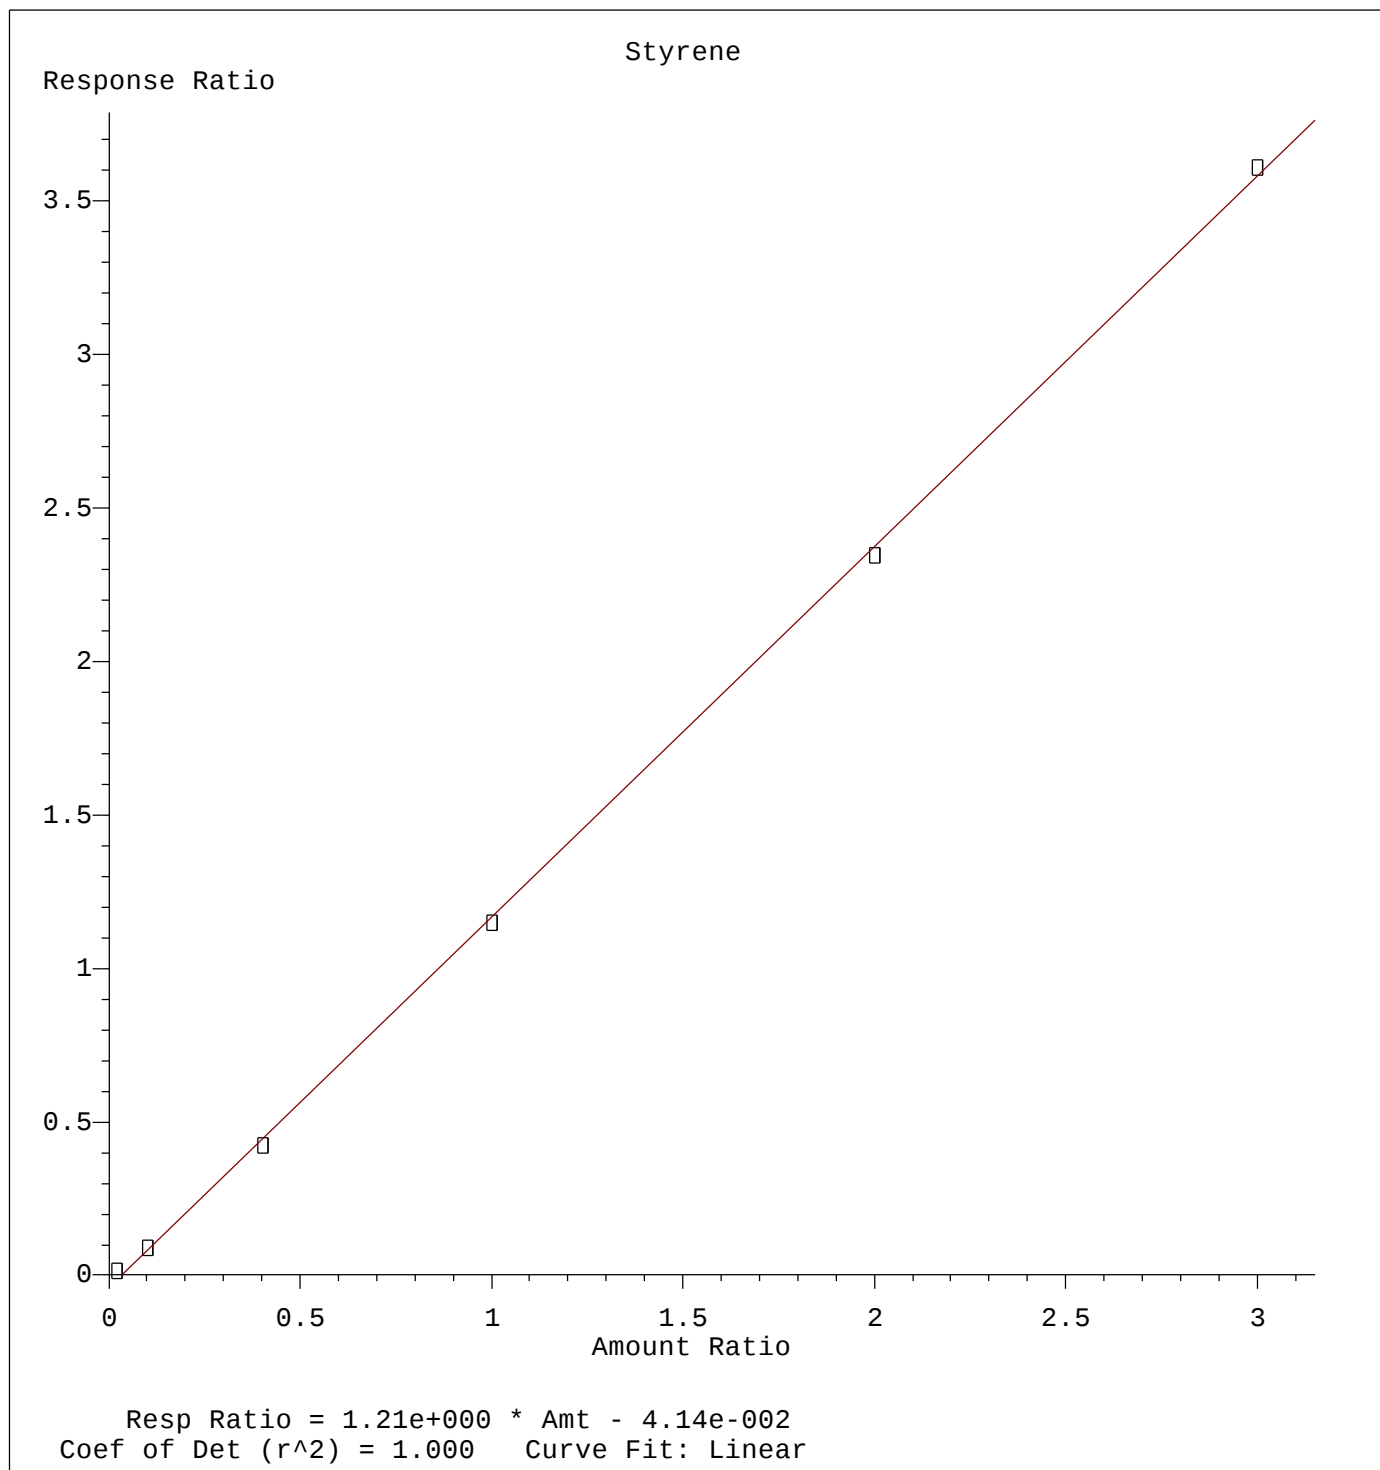

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
Calibration Table Last Updated: Sat Oct 19 00:16:20 2019

1,2,4-Trichlorobenzene

Response Ratio

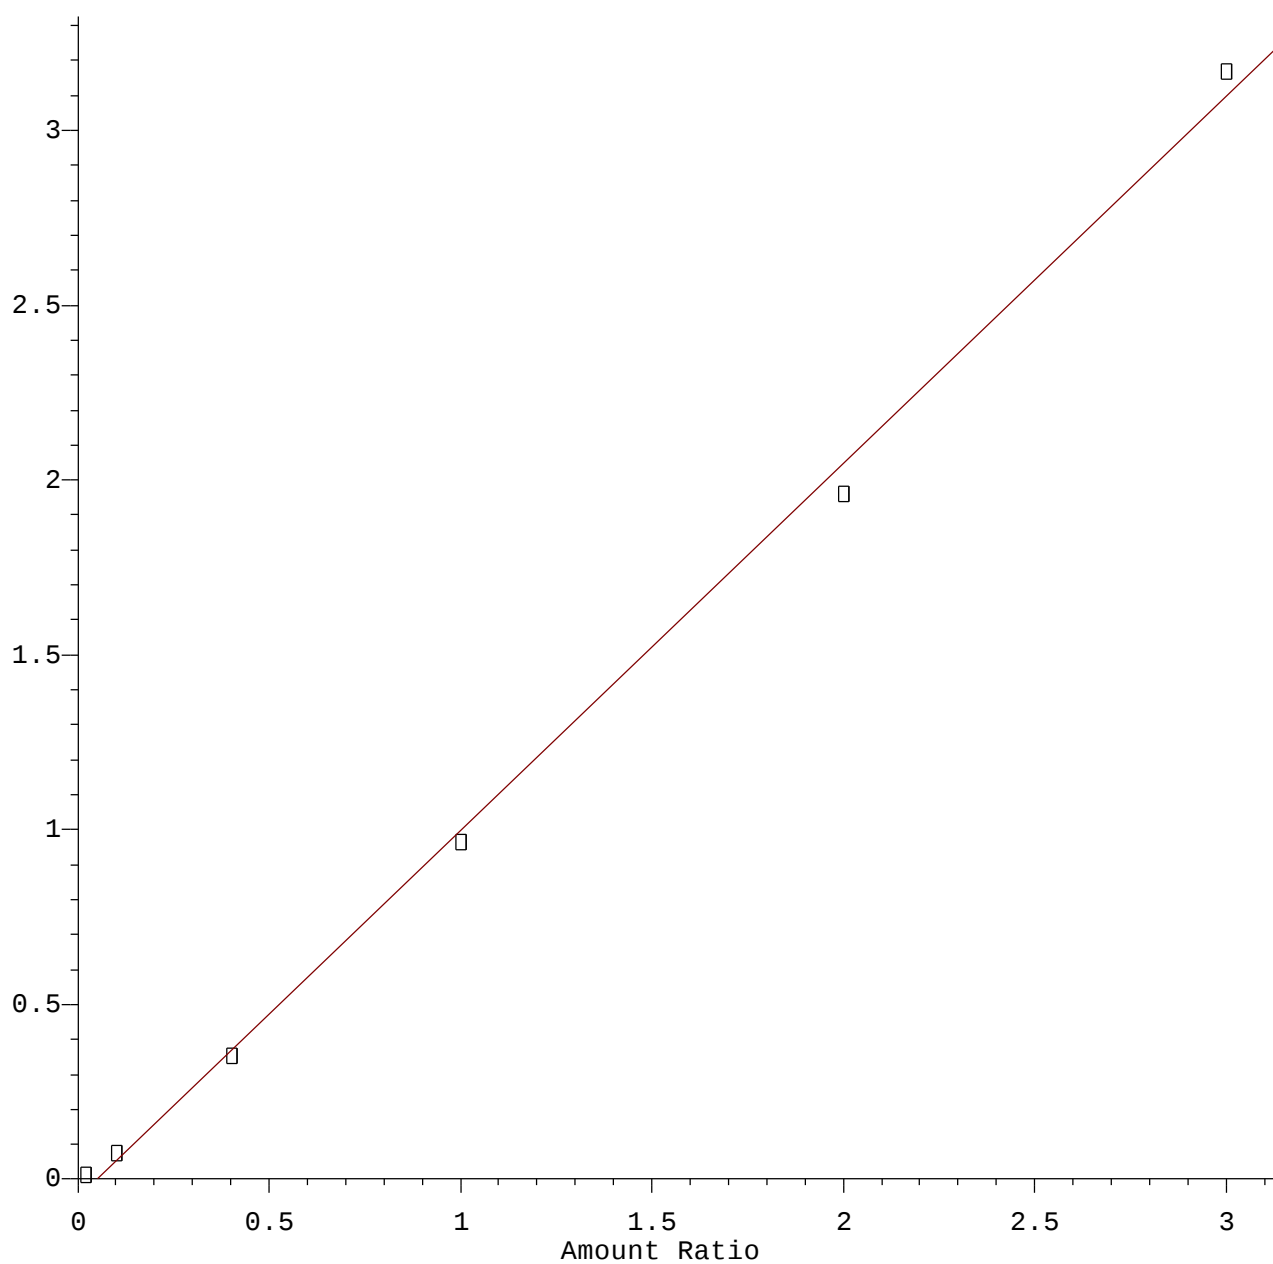


Resp Ratio = 1.05e+000 * Amt - 5.29e-002
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
Calibration Table Last Updated: Sat Oct 19 00:16:20 2019

Naphthalene

Response Ratio

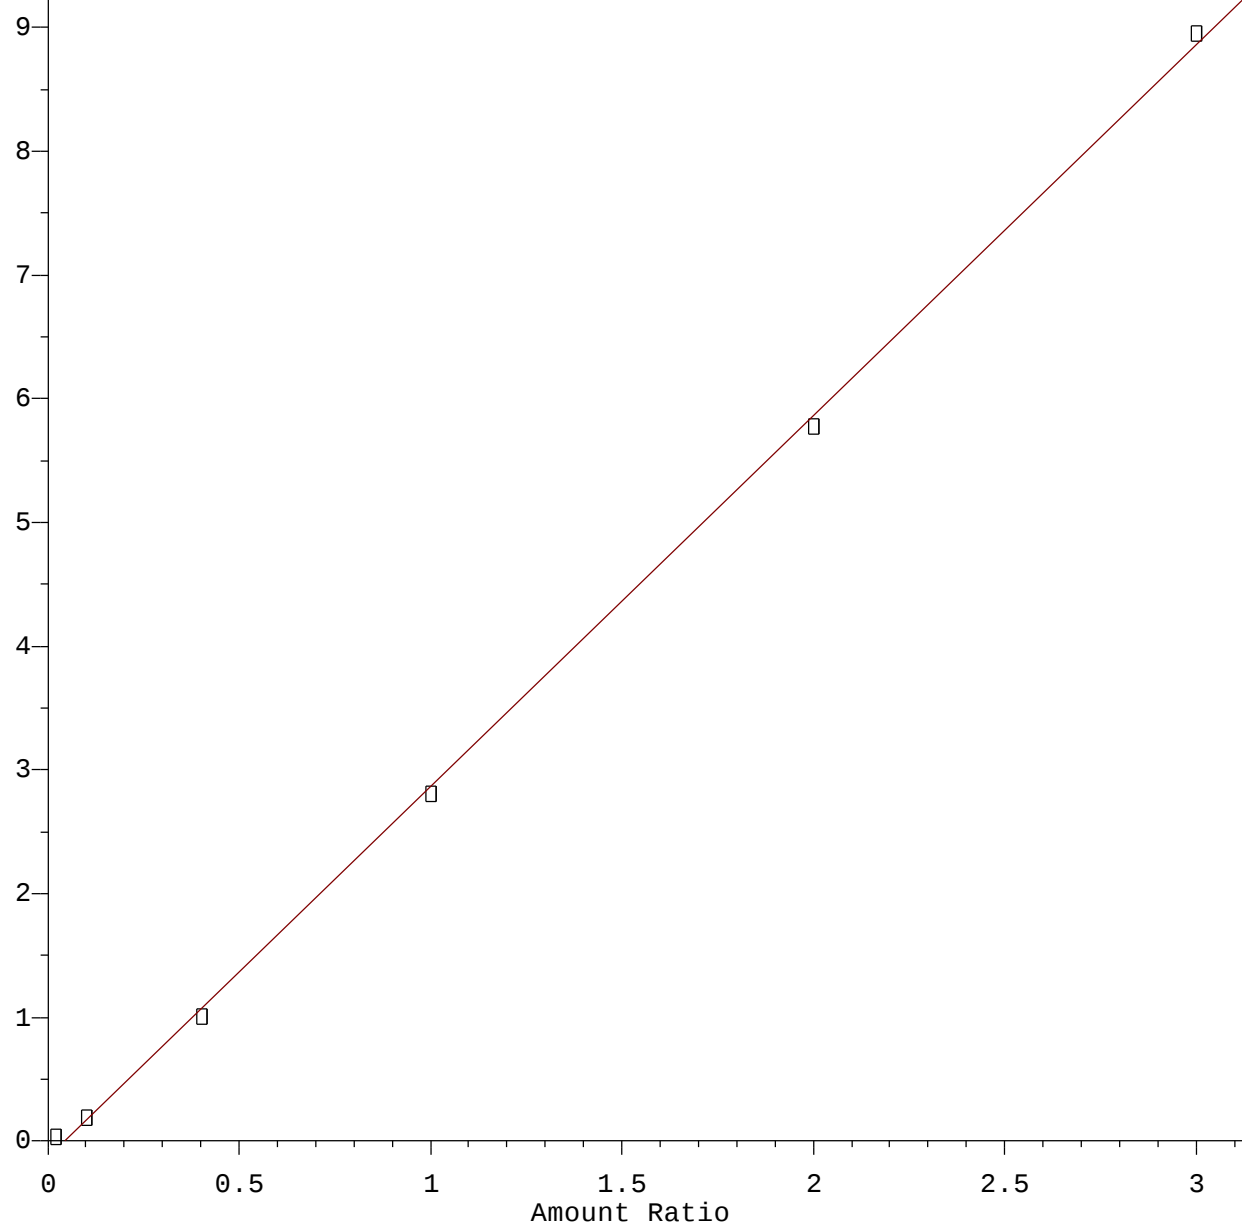


Resp Ratio = 3.00e+000 * Amt - 1.33e-001
Coef of Det (r²) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
Calibration Table Last Updated: Sat Oct 19 00:16:20 2019

1,2,3-Trichlorobenzene

Response Ratio

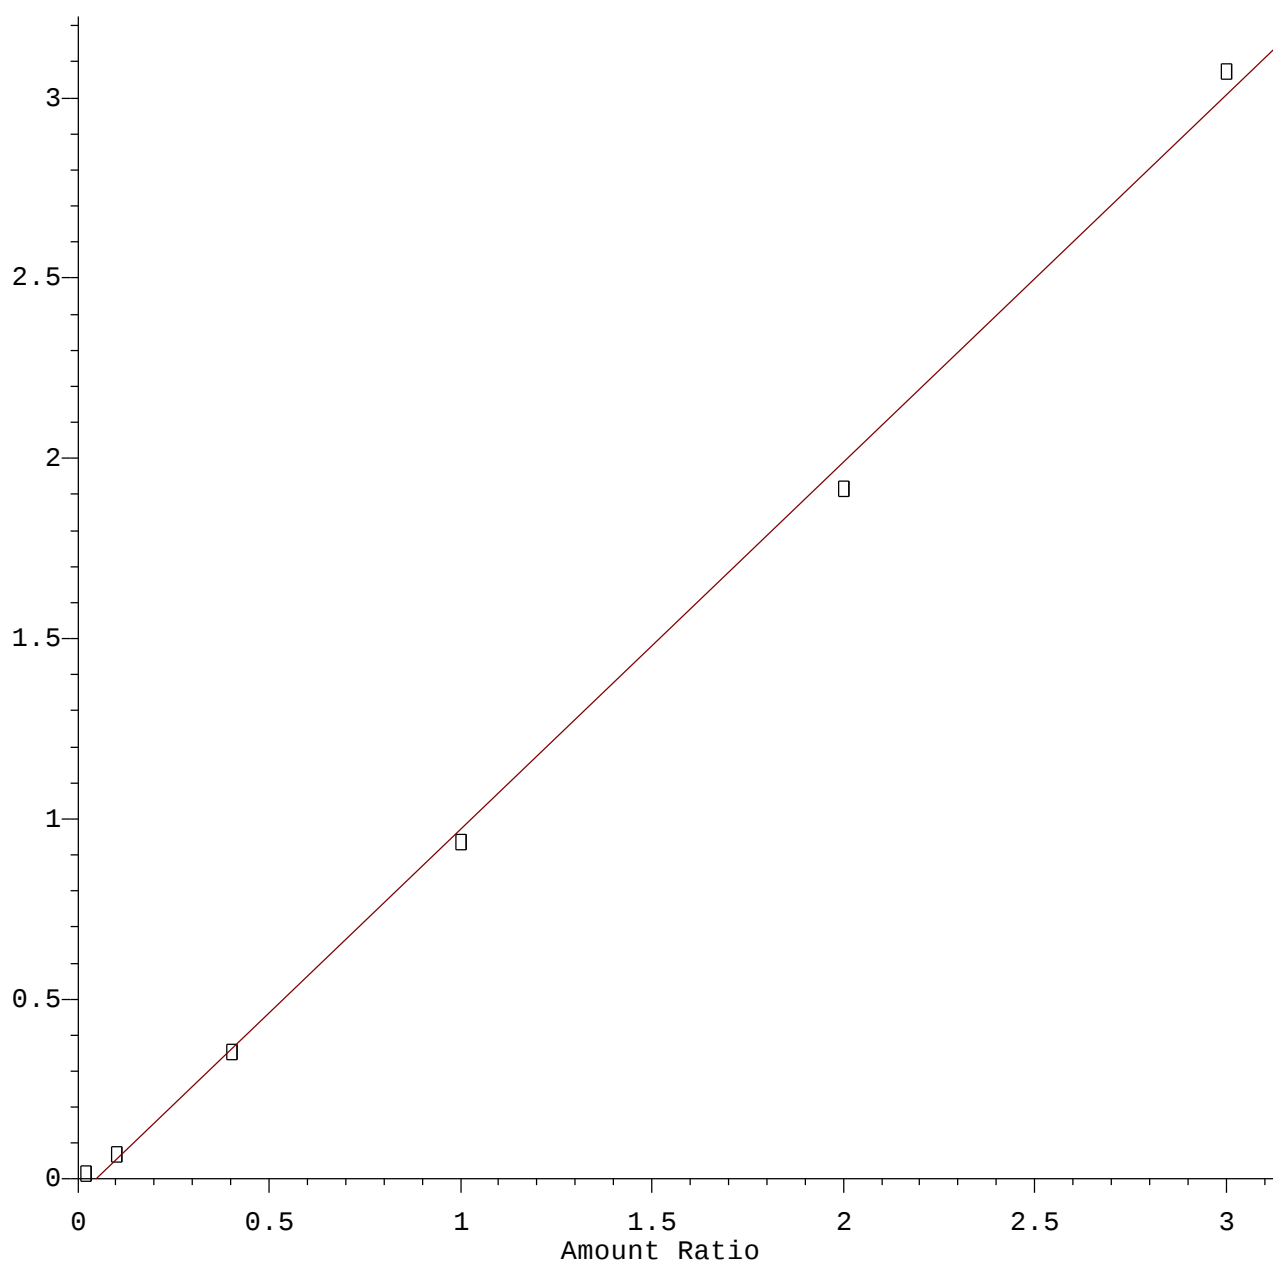

Resp Ratio = 1.02e+000 * Amt - 4.88e-002
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
Calibration Table Last Updated: Sat Oct 19 00:16:20 2019