


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN101819\
Data File : VN058842.D
Acq On : 18 Oct 2019 8:24
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N101819W.M
Title : SW846 8260
Last Update : Sat Oct 19 00:16:20 2019

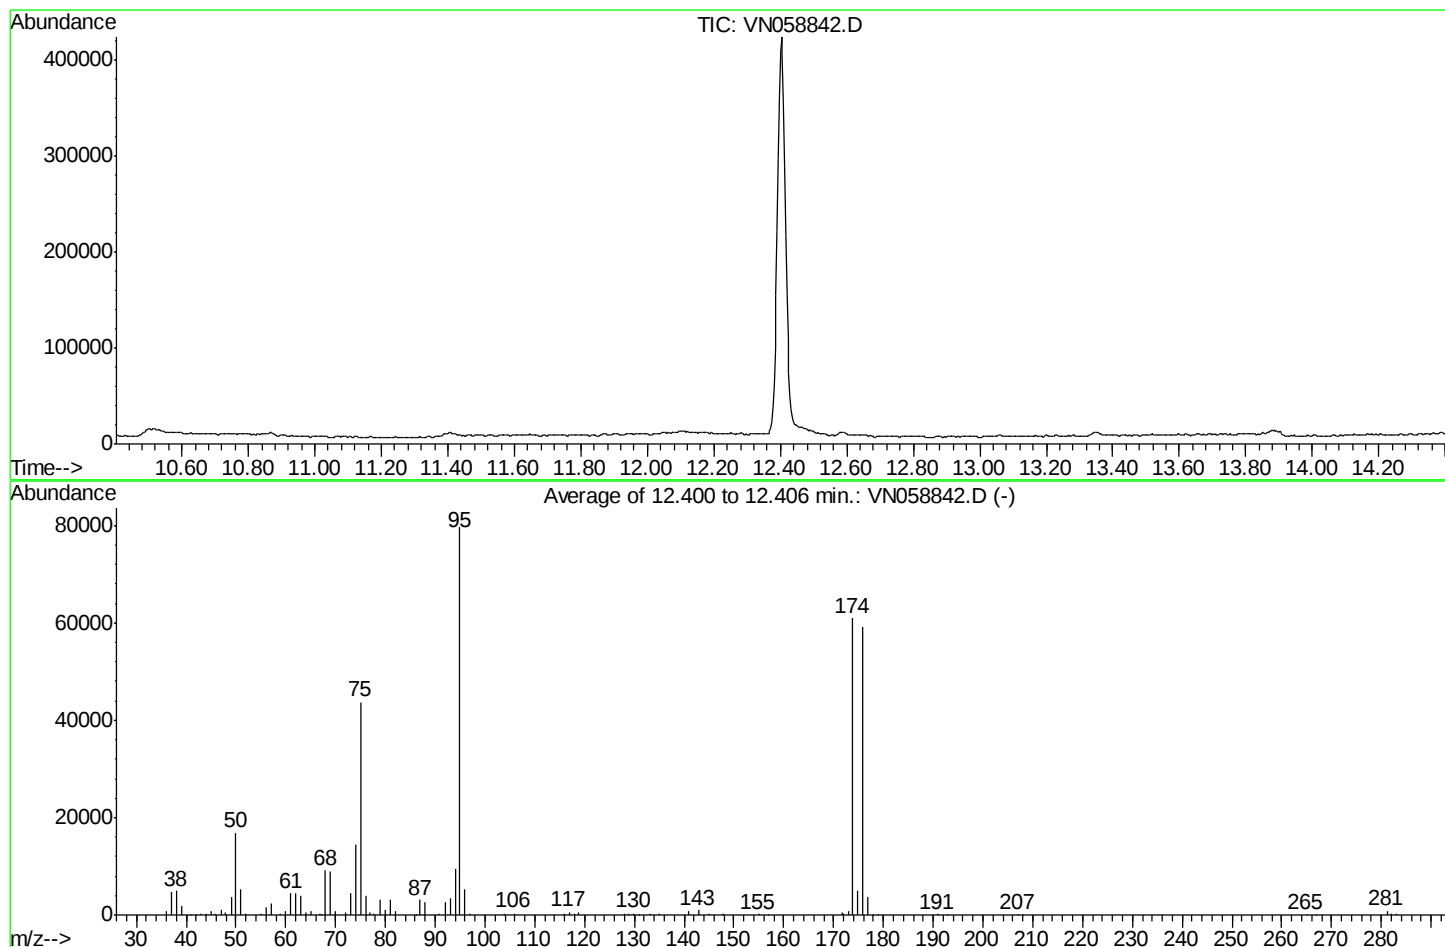

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	16922	PASS
75	95	30	60	54.9	43722	PASS
95	95	100	100	100.0	79642	PASS
96	95	5	9	6.7	5357	PASS
173	174	0.00	2	1.5	899	PASS
174	95	50	100	76.5	60965	PASS
175	174	5	9	8.1	4911	PASS
176	174	95	101	97.2	59234	PASS
177	176	5	9	6.1	3634	PASS