


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101821\
Data File : VN068966.D
Acq On : 18 Oct 2021 9:18
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Title : SW846 8260
Last Update : Wed Oct 13 05:44:40 2021

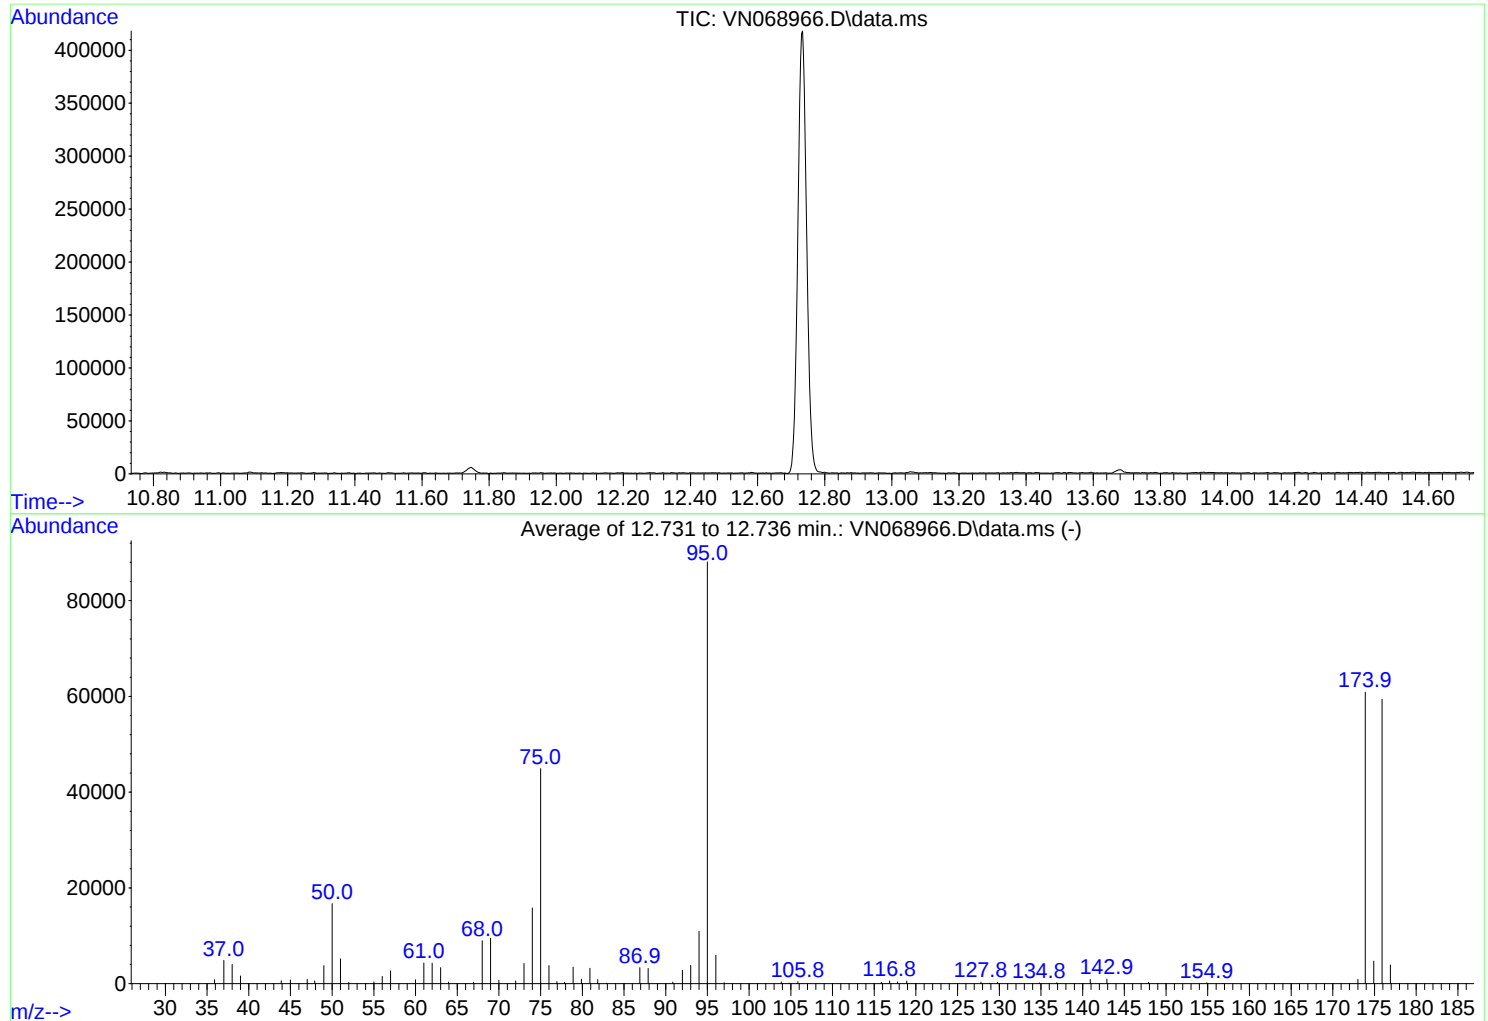

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3987

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	16715	PASS
75	95	30	60	51.0	44904	PASS
95	95	100	100	100.0	88109	PASS
96	95	5	9	6.7	5926	PASS
173	174	0.00	2	1.5	907	PASS
174	95	50	100	69.1	60885	PASS
175	174	5	9	7.7	4717	PASS
176	174	95	101	97.6	59400	PASS
177	176	5	9	6.6	3898	PASS