
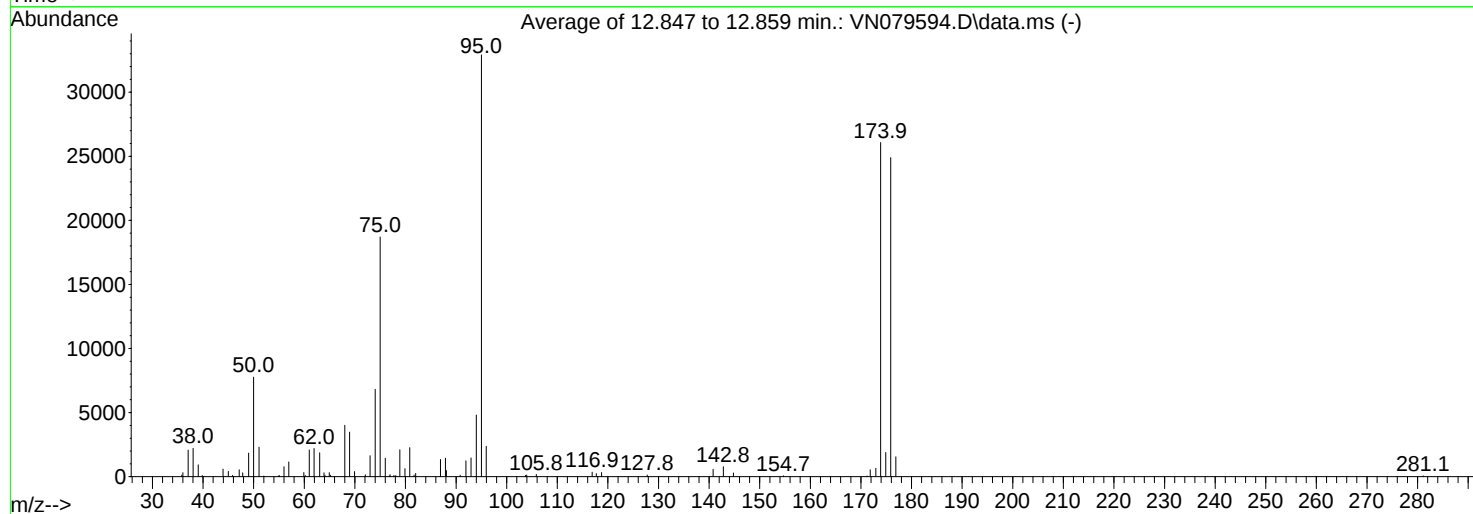


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101823\
 Data File : VN079594.D
 Acq On : 18 Oct 2023 10:22
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N101723W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Oct 18 02:19:15 2023

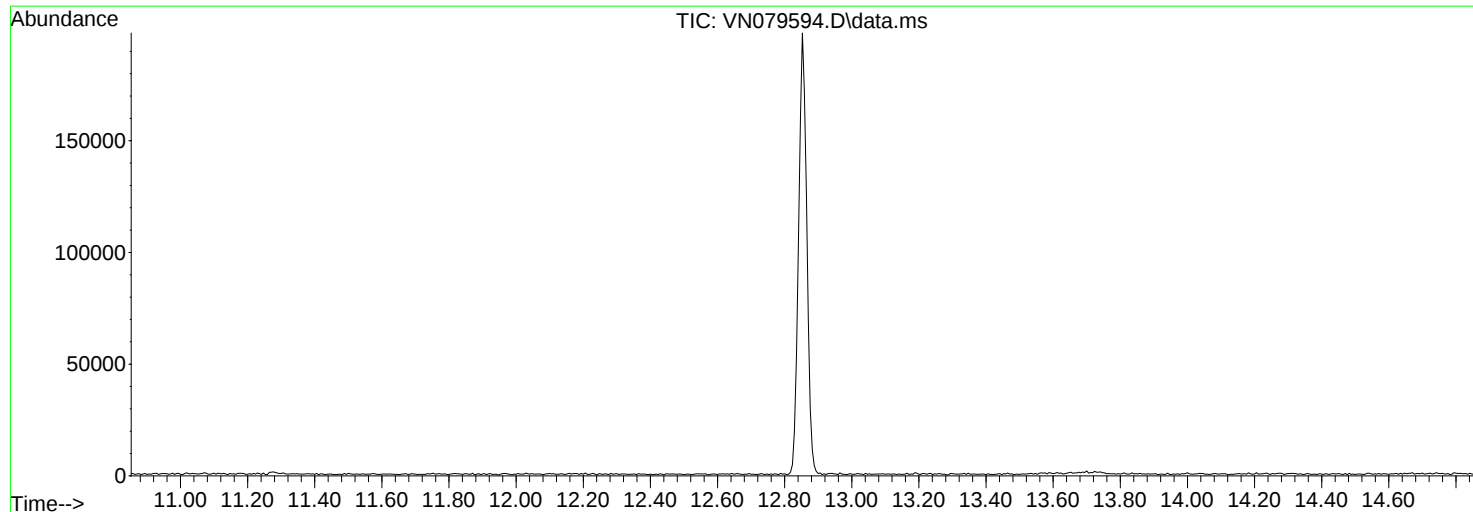

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	7773	PASS
75	95	30	60	56.8	18709	PASS
95	95	100	100	100.0	32915	PASS
96	95	5	9	7.2	2377	PASS
173	174	0.00	2	2.5	645	FAIL*
174	95	50	100	79.2	26067	PASS
175	174	5	9	7.3	1891	PASS
176	174	95	101	95.5	24899	PASS
177	176	5	9	6.2	1551	PASS