
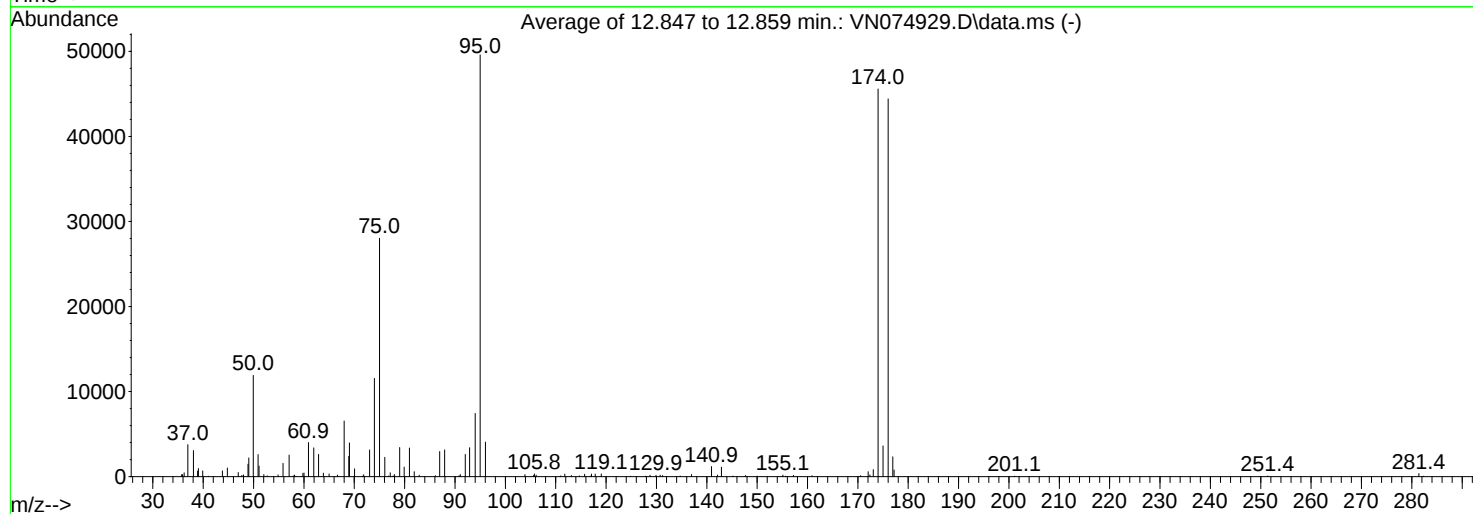


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101922\
Data File : VN074929.D
Acq On : 19 Oct 2022 13:57
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101922W.M
Title : SW846 8260
Last Update : Thu Oct 20 06:14:51 2022

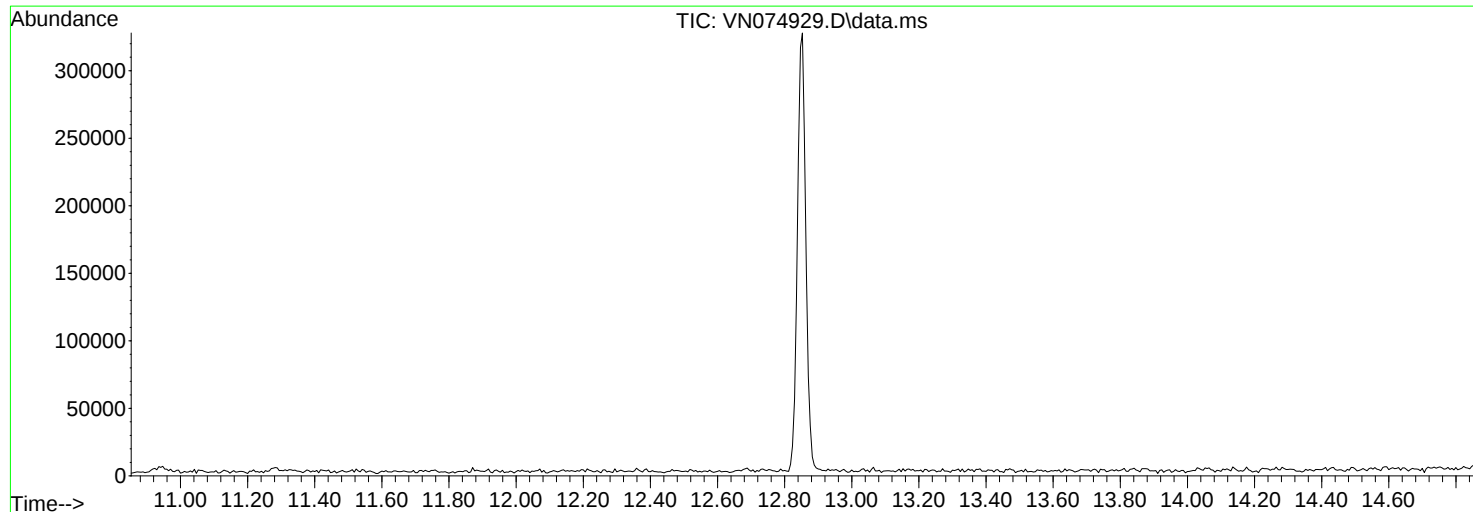

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.0	11911	PASS
75	95	30	60	56.5	28027	PASS
95	95	100	100	100.0	49589	PASS
96	95	5	9	8.2	4072	PASS
173	174	0.00	2	1.8	829	PASS
174	95	50	100	91.9	45576	PASS
175	174	5	9	7.9	3607	PASS
176	174	95	101	97.4	44405	PASS
177	176	5	9	5.2	2328	PASS

Average of 12.847 to 12.859 min.: VN074929.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.70	227	46.95	490	55.85	1564	66.65	181
35.90	251	47.70	149	57.05	2548	68.00	654
36.20	445	48.00	207	57.90	87	68.90	238
36.95	3759	48.90	1477	58.15	195	69.05	397
38.05	3070	49.05	2210	59.80	389	70.05	922
38.90	657	49.95	11911	60.00	433	71.60	61
39.05	953	50.90	2599	60.90	4004	71.85	230
39.90	685	51.10	1241	61.95	3382	73.05	3137
41.00	65	52.05	240	62.90	2620	74.00	11549
43.80	674	52.70	90	63.85	407	75.00	28027
44.80	1020	54.85	215	65.00	323	76.05	2277

Average of 12.847 to 12.859 min.: VN074929.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.80	73	87.95	3147	106.10	199	127.80	61
77.15	458	90.80	108	111.00	104	128.75	171
77.70	73	91.05	236	111.80	297	129.90	177
77.95	255	92.05	2606	113.10	130	130.75	191
79.00	3431	92.90	3411	114.70	101	131.20	130
79.90	1126	94.00	7434	115.75	274	134.70	75
80.95	3366	95.00	49589	116.90	61	136.95	245
81.90	588	96.05	4072	117.10	298	140.95	1178
82.90	170	103.90	242	117.85	297	142.15	188
86.10	108	105.60	148	119.05	318	142.90	1118
86.95	2953	105.75	323	124.80	59	145.20	72

Average of 12.847 to 12.859 min.: VN074929.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
147.70	131	175.00	3607				
150.00	55	176.00	44405				
155.10	187	176.95	2328				
155.60	58	177.20	785				
157.20	160	201.10	53				
160.90	107	251.40	75				
170.55	120	281.40	367				
172.05	579	282.30	64				
172.40	204						
173.05	829						
174.00	45576						

Instrument :

MSVOA_N

ClientSampleId :

BFB