
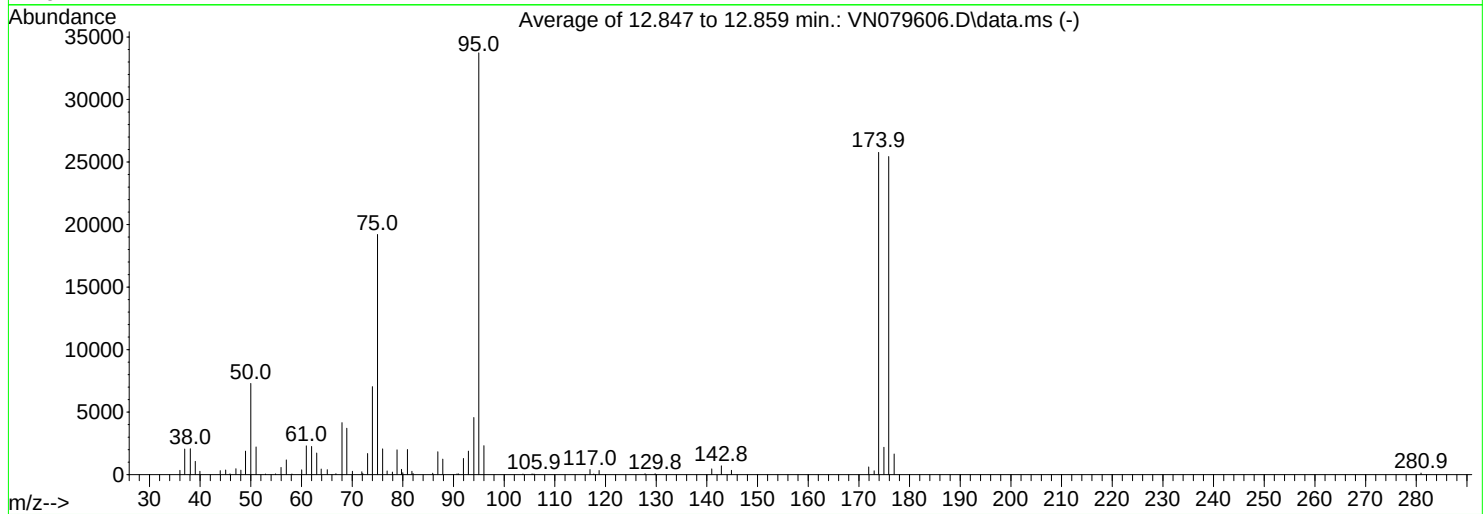


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN101923\
Data File : VN079606.D
Acq On : 19 Oct 2023 08:36
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100523W.M
Title : SW846 8260
Last Update : Fri Oct 06 03:34:49 2023

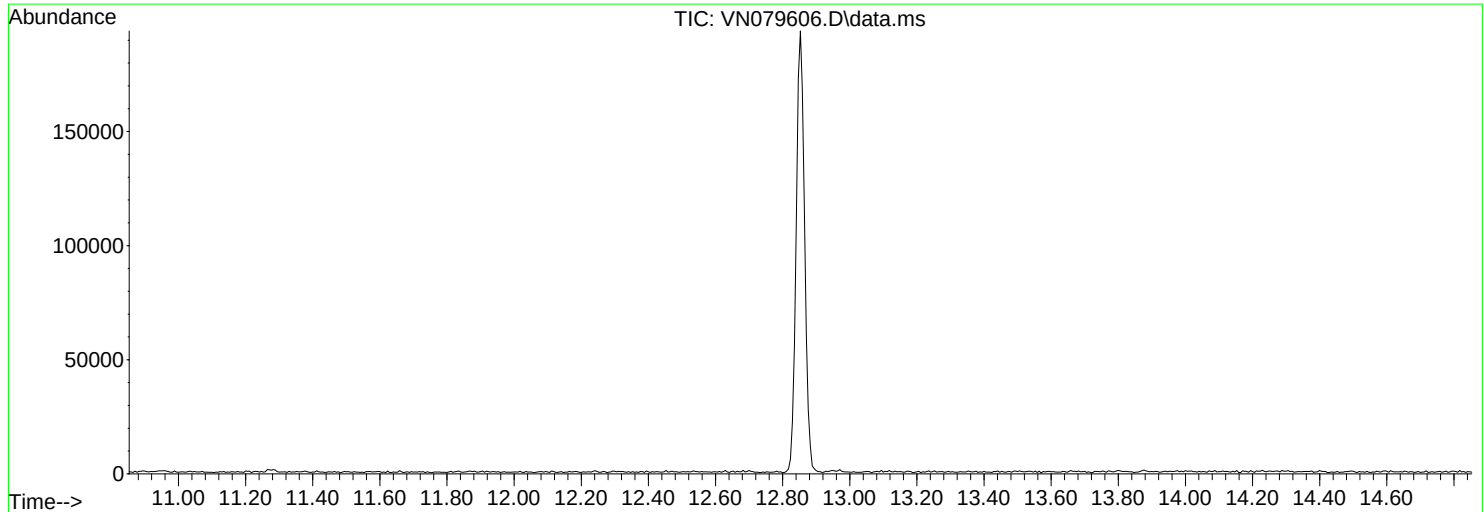

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	7292	PASS
75	95	30	60	56.9	19203	PASS
95	95	100	100	100.0	33731	PASS
96	95	5	9	6.9	2315	PASS
173	174	0.00	2	1.2	305	PASS
174	95	50	100	76.4	25776	PASS
175	174	5	9	8.5	2190	PASS
176	174	95	101	98.7	25443	PASS
177	176	5	9	6.5	1648	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	353	50.00	7292	63.90	444	76.00	205
36.95	2045	51.05	2209	65.10	402	76.90	29
38.05	2075	52.90	50	66.80	72	77.95	20
39.05	1069	54.90	66	68.00	4160	78.85	198
39.95	273	55.95	574	68.95	3709	79.75	418
43.95	326	57.00	1180	70.05	266	80.00	157
45.05	368	58.10	54	71.90	234	80.90	2015
45.90	61	60.05	390	72.10	88	81.80	271
47.05	481	60.95	2303	73.05	1686	82.00	89
48.05	364	62.00	2249	74.00	7041	85.90	114
48.95	1885	63.00	1734	75.00	19203	86.90	1827

Average of 12.847 to 12.859 min.: VN079606.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.90	1244	116.95	411	174.95	2190		
90.70	63	117.70	53	175.90	25443		
91.00	65	118.75	331	176.95	1648		
91.95	1290	127.80	73	280.95	134		
92.95	1878	129.80	83				
94.00	4567	140.95	464				
95.00	33731	142.85	700				
96.00	2315	144.85	344				
103.70	52	171.95	612				
105.50	59	173.00	305				
105.90	54	173.90	25776				