


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN102020\
 Data File : VN064189.D
 Acq On : 20 Oct 2020 9:15
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N102020W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue Oct 20 11:51:57 2020

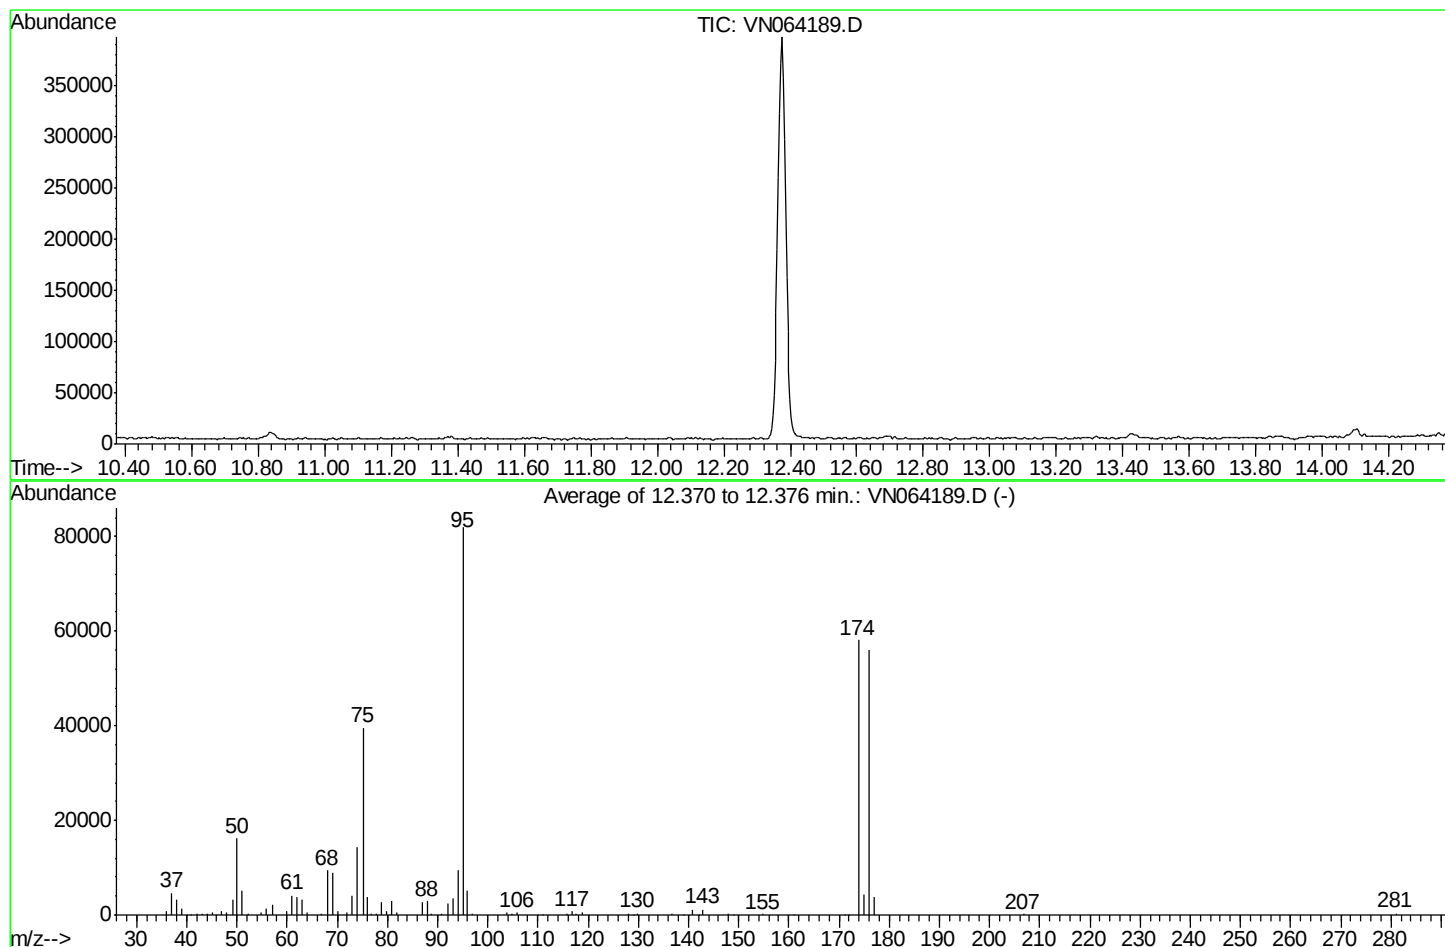

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	16138	PASS
75	95	30	60	48.3	39560	PASS
95	95	100	100	100.0	81930	PASS
96	95	5	9	6.4	5226	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.9	58125	PASS
175	174	5	9	7.6	4441	PASS
176	174	95	101	96.1	55877	PASS
177	176	5	9	6.7	3769	PASS