

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102021\
 Data File : VN069073.D
 Acq On : 20 Oct 2021 19:57
 Operator : JC/MD
 Sample : M4253-05
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 135-136

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M

Title : SW846 8260

Signal : TIC: VN069073.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.578	945	965	985	rBV3	5899	18458	1.01%	0.194%
2	7.313	1966	1985	2003	rBV2	7558	20312	1.11%	0.214%
3	8.027	2228	2251	2261	rBV	221738	531360	29.01%	5.591%
4	8.088	2262	2274	2302	rVB	424481	967740	52.84%	10.183%
5	8.440	2383	2405	2430	rBV	249671	572075	31.24%	6.020%
6	8.627	2440	2475	2477	rBV2	51118	165546	9.04%	1.742%
7	8.971	2584	2603	2631	rBV	631306	1306796	71.36%	13.750%
8	10.443	3133	3152	3193	rBV	970856	1831393	100.00%	19.270%
9	11.095	3382	3395	3414	rBV2	18697	34147	1.86%	0.359%
10	11.747	3621	3638	3666	rBV	894864	1607617	87.78%	16.916%
11	12.734	3990	4006	4030	rBV	676864	1169924	63.88%	12.310%
12	13.678	4341	4358	4384	rBV	738844	1278297	69.80%	13.451%


Sum of corrected areas: 9503665

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102021\
Data File : VN069073.D
Acq On : 20 Oct 2021 19:57
Operator : JC/MD
Sample : M4253-05
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
135-136

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

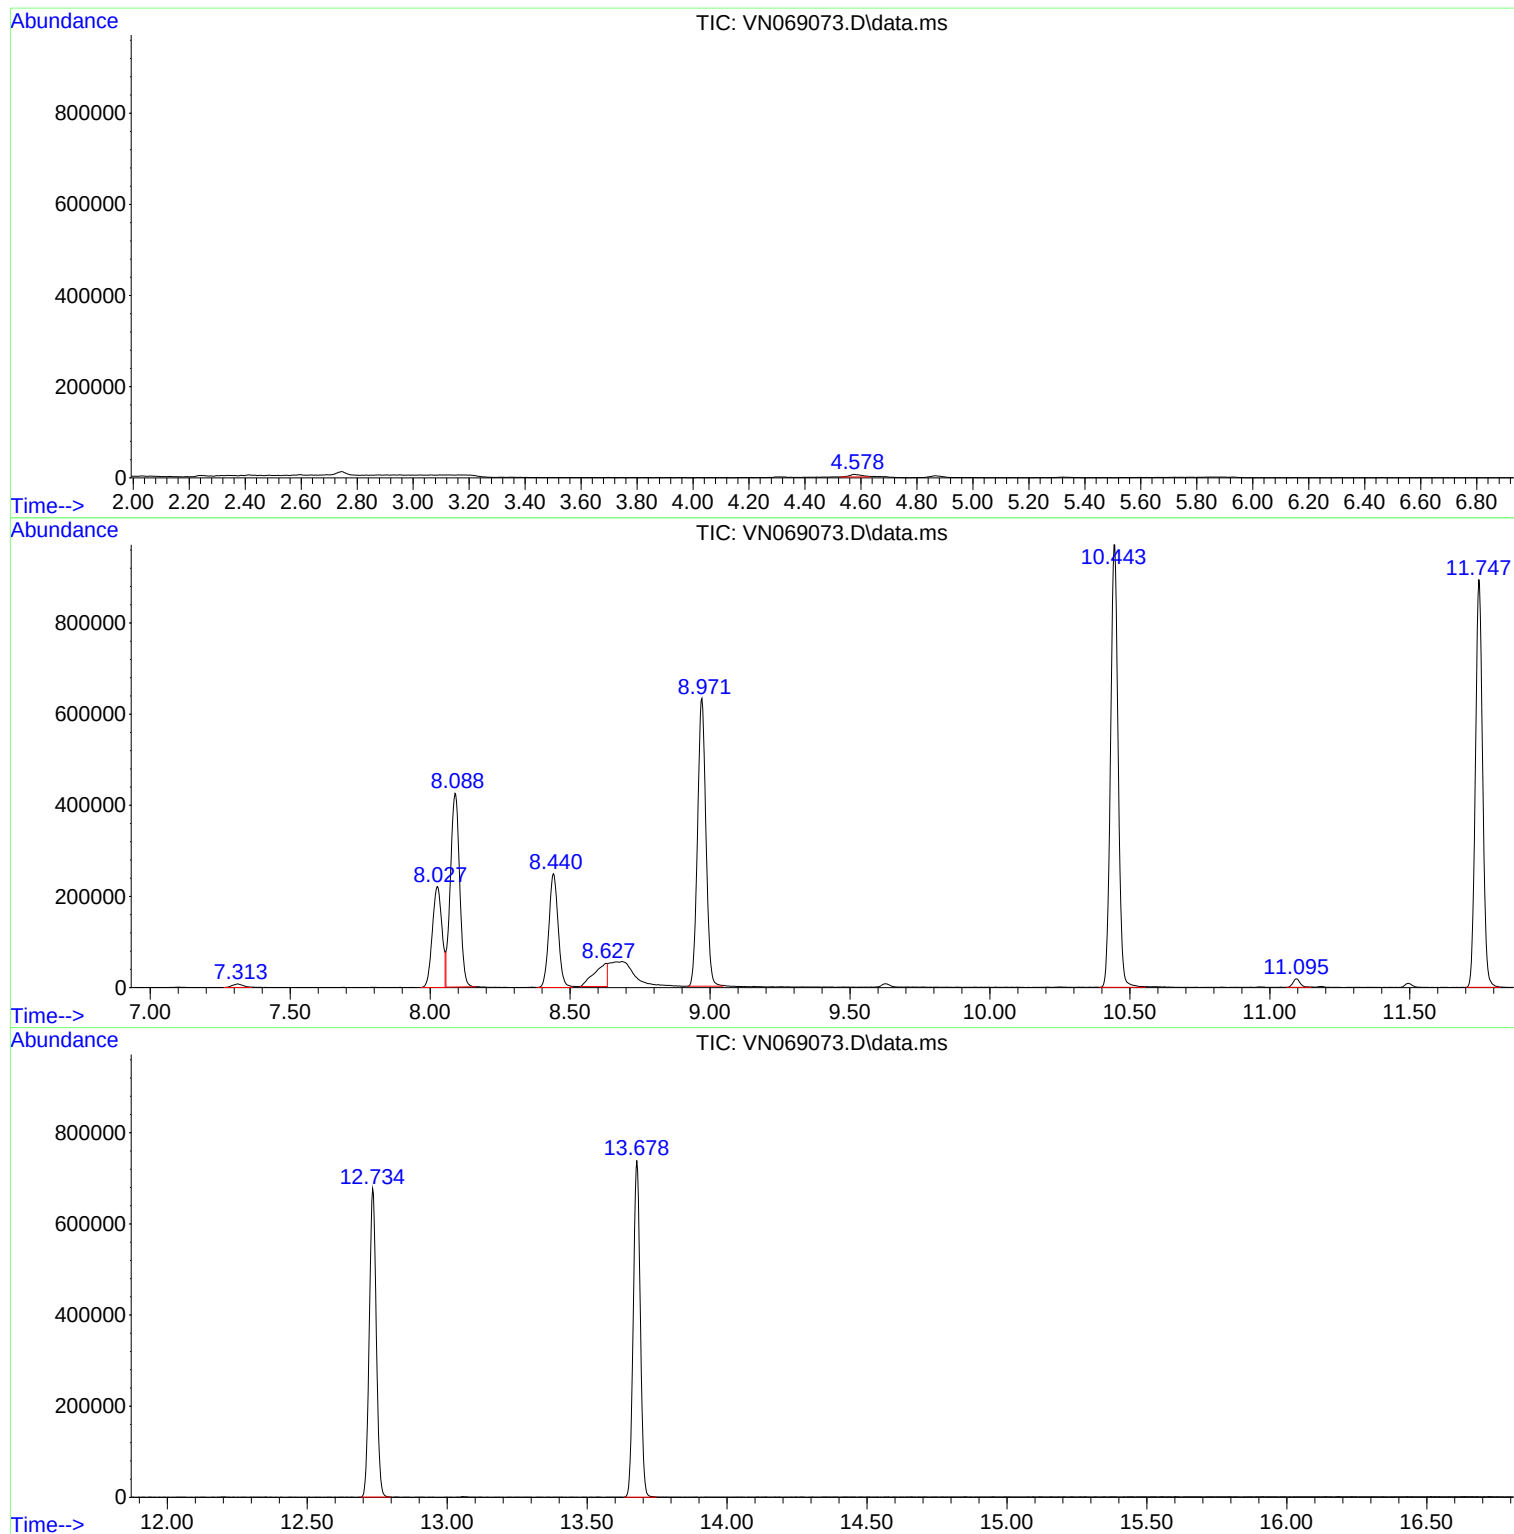

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102021\
Data File : VN069073.D
Acq On : 20 Oct 2021 19:57
Operator : JC/MD
Sample : M4253-05
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
135-136










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Acetic acid Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.627	6.33 ug/l	165546	1,4-Difluorobenzene	8.971

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Acetic acid	60	C2H4O2	000064-19-7	90
2			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	72
3			Ammonium acetate	77	C2H7NO2	000631-61-8	64
4			Hydrazine, 1,1-dimethyl-	60	C2H8N2	000057-14-7	5
5			Thiirane	60	C2H4S	000420-12-2	5

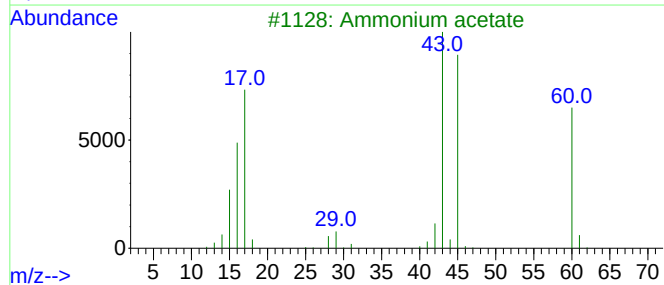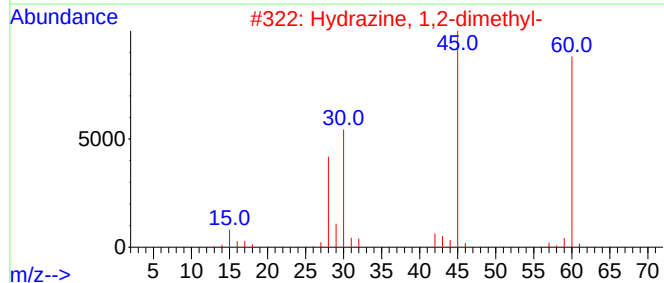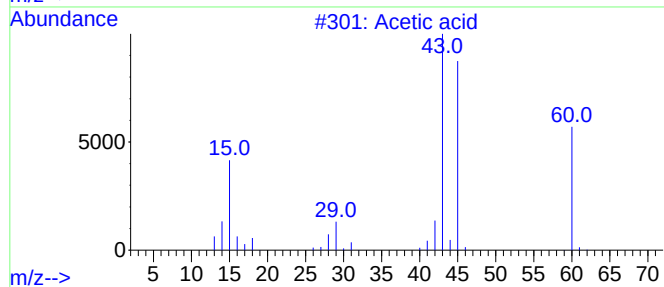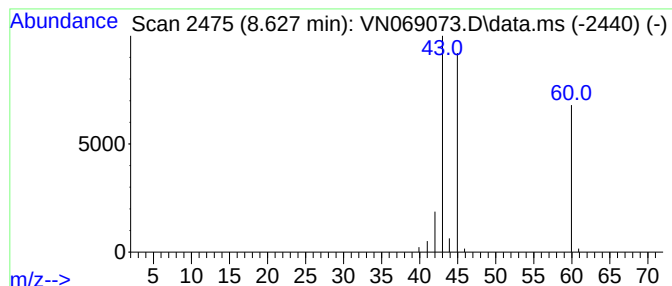

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102021\
Data File : VN069073.D
Acq On : 20 Oct 2021 19:57
Operator : JC/MD
Sample : M4253-05
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
135-136

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N101221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Acetic acid	8.627	6.3	ug/l	165546	2	8.971	1306800	50.0