

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102022\
 Data File : VN074946.D
 Acq On : 20 Oct 2022 16:52
 Operator : JC\MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102022W.M
 Title : SW846 8260

Signal : TIC: VN074946.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.295	36	41	46	rBV3	38942	75578	1.49%	0.259%
2	2.824	125	131	133	rBV2	70495	142487	2.82%	0.488%
3	2.865	136	138	147	rVB3	142630	270027	5.34%	0.924%
4	7.447	909	917	926	rBV	51090	159673	3.16%	0.546%
5	8.171	1031	1040	1045	rBV	714566	1736667	34.33%	5.942%
6	8.230	1045	1050	1063	rVB	1171175	2524235	49.90%	8.637%
7	8.582	1101	1110	1123	rBV	695792	1531639	30.28%	5.241%
8	9.106	1189	1199	1209	rBV	1660697	3495144	69.09%	11.959%
9	10.571	1436	1448	1456	rBV	2466019	4519853	89.35%	15.466%
10	11.865	1660	1668	1679	rBV	2712102	4734831	93.60%	16.201%
11	12.076	1695	1704	1710	rVV4	34945	76774	1.52%	0.263%
12	12.412	1753	1761	1765	rBV6	30456	65571	1.30%	0.224%
13	12.853	1827	1836	1845	rBV	2254593	3858556	76.28%	13.203%
14	13.123	1873	1882	1888	rBV6	27454	60934	1.20%	0.208%
15	13.223	1895	1899	1907	rVB4	39077	71000	1.40%	0.243%
16	13.482	1938	1943	1948	rVB2	33836	53352	1.05%	0.183%
17	13.735	1978	1986	1989	rBV4	61323	110835	2.19%	0.379%
18	13.794	1989	1996	2008	rVB	2980665	5058484	100.00%	17.309%
19	14.053	2034	2040	2045	rBV3	34378	64708	1.28%	0.221%
20	14.112	2045	2050	2056	rVB3	34359	61657	1.22%	0.211%
21	15.035	2202	2207	2213	rVB5	32306	53816	1.06%	0.184%
22	15.394	2261	2268	2276	rVB4	61160	108271	2.14%	0.370%
23	15.641	2301	2310	2320	rBV	112079	255926	5.06%	0.876%
24	15.841	2338	2344	2351	rVB3	66833	135227	2.67%	0.463%




Sum of corrected areas: 29225245

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102022\
Data File : VN074946.D
Acq On : 20 Oct 2022 16:52
Operator : JC\MD
Sample : IBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

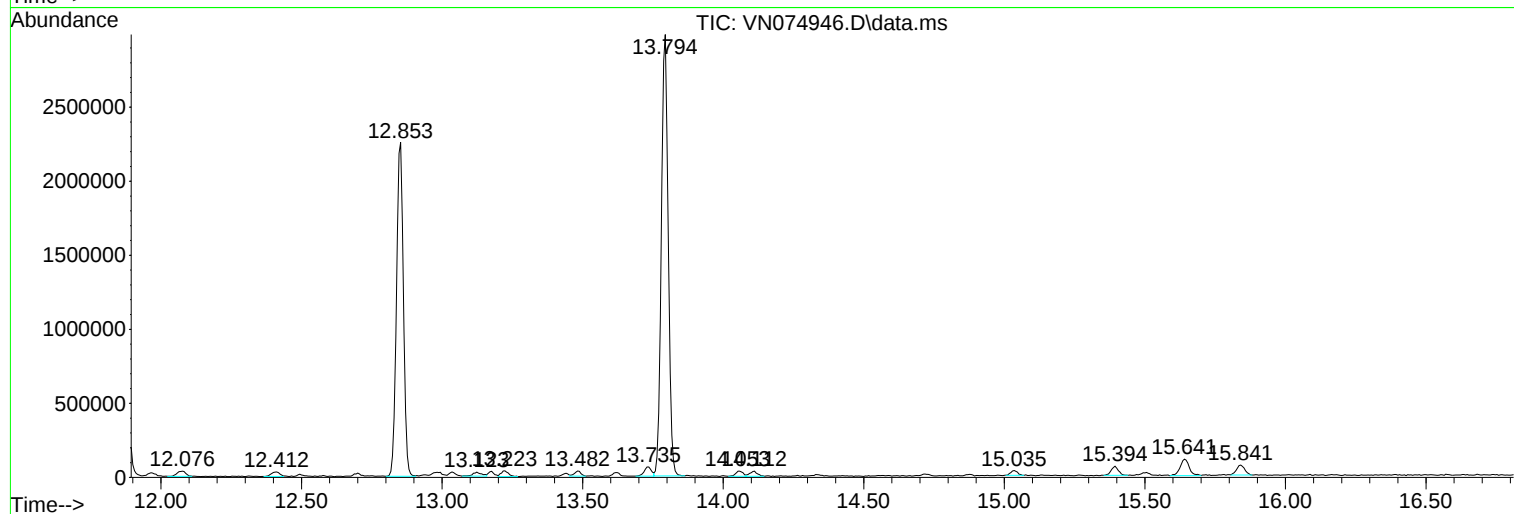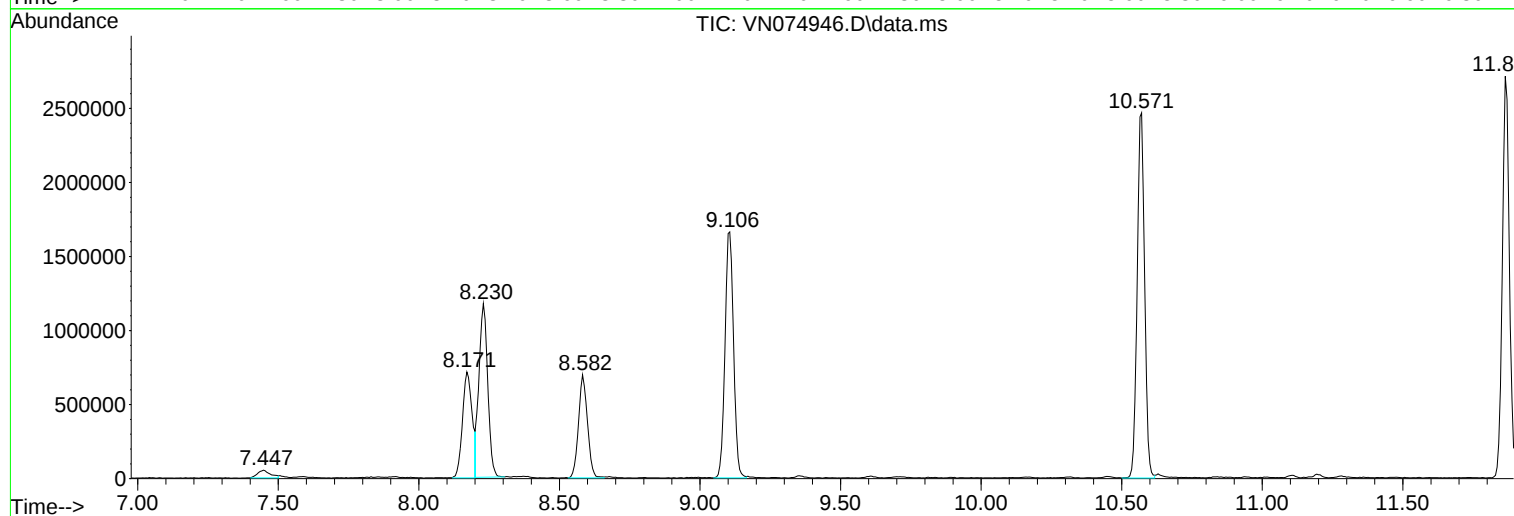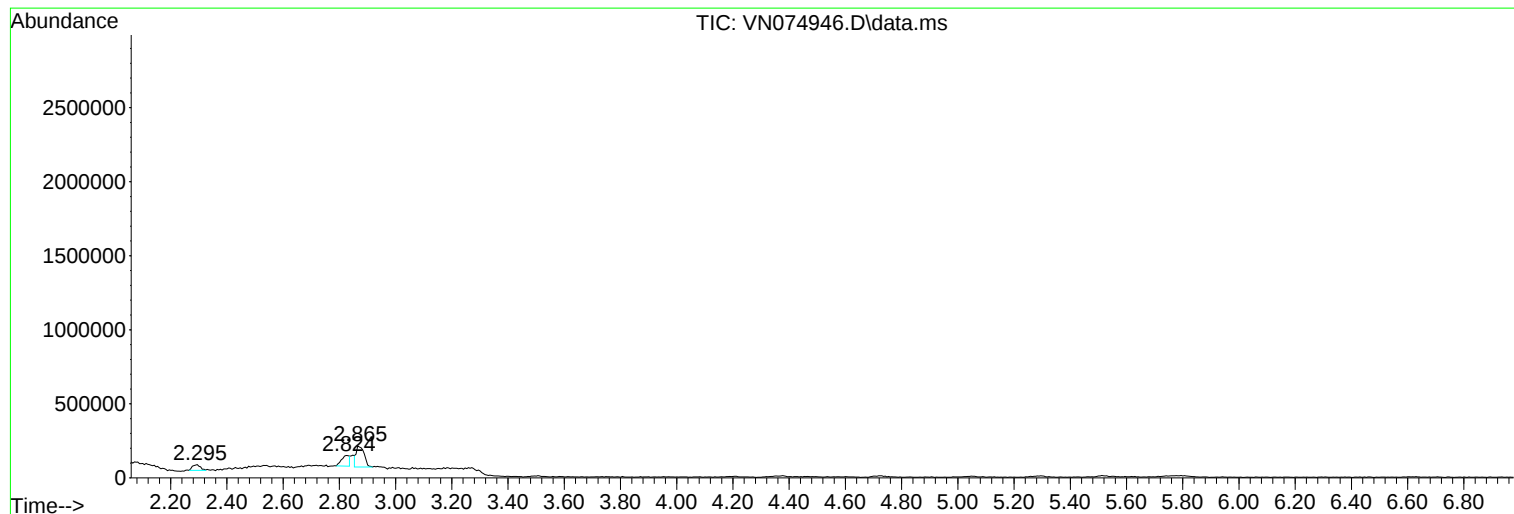

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN102022\
Data File : VN074946.D
Acq On : 20 Oct 2022 16:52
Operator : JC\MD
Sample : IBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	2.865	5.3	ug/l	270027	1	8.230	2524240	50.0